

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL050522\
 Data File : VL038967.D
 Acq On : 5 May 2022 11:18
 Operator : SY/AP
 Sample : N2682-01
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 1

Quant Time: May 06 07:27:07 2022
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL050522AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LThu May 05 07:41:27 2022
 QLast Update : Thu May 05 07:41:27 2022
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.66	49	1080793	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.16	114	2573066	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.07	117	2178233	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.39	95	1769921	10.26	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.60%


Target Compounds					Ovalue
2) Dichlorodifluoromethane	3.05	85	41601	0.246 ppbv	99
3) Chlorodifluoromethane	2.99	51	1163376	8.675 ppbv #	88
4) Chloromethane	3.14	50	20785	0.309 ppbv	99
9) Propene	3.02	41	52175	0.891 ppbv #	83
10) Heptane	8.10	43	24559	0.171 ppbv	93
11) Trichlorofluoromethane	3.95	101	32490	0.224 ppbv	93
13) Ethanol	3.60	45	622096	136.020 ppbv	96
15) Acetone	3.84	43	1231543	12.080 ppbv	99
16) 1,3-Butadiene	3.33	39	4473	0.076 ppbv #	1
17) tert-Butyl alcohol	3.96	59	108993	1.391 ppbv	99
19) Isopropyl Alcohol	3.95	45	3206644	66.152 ppbv	99
20) Methylene Chloride	4.34	84	237364	6.177 ppbv	97
21) Allyl Chloride	4.34	41	3856	0.056 ppbv #	20
23) Vinyl Acetate	5.05	43	36882	0.457 ppbv #	1
25) Ethyl Acetate	5.68	43	453665	1.859 ppbv #	81
26) Hexane	5.68	57	565902	5.219 ppbv #	43
29) Chloroform	5.74	83	5790	0.033 ppbv	93
30) Cyclohexane	7.12	84	4051	0.045 ppbv #	1
34) 2-Butanone	5.24	43	60654	0.462 ppbv #	34
36) Benzene	6.88	78	115577	0.525 ppbv #	92
39) 1,2-Dichloropropane	7.17	63	716888	8.367 ppbv #	26
41) Tetrahydrofuran	6.05	42	48974	0.555 ppbv	88
43) Methyl Methacrylate	8.00	69	499011	5.582 ppbv	95
44) 2,2,4-Trimethylpentane	7.85	57	21286	0.055 ppbv #	6
53) Toluene	9.79	91	294262	1.192 ppbv	98
58) Ethyl Benzene	12.69	91	29698	0.095 ppbv	91
59) m/p-Xylene	12.99	91	36361	0.136 ppbv #	33
60) o-Xylene	13.67	91	34323	0.136 ppbv #	32
61) Styrene	13.50	104	7960	0.059 ppbv #	25
72) 4-Ethyltoluene	15.82	105	20170	0.070 ppbv #	22
73) 1,3,5-Trimethylbenzene	15.97	105	10391	0.040 ppbv #	33
74) 1,2,4-Trimethylbenzene	16.74	105	109370	0.387 ppbv #	67
80) Naphthalene,2-methyl-	24.95	142	4457	0.064 ppbv #	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL050522\
Data File : VL038967.D
Acq On : 5 May 2022 11:18
Operator : SY/AP
Sample : N2682-01
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
1

Quant Time: May 06 07:27:07 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL050522AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 05 07:41:27 2022
QLast Update : Thu May 05 07:41:27 2022
Response via : Initial Calibration

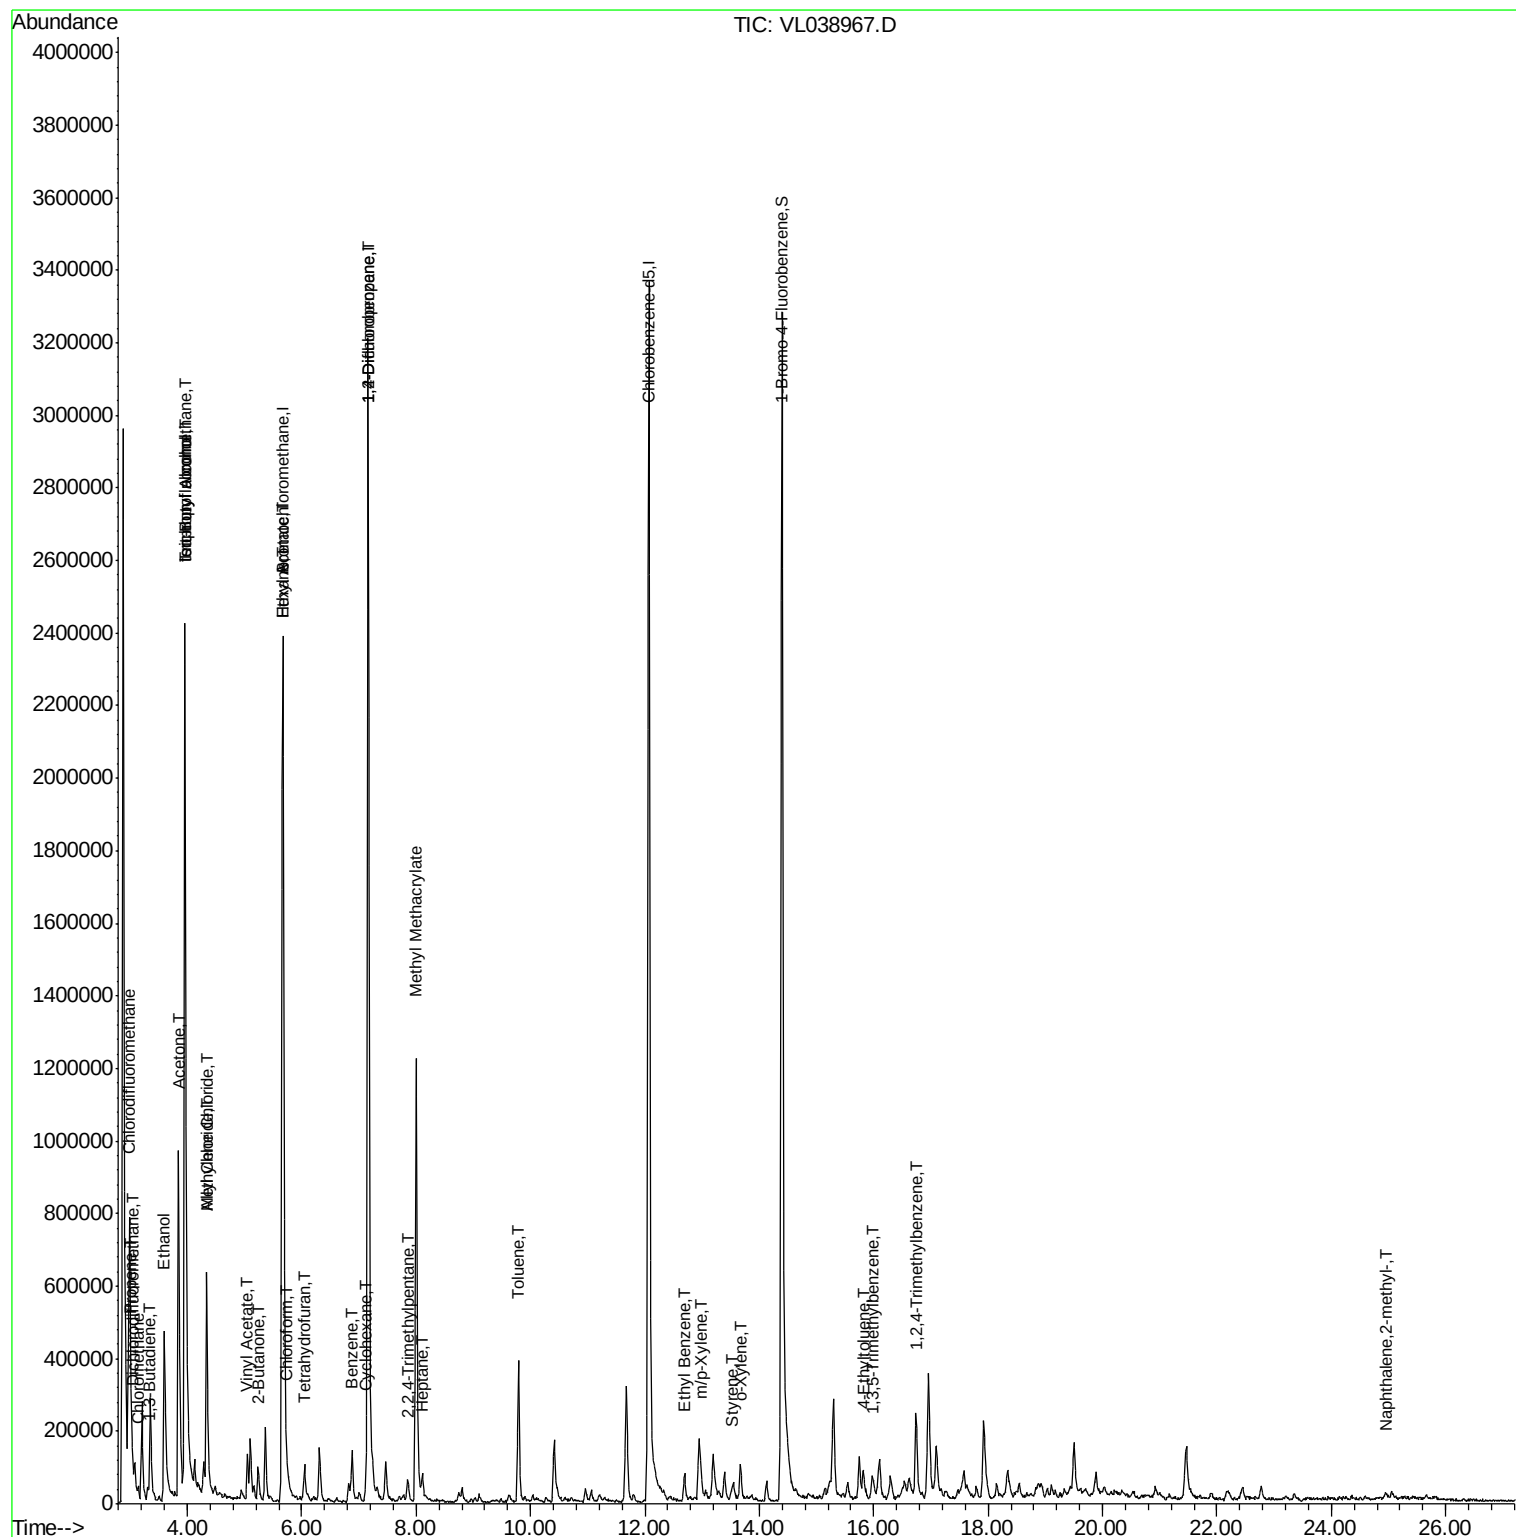

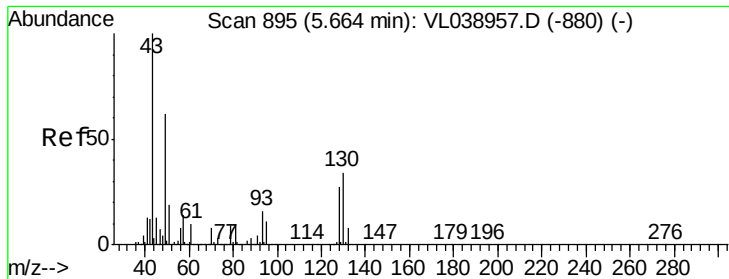

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.66 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 5 May 2022 11:18


Tot Ion: 49 Resp: 1080793

Ion Ratio Lower Upper

49 100

128 46.0 23.3 69.8




130 59.8 29.8 89.3

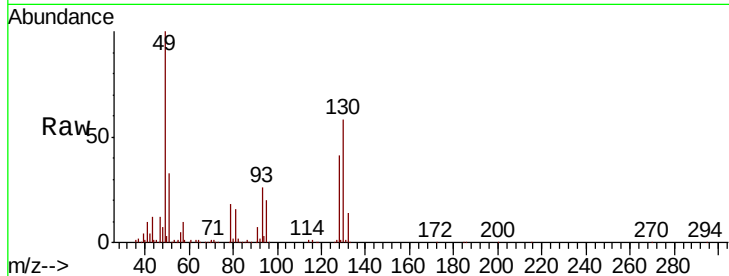

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

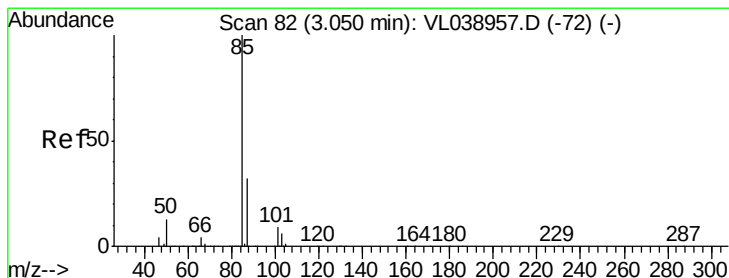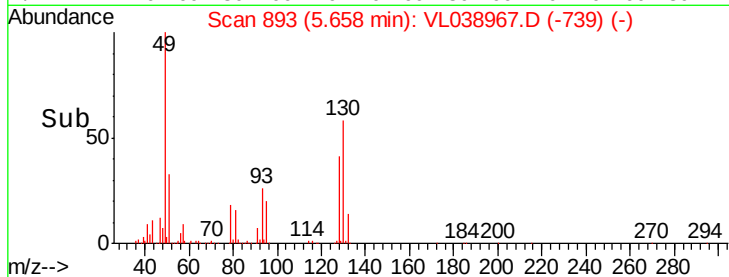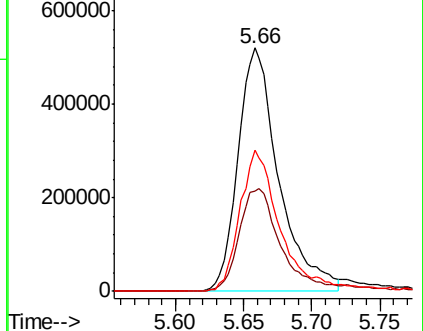

#2

Dichlorodifluoromethane

Concen: 0.246 ppbv

RT: 3.05 min Scan# 81

Delta R.T. -0.00 min

Lab File: VL038967.D


Acq: 5 May 2022 11:18

Tgt Ion: 85 Resp: 41601

Ion Ratio Lower Upper



85 100


87 31.3 25.7 38.5

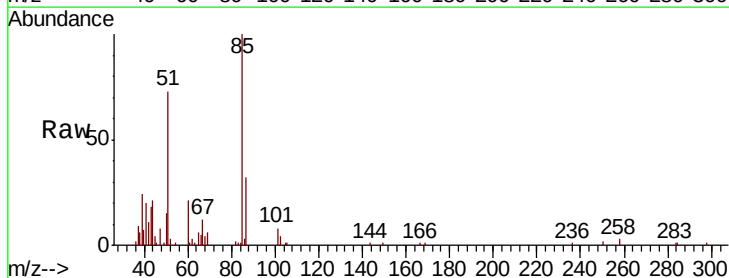

Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

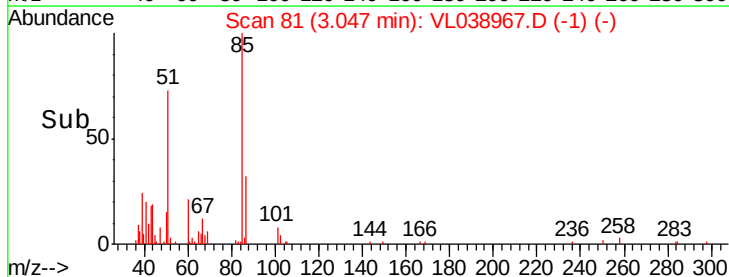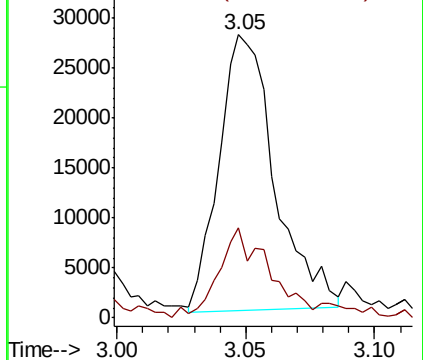

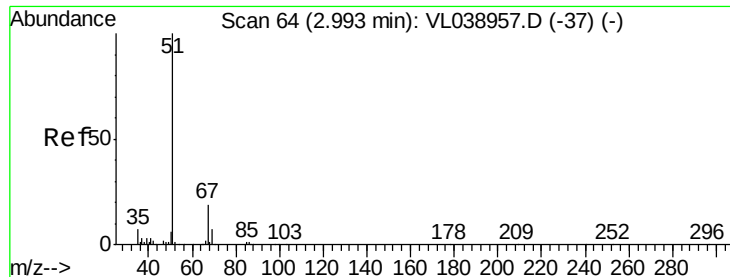

#3

Chlorodifluoromethane

Concen: 8.675 ppbv

RT: 2.99 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:





Acq: 5 May 2022 11:18

Tot Ion: 51 Resp: 1163376

Ion Ratio Lower Upper

51 100

67 14.5 15.8 23.8#

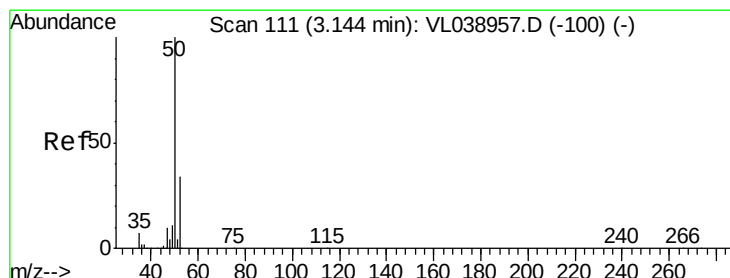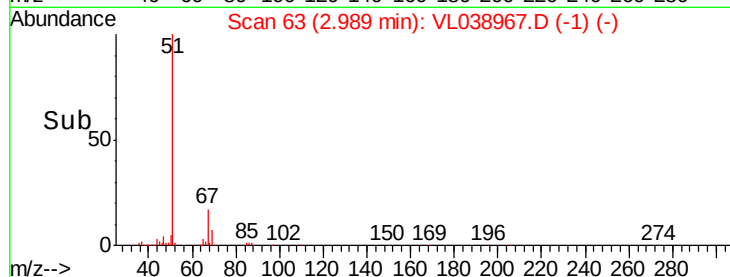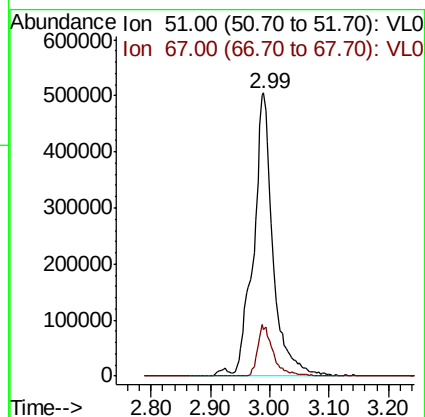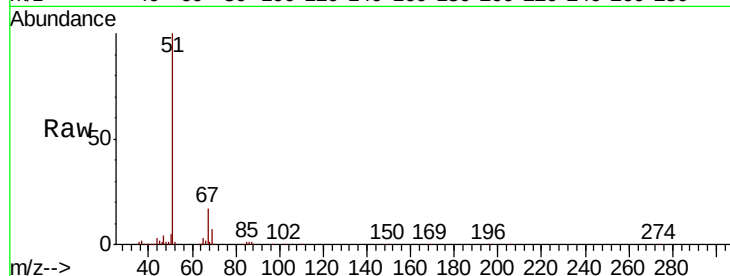

#4

Chloromethane

Concen: 0.309 ppbv

RT: 3.14 min Scan# 111

Delta R.T. 0.00 min

Lab File: VL038967.D




Acq: 5 May 2022 11:18


Tgt Ion: 50 Resp: 20785

Ion Ratio Lower Upper

50 100

52 33.7 27.3 40.9

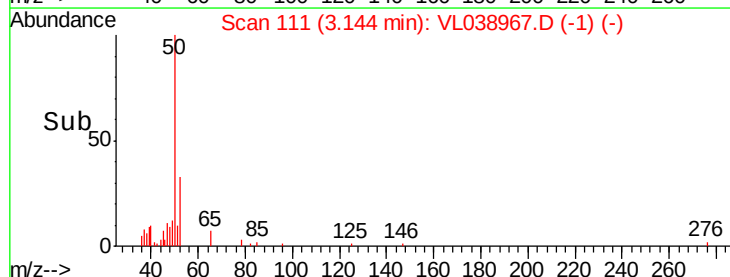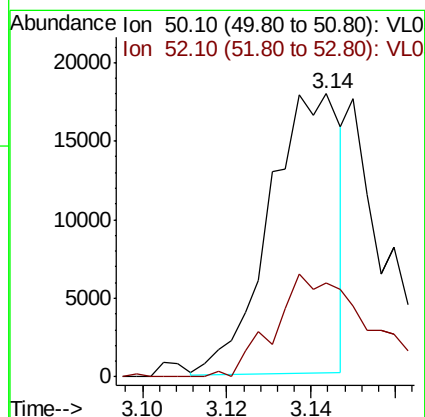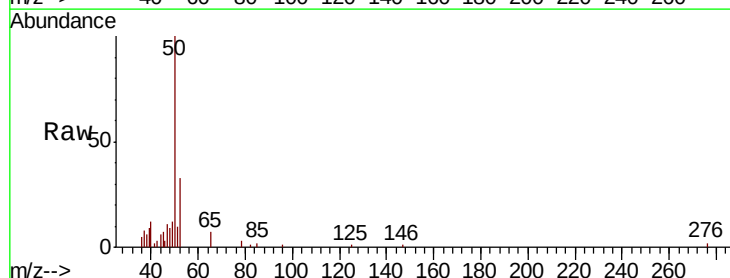

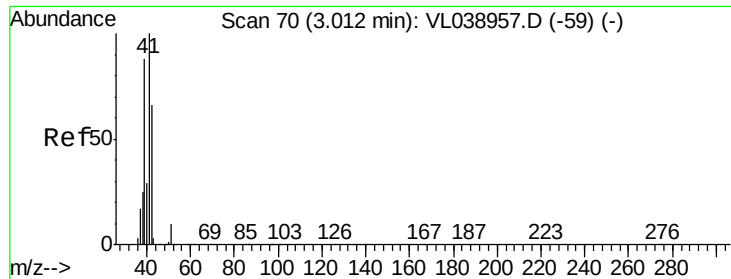

#9

Propene

Concen: 0.891 ppbv

RT: 3.02 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:





Acq: 5 May 2022 11:18

Tot Ion: 41 Resp: 52175

Ion Ratio Lower Upper

41 100

42 58.2 58.3 87.5#

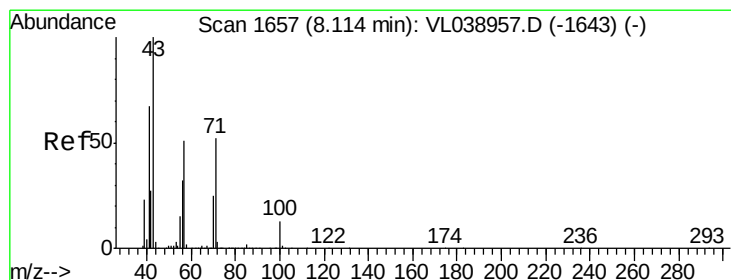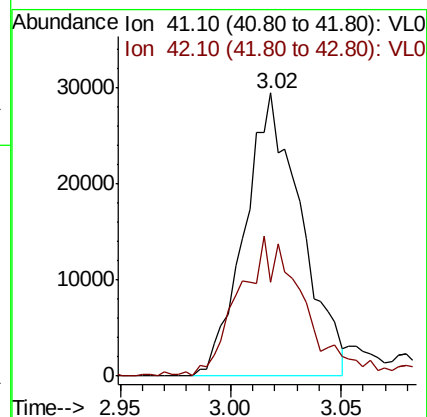

#10

Heptane

Concen: 0.171 ppbv

RT: 8.10 min Scan# 1654

Delta R.T. -0.01 min

Lab File: VL038967.D




Acq: 5 May 2022 11:18


Tgt Ion: 43 Resp: 24559

Ion Ratio Lower Upper

43 100





57 55.3 40.5 60.7

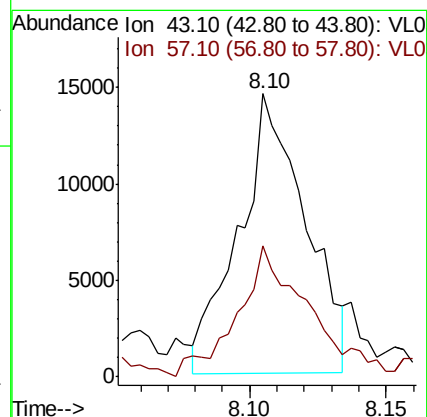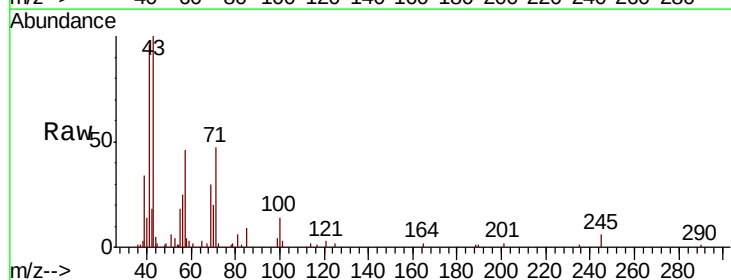






#11
 Trichlorofluoromethane
 Concen: 0.224 ppbv
 RT: 3.95 min
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 Acq: 5 May 2022 11:18


Tot Ion: 101 Resp: 32490
 Ion Ratio Lower Upper
 101 100
 103 70.1 51.5 77.3

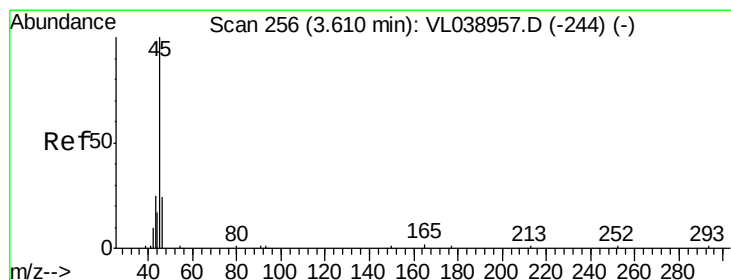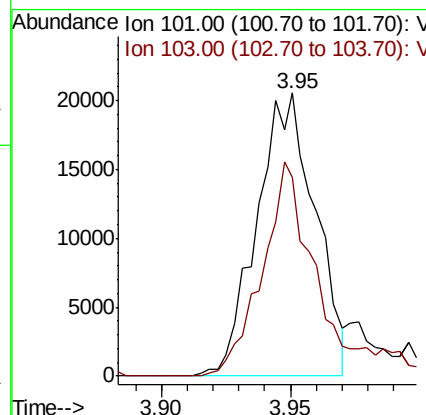

#13
 Ethanol
 Concen: 136.020 ppbv
 RT: 3.60 min Scan# 252
 Delta R.T. -0.01 min
 Lab File: VL038967.D
 Acq: 5 May 2022 11:18

Tgt Ion: 45 Resp: 622096
 Ion Ratio Lower Upper
 45 100
 46 42.6 18.0 72.2

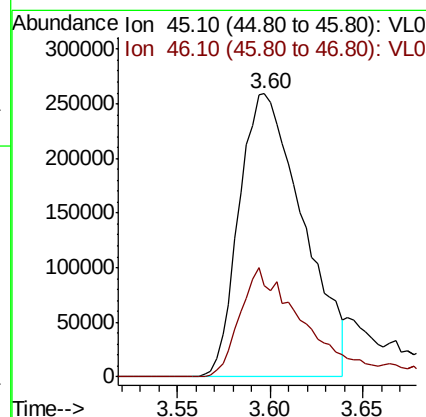



#15

Acetone

Concen: 12.080 ppbv

RT: 3.84 Instrument: MSVOA_1

Delta R.T. 0.00 min

Lab File: ClientSampleId: 1


Acq: 5 May 2022 11:18

Tot Ion: 43 Resp: 1231543

Ion Ratio Lower Upper




43 100

58 26.3 21.3 31.9

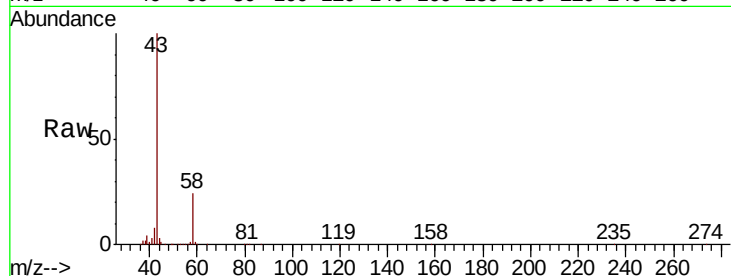

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 58.10 (57.80 to 58.80): VL0

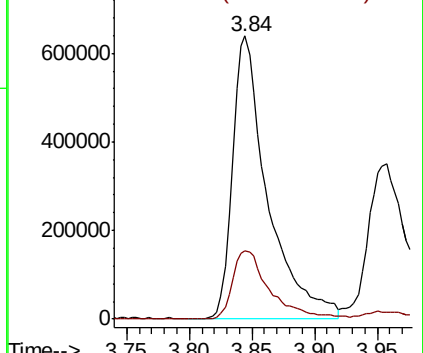

#16

1,3-Butadiene

Concen: 0.076 ppbv

RT: 3.33 min Scan# 168

Delta R.T. 0.00 min

Lab File: VL038967.D


Acq: 5 May 2022 11:18

Tgt Ion: 39 Resp: 4473

Ion Ratio Lower Upper



39 100


54 230.4 65.2 97.8#



Abundance Ion 39.10 (38.80 to 39.80): VL0

Ion 54.10 (53.80 to 54.80): VL0

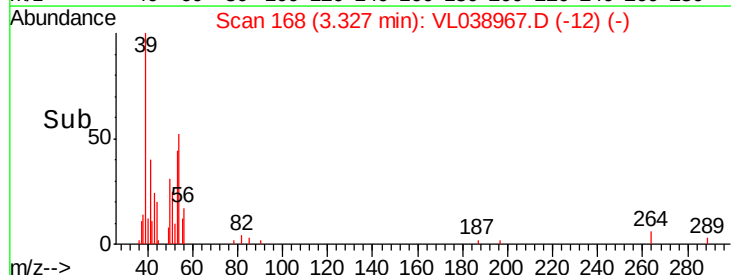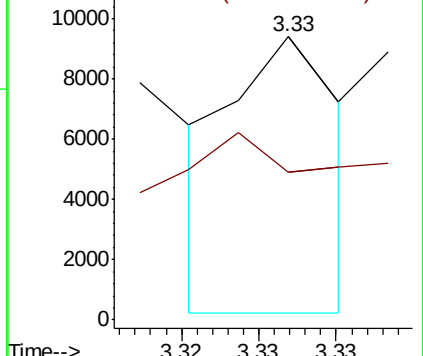



#17

tert-Butyl alcohol

Concen: 1.391 ppbv

RT: 3.96 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:




Acq: 5 May 2022 11:18

Tot Ion: 59 Resp: 108993

Ion Ratio Lower Upper

59 100

57 11.2 9.2 13.8

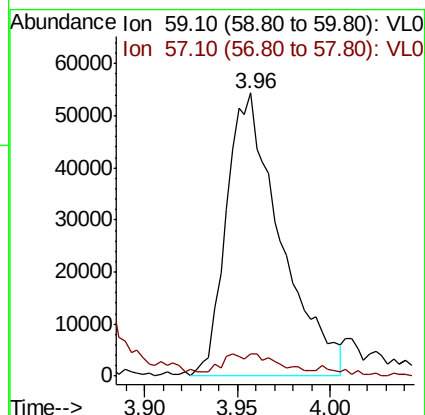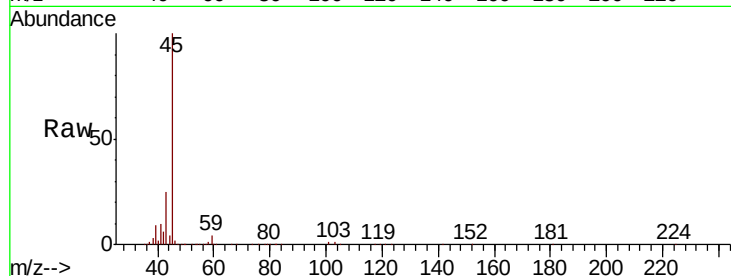

#19

Isopropyl Alcohol

Concen: 66.152 ppbv

RT: 3.95 min Scan# 363

Delta R.T. -0.00 min

Lab File: VL038967.D





Acq: 5 May 2022 11:18


Tgt Ion: 45 Resp: 3206644

Ion Ratio Lower Upper

45 100

58 1.6 1.4 2.2

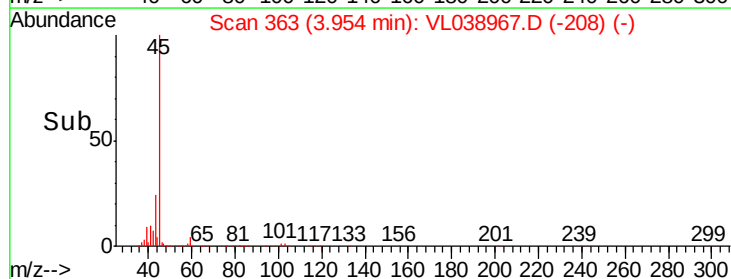
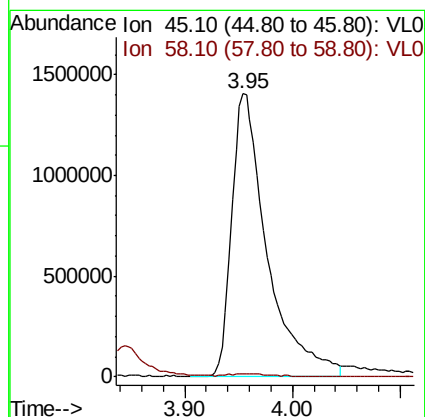



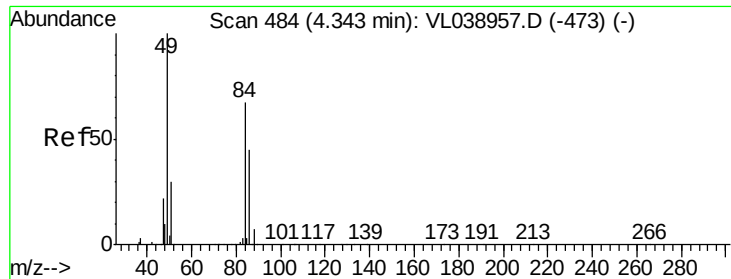

#20
Methylene Chloride
Concen: 6.177 ppbv
RT: 4.34
Delta R.T. MSVOA_1
Lab File: ClientSampleId :
Acq: 5 May 2022 11:18

Tot Ion: 84 Resp: 237364





Ion	Ratio	Lower	Upper
84	100		
49	154.8	119.9	179.9
51	46.2	35.7	53.5
86	67.7	53.8	80.6

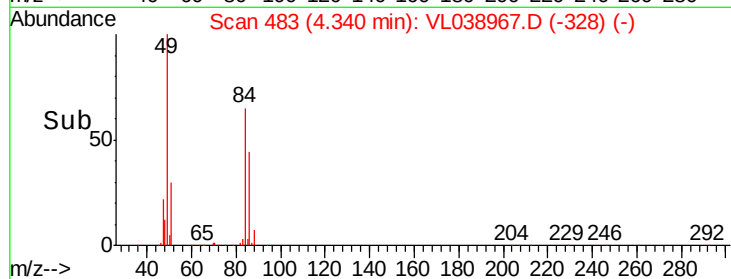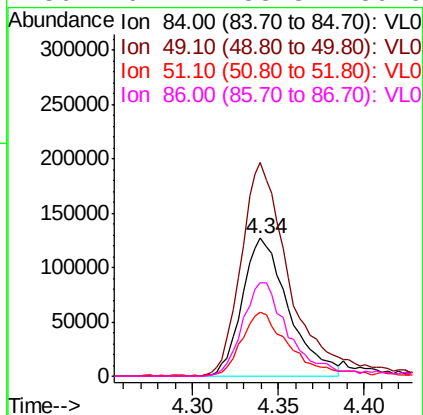


#21
Allyl Chloride
Concen: 0.056 ppbv
RT: 4.34 min Scan# 483
Delta R.T. -0.07 min
Lab File: VL038967.D
Acq: 5 May 2022 11:18

Tgt Ion: 41 Resp: 3856

Ion	Ratio	Lower	Upper
41	100		
76	2.3	24.2	36.4#
39	0.0	63.8	95.8#

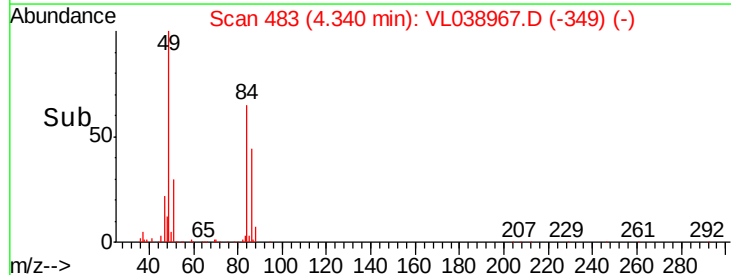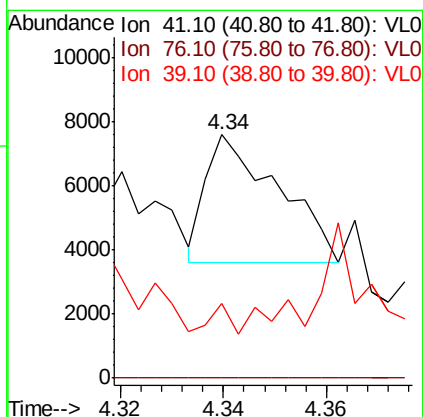

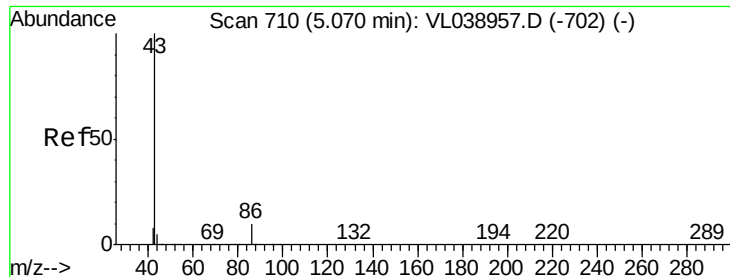

#23

Vinyl Acetate

Concen: 0.457 ppbv

RT: 5.05 Instrument: MSVOA_1


Delta R.T.

Lab File: ClientSampleId:

Acq: 5 May 2022 11:18

Tot Ion: 43 Resp: 36882

Ion	Ratio	Lower	Upper
43	100		
86	7.1	6.6	9.8
42	184.1	8.1	12.1#
44	2.2	3.5	5.3#



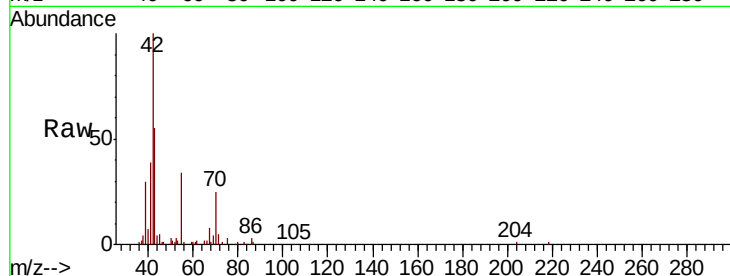


Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 86.10 (85.80 to 86.80): VL0

Ion 42.10 (41.80 to 42.80): VL0

Ion 44.10 (43.80 to 44.80): VL0

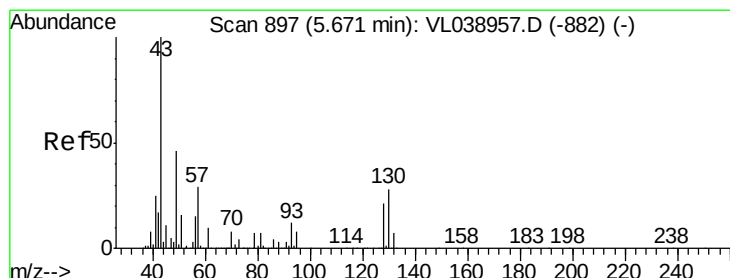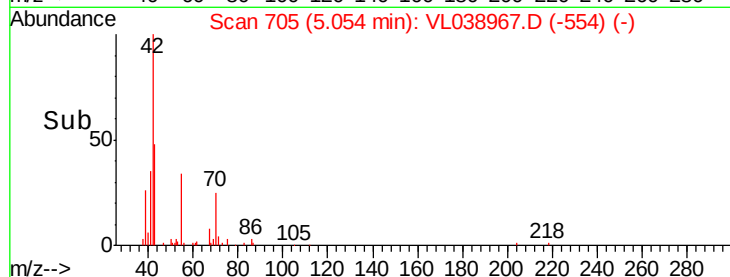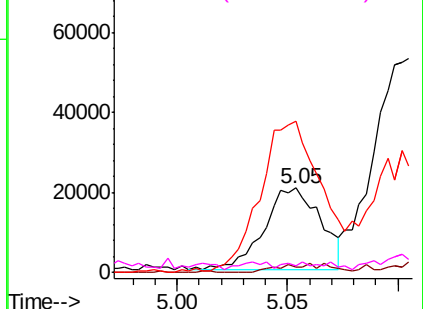

#25

Ethyl Acetate

Concen: 1.859 ppbv

RT: 5.68 min Scan# 900


Delta R.T. 0.01 min

Lab File: VL038967.D

Acq: 5 May 2022 11:18

Tgt Ion: 43 Resp: 453665

Ion	Ratio	Lower	Upper
43	100		
45	2.8	8.1	12.1#
61	1.8	7.8	11.6#
70	2.1	5.6	8.4#


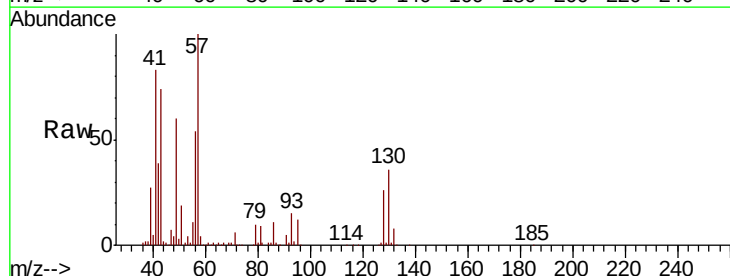



Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 45.10 (44.80 to 45.80): VL0

Ion 61.10 (60.80 to 61.80): VL0

Ion 70.10 (69.80 to 70.80): VL0

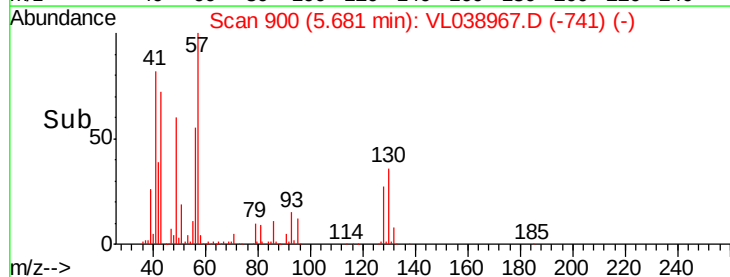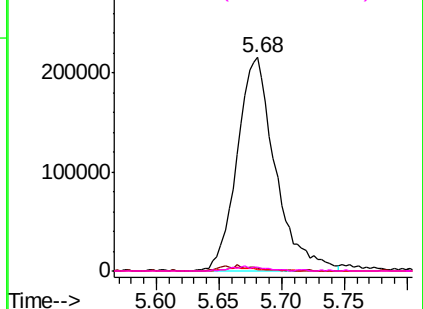



#26

Hexane

Concen: 5.219 ppbv

RT: 5.68 Instrument:


Delta R.T. MSVOA_1

Lab File: ClientSampleId:



Acq: 5 May 2022 11:18

Tot Ion: 57 Resp: 565902

Ion	Ratio	Lower	Upper
57	100		
41	93.8	75.2	112.8
43	81.7	190.8	286.2#
56	54.5	43.0	64.6

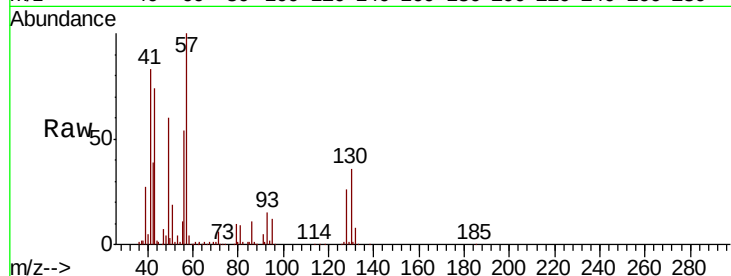

Abundance Ion 57.10 (56.80 to 57.80): VL0
 Ion 41.10 (40.80 to 41.80): VL0
 Ion 43.10 (42.80 to 43.80): VL0
 Ion 56.10 (55.80 to 56.80): VL0

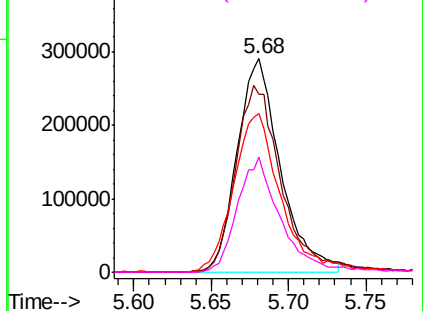

#29

Chloroform

Concen: 0.033 ppbv

RT: 5.74 min Scan# 918



Delta R.T. -0.01 min

Lab File: VL038967.D



Acq: 5 May 2022 11:18


Tgt Ion: 83 Resp: 5790

Ion	Ratio	Lower	Upper
83	100		
85	59.3	51.8	77.6

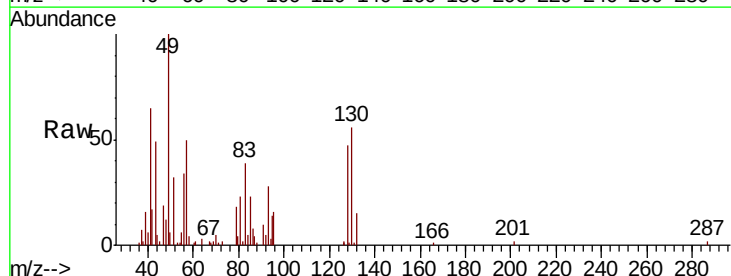





Abundance Ion 83.00 (82.70 to 83.70): VL0
 Ion 85.00 (84.70 to 85.70): VL0

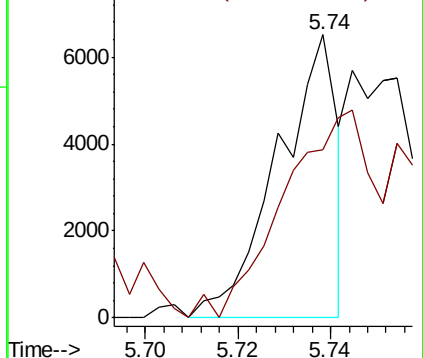

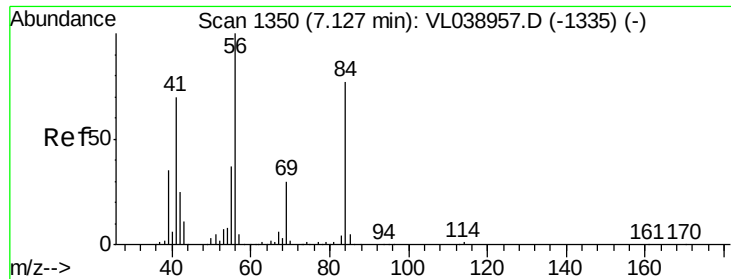




#30
Cyclohexane
Concen: 0.045 ppbv
RT: 7.12 min
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 5 May 2022 11:18


Tot Ion	Ratio	Lower	Upper
84	100		
56	0.0	115.3	172.9#
41	331.5	72.0	108.0#

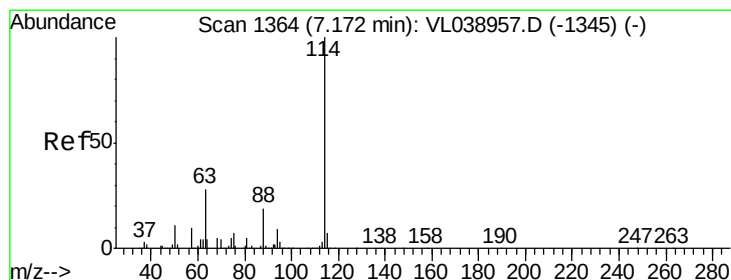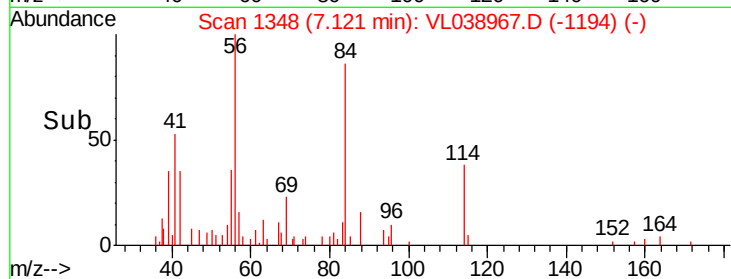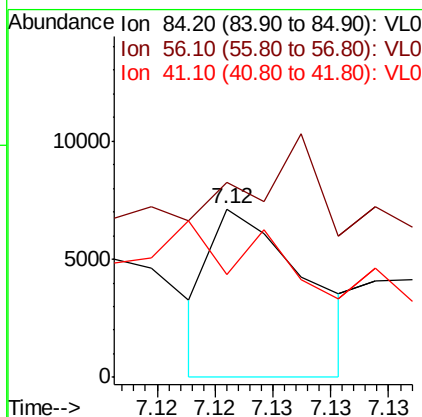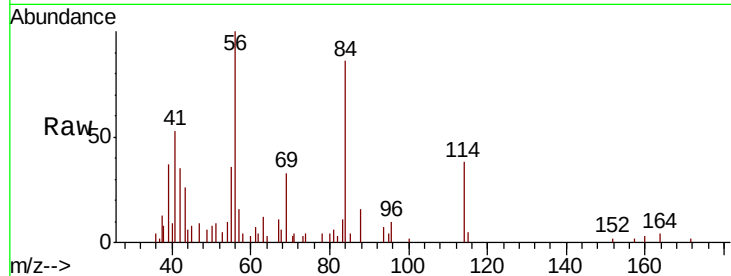

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.16 min Scan# 1361
Delta R.T. -0.01 min
Lab File: VL038967.D
Acq: 5 May 2022 11:18





Tgt Ion	Ratio	Lower	Upper
114	100		
63	28.6	22.6	33.8
88	19.4	15.4	23.0

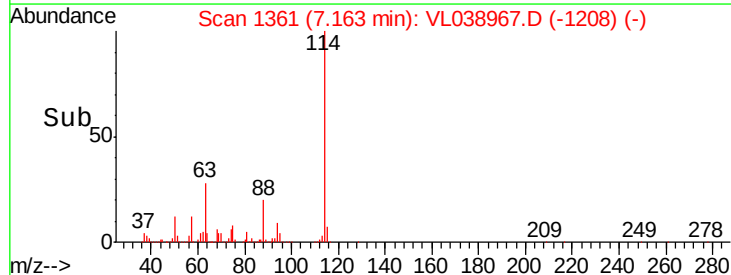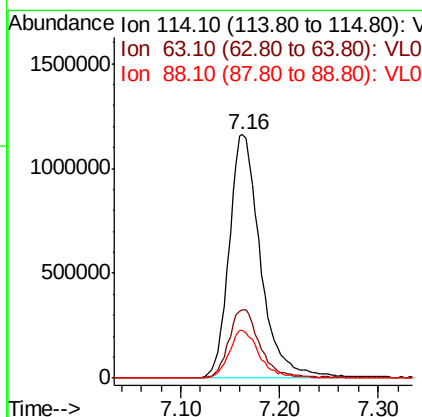

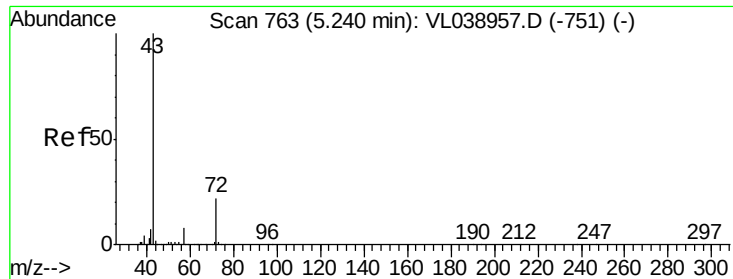




#34
 2-Butanone
 Concen: 0.462 ppbv
 RT: 5.24
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 Acq: 5 May 2022 11:18


Tot Ion: 43 Resp: 60654
 Ion Ratio Lower Upper
 43 100
 72 54.0 17.8 26.6#

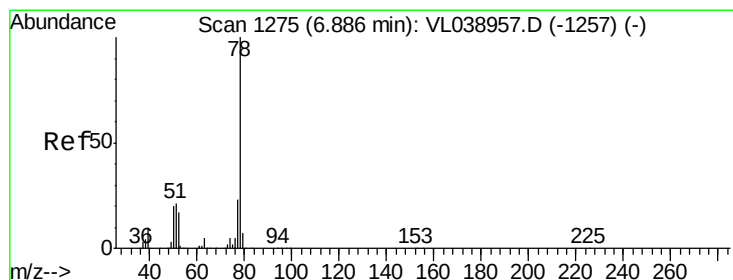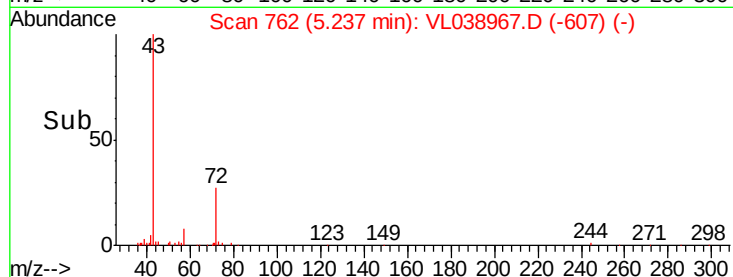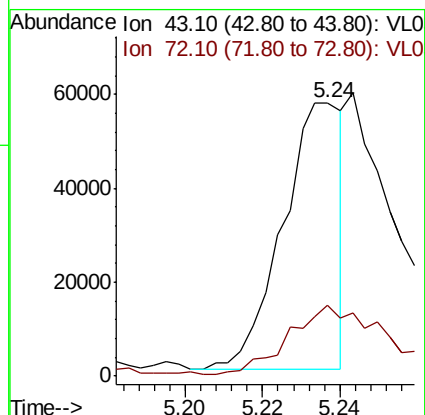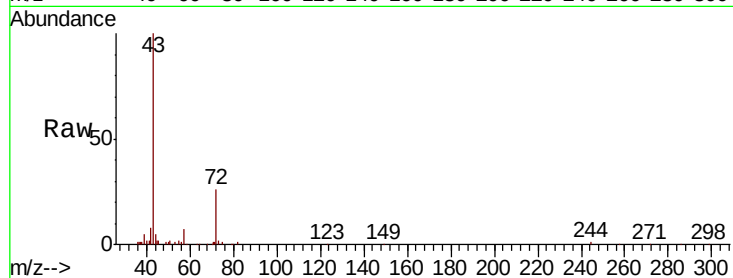

#36
 Benzene
 Concen: 0.525 ppbv
 RT: 6.88 min Scan# 1272
 Delta R.T. -0.01 min
 Lab File: VL038967.D
 Acq: 5 May 2022 11:18

Tgt Ion: 78 Resp: 115577
 Ion Ratio Lower Upper
 78 100
 77 17.1 18.6 28.0#
 50 18.6 15.6 23.4

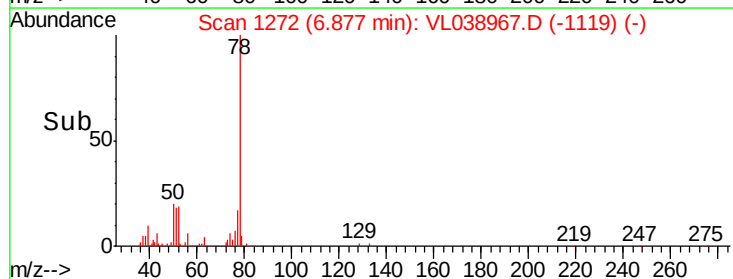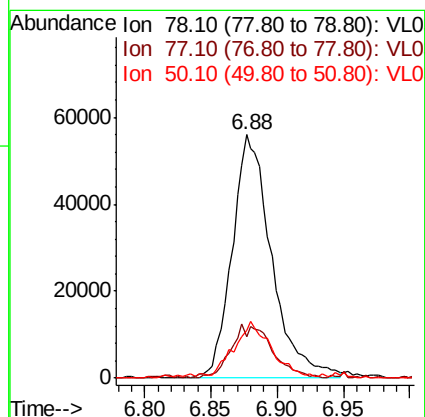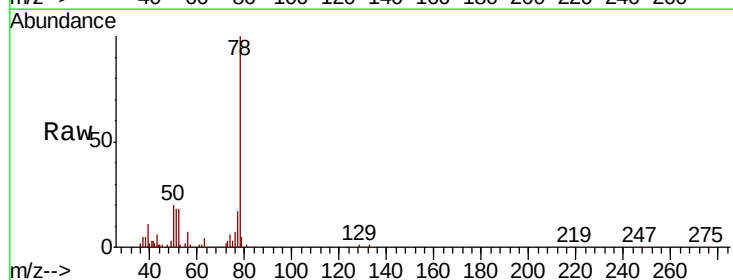



#39

1,2-Dichloropropane

Concen: 8.367 ppbv

RT: 7.17 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 5 May 2022 11:18





Tot Ion: 63 Resp: 716888

Ion Ratio Lower Upper

63 100

41 0.0 55.9 83.9#

62 17.4 53.8 80.6#

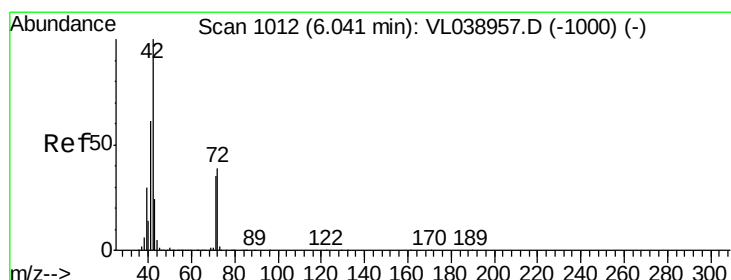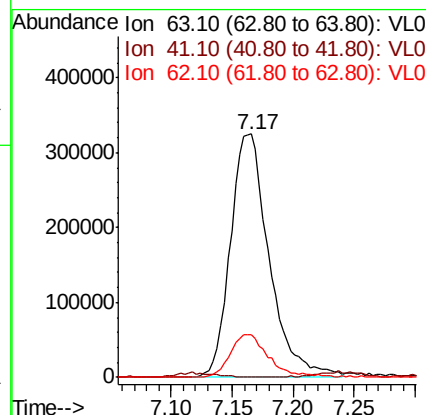

#41

Tetrahydrofuran

Concen: 0.555 ppbv

RT: 6.05 min Scan# 1014

Delta R.T. 0.01 min

Lab File: VL038967.D

Acq: 5 May 2022 11:18




Tgt Ion: 42 Resp: 48974


Ion Ratio Lower Upper

42 100

72 46.8 31.8 47.6

71 45.6 30.6 45.8

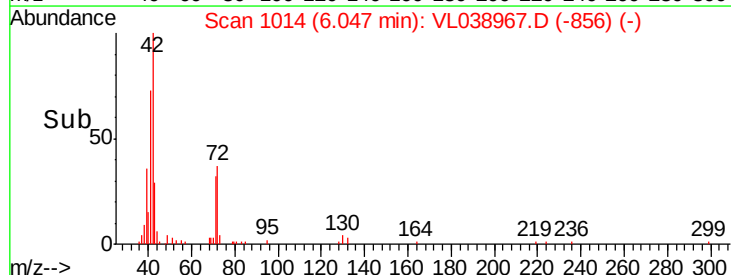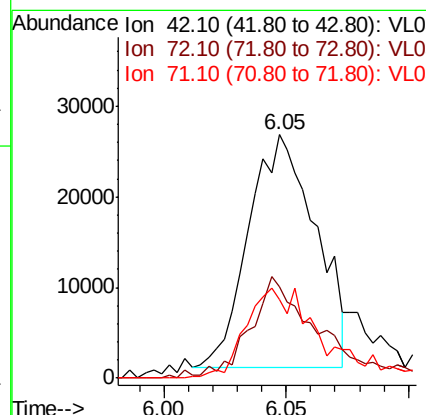

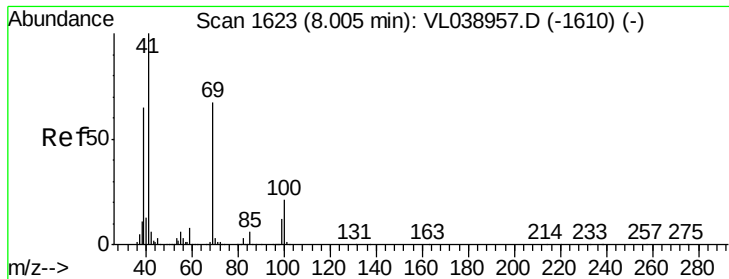

#43

Methyl Methacrylate

Concen: 5.582 ppbv

RT: 8.00 Instrument:

Delta R.T. MSVOA_1

Lab File: ClientSampleId:

Acq: 5 May 2022 11:18


Tot Ion: 69 Resp: 499011

Ion Ratio Lower Upper

69 100

41 159.7 121.9 182.9




100 28.8 24.6 36.8

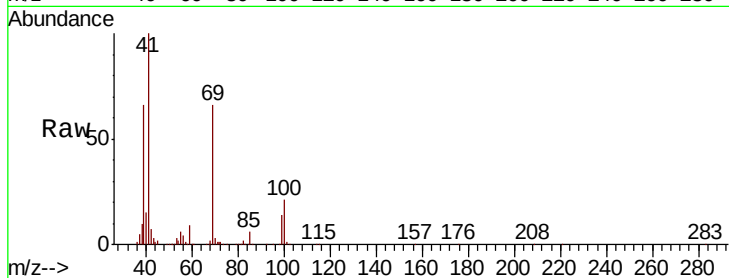

Abundance Ion 69.10 (68.80 to 69.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 100.10 (99.80 to 100.80): VL0

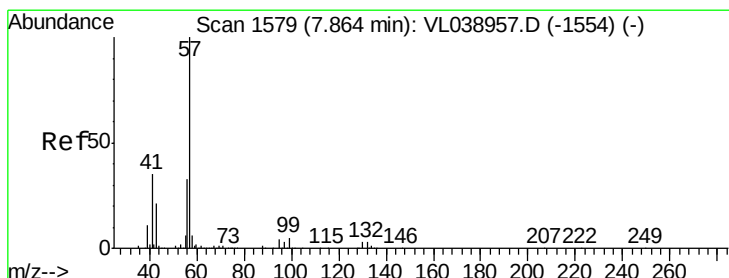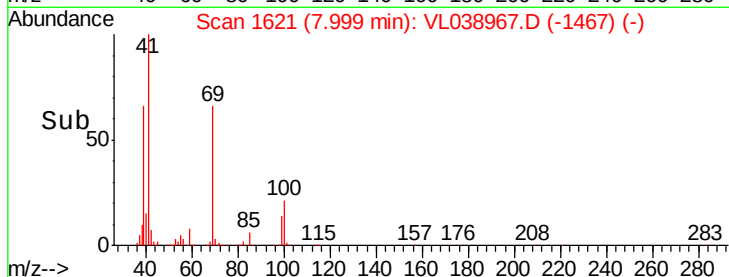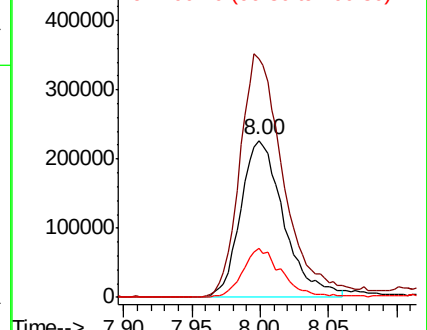

#44

2,2,4-Trimethylpentane

Concen: 0.055 ppbv

RT: 7.85 min Scan# 1576

Delta R.T. -0.01 min

Lab File: VL038967.D

Acq: 5 May 2022 11:18


Tgt Ion: 57 Resp: 21286

Ion Ratio Lower Upper

57 100

41 0.0 26.3 39.5#



56 103.7 24.6 37.0#

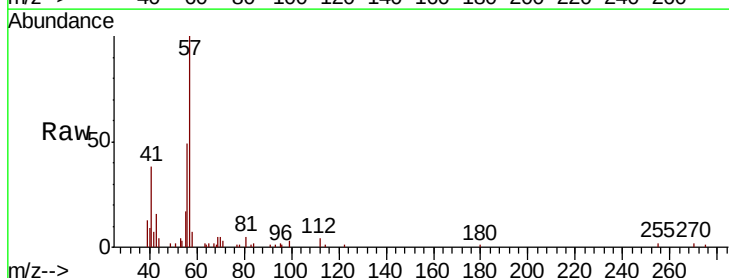


Abundance Ion 57.10 (56.80 to 57.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 56.10 (55.80 to 56.80): VL0

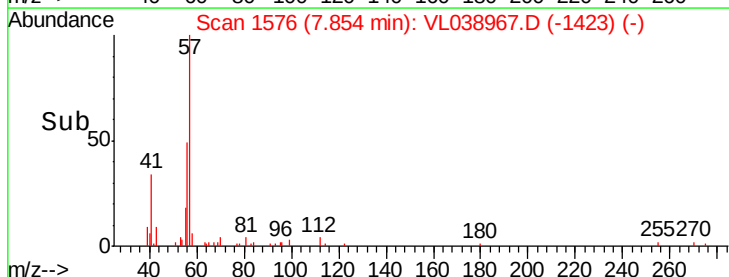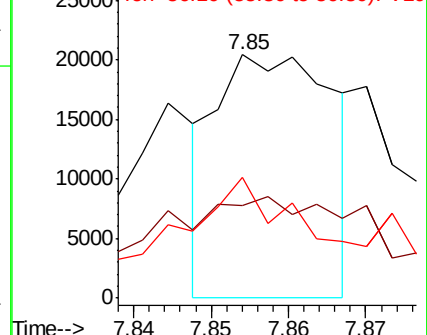



#53

Toluene

Concen: 1.192 ppbv

RT: 9.79 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:





Acq: 5 May 2022 11:18

Tot Ion: 91 Resp: 294262

Ion Ratio Lower Upper

91 100

92 61.7 48.2 72.2

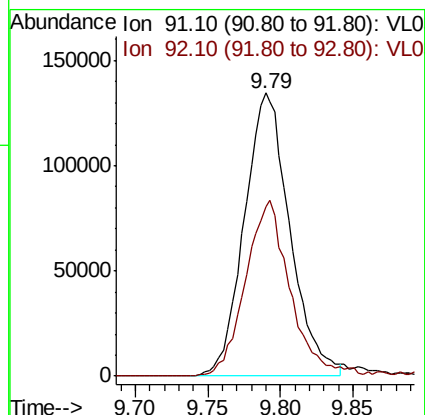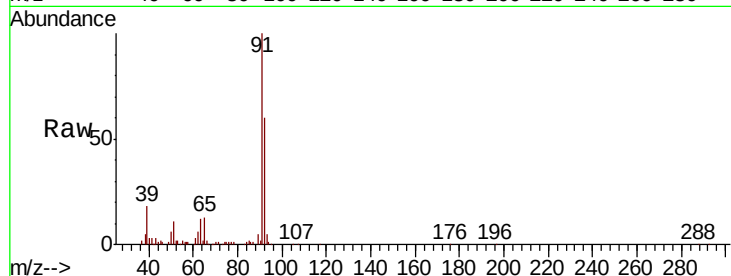

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.07 min Scan# 2886

Delta R.T. -0.01 min

Lab File: VL038967.D

Acq: 5 May 2022 11:18




Tgt Ion: 117 Resp: 2178233


Ion Ratio Lower Upper

117 100

82 75.0 57.0 85.6





119 34.0 27.2 40.8

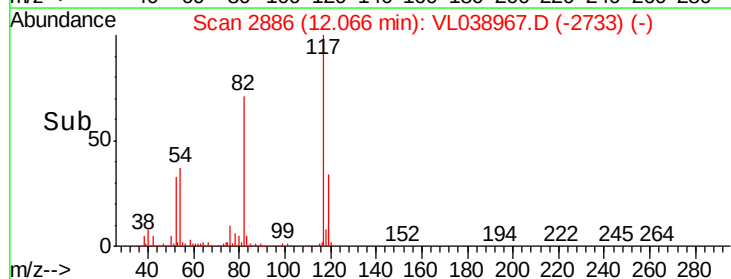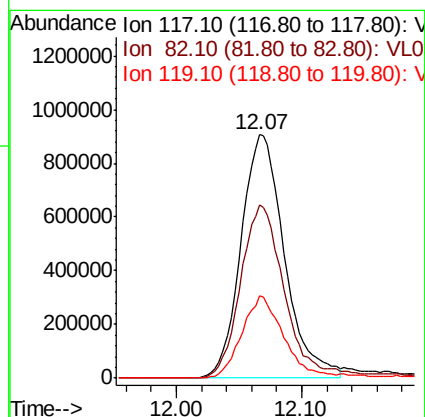

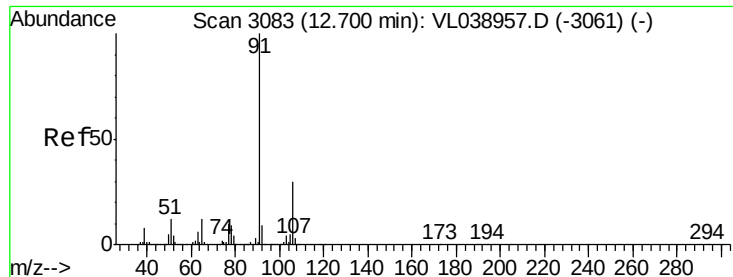




#58
Ethyl Benzene
Concen: 0.095 ppbv
RT: 12.69 min
Delta R.T. MSVOA_1
Lab File: ClientSampleId :
Acq: 5 May 2022 11:18


Tot Ion: 91 Resp: 29698
Ion Ratio Lower Upper
91 100
106 25.3 24.2 36.4

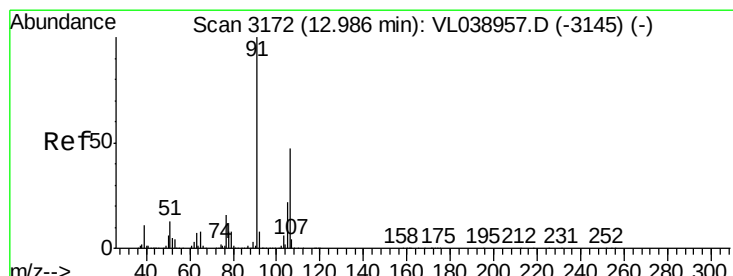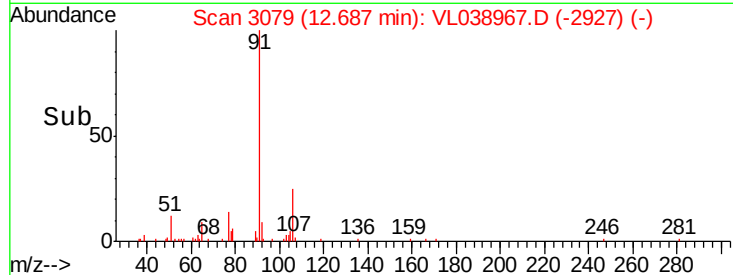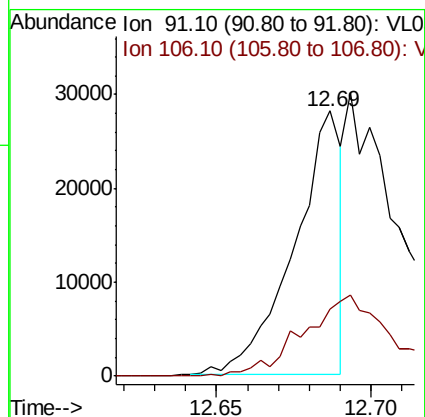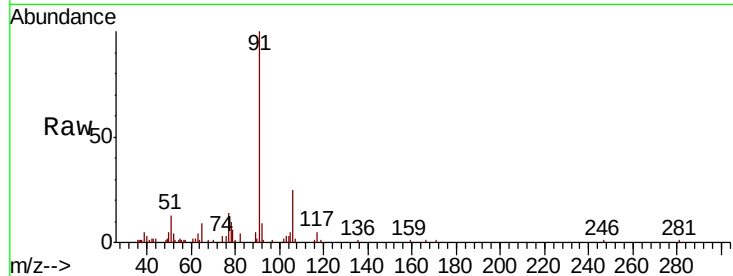

#59
m/p-Xylene
Concen: 0.136 ppbv
RT: 12.99 min Scan# 3172
Delta R.T. 0.00 min
Lab File: VL038967.D
Acq: 5 May 2022 11:18





Tgt Ion: 91 Resp: 36361
Ion Ratio Lower Upper
91 100
106 0.0 34.6 52.0#

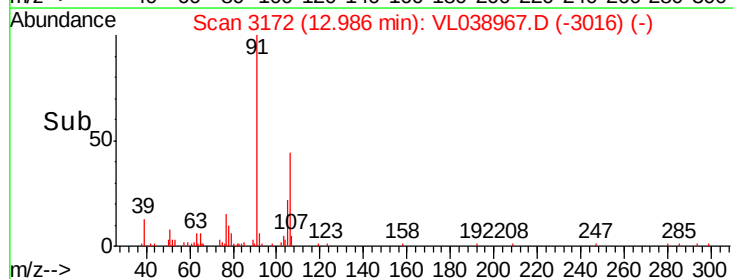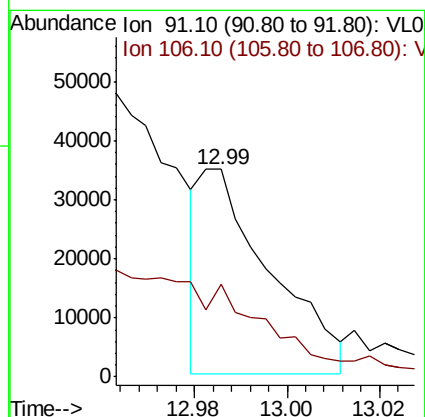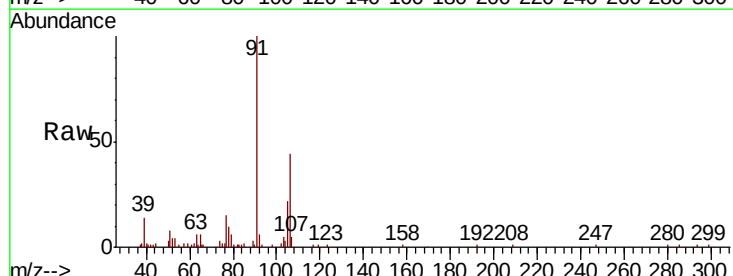

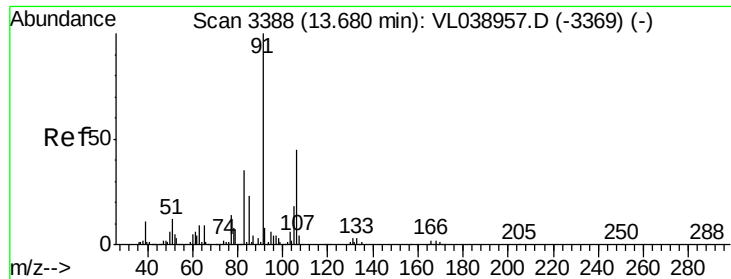




#60
o-Xylene
Concen: 0.136 ppbv
RT: 13.67
Delta R.T. MSVOA_L
Lab File: ClientSampled :
Acq: 5 May 2022 11:18


Tot Ion: 91 Resp: 34323
Ion Ratio Lower Upper
91 100
106 0.0 22.2 66.6#

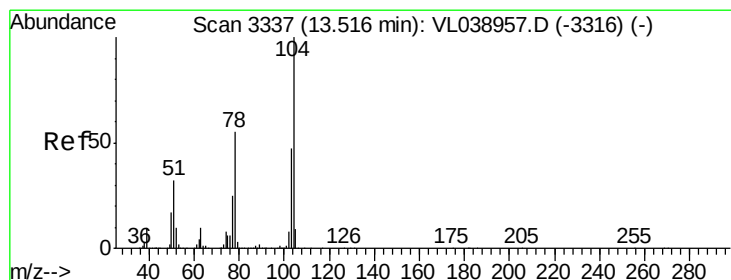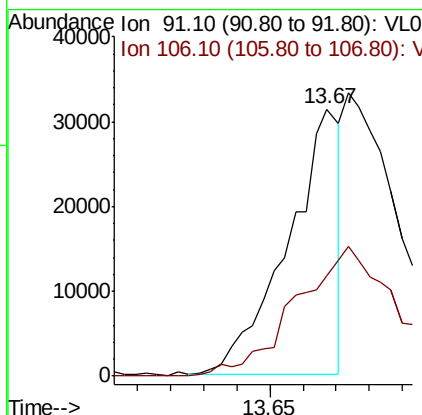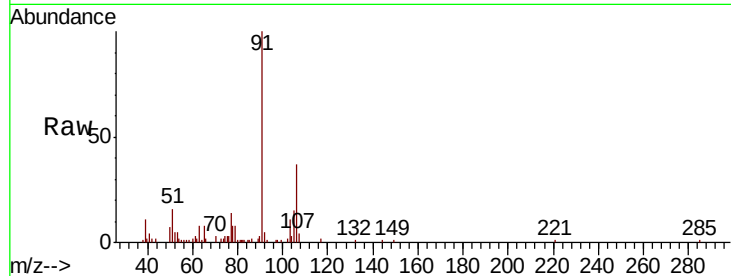

#61
Styrene
Concen: 0.059 ppbv
RT: 13.50 min Scan# 3333
Delta R.T. -0.01 min
Lab File: VL038967.D
Acq: 5 May 2022 11:18





Tgt Ion:104 Resp: 7960
Ion Ratio Lower Upper
104 100
78 0.0 46.4 69.6#
103 0.0 39.3 58.9#

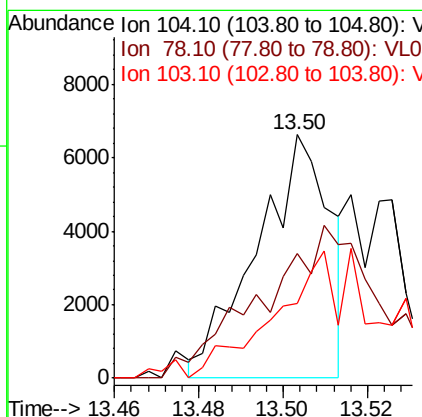






#68
 1-Bromo-4-Fluorobenzene
 Concen: 10.260 ppbv
 RT: 14.39
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 Acq: 5 May 2022 11:18


Tot Ion:	95	Resp:	1769921
Ion	Ratio	Lower	Upper
95	100		
174	64.9	50.8	76.2
175	4.6	3.8	5.6

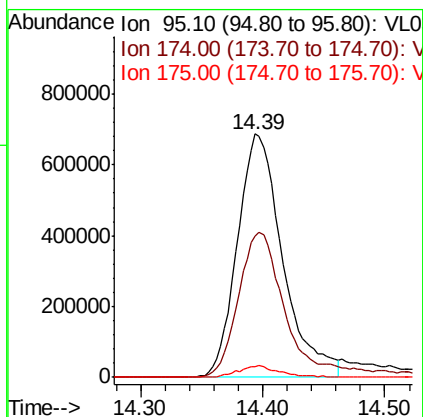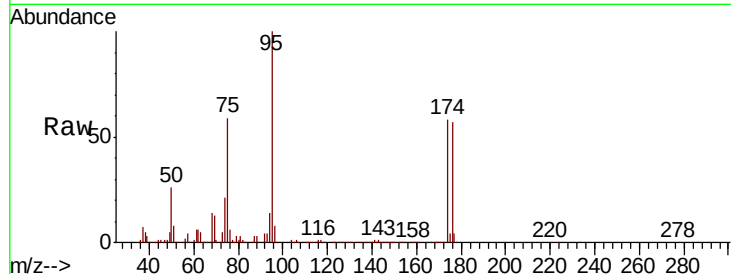

#72
 4-Ethyltoluene
 Concen: 0.070 ppbv
 RT: 15.82 min Scan# 4053
 Delta R.T. -0.01 min
 Lab File: VL038967.D
 Acq: 5 May 2022 11:18





Tgt Ion:	105	Resp:	20170
Ion	Ratio	Lower	Upper
105	100		
120	72.2	23.4	35.0#
91	47.2	10.6	16.0#
77	44.5	12.5	18.7#

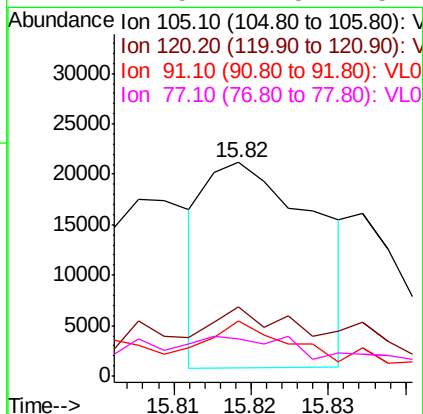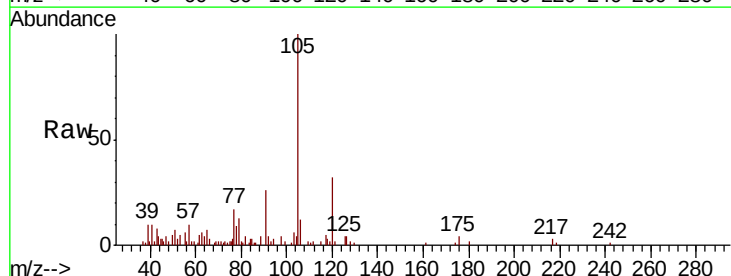

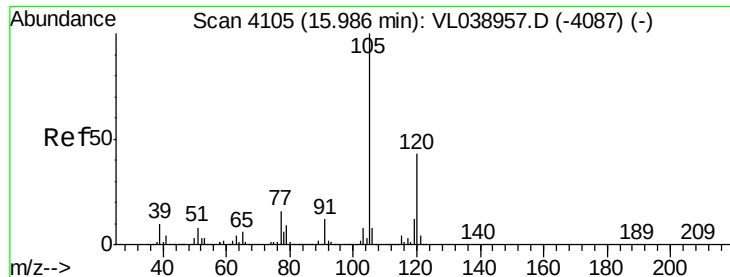




#73
 1,3,5-Trimethylbenzene
 Concen: 0.040 ppbv
 RT: 15.97 min
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId:
 Acq: 5 May 2022 11:18


Tot Ion:105 Resp: 10391
 Ion Ratio Lower Upper
 105 100
 120 0.0 34.4 51.6#

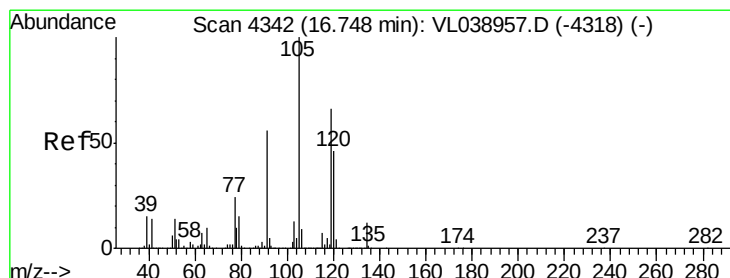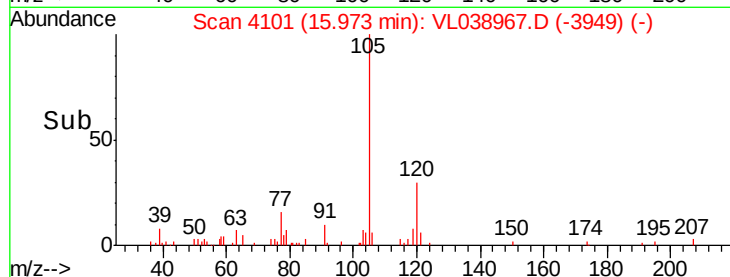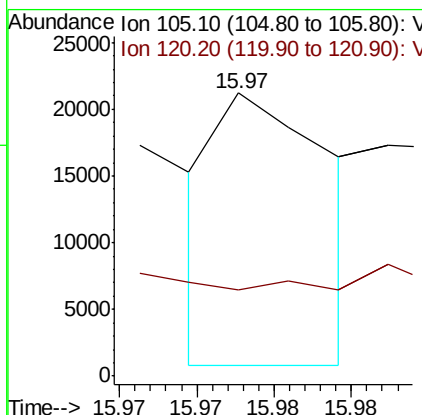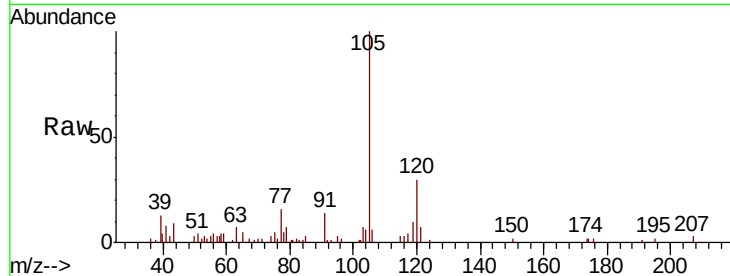

#74
 1,2,4-Trimethylbenzene
 Concen: 0.387 ppbv
 RT: 16.74 min Scan# 4340
 Delta R.T. -0.01 min
 Lab File: VL038967.D
 Acq: 5 May 2022 11:18

Tgt Ion:105 Resp: 109370
 Ion Ratio Lower Upper
 105 100
 120 42.5 36.9 55.3
 91 11.1 45.0 67.4#
 77 14.9 19.2 28.8#

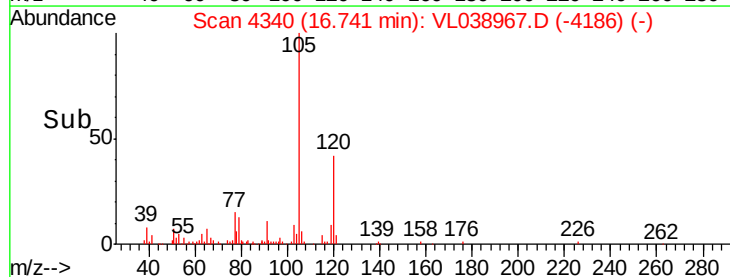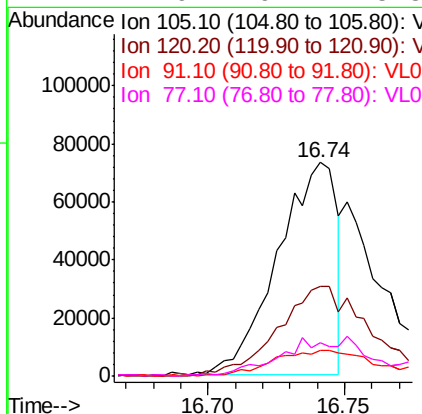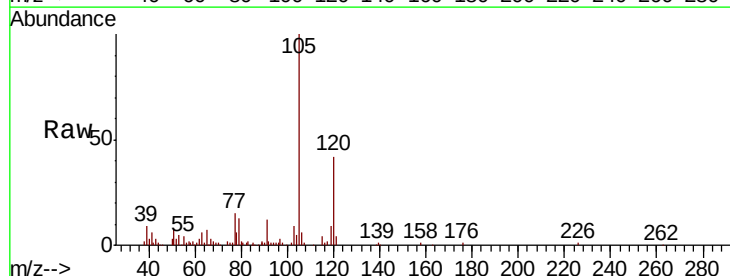

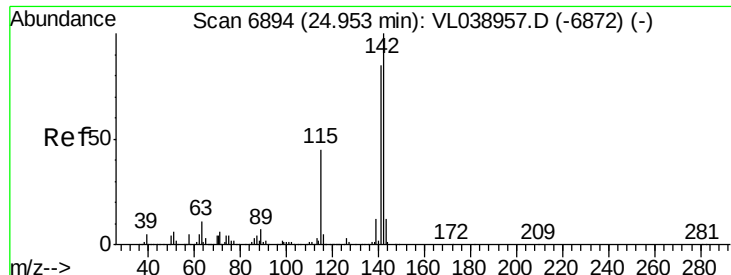

#80

Naphthalene, 2-methyl-

Concen: 0.064 ppbv

RT: 24.95

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 5 May 2022 11:18


Tot Ion: 142 Resp: 4457

Ion Ratio Lower Upper

142 100

141 0.0 70.8 106.2#

115 37.0 35.1 52.7

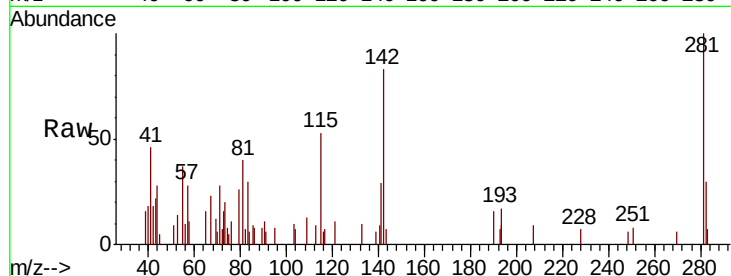

Abundance

Ion 142.00 (141.70 to 142.70): V

Ion 141.00 (140.70 to 141.70): V

Ion 115.00 (114.70 to 115.70): V

