

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL050522\
Data File : VL038982.D
Acq On : 5 May 2022 21:17
Operator : SY/AP
Sample : QC050322 CAN 10267
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC050322 CAN 10267

Quant Time: May 06 08:56:24 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL050522AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 05 07:41:27 2022
QLast Update : Thu May 05 07:41:27 2022
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.66	49	1031281	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.17	114	2543595	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.08	117	2106487	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.40	95	1639273	9.83	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.30%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL050522\
Data File : VL038982.D
Acq On : 5 May 2022 21:17
Operator : SY/AP
Sample : OC050322 CAN 10267
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC050322 CAN 10267

Quant Time: May 06 08:56:24 2022
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL050522AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 05 07:41:27 2022
QLast Update : Thu May 05 07:41:27 2022
Response via : Initial Calibration

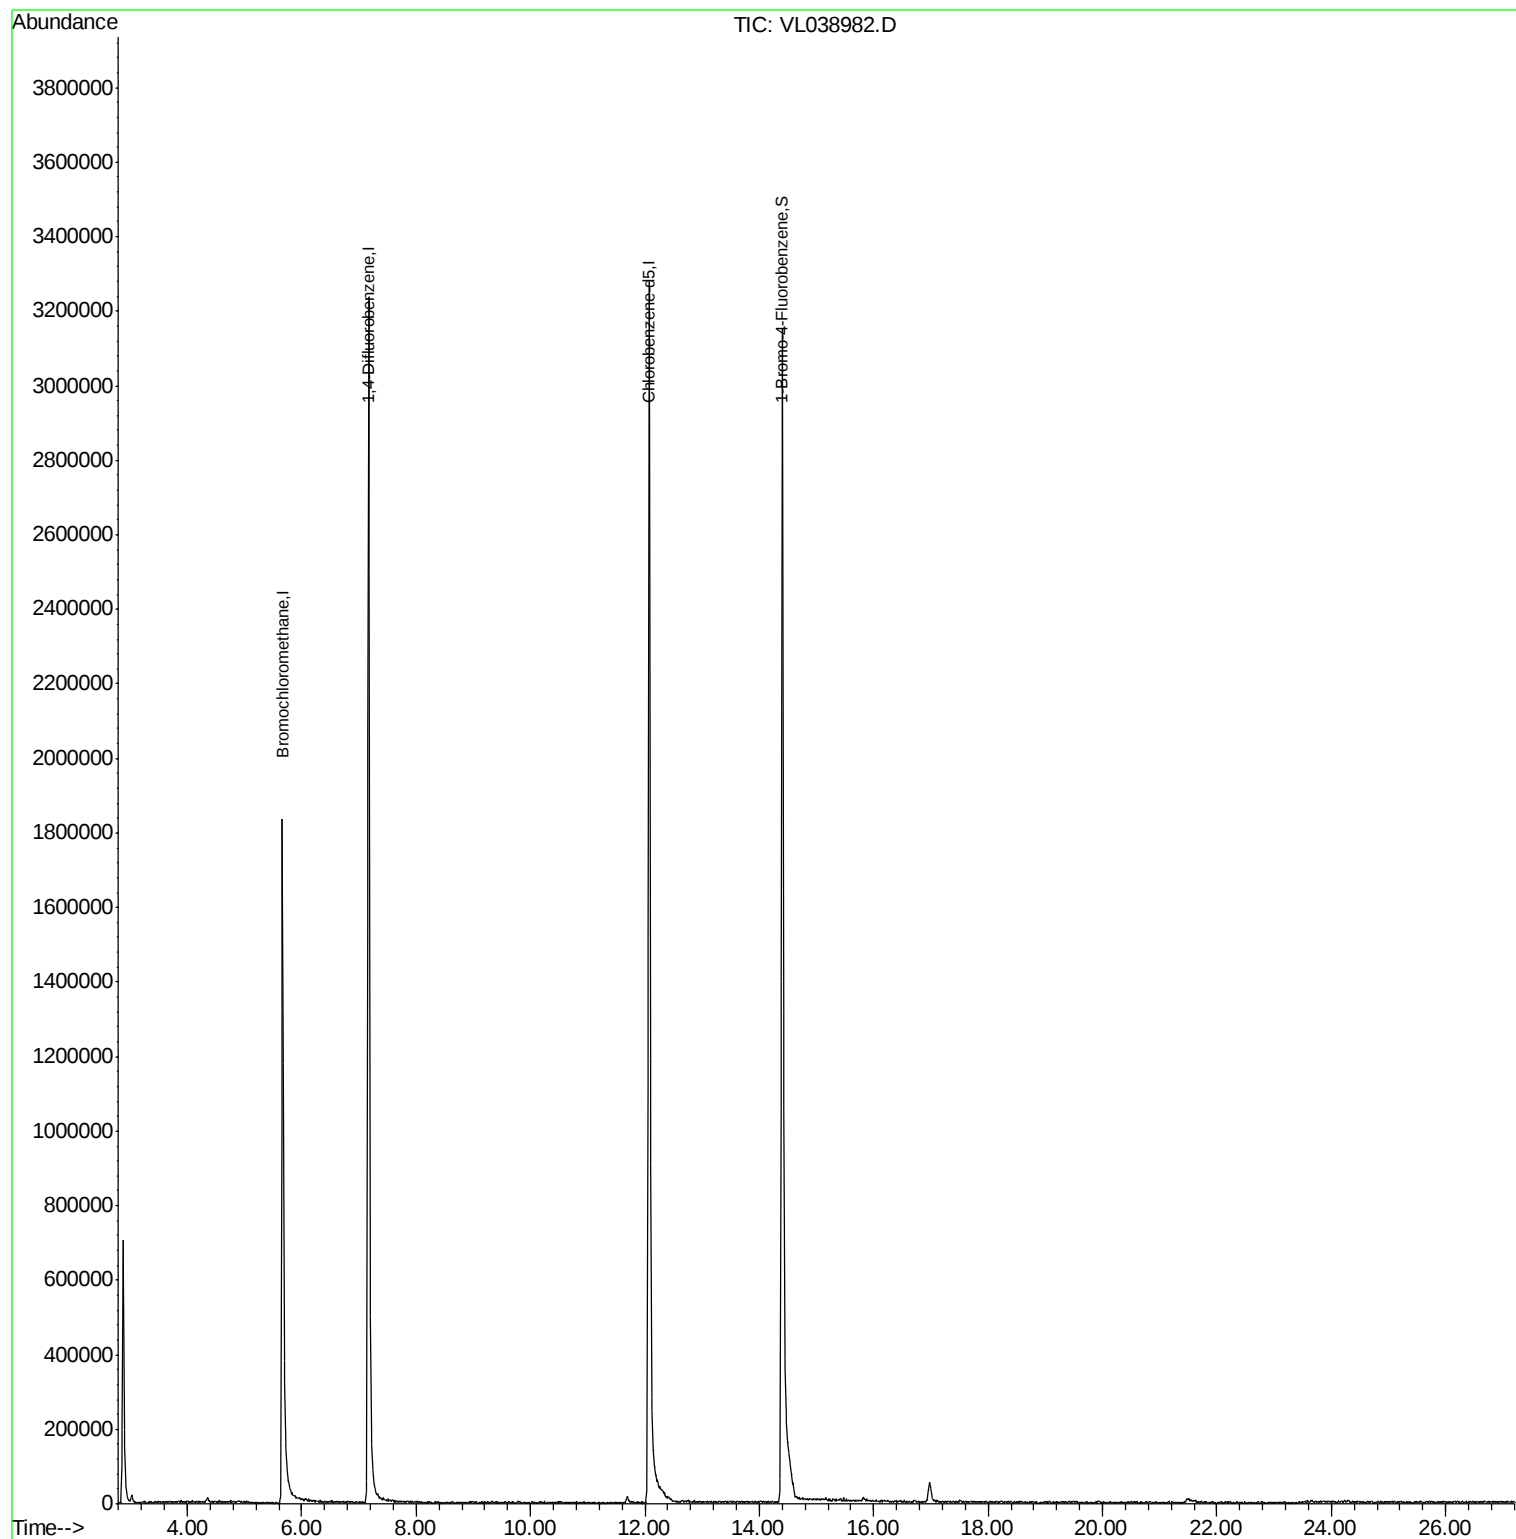

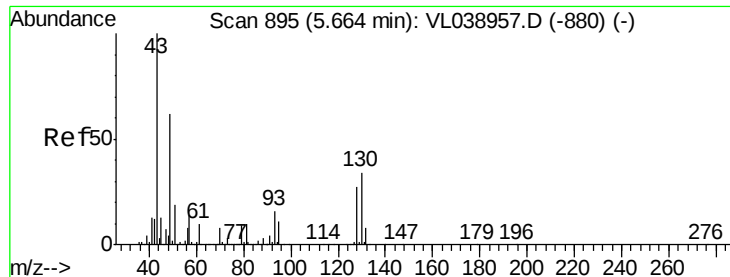

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.66 Instrument: MSVOA_1

Delta R.T.

Lab File: ClientSampleId: OC050322 CAN 10267

Acq: 5 May 2022 21:17


Tot Ion: 49 Resp: 1031281

Ion	Ratio	Lower	Upper
49	100		
128	49.3	23.3	69.8
130	63.8	29.8	89.3

49 100

128 49.3 23.3 69.8




130 63.8 29.8 89.3

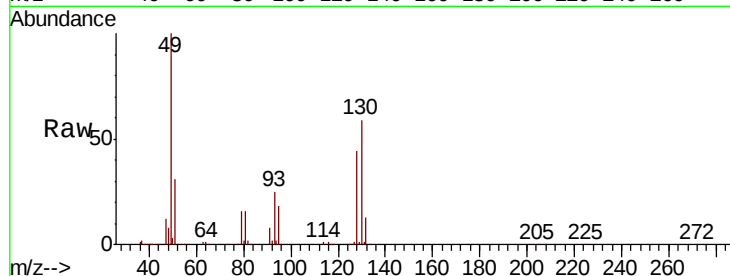

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

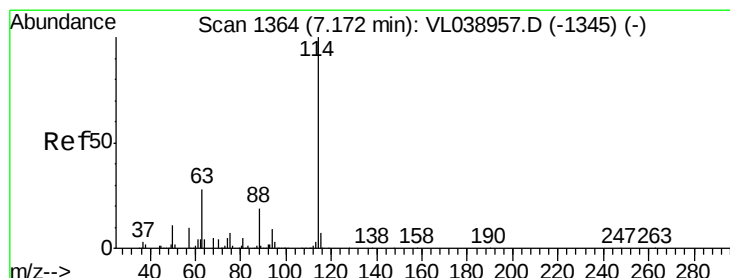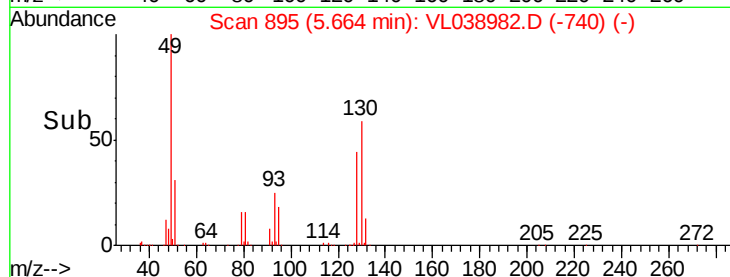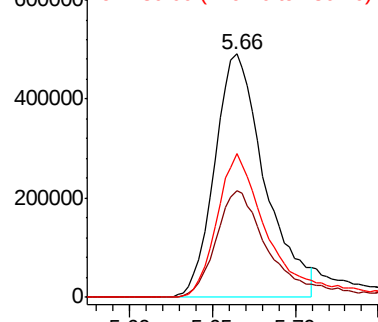

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.17 min Scan# 1363

Delta R.T. -0.00 min

Lab File: VL038982.D

Acq: 5 May 2022 21:17


Tgt Ion: 114 Resp: 2543595

Ion	Ratio	Lower	Upper
114	100		
63	29.6	22.6	33.8
88	19.9	15.4	23.0

114 100

63 29.6 22.6 33.8



88 19.9 15.4 23.0

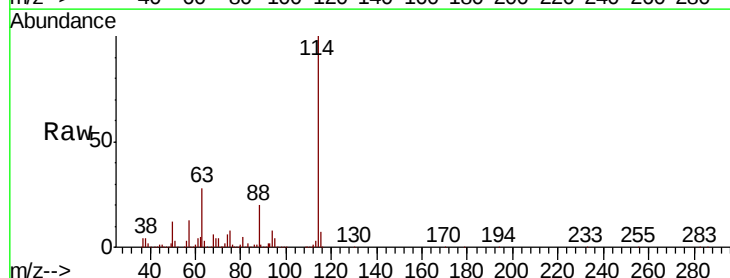


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



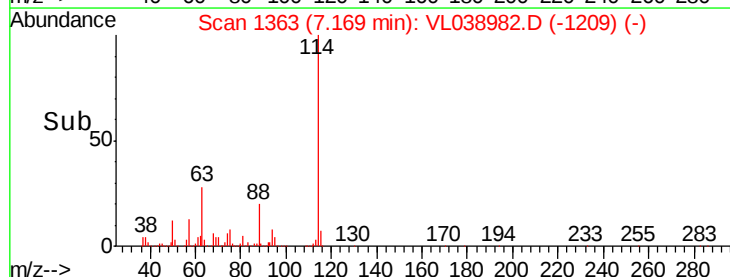
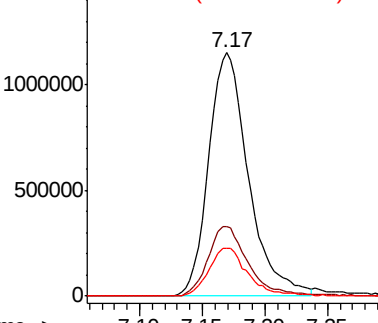


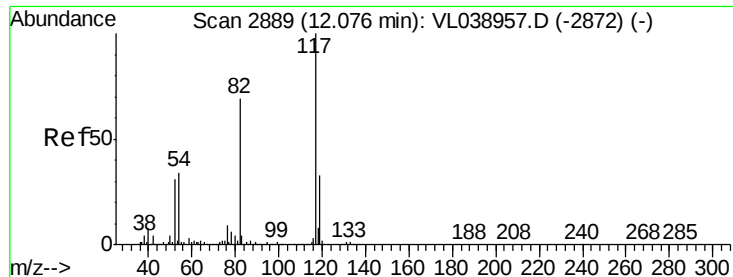

#55
 Chlorobenzene-d5
 Concen: 10.000 ppbv
 RT: 12.08 min
 Instrument: MSVOA_1
 Delta R.T.:
 ClientSampleId:
 Lab File: OC050322 CAN 10267
 Acq: 5 May 2022 21:17

Tot Ion: 117 Resp: 2106487

Ion	Ratio	Lower	Upper
117	100		
82	78.0	57.0	85.6
119	34.7	27.2	40.8

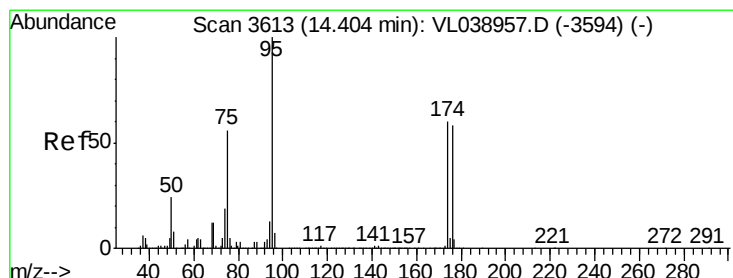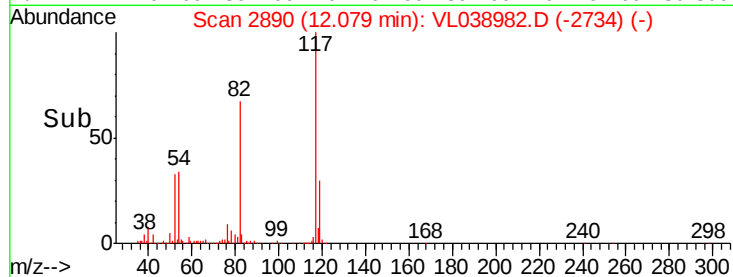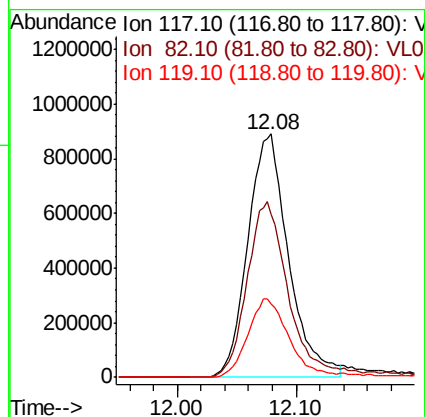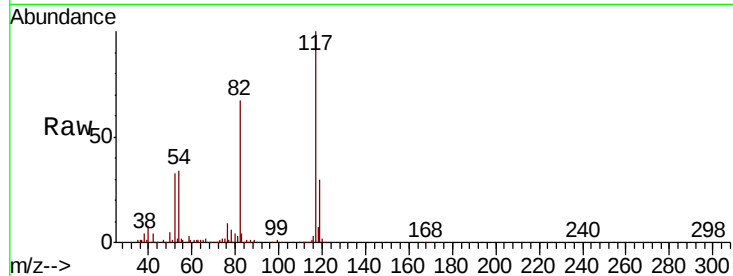

#68
 1-Bromo-4-Fluorobenzene
 Concen: 9.826 ppbv
 RT: 14.40 min Scan# 3612
 Delta R.T.: -0.00 min
 Lab File: VL038982.D
 Acq: 5 May 2022 21:17

Tgt Ion: 95 Resp: 1639273

Ion	Ratio	Lower	Upper
95	100		
174	67.3	50.8	76.2
175	4.7	3.8	5.6

