


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL050522\
 Data File : VL038956.D
 Acq On : 5 May 2022 2:04
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu May 05 10:12:15 2022
 Last Update : Thu May 05 10:12:15 2022

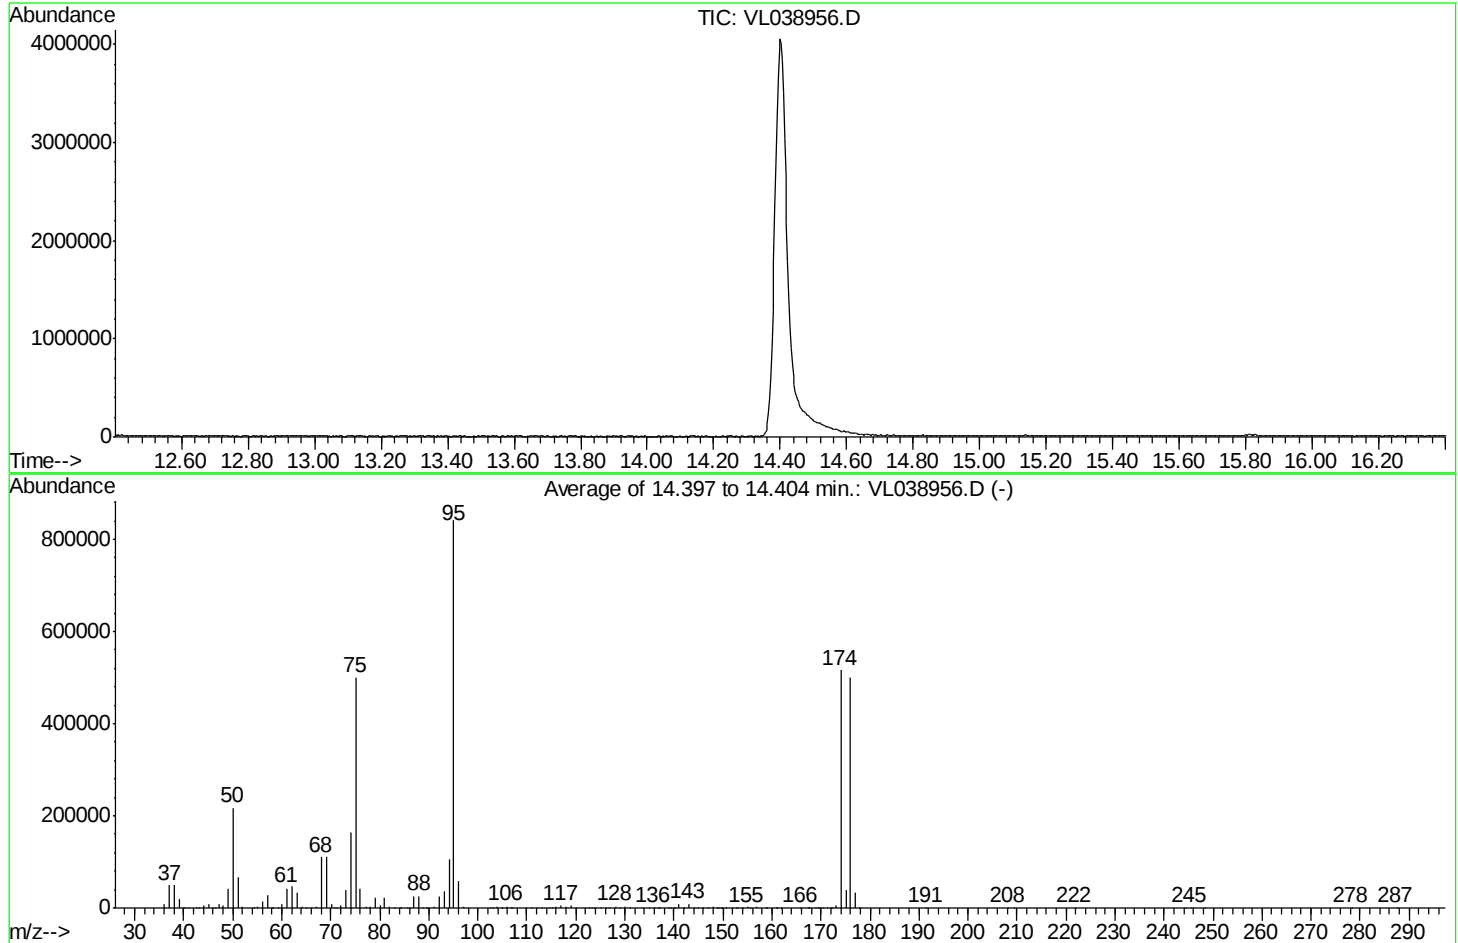

AutoFind: Scans 3611, 3612, 3613; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.8	217216	PASS
75	95	30	66	59.3	499178	PASS
95	95	100	100	100.0	841216	PASS
96	95	5	9	6.9	58000	PASS
173	174	0.00	2	1.2	5994	PASS
174	95	50	120	61.3	515882	PASS
175	174	4	9	7.6	39354	PASS
176	174	93	101	96.9	499776	PASS
177	176	5	9	6.6	32890	PASS