

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050525\
 Data File : VL042477.D
 Acq On : 05 May 2025 15:53
 Operator : SY/MD
 Sample : Q1927-01DUP
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 EBR-P06-SC-IA01-20250428DUP

Quant Time: May 06 01:42:48 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL050125AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri May 02 03:16:31 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Bromochloromethane	2.790	49	73750	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.965	114	201304	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.888	117	172499	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.383	95	158397	9.904	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.000%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.499	85	5732	0.470	ppbv	90
4) Chloromethane	1.534	50	2300	0.451	ppbv #	75
6) Bromomethane	1.674	94	88	0.036	ppbv #	6
9) Propene	1.622	41	3258	0.772	ppbv	97
13) Ethanol	1.722	45	17711	20.679	ppbv #	37
15) Acetone	1.839	43	170449	12.660	ppbv	100
16) 1,3-Butadiene	1.622	39	1761	0.297	ppbv #	37
17) tert-Butyl alcohol	2.046	59	2899	0.244	ppbv #	75
19) Isopropyl Alcohol	1.890	45	11026	1.480	ppbv #	1
20) Methylene Chloride	2.065	84	6814	1.684	ppbv #	79
23) Vinyl Acetate	2.457	43	7863	0.612	ppbv #	61
25) Ethyl Acetate	2.845	43	1490	0.069	ppbv #	74
26) Hexane	2.829	57	2340	0.249	ppbv #	79
27) Carbon Disulfide	2.153	76	526	0.048	ppbv #	1
34) 2-Butanone	2.564	43	8535	0.586	ppbv	98
35) Carbon Tetrachloride	3.771	117	1344	0.073	ppbv #	81
36) Benzene	3.664	78	989	0.052	ppbv #	62
37) 1,2-Dichloroethane	3.217	62	454	0.031	ppbv #	96
39) 1,2-Dichloropropane	3.962	63	56653	7.966	ppbv #	22
40) 1,4-Dioxane	4.680	88	102	0.031	ppbv #	100
53) Toluene	6.952	91	2089	0.104	ppbv #	21
58) Ethyl Benzene	9.357	91	2175	0.075	ppbv	91
59) m/p-Xylene	9.535	91	4290	0.178	ppbv #	33
60) o-Xylene	9.966	91	3592	0.148	ppbv	92
61) Styrene	9.875	104	1295	0.143	ppbv #	90
72) 4-Ethyltoluene	11.131	105	864	0.030	ppbv #	56
73) 1,3,5-Trimethylbenzene	11.205	105	1235	0.049	ppbv	94
74) 1,2,4-Trimethylbenzene	11.542	105	5187	0.171	ppbv #	55

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_L
ClientSampleId :
EBR-P06-SC-IA01-20250428DUP

The chromatogram displays the abundance of various chemical compounds over time. The y-axis represents abundance, ranging from 0 to 750,000. The x-axis represents time in minutes, ranging from 1.00 to 21.00. The following table lists the labeled compounds and their approximate retention times:





Compound	Retention Time (min)
Chlorobenzene-d5, I	1.50
Bromochloromethane, I	1.80
Acetone, T	2.00
Carbon Disulfide, T	2.20
1,2-Dichloroethane, T	2.50
1,2-Dichloroethane, I	2.80
1,2-Dichloroethane, T	3.00
1,2-Dichloroethane, I	3.20
1,2-Dichloroethane, T	3.50
1,2-Dichloroethane, I	3.80
1,2-Dichloroethane, T	4.00
1,2-Dichloroethane, I	4.20
1,2-Dichloroethane, T	4.50
1,2-Dichloroethane, I	4.80
1,2-Dichloroethane, T	5.00
1,2-Dichloroethane, I	5.20
1,2-Dichloroethane, T	5.50
1,2-Dichloroethane, I	5.80
1,2-Dichloroethane, T	6.00
1,2-Dichloroethane, I	6.20
1,2-Dichloroethane, T	6.50
1,2-Dichloroethane, I	6.80
1,2-Dichloroethane, T	7.00
1,2-Dichloroethane, I	7.20
1,2-Dichloroethane, T	7.50
1,2-Dichloroethane, I	7.80
1,2-Dichloroethane, T	8.00
1,2-Dichloroethane, I	8.20
1,2-Dichloroethane, T	8.50
1,2-Dichloroethane, I	8.80
1,2-Dichloroethane, T	9.00
1,2-Dichloroethane, I	9.20
1,2-Dichloroethane, T	9.50
1,2-Dichloroethane, I	9.80
1,2-Dichloroethane, T	10.00
1,2-Dichloroethane, I	10.20
1,2-Dichloroethane, T	10.50
1,2-Dichloroethane, I	10.80
1,2-Dichloroethane, T	11.00
1,2-Dichloroethane, I	11.20
1,2-Dichloroethane, T	11.50
1,2-Dichloroethane, I	11.80
1,2-Dichloroethane, T	12.00
1,2-Dichloroethane, I	12.20
1,2-Dichloroethane, T	12.50
1,2-Dichloroethane, I	12.80
1,2-Dichloroethane, T	13.00
1,2-Dichloroethane, I	13.20
1,2-Dichloroethane, T	13.50
1,2-Dichloroethane, I	13.80
1,2-Dichloroethane, T	14.00
1,2-Dichloroethane, I	14.20
1,2-Dichloroethane, T	14.50
1,2-Dichloroethane, I	14.80
1,2-Dichloroethane, T	15.00
1,2-Dichloroethane, I	15.20
1,2-Dichloroethane, T	15.50
1,2-Dichloroethane, I	15.80
1,2-Dichloroethane, T	16.00
1,2-Dichloroethane, I	16.20
1,2-Dichloroethane, T	16.50
1,2-Dichloroethane, I	16.80
1,2-Dichloroethane, T	17.00
1,2-Dichloroethane, I	17.20
1,2-Dichloroethane, T	17.50
1,2-Dichloroethane, I	17.80
1,2-Dichloroethane, T	18.00
1,2-Dichloroethane, I	18.20
1,2-Dichloroethane, T	18.50
1,2-Dichloroethane, I	18.80
1,2-Dichloroethane, T	19.00
1,2-Dichloroethane, I	19.20
1,2-Dichloroethane, T	19.50
1,2-Dichloroethane, I	19.80
1,2-Dichloroethane, T	20.00
1,2-Dichloroethane, I	20.20
1,2-Dichloroethane, T	20.50
1,2-Dichloroethane, I	20.80
1,2-Dichloroethane, T	21.00



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.790 min Scan# 81
Delta R.T. 0.006 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53




Instrument :
MSVOA_L
ClientSampleId :
EBR-P06-SC-IA01-20250428DUP


Tgt Ion: 49 Resp: 73750
Ion Ratio Lower Upper
49 100
128 47.2 23.3 69.9
130 62.1 29.5 88.6

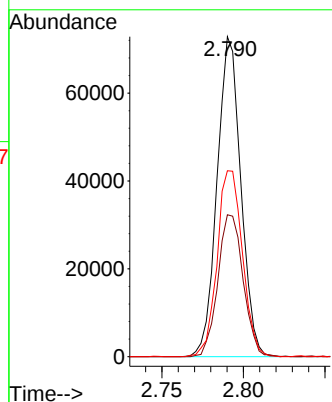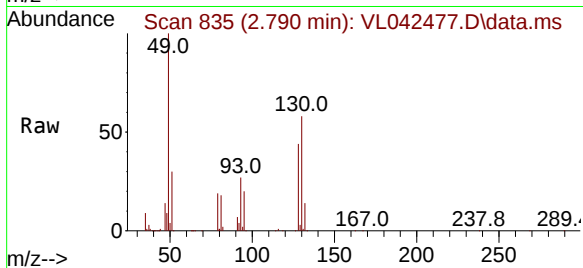

#2
Dichlorodifluoromethane
Concen: 0.470 ppbv
RT: 1.499 min Scan# 436
Delta R.T. 0.000 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53

Tgt Ion: 85 Resp: 5732
Ion Ratio Lower Upper
85 100
87 27.7 26.9 40.3


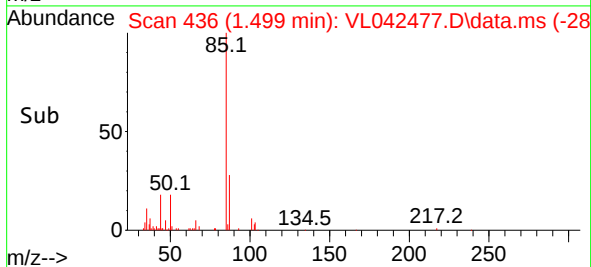
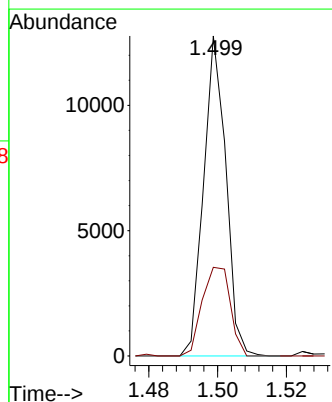
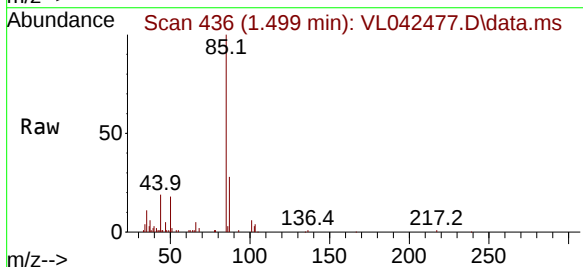




#4
Chloromethane
Concen: 0.451 ppbv
RT: 1.534 min Scan# 446
Delta R.T. 0.003 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53




Instrument : MSVOA_1
ClientSampleId : EBR-P06-SC-IA01-20250428DUP


Tgt Ion: 50 Resp: 2300
Ion Ratio Lower Upper
50 100
52 42.6 23.5 35.3#

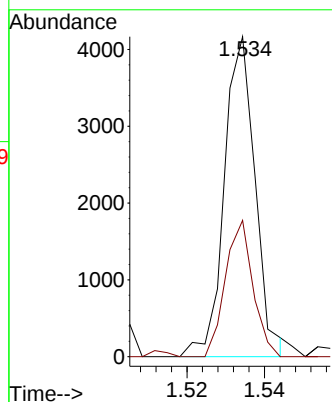

#6
Bromomethane
Concen: 0.036 ppbv
RT: 1.674 min Scan# 490
Delta R.T. 0.007 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53

Tgt Ion: 94 Resp: 88
Ion Ratio Lower Upper
94 100
96 0.0 68.8 103.2#

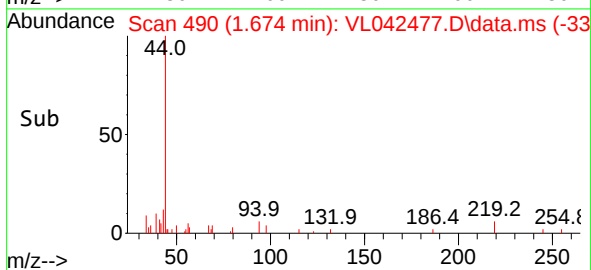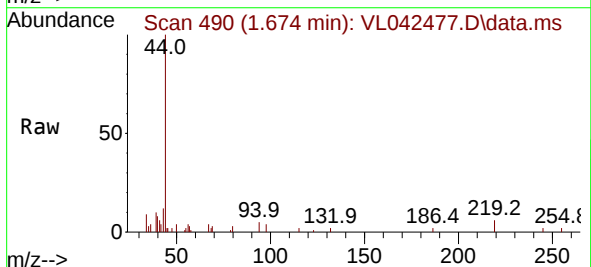



#9

Propene

Concen: 0.772 ppbv

RT: 1.622 min Scan# 41

Delta R.T. 0.139 min

Lab File: VL042477.D

Acq: 05 May 2025 15:53

Instrument :

MSVOA_L

ClientSampleId :





EBR-P06-SC-IA01-20250428DUP

Tgt Ion: 41 Resp: 3258

Ion Ratio Lower Upper

41 100

42 69.9 54.3 81.5

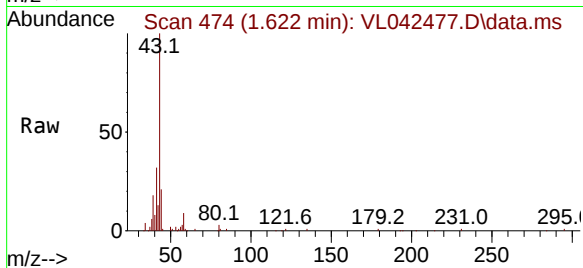

#13

Ethanol

Concen: 20.679 ppbv

RT: 1.722 min Scan# 505

Delta R.T. 0.003 min

Lab File: VL042477.D




Acq: 05 May 2025 15:53


Tgt Ion: 45 Resp: 17711

Ion Ratio Lower Upper

45 100

46 0.0 15.3 61.1#


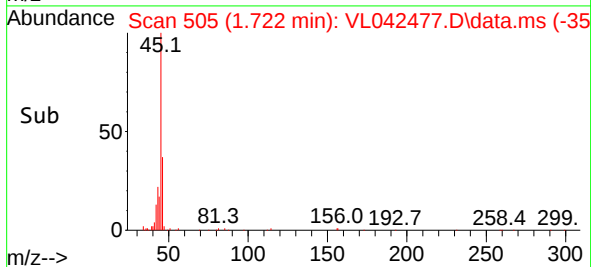

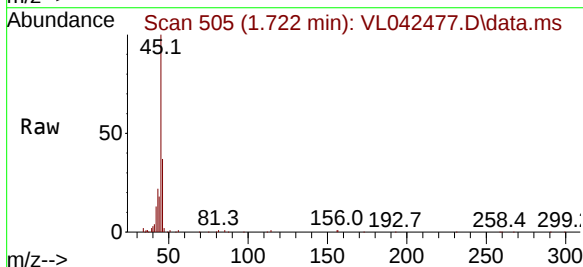




#15
Acetone
Concen: 12.660 ppbv
RT: 1.839 min Scan# 541
Delta R.T. 0.003 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53




Instrument :
MSVOA_L
ClientSampleId :
EBR-P06-SC-IA01-20250428DUP


Tgt Ion: 43 Resp: 170449
Ion Ratio Lower Upper
43 100
58 24.9 19.8 29.8

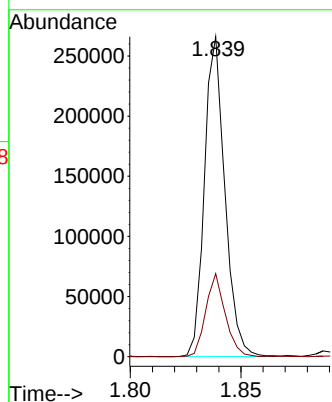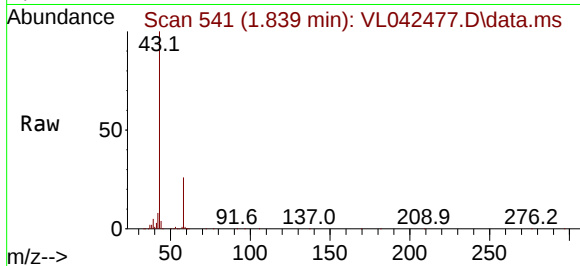

#16
1,3-Butadiene
Concen: 0.297 ppbv
RT: 1.622 min Scan# 474
Delta R.T. 0.013 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53

Tgt Ion: 39 Resp: 1761
Ion Ratio Lower Upper
39 100
54 17.6 55.2 82.8#

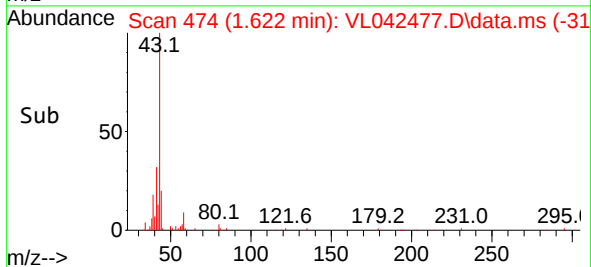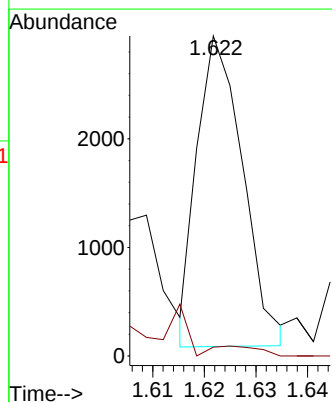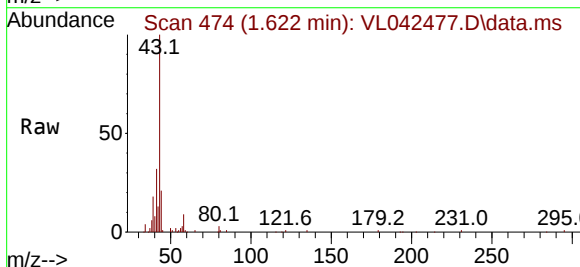



#17

tert-Butyl alcohol

Concen: 0.244 ppbv

RT: 2.046 min Scan# 603

Delta R.T. 0.007 min

Lab File: VL042477.D

Acq: 05 May 2025 15:53

Instrument :

MSVOA_L

ClientSampleId :





EBR-P06-SC-IA01-20250428DUP

Tgt Ion: 59 Resp: 2899

Ion Ratio Lower Upper

59 100

57 19.8 8.3 12.5#

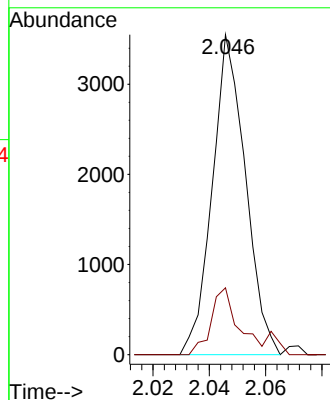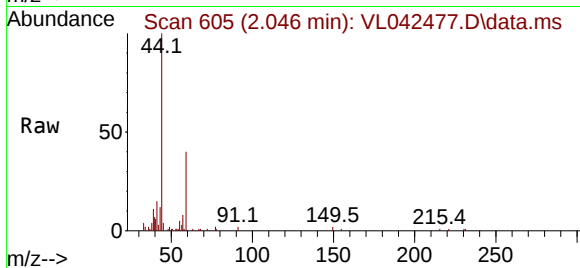

#19

Isopropyl Alcohol

Concen: 1.480 ppbv

RT: 1.890 min Scan# 557

Delta R.T. 0.007 min

Lab File: VL042477.D




Acq: 05 May 2025 15:53


Tgt Ion: 45 Resp: 11026

Ion Ratio Lower Upper

45 100

58 385.1 1.6 2.4#

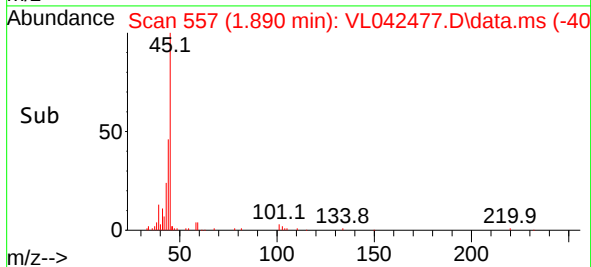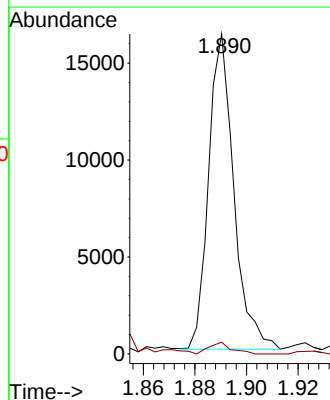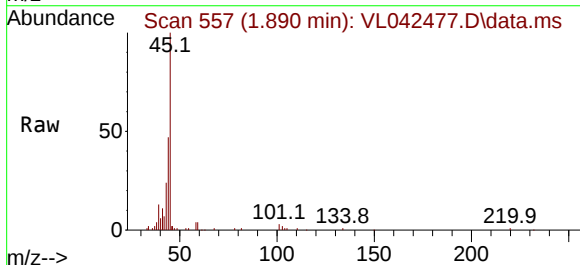



#20

Methylene Chloride

Concen: 1.684 ppbv

RT: 2.065 min Scan# 611

Delta R.T. 0.007 min

Lab File: VL042477.D


Acq: 05 May 2025 15:53

Instrument :

MSVOA_L

ClientSampleId :

EBR-P06-SC-IA01-20250428DUP

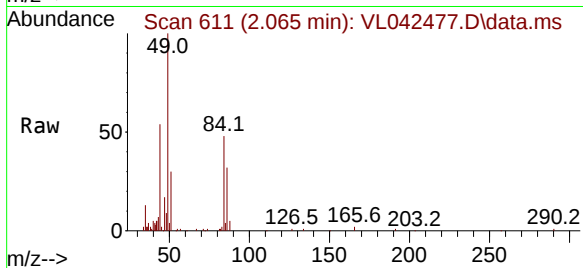

Tgt Ion: 84 Resp: 6814




Ion Ratio Lower Upper

84 100

49 209.8 133.9 200.9#

51 60.2 41.0 61.6

86 66.9 51.9 77.9



#23

Vinyl Acetate

Concen: 0.612 ppbv

RT: 2.457 min Scan# 732

Delta R.T. -0.003 min

Lab File: VL042477.D

Acq: 05 May 2025 15:53

Tgt Ion: 43 Resp: 7863




Ion Ratio Lower Upper


43 100

86 12.1 5.5 8.3#

42 1.7 8.3 12.5#

44 38.5 4.6 7.0#

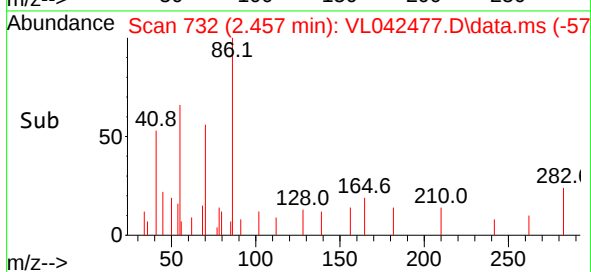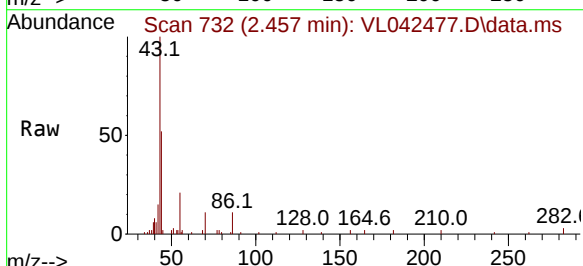



#25

Ethyl Acetate

Concen: 0.069 ppbv

RT: 2.845 min Scan# 81

Delta R.T. 0.010 min

Lab File: VL042477.D

Acq: 05 May 2025 15:53

Instrument :

MSVOA_L

ClientSampleId :

EBR-P06-SC-IA01-20250428DUP

Tgt Ion: 43 Resp: 1490





Ion Ratio Lower Upper

43 100

45 0.0 7.8 11.6#

61 12.8 7.2 10.8#

70 23.4 7.2 10.8#

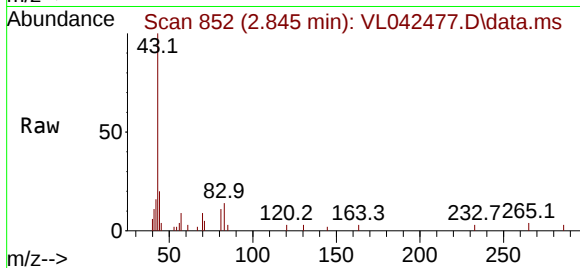

#26

Hexane

Concen: 0.249 ppbv

RT: 2.829 min Scan# 847

Delta R.T. 0.003 min

Lab File: VL042477.D

Acq: 05 May 2025 15:53

Tgt Ion: 57 Resp: 2340




Ion Ratio Lower Upper


57 100

41 98.2 77.8 116.8

43 180.1 187.0 280.6#

56 59.8 43.9 65.9


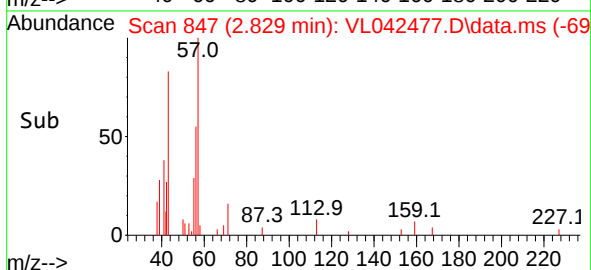
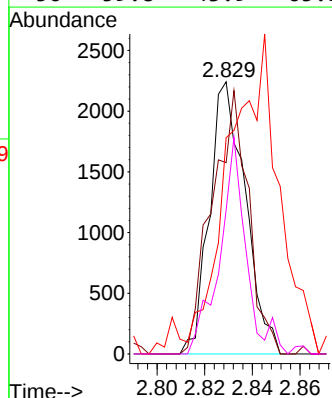
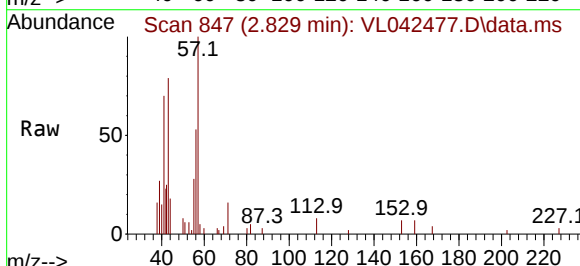




#27
Carbon Disulfide
Concen: 0.048 ppbv
RT: 2.153 min Scan# 61
Delta R.T. 0.006 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53




Instrument :
MSVOA_1
ClientSampleId :
EBR-P06-SC-IA01-20250428DUP


Tgt Ion: 76 Resp: 526
Ion Ratio Lower Upper
76 100
44 7213.5 21.0 31.6#
78 30.0 8.6 13.0#

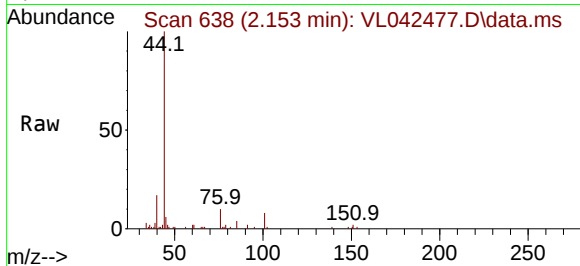

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.965 min Scan# 1198
Delta R.T. 0.010 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53

Tgt Ion: 114 Resp: 201304
Ion Ratio Lower Upper
114 100
63 28.4 23.1 34.7
88 19.8 16.1 24.1


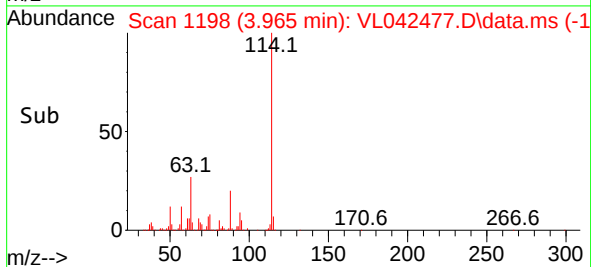

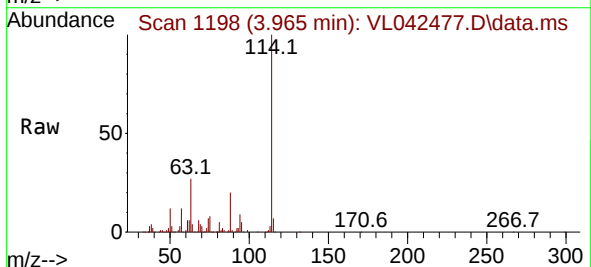




#34
2-Butanone
Concen: 0.586 ppbv
RT: 2.564 min Scan# 765
Delta R.T. 0.007 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53




Instrument :
MSVOA_L
ClientSampleId :
EBR-P06-SC-IA01-20250428DUP


Tgt Ion: 43 Resp: 8535
Ion Ratio Lower Upper
43 100
72 22.0 16.7 25.1

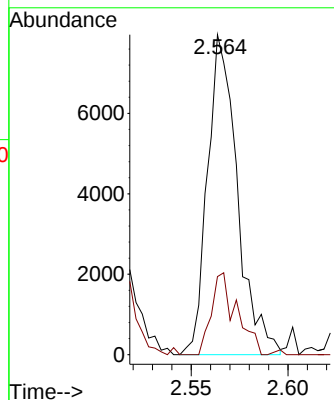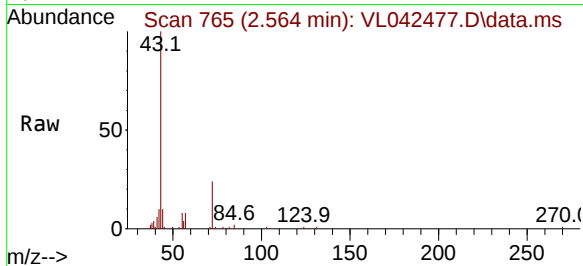

#35
Carbon Tetrachloride
Concen: 0.073 ppbv
RT: 3.771 min Scan# 1138
Delta R.T. 0.013 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53

Tgt Ion: 117 Resp: 1344
Ion Ratio Lower Upper
117 100
119 76.0 78.1 117.1#
121 33.8 23.0 34.6


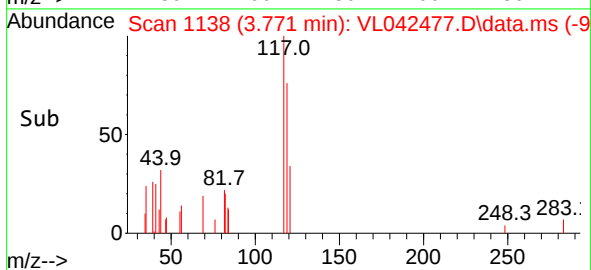
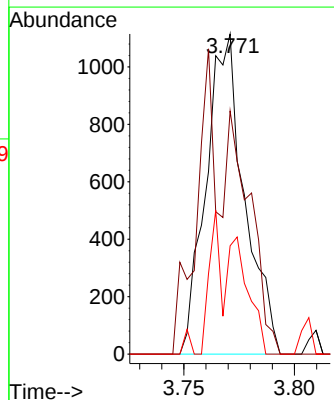
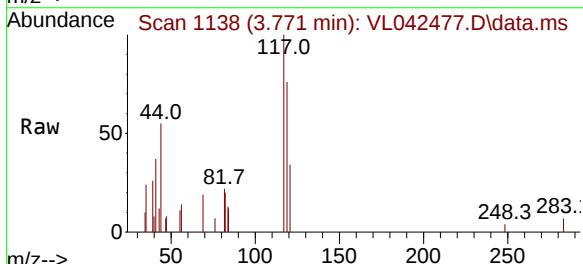




#36
Benzene
Concen: 0.052 ppbv
RT: 3.664 min Scan# 1105
Delta R.T. 0.010 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53




Instrument :
MSVOA_L
ClientSampleId :
EBR-P06-SC-IA01-20250428DUP


Tgt Ion: 78 Resp: 989
Ion Ratio Lower Upper
78 100
77 33.9 18.9 28.3#
50 49.7 18.4 27.6#

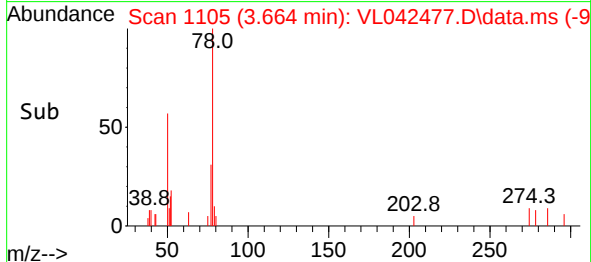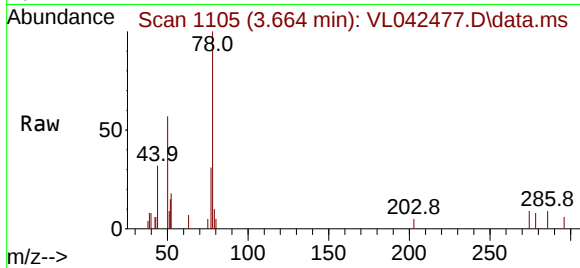

#37
1,2-Dichloroethane
Concen: 0.031 ppbv
RT: 3.217 min Scan# 967
Delta R.T. 0.000 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53

Tgt Ion: 62 Resp: 454
Ion Ratio Lower Upper
62 100
98 6.8 4.3 6.5#

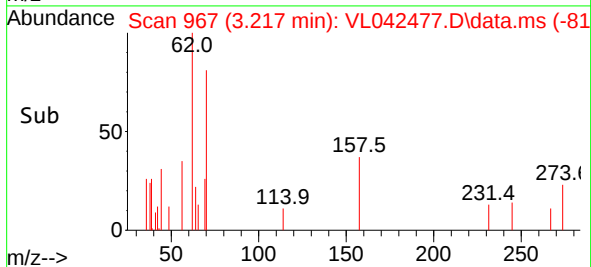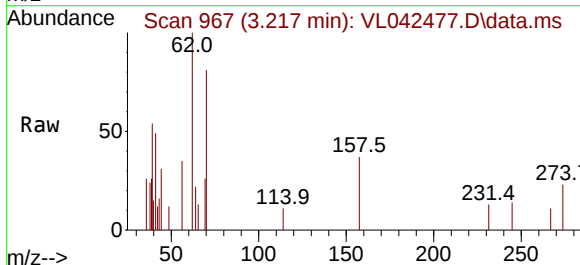



#39

1,2-Dichloropropane

Concen: 7.966 ppbv

RT: 3.962 min Scan# 1197

Delta R.T. -0.350 min

Lab File: VL042477.D

Acq: 05 May 2025 15:53

Instrument :

MSVOA_L

ClientSampleId :

EBR-P06-SC-IA01-20250428DUP





Tgt Ion: 63 Resp: 56653

Ion Ratio Lower Upper

63 100

41 0.1 69.8 104.6#

62 20.7 54.3 81.5#

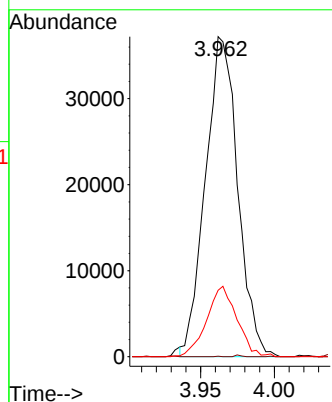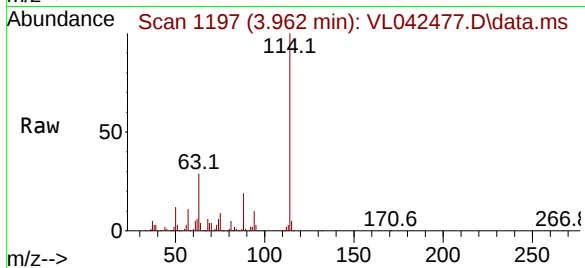

#40

1,4-Dioxane

Concen: 0.031 ppbv

RT: 4.680 min Scan# 1419

Delta R.T. 0.097 min

Lab File: VL042477.D

Acq: 05 May 2025 15:53

Tgt Ion: 88 Resp: 102




Ion Ratio Lower Upper


88 100

58 0.0 0.0 0.0

43 620.6 0.0 0.0#

57 1759.8 0.0 0.0#


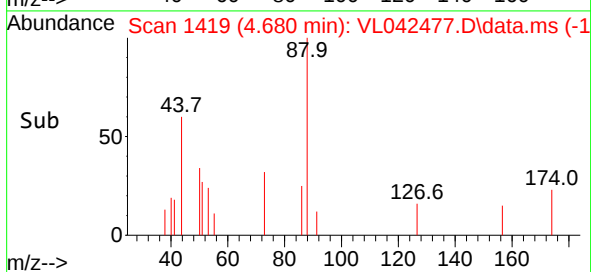

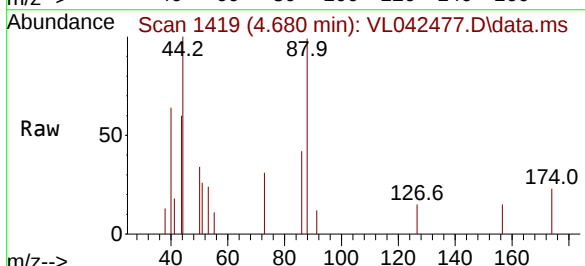




#53
Toluene
Concen: 0.104 ppbv
RT: 6.952 min Scan# 2114
Delta R.T. 0.023 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53




Instrument : MSVOA_L
ClientSampleId : EBR-P06-SC-IA01-20250428DUP


Tgt Ion: 91 Resp: 2089
Ion Ratio Lower Upper
91 100
92 0.0 47.9 71.9#



#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.888 min Scan# 2719
Delta R.T. 0.007 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53

Tgt Ion: 117 Resp: 172499
Ion Ratio Lower Upper
117 100
82 71.0 63.5 95.3
119 30.4 25.8 38.8


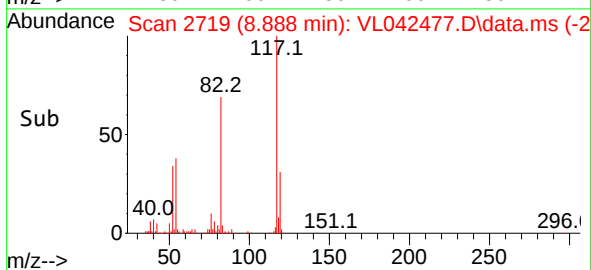






#58
Ethyl Benzene
Concen: 0.075 ppbv
RT: 9.357 min Scan# 2175
Delta R.T. 0.003 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53




Instrument :
MSVOA_L
ClientSampleId :
EBR-P06-SC-IA01-20250428DUP


Tgt Ion: 91 Resp: 2175
Ion Ratio Lower Upper
91 100
106 23.0 21.9 32.9

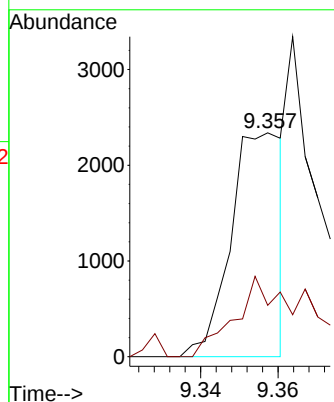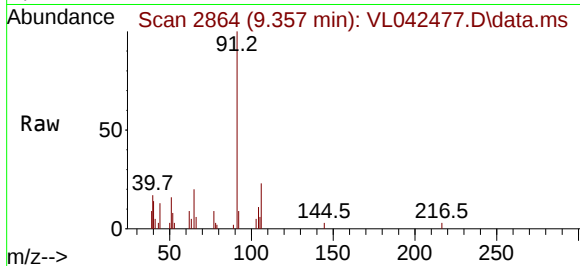

#59
m/p-Xylene
Concen: 0.178 ppbv
RT: 9.535 min Scan# 2919
Delta R.T. 0.007 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53

Tgt Ion: 91 Resp: 4290
Ion Ratio Lower Upper
91 100
106 0.0 34.2 51.2#


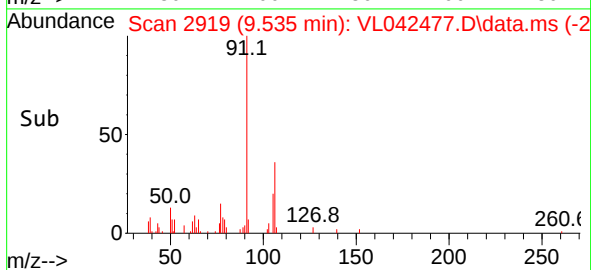
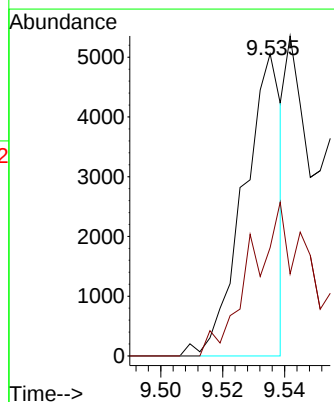
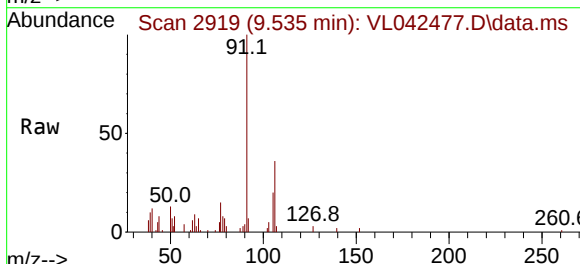




#60
o-Xylene
Concen: 0.148 ppbv
RT: 9.966 min Scan# 3052
Delta R.T. 0.003 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53




Instrument :
MSVOA_L
ClientSampleId :
EBR-P06-SC-IA01-20250428DUP


Tgt Ion: 91 Resp: 3592
Ion Ratio Lower Upper
91 100
106 45.3 20.1 60.2

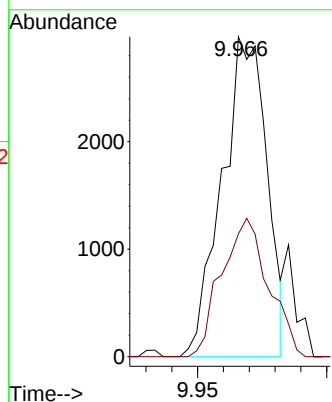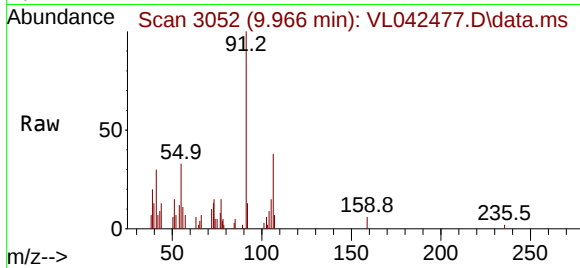

#61
Styrene
Concen: 0.143 ppbv
RT: 9.875 min Scan# 3024
Delta R.T. 0.003 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53

Tgt Ion: 104 Resp: 1295
Ion Ratio Lower Upper
104 100
78 60.1 46.9 70.3
103 59.5 36.6 55.0#


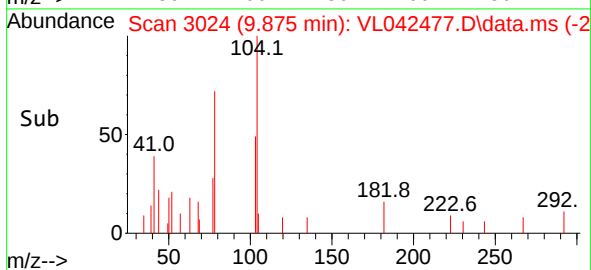

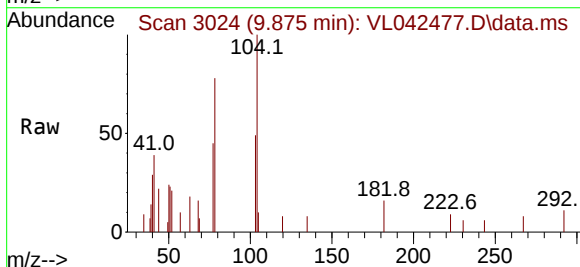




#68
1-Bromo-4-Fluorobenzene
Concen: 9.904 ppbv
RT: 10.383 min Scan# 3179
Delta R.T. 0.007 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53




Instrument :
MSVOA_L
ClientSampleId :
EBR-P06-SC-IA01-20250428DUP


Tgt Ion: 95 Resp: 158397
Ion Ratio Lower Upper
95 100
174 54.3 42.7 64.1
175 3.9 3.6 5.4

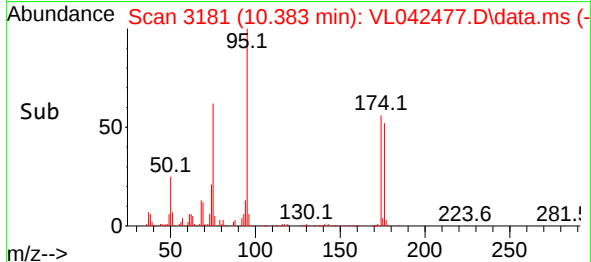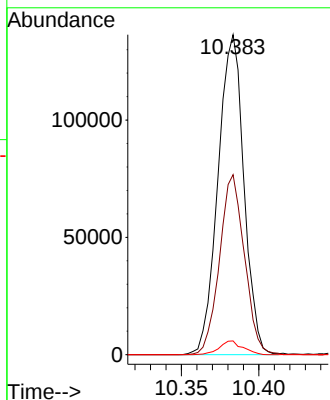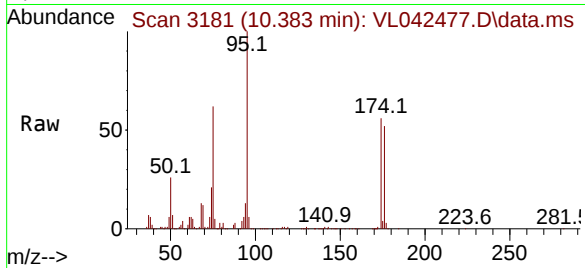

#72
4-Ethyltoluene
Concen: 0.030 ppbv
RT: 11.131 min Scan# 3412
Delta R.T. 0.007 min
Lab File: VL042477.D
Acq: 05 May 2025 15:53

Tgt Ion: 105 Resp: 864
Ion Ratio Lower Upper
105 100
120 0.0 22.0 33.0#
91 0.0 11.2 16.8#
77 0.0 12.2 18.4#


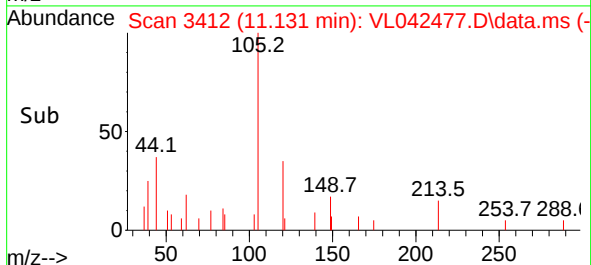
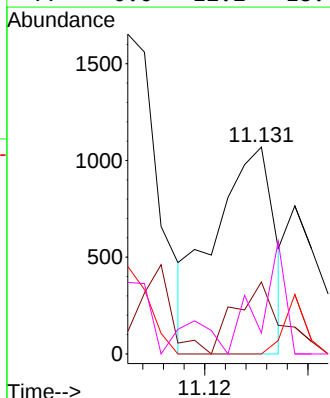
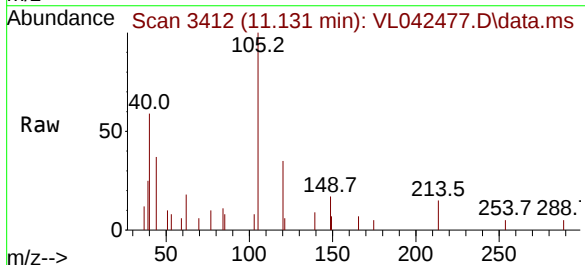




#73
 1,3,5-Trimethylbenzene
 Concen: 0.049 ppbv
 RT: 11.205 min Scan# 3434
 Delta R.T. 0.003 min
 Lab File: VL042477.D
 Acq: 05 May 2025 15:53

Instrument :
 MSVOA_L
 ClientSampleId :
 EBR-P06-SC-IA01-20250428DUP

Tgt Ion:105 Resp: 1235
 Ion Ratio Lower Upper
 105 100
 120 46.7 34.4 51.6

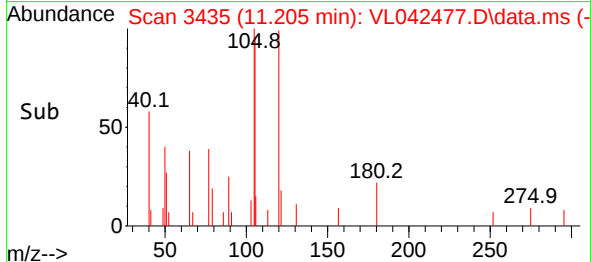

#74
 1,2,4-Trimethylbenzene
 Concen: 0.171 ppbv
 RT: 11.542 min Scan# 3539
 Delta R.T. 0.007 min
 Lab File: VL042477.D
 Acq: 05 May 2025 15:53

Tgt Ion:105 Resp: 5187
 Ion Ratio Lower Upper
 105 100
 120 37.3 36.1 54.1
 91 10.0 57.6 86.4#
 77 16.5 22.1 33.1#

