


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050620\
 Data File : VL034935.D
 Acq On : 6 May 2020 9:07
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050620AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Mar 09 16:42:53 2020
 Last Update : Mon Mar 09 16:42:53 2020

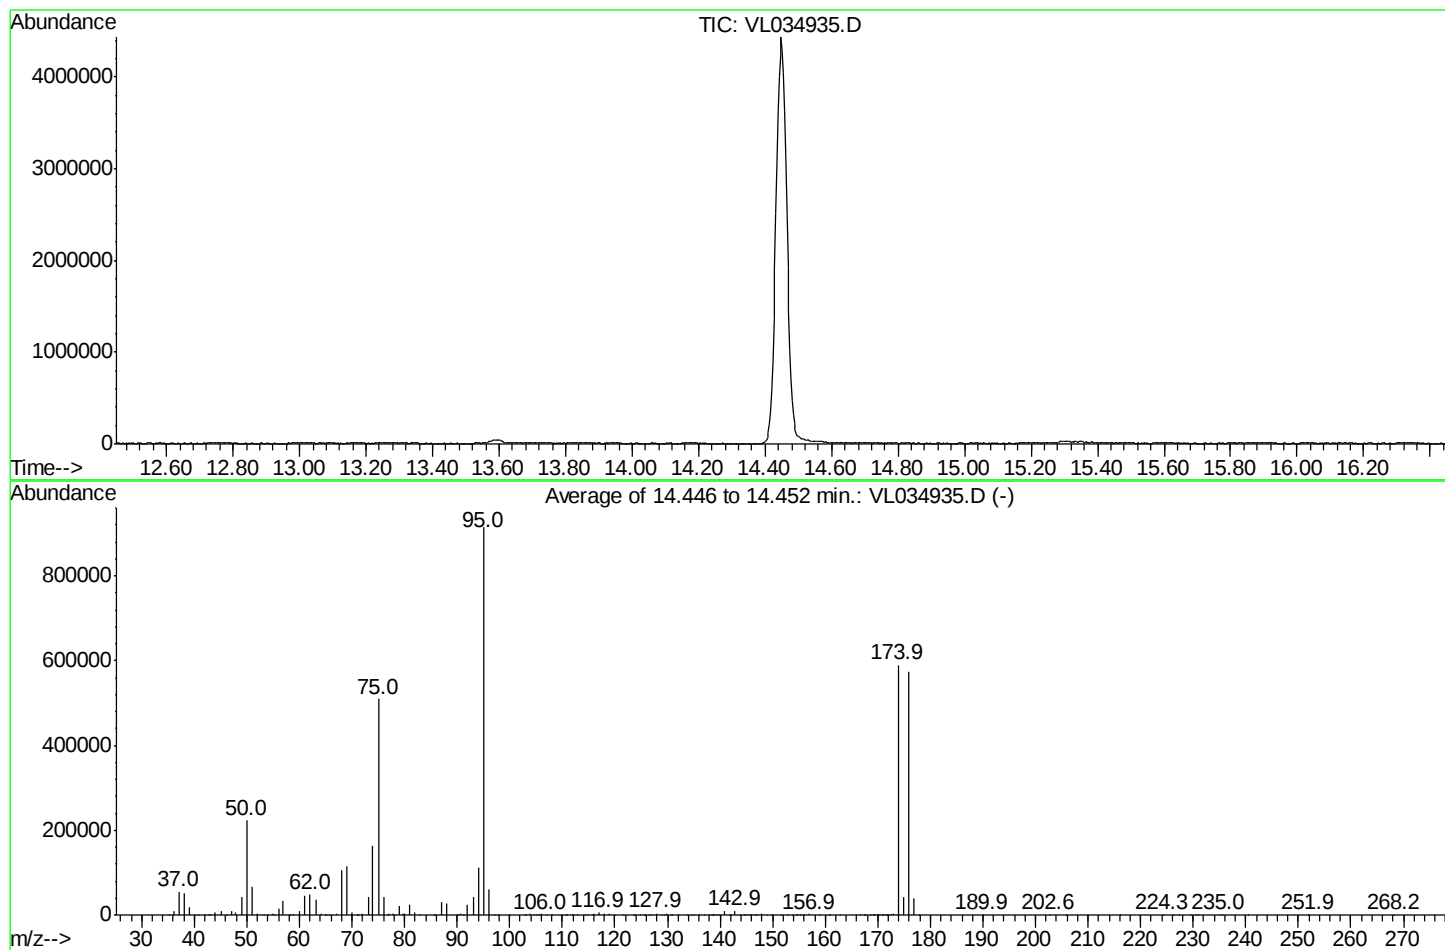

AutoFind: Scans 3626, 3627, 3628; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	222103	PASS
75	95	30	66	55.8	510250	PASS
95	95	100	100	100.0	914645	PASS
96	95	5	9	6.7	61328	PASS
173	174	0.00	2	0.8	4466	PASS
174	95	50	120	64.5	590122	PASS
175	174	4	9	7.3	43088	PASS
176	174	93	101	97.5	575402	PASS
177	176	5	9	6.8	39165	PASS