

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050624\
 Data File : VL041221.D
 Acq On : 6 May 2024 17:00
 Operator : SY/MD
 Sample : P2334-11
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BA-03-IA03-20240425

Quant Time: May 07 05:25:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue May 07 05:19:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	5.195	49	818706	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.658	114	2139757	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.468	117	1979374	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.780	95	1472830	9.856	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.600%
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	2.739	85	42942	0.388	ppbv	98
3) Chlorodifluoromethane	2.661	51	4439460	35.703	ppbv #	60
4) Chloromethane	2.822	50	27552	0.565	ppbv	97
8) Dichlorotetrafluoroethane	2.864	85	3590	0.031	ppbv #	66
9) Propene	2.716	41	71282	1.465	ppbv #	71
10) Heptane	7.581	43	12391	0.105	ppbv #	29
11) Trichlorofluoromethane	3.575	101	30299	0.269	ppbv	85
12) 1,1,2-Trichlorotrifluoro...	4.073	101	4340	0.052	ppbv #	52
13) Ethanol	3.253	45	7446042	682.598	ppbv	99
15) Acetone	3.472	43	1340913	13.878	ppbv	99
16) 1,3-Butadiene	2.986	39	2350	0.048	ppbv #	1
17) tert-Butyl alcohol	3.896	59	19913	0.191	ppbv #	79
19) Isopropyl Alcohol	3.591	45	1387720	21.887	ppbv #	44
20) Methylene Chloride	3.944	84	42649	1.269	ppbv	84
21) Allyl Chloride	3.899	41	4915	0.078	ppbv #	35
22) trans-1,2-Dichloroethene	4.456	96	1793	0.046	ppbv #	32
23) Vinyl Acetate	4.623	43	35021	0.329	ppbv #	59
25) Ethyl Acetate	5.211	43	435324	2.257	ppbv #	97
26) Hexane	5.218	57	188787	2.194	ppbv	97
29) Chloroform	5.279	83	4407	0.037	ppbv	98
30) Cyclohexane	6.600	84	2242	0.033	ppbv #	1
31) cis-1,2-Dichloroethene	5.208	61	37522	0.466	ppbv #	28
34) 2-Butanone	4.796	43	72874	0.669	ppbv	98
36) Benzene	6.372	78	37722	0.210	ppbv #	92
37) 1,2-Dichloroethane	5.809	62	30929	0.330	ppbv	100
39) 1,2-Dichloropropane	6.655	63	543600	7.855	ppbv #	23
50) 4-Methyl-2-Pentanone	8.188	43	8100	0.041	ppbv #	40
52) Tetrachloroethene	10.622	164	8326	0.132	ppbv #	72
53) Toluene	9.224	91	175777	0.844	ppbv	98
58) Ethyl Benzene	12.089	91	24219	0.089	ppbv	100
59) m/p-Xylene	12.368	91	14641	0.064	ppbv #	31
60) o-Xylene	13.056	91	16175	0.076	ppbv	79
61) Styrene	12.902	104	8943	0.079	ppbv #	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050624\
Data File : VL041221.D
Acq On : 6 May 2024 17:00
Operator : SY/MD
Sample : P2334-11
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Quant Time: May 07 05:25:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue May 07 05:19:44 2024
Response via : Initial Calibration

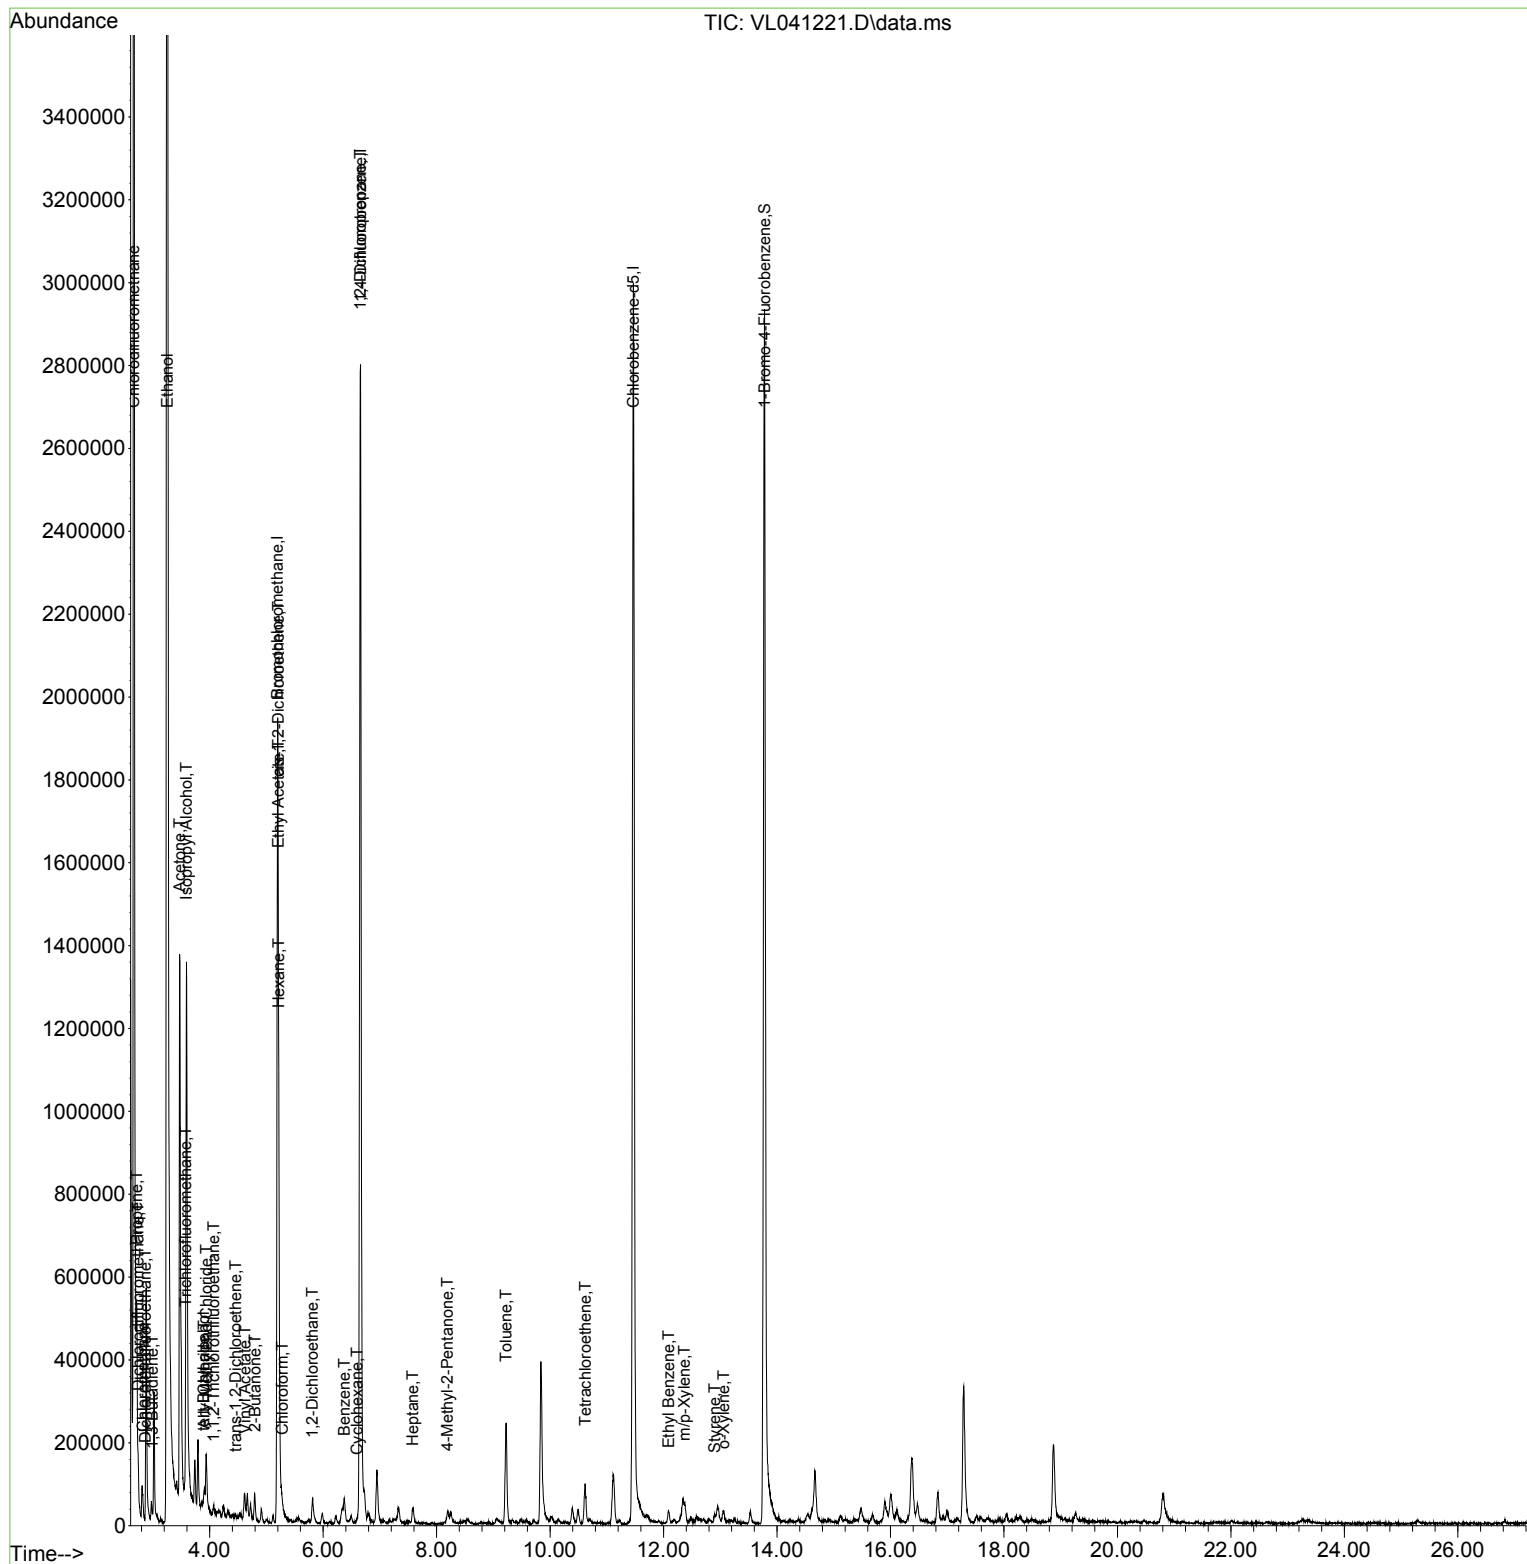






#1
 Bromochloromethane
 Concen: 10.000 ppbv
 RT: 5.195 min Scan# 804
 Delta R.T. 0.000 min
 Lab File: VL041221.D
 Acq: 6 May 2024 17:00

Instrument :
 MSVOA_L
 ClientSampleId :
 BA-03-IA03-20240425



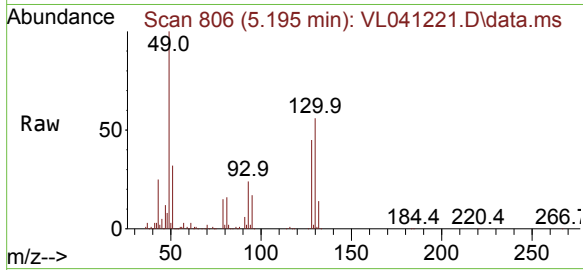



Tgt Ion: 49 Resp: 818706
 Ion Ratio Lower Upper
 49 100
 128 45.4 21.5 64.5
 130 57.5 27.2 81.6

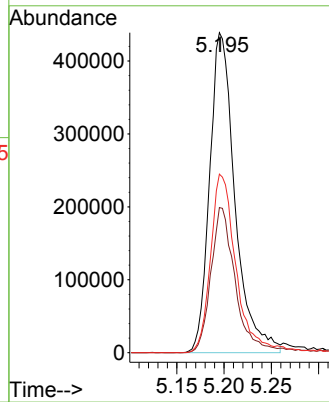

#2
 Dichlorodifluoromethane
 Concen: 0.388 ppbv
 RT: 2.739 min Scan# 42
 Delta R.T. 0.000 min
 Lab File: VL041221.D
 Acq: 6 May 2024 17:00

Tgt Ion: 85 Resp: 42942
 Ion Ratio Lower Upper
 85 100
 87 30.9 25.7 38.5

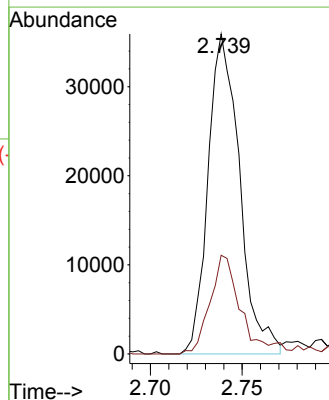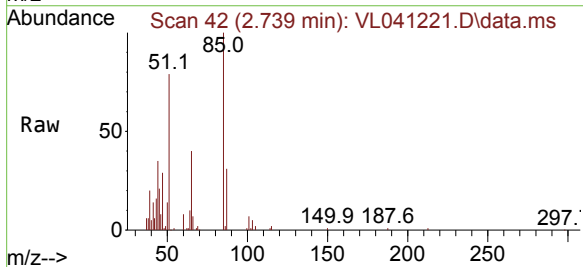

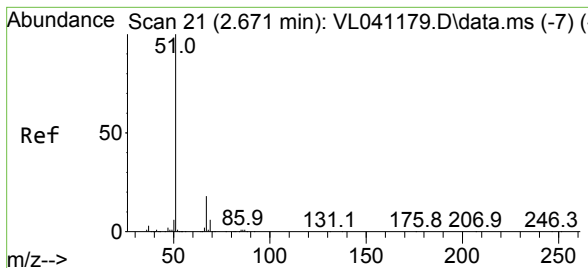

#3

Chlorodifluoromethane

Concen: 35.703 ppbv

RT: 2.661 min Scan# 18

Delta R.T. -0.022 min

Lab File: VL041221.D

Acq: 6 May 2024 17:00

Instrument :

MSVOA_L

ClientSampleId :





BA-03-IA03-20240425

Tgt Ion: 51 Resp: 4439460

Ion Ratio Lower Upper

51 100

67 0.2 14.0 21.0#

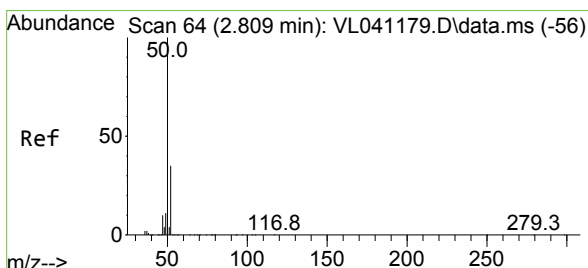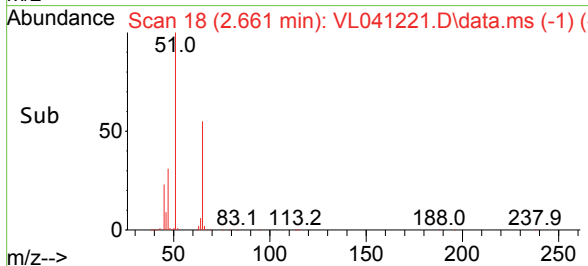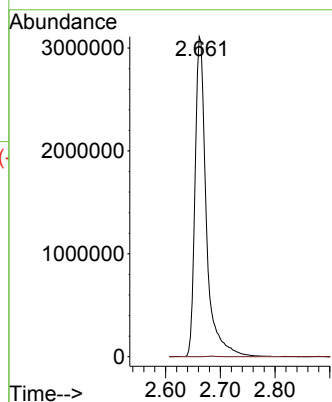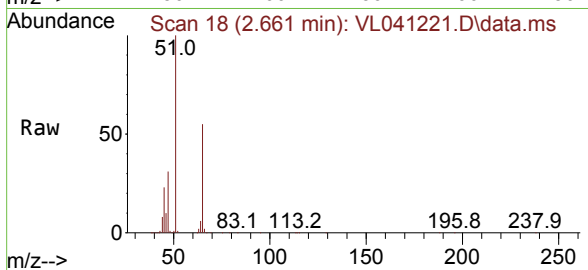

#4

Chloromethane

Concen: 0.565 ppbv

RT: 2.822 min Scan# 68

Delta R.T. 0.000 min

Lab File: VL041221.D




Acq: 6 May 2024 17:00


Tgt Ion: 50 Resp: 27552

Ion Ratio Lower Upper

50 100

52 37.2 28.3 42.5


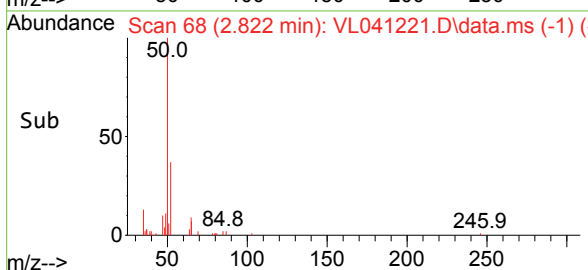
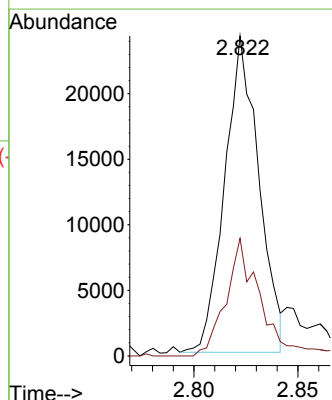
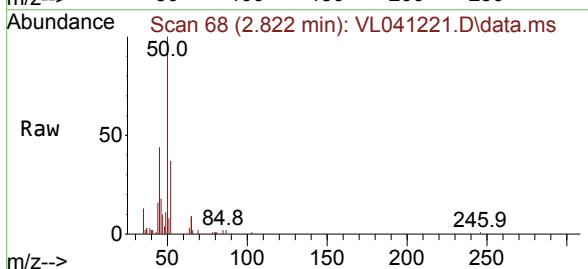


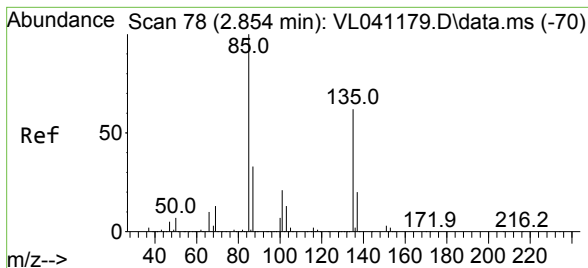

#8
Dichlorotetrafluoroethane
Concen: 0.031 ppbv
RT: 2.864 min Scan# 81
Delta R.T. -0.003 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00




Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Tgt Ion: 85 Resp: 3590
Ion Ratio Lower Upper
85 100
135 38.0 51.5 77.3#

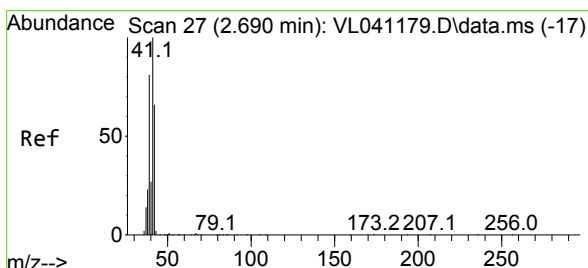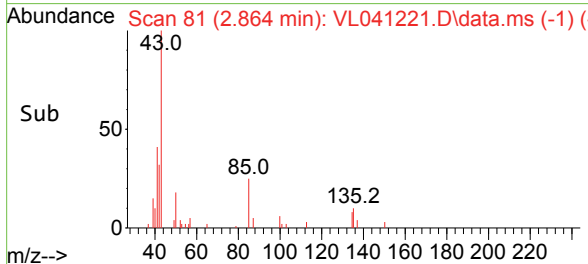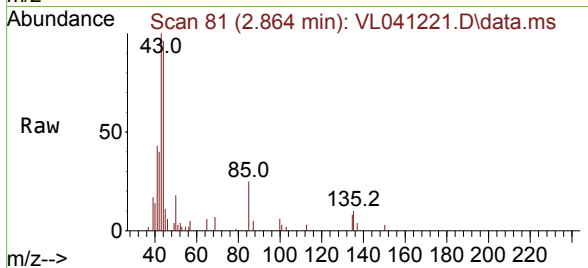

#9
Propene
Concen: 1.465 ppbv
RT: 2.716 min Scan# 35
Delta R.T. 0.013 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Tgt Ion: 41 Resp: 71282
Ion Ratio Lower Upper
41 100
42 45.4 55.3 82.9#


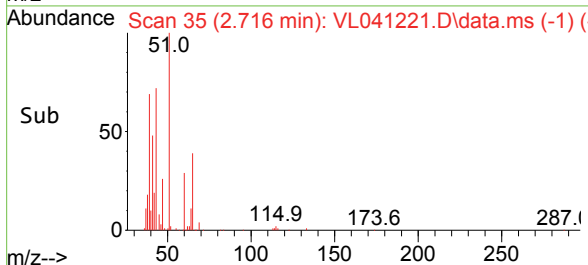

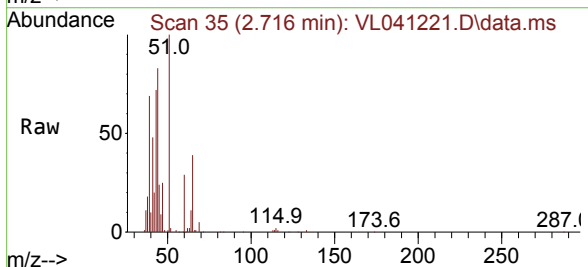




#10
Heptane
Concen: 0.105 ppbv
RT: 7.581 min Scan# 11
Delta R.T. 0.003 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00




Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Tgt Ion: 43 Resp: 12391
Ion Ratio Lower Upper
43 100
57 0.0 38.7 58.1#

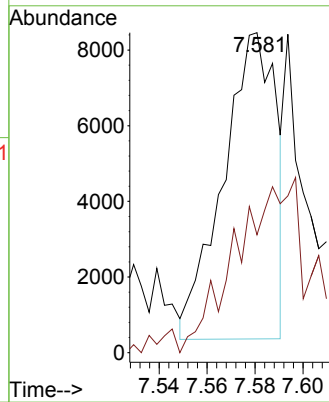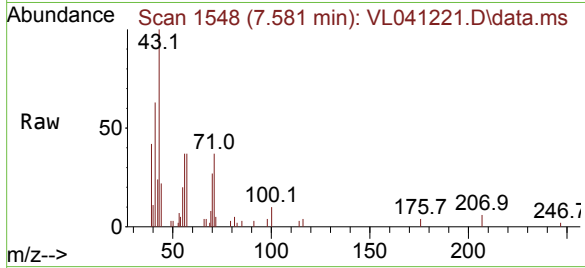

#11
Trichlorofluoromethane
Concen: 0.269 ppbv
RT: 3.575 min Scan# 302
Delta R.T. 0.007 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Tgt Ion: 101 Resp: 30299
Ion Ratio Lower Upper
101 100
103 52.5 51.6 77.4

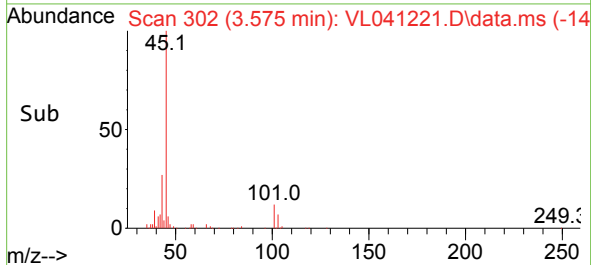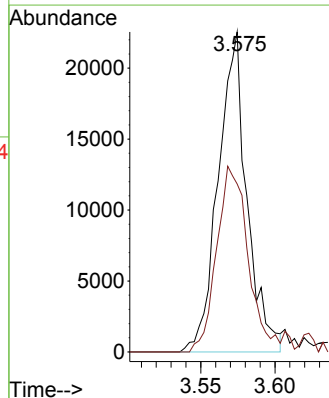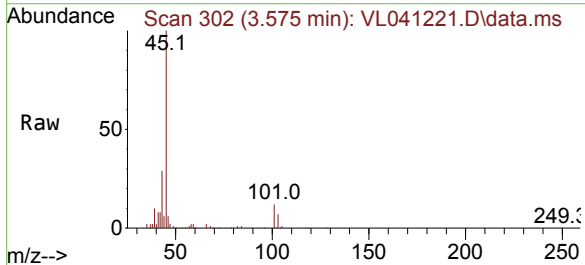



#12

1,1,2-Trichlorotrifluoroethane

Concen: 0.052 ppbv

RT: 4.073 min Scan# 4

Delta R.T. 0.003 min

Lab File: VL041221.D

Acq: 6 May 2024 17:00

Instrument :

MSVOA_L

ClientSampleId :





BA-03-IA03-20240425

Tgt Ion:101 Resp: 4340

Ion Ratio Lower Upper

101 100

151 111.0 56.8 85.2#

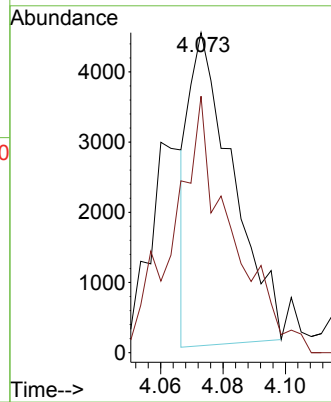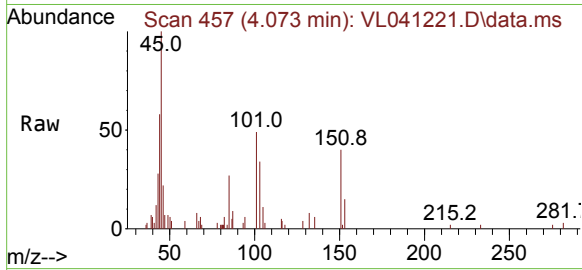

#13

Ethanol

Concen: 682.598 ppbv

RT: 3.253 min Scan# 202

Delta R.T. 0.010 min

Lab File: VL041221.D




Acq: 6 May 2024 17:00


Tgt Ion: 45 Resp: 7446042

Ion Ratio Lower Upper

45 100

46 37.3 14.8 59.0



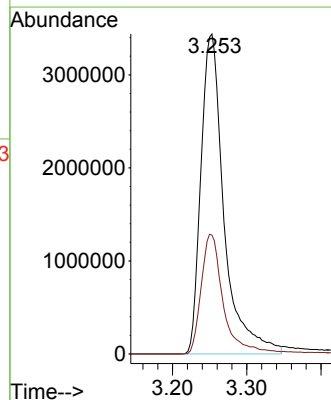
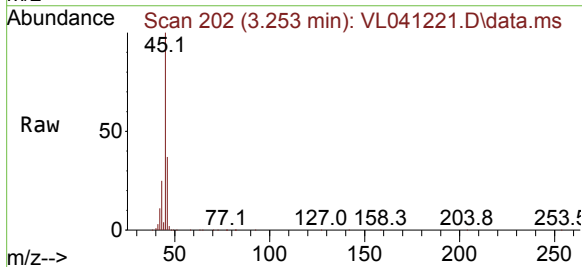




#15
Acetone
Concen: 13.878 ppbv
RT: 3.472 min Scan# 21
Delta R.T. -0.003 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00




Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Tgt Ion: 43 Resp: 1340913
Ion Ratio Lower Upper
43 100
58 26.3 21.4 32.0

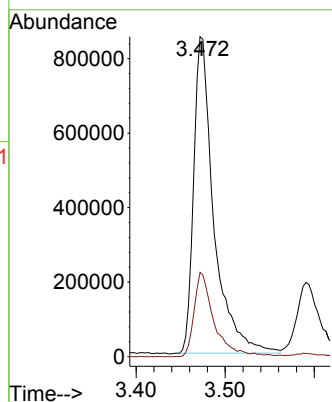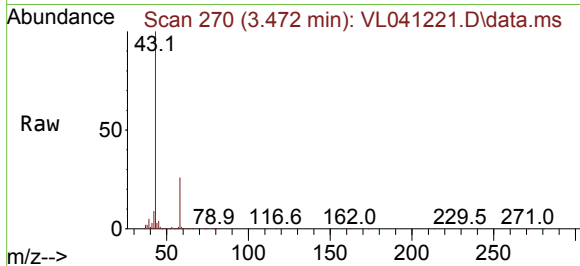

#16
1,3-Butadiene
Concen: 0.048 ppbv
RT: 2.986 min Scan# 119
Delta R.T. -0.006 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Tgt Ion: 39 Resp: 2350
Ion Ratio Lower Upper
39 100
54 176.3 62.2 93.4#



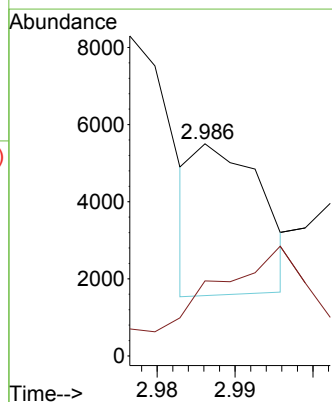
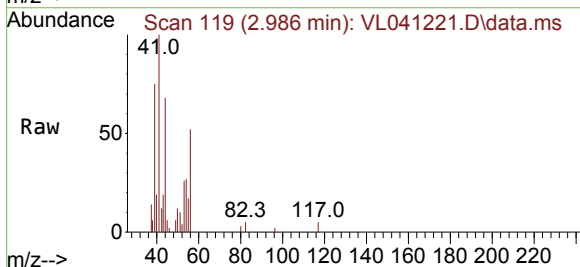




#17
tert-Butyl alcohol
Concen: 0.191 ppbv
RT: 3.896 min Scan# 402
Delta R.T. 0.013 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00




Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Tgt Ion: 59 Resp: 19913
Ion Ratio Lower Upper
59 100
57 18.2 8.4 12.6#

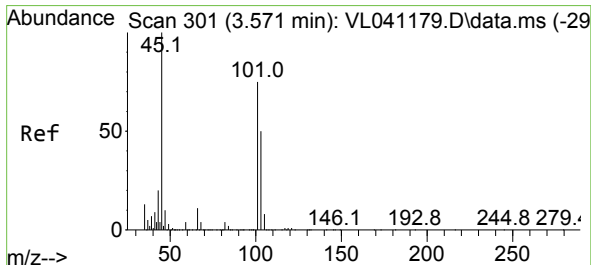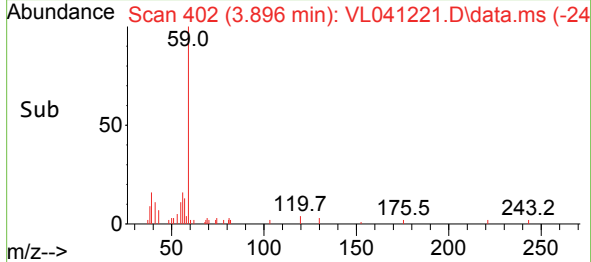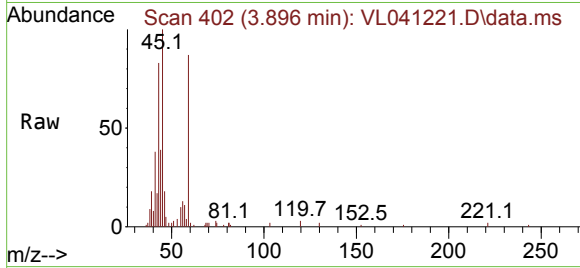

#19
Isopropyl Alcohol
Concen: 21.887 ppbv
RT: 3.591 min Scan# 307
Delta R.T. 0.010 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Tgt Ion: 45 Resp: 1387720
Ion Ratio Lower Upper
45 100
58 1.5 26.8 40.2#

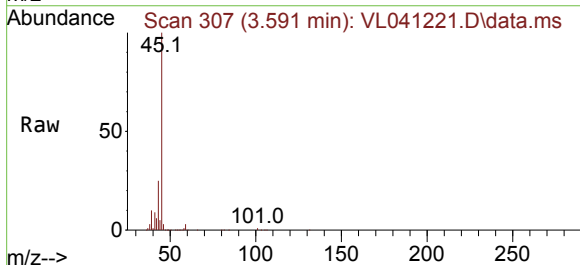







#20
Methylene Chloride
Concen: 1.269 ppbv
RT: 3.944 min Scan# 41
Delta R.T. 0.007 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425

Tgt Ion: 84 Resp: 42649




Ion	Ratio	Lower	Upper
84	100		
49	133.0	130.4	195.6
51	40.8	38.0	57.0
86	58.8	50.3	75.5

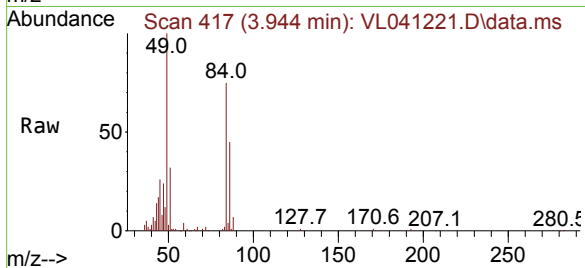


#21
Allyl Chloride
Concen: 0.078 ppbv
RT: 3.899 min Scan# 403
Delta R.T. -0.103 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Tgt Ion: 41 Resp: 4915

Ion	Ratio	Lower	Upper
41	100		
76	0.0	23.7	35.5#
39	141.6	64.7	97.1#




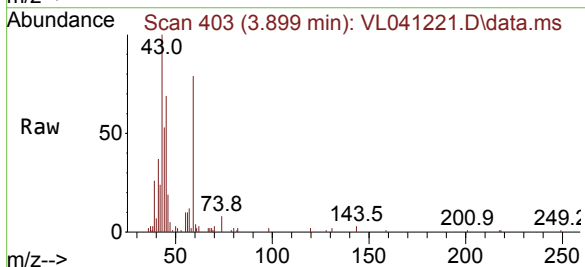




#22
trans-1,2-Dichloroethene
Concen: 0.046 ppbv
RT: 4.456 min Scan# 571
Delta R.T. 0.007 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00




Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Tgt Ion: 96 Resp: 1793
Ion Ratio Lower Upper
96 100
61 61.5 137.6 206.4#
98 36.9 50.6 76.0#

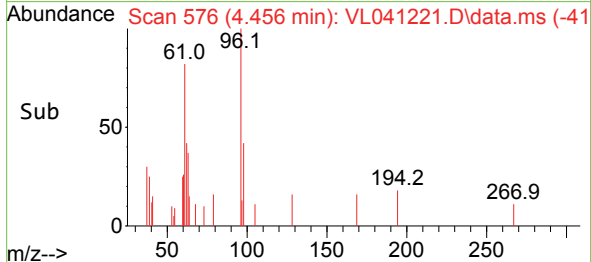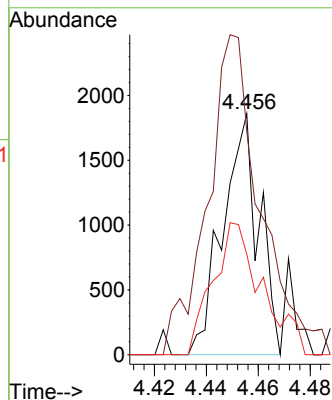

#23
Vinyl Acetate
Concen: 0.329 ppbv
RT: 4.623 min Scan# 628
Delta R.T. -0.006 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Tgt Ion: 43 Resp: 35021
Ion Ratio Lower Upper
43 100
86 8.0 4.9 7.3#
42 39.8 8.0 12.0#
44 3.3 3.7 5.5#


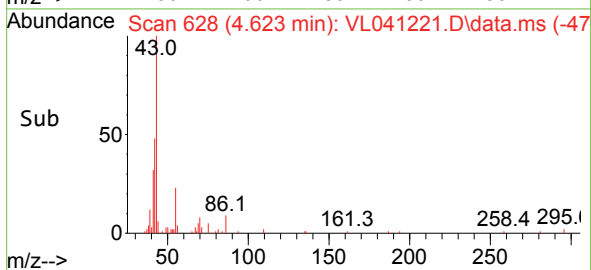
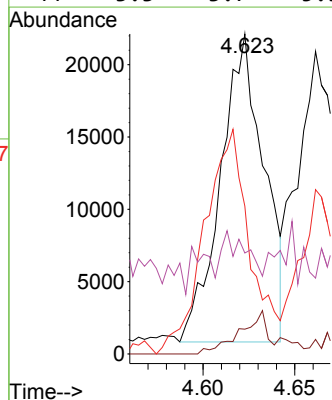





#25
Ethyl Acetate
Concen: 2.257 ppbv
RT: 5.211 min Scan# 811
Delta R.T. 0.007 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00




Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Tgt Ion: 43 Resp: 435324
Ion Ratio Lower Upper
43 100
45 13.1 8.2 12.2#
61 9.3 7.7 11.5
70 7.3 5.8 8.6

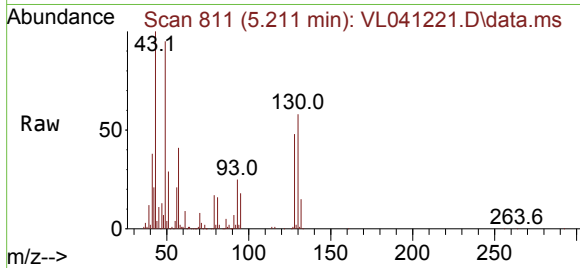

#26
Hexane
Concen: 2.194 ppbv
RT: 5.218 min Scan# 813
Delta R.T. 0.003 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Tgt Ion: 57 Resp: 188787
Ion Ratio Lower Upper
57 100
41 99.1 75.8 113.8
43 238.8 187.0 280.4
56 53.8 42.7 64.1

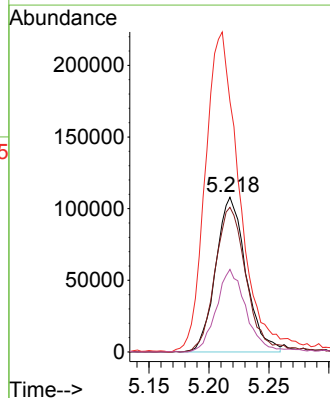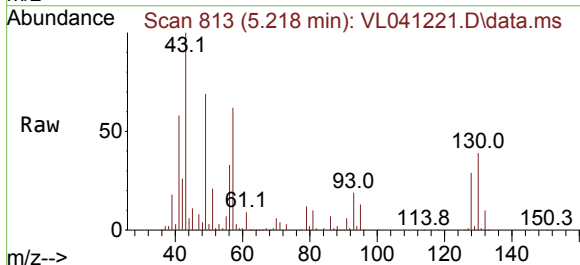



#29

Chloroform

Concen: 0.037 ppbv

RT: 5.279 min Scan# 81

Delta R.T. 0.000 min

Lab File: VL041221.D

Acq: 6 May 2024 17:00

Instrument :

MSVOA_L

ClientSampleId :





BA-03-IA03-20240425

Tgt Ion: 83 Resp: 4407

Ion Ratio Lower Upper

83 100

85 66.5 51.7 77.5

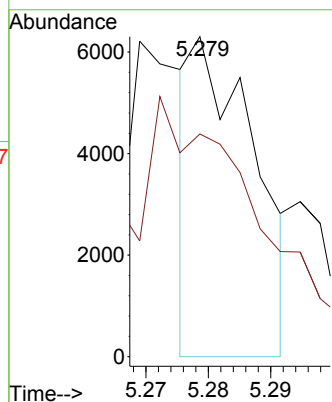

#30

Cyclohexane

Concen: 0.033 ppbv

RT: 6.600 min Scan# 1243

Delta R.T. 0.000 min

Lab File: VL041221.D

Acq: 6 May 2024 17:00




Tgt Ion: 84 Resp: 2242


Ion Ratio Lower Upper

84 100

56 0.0 116.8 175.2#

41 326.6 73.8 110.8#


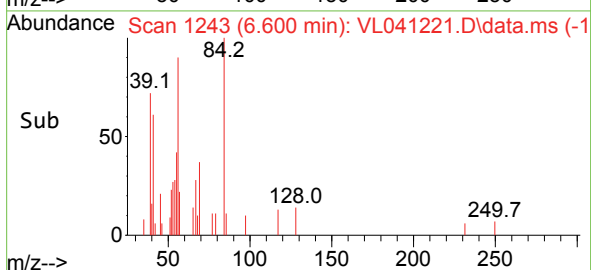
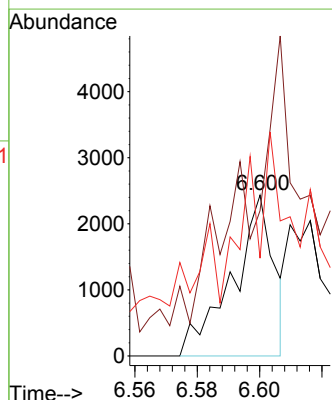





#31
 cis-1,2-Dichloroethene
 Concen: 0.466 ppbv
 RT: 5.208 min Scan# 81
 Delta R.T. 0.129 min
 Lab File: VL041221.D
 Acq: 6 May 2024 17:00




Instrument :
 MSVOA_L
 ClientSampleId :
 BA-03-IA03-20240425


Tgt Ion: 61 Resp: 37522
 Ion Ratio Lower Upper
 61 100
 96 2.4 49.8 74.6#
 98 0.0 30.0 45.0#

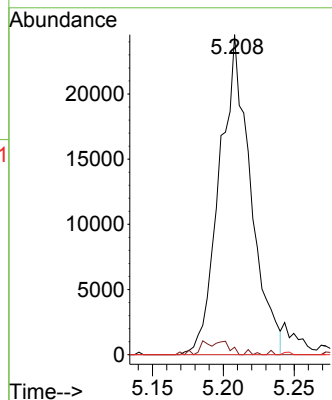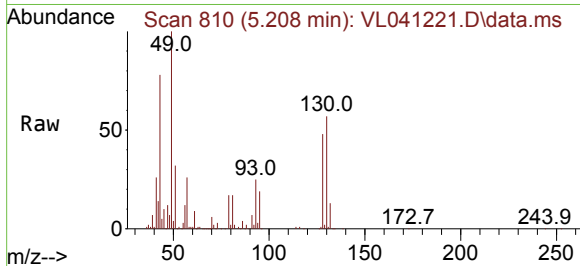

#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 6.658 min Scan# 1261
 Delta R.T. 0.003 min
 Lab File: VL041221.D
 Acq: 6 May 2024 17:00

Tgt Ion: 114 Resp: 2139757
 Ion Ratio Lower Upper
 114 100
 63 25.9 21.8 32.6
 88 18.1 15.2 22.8


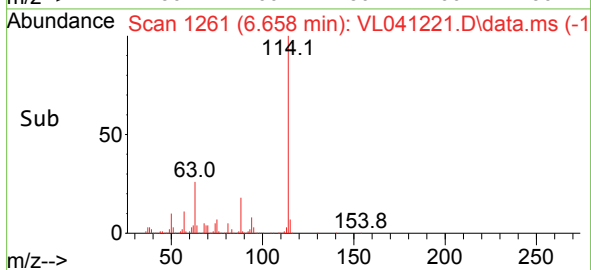
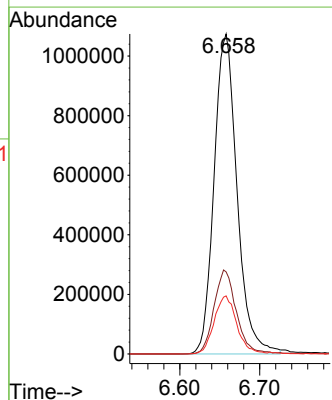
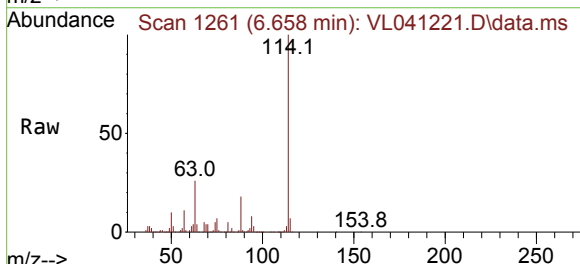




#34
2-Butanone
Concen: 0.669 ppbv
RT: 4.796 min Scan# 61
Delta R.T. 0.010 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00




Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Tgt Ion: 43 Resp: 72874
Ion Ratio Lower Upper
43 100
72 22.3 17.3 25.9

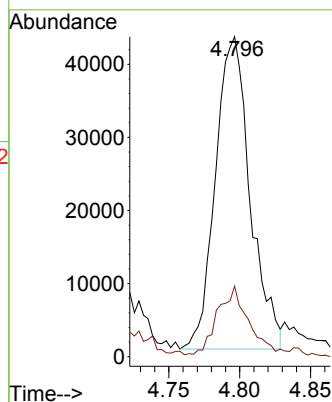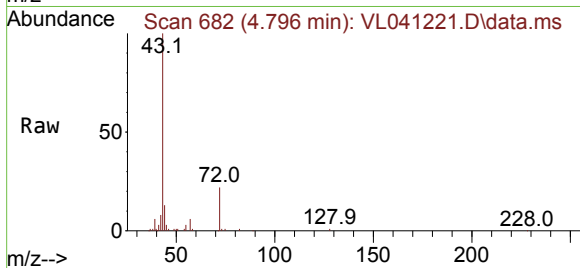

#36
Benzene
Concen: 0.210 ppbv
RT: 6.372 min Scan# 1172
Delta R.T. 0.000 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Tgt Ion: 78 Resp: 37722
Ion Ratio Lower Upper
78 100
77 20.6 18.3 27.5
50 14.4 15.9 23.9#



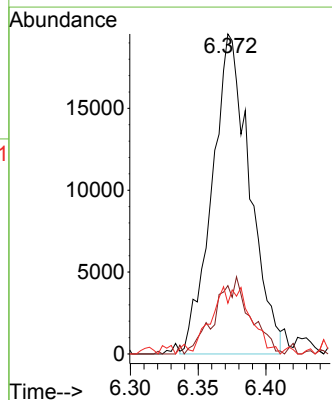
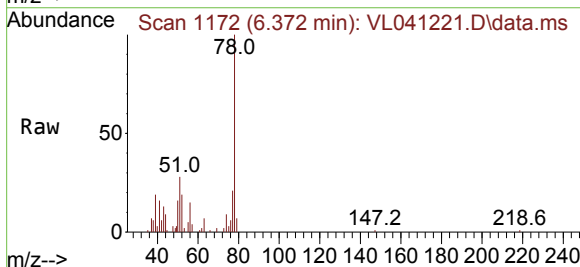




#37
1,2-Dichloroethane
Concen: 0.330 ppbv
RT: 5.809 min Scan# 996
Delta R.T. 0.000 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00




Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Tgt Ion: 62 Resp: 30929
Ion Ratio Lower Upper
62 100
98 6.3 5.0 7.4



#39
1,2-Dichloropropane
Concen: 7.855 ppbv
RT: 6.655 min Scan# 1260
Delta R.T. -0.418 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Tgt Ion: 63 Resp: 543600
Ion Ratio Lower Upper
63 100
41 0.0 59.4 89.0#
62 17.4 56.8 85.2#



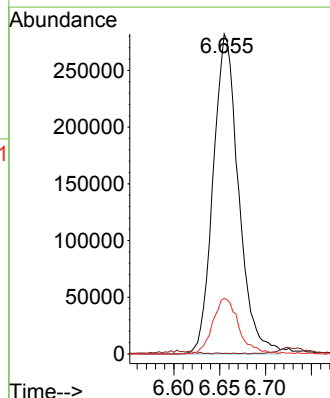





#50
 4-Methyl-2-Pentanone
 Concen: 0.041 ppbv
 RT: 8.188 min Scan# 1737
 Delta R.T. 0.010 min
 Lab File: VL041221.D
 Acq: 6 May 2024 17:00




Instrument :
 MSVOA_L
 ClientSampleId :
 BA-03-IA03-20240425


Tgt Ion: 43 Resp: 8100
 Ion Ratio Lower Upper
 43 100
 58 0.0 27.7 41.5#

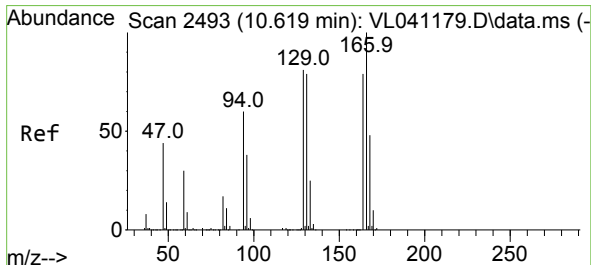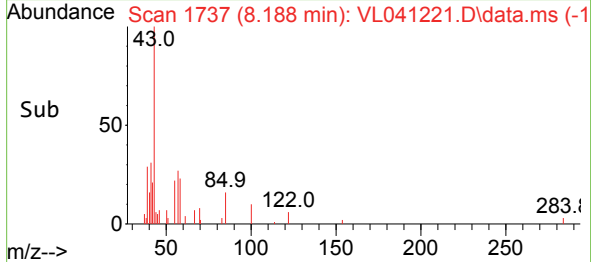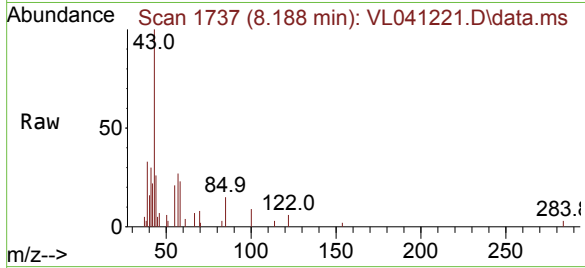

#52
 Tetrachloroethene
 Concen: 0.132 ppbv
 RT: 10.622 min Scan# 2494
 Delta R.T. 0.010 min
 Lab File: VL041221.D
 Acq: 6 May 2024 17:00

Tgt Ion: 164 Resp: 8326
 Ion Ratio Lower Upper
 164 100
 166 93.3 101.1 151.7#
 129 83.9 81.7 122.5
 131 64.4 80.4 120.6#



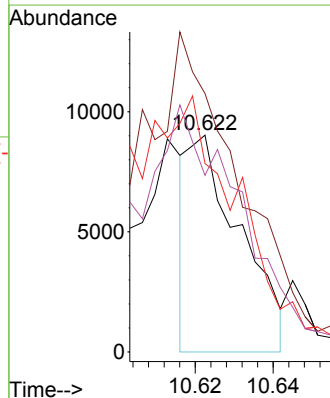
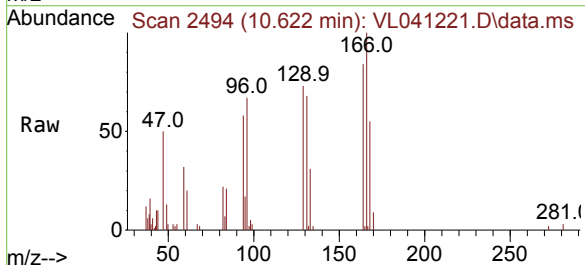


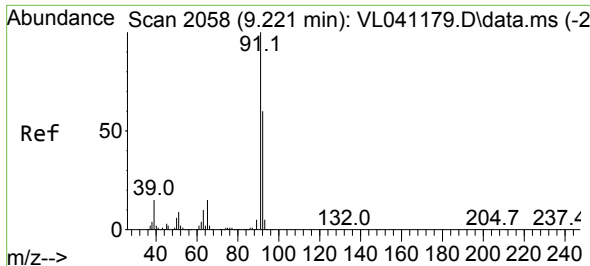

#53
Toluene
Concen: 0.844 ppbv
RT: 9.224 min Scan# 2058
Delta R.T. 0.003 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00




Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Tgt Ion: 91 Resp: 175777
Ion Ratio Lower Upper
91 100
92 61.9 48.2 72.4

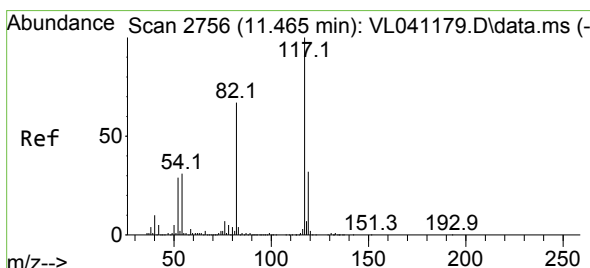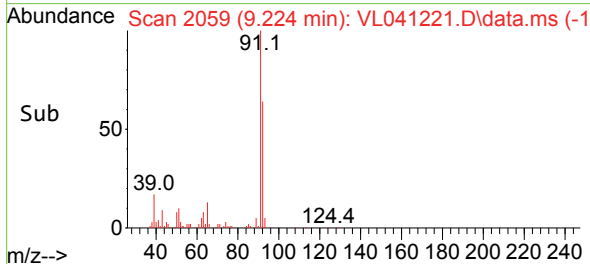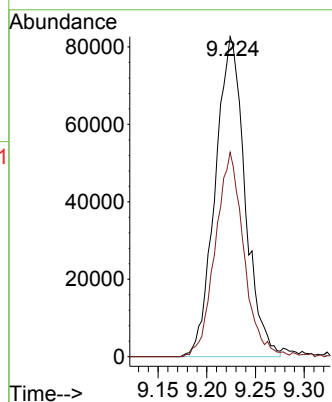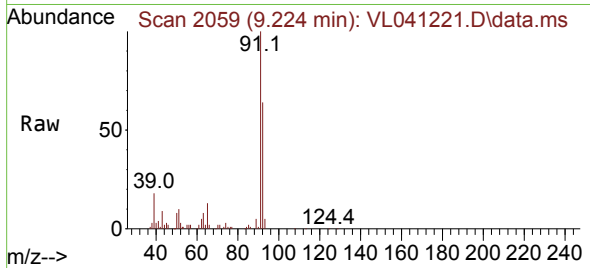

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.468 min Scan# 2757
Delta R.T. 0.003 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00

Tgt Ion: 117 Resp: 1979374
Ion Ratio Lower Upper
117 100
82 66.4 53.6 80.4
119 33.3 27.2 40.8

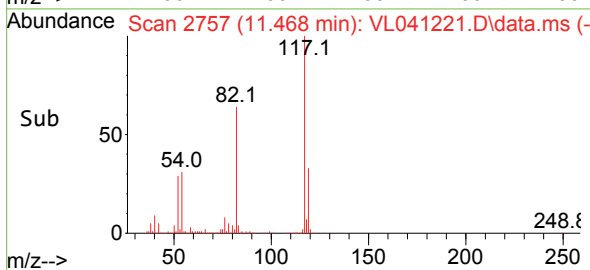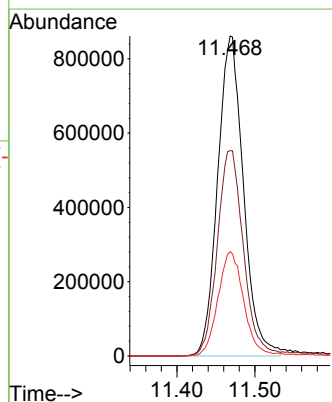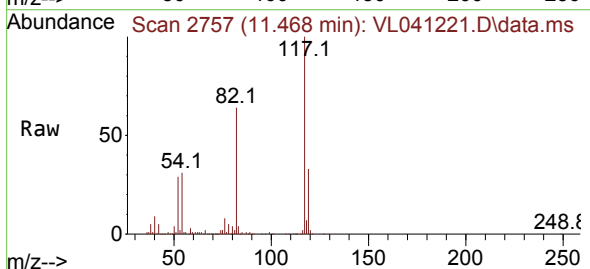

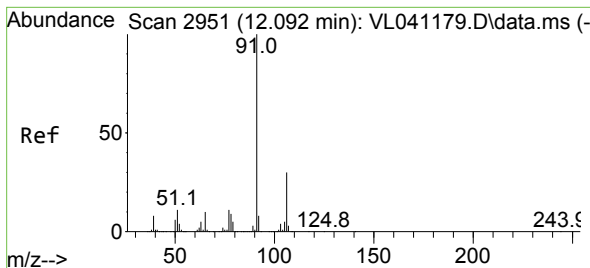

#58

Ethyl Benzene

Concen: 0.089 ppbv

RT: 12.089 min Scan# 2951

Delta R.T. 0.003 min

Lab File: VL041221.D

Acq: 6 May 2024 17:00

Instrument :

MSVOA_L

ClientSampleId :





BA-03-IA03-20240425

Tgt Ion: 91 Resp: 24219

Ion Ratio Lower Upper

91 100

106 30.6 24.3 36.5

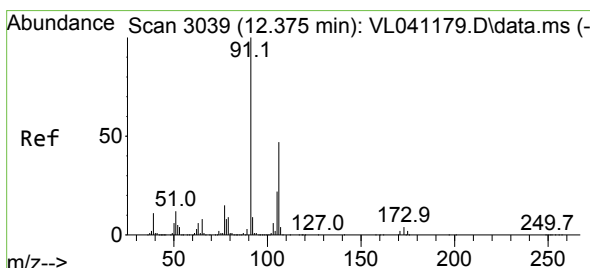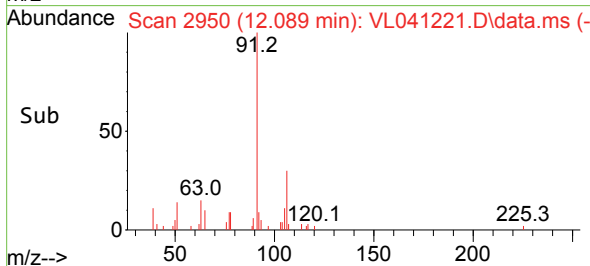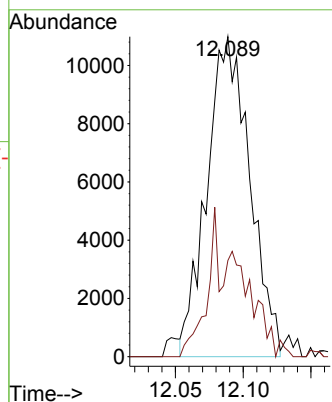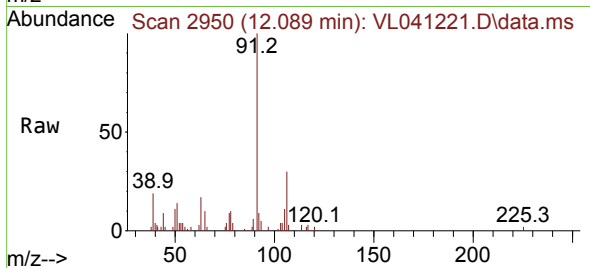

#59

m/p-Xylene

Concen: 0.064 ppbv

RT: 12.368 min Scan# 3037

Delta R.T. 0.000 min

Lab File: VL041221.D




Acq: 6 May 2024 17:00


Tgt Ion: 91 Resp: 14641

Ion Ratio Lower Upper

91 100

106 0.0 35.7 53.5#


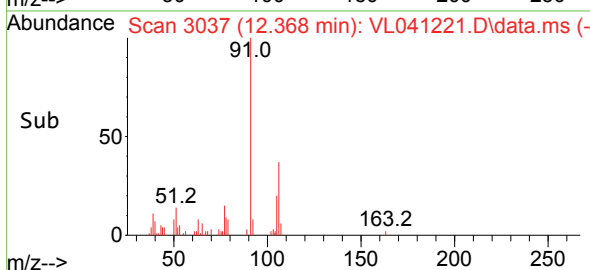
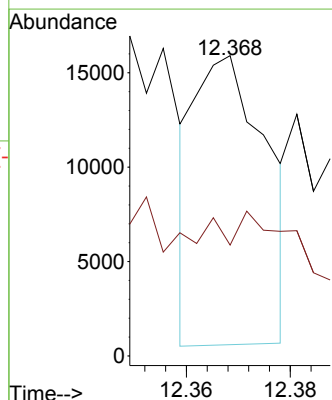
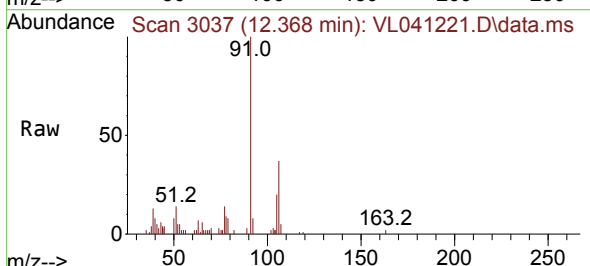




#60
o-Xylene
Concen: 0.076 ppbv
RT: 13.056 min Scan# 31
Delta R.T. 0.000 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00




Instrument :
MSVOA_L
ClientSampleId :
BA-03-IA03-20240425


Tgt Ion: 91 Resp: 16175
Ion Ratio Lower Upper
91 100
106 58.3 22.4 67.3

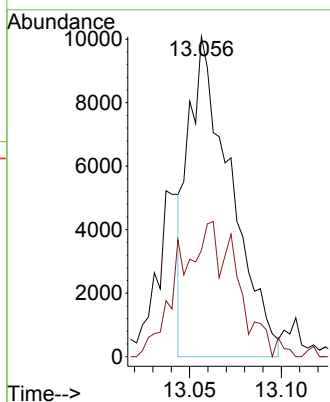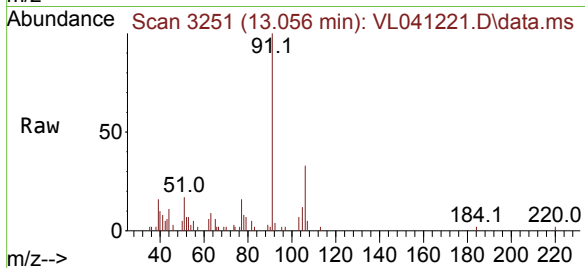

#61
Styrene
Concen: 0.079 ppbv
RT: 12.902 min Scan# 3203
Delta R.T. 0.007 min
Lab File: VL041221.D
Acq: 6 May 2024 17:00


Tgt Ion: 104 Resp: 8943
Ion Ratio Lower Upper
104 100
78 68.5 42.6 63.8#
103 57.9 38.4 57.6#

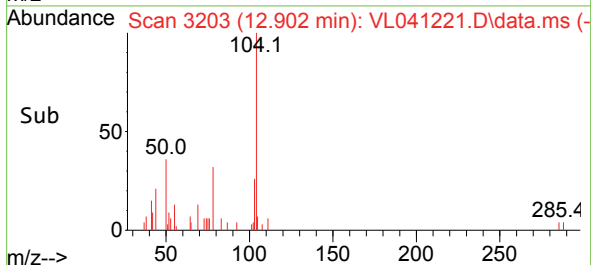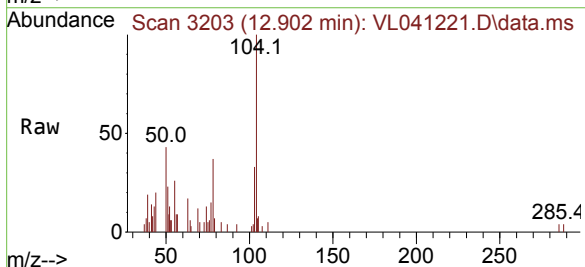

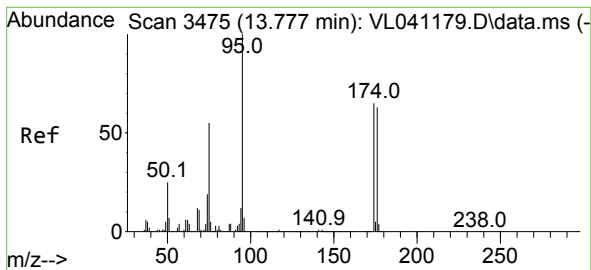

#68
 1-Bromo-4-Fluorobenzene
 Concen: 9.856 ppbv
 RT: 13.780 min Scan# 3476
 Delta R.T. 0.007 min
 Lab File: VL041221.D
 Acq: 6 May 2024 17:00

Instrument :
 MSVOA_L
 ClientSampleId :
 BA-03-IA03-20240425

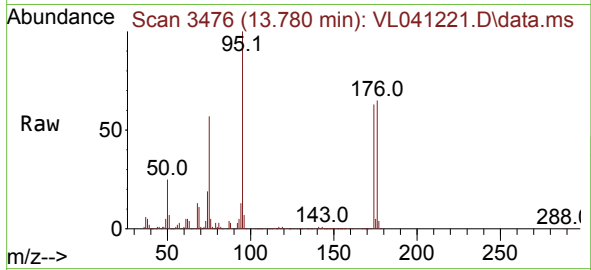

Tgt Ion: 95 Resp: 1472830
 Ion Ratio Lower Upper
 95 100
 174 67.5 53.6 80.4
 175 4.7 4.2 6.4

