
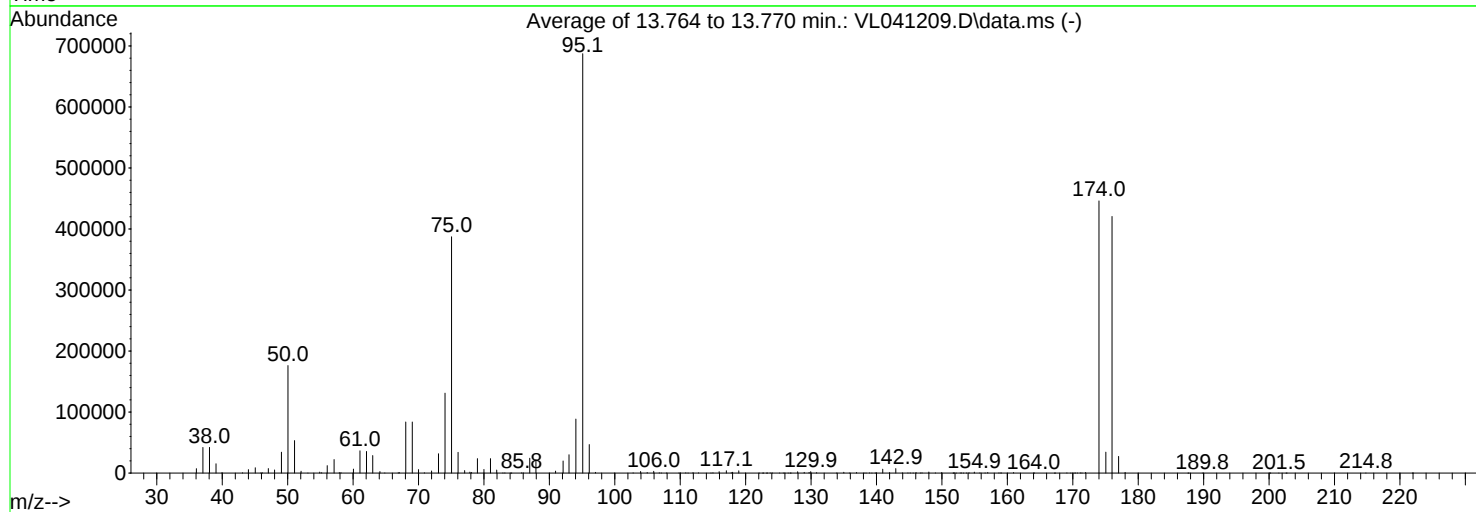


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050624\
Data File : VL041209.D
Acq On : 6 May 2024 8:43
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue May 07 05:19:44 2024

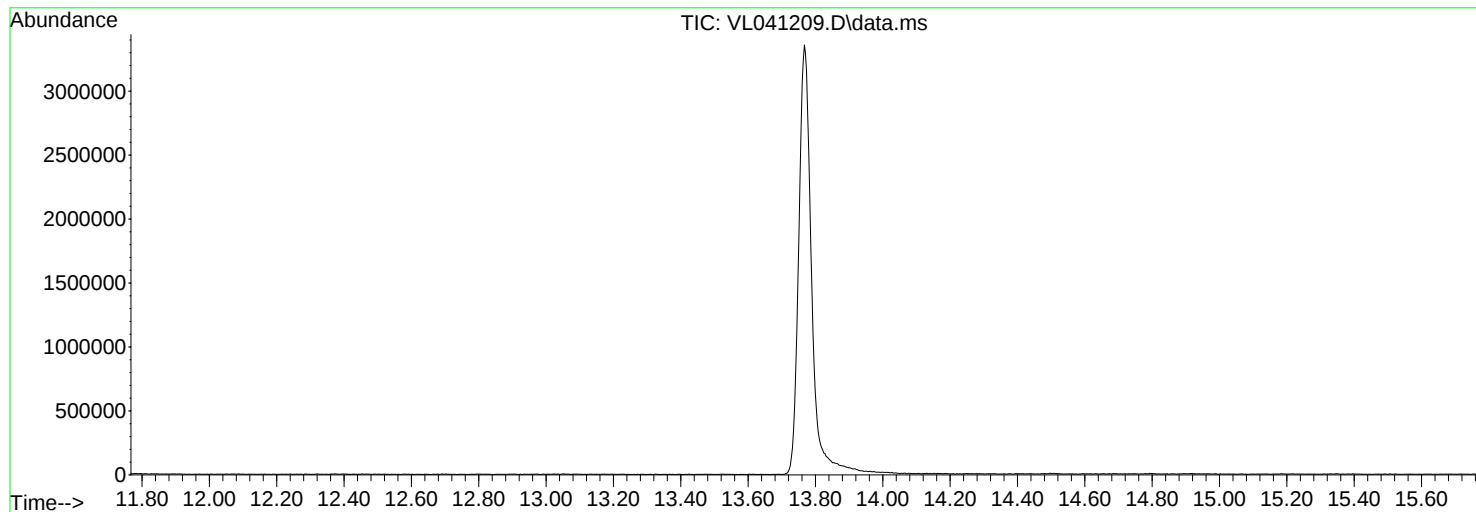

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.6	176192	PASS
75	95	30	66	56.4	387307	PASS
95	95	100	100	100.0	687296	PASS
96	95	5	9	6.8	46747	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	64.9	446080	PASS
175	174	4	9	7.7	34283	PASS
176	174	93	101	94.3	420544	PASS
177	176	5	9	6.5	27275	PASS

Average of 13.764 to 13.770 min.: VL041209.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7275	48.00	5110	58.15	655	70.00	5729
37.05	42064	49.05	34269	60.05	6558	70.90	503
38.05	42083	50.05	176192	61.05	36517	72.00	3459
39.05	15263	51.05	53253	62.05	35432	73.05	3171
39.95	389	52.05	3051	63.00	28757	74.05	131005
43.10	476	53.10	67	64.10	2499	75.05	387307
44.00	5658	54.90	1616	64.85	274	76.05	33963
45.05	8743	55.20	638	66.90	491	77.05	4105
45.90	320	56.05	12231	67.05	1077	77.85	1619
46.15	387	57.10	22211	68.05	83699	78.10	953
47.05	7398	57.90	723	69.05	83731	79.00	23656

Average of 13.764 to 13.770 min.: VL041209.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.00	5954	92.10	19827	107.10	246	117.05	3887
81.00	23692	93.00	30051	107.90	146	117.80	719
81.95	4957	94.05	88533	109.80	137	118.00	1371
82.90	243	95.10	687296	110.00	159	118.95	3711
83.20	348	96.10	46747	110.85	491	122.10	66
84.10	54	97.05	1242	111.20	162	122.60	53
85.75	386	102.80	390	111.95	641	123.20	60
86.00	134	103.95	2640	112.80	436	123.75	301
87.00	24291	104.95	937	114.70	199	124.10	152
87.95	22117	105.95	2971	115.00	597	125.20	154
90.95	3228	106.80	513	115.95	2362	125.75	162

Average of 13.764 to 13.770 min.: VL041209.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.00	83	136.95	969	144.80	240	152.20	119
126.50	100	138.10	121	145.15	340	152.80	249
126.80	53	138.40	123	145.60	183	153.00	266
127.95	2247	138.95	369	146.05	771	153.30	83
128.95	1160	139.30	114	146.70	241	153.75	206
129.70	1108	139.80	221	146.95	479	154.15	453
129.95	2377	139.95	418	148.00	1743	154.95	1628
130.85	687	140.95	6409	149.00	370	155.80	334
133.90	93	142.00	759	149.95	661	156.60	206
135.00	1332	142.95	7411	151.70	55	157.00	986
135.85	163	143.95	272	151.85	434	158.70	194

Average of 13.764 to 13.770 min.: VL041209.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
158.90	301	171.40	225	202.60	55		
159.10	253	171.95	861	214.80	133		
160.95	924	174.00	446080	221.90	54		
164.00	57	175.05	34283				
167.20	63	176.00	420544				
169.10	293	177.00	27275				
169.70	74	178.00	947				
170.20	123	187.60	62				
170.40	205	189.80	66				
170.70	143	200.10	55				
171.15	425	201.50	64				

Instrument :

MSVOA_L

ClientSampleId :

BFB