

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050625\
 Data File : VL042488.D
 Acq On : 06 May 2025 09:49
 Operator : SY/MD
 Sample : VL0506ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0506ABL01

Quant Time: May 07 01:36:30 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL050125AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri May 02 03:16:31 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	71766	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.959	114	194806	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	158449	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.380	95	146316	9.960	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050625\
Data File : VL042488.D
Acq On : 06 May 2025 09:49
Operator : SY/MD
Sample : VL0506ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0506ABL01

Quant Time: May 07 01:36:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL050125AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri May 02 03:16:31 2025
Response via : Initial Calibration




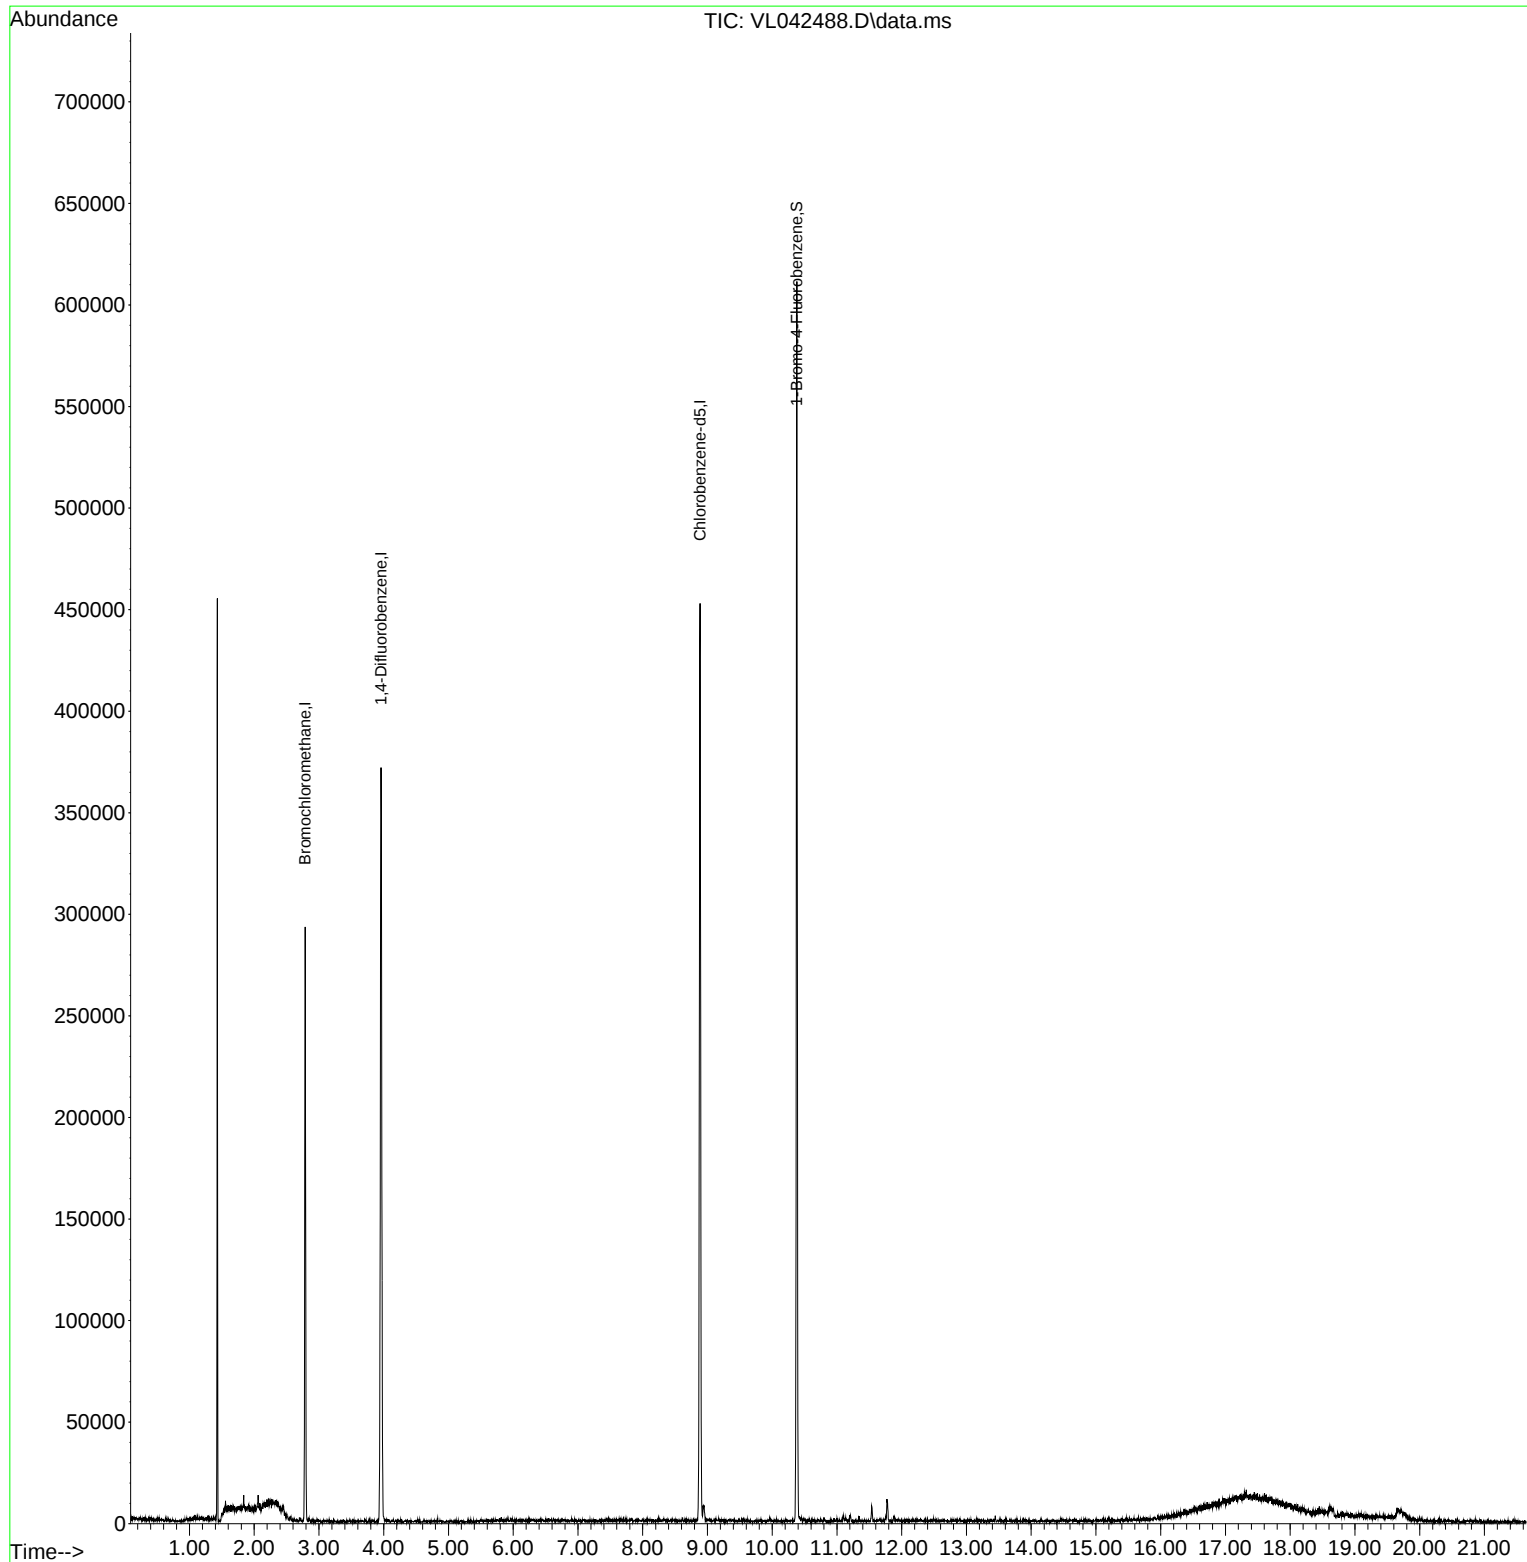


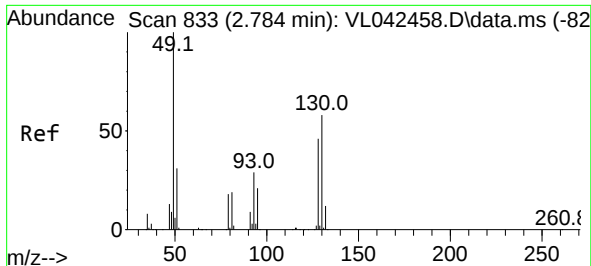

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.787 min Scan# 81
Delta R.T. 0.003 min
Lab File: VL042488.D
Acq: 06 May 2025 09:49




Instrument :
MSVOA_1
ClientSampleId :
VL0506ABL01


Tgt Ion: 49 Resp: 71766
Ion Ratio Lower Upper
49 100
128 47.5 23.3 69.9
130 59.6 29.5 88.6

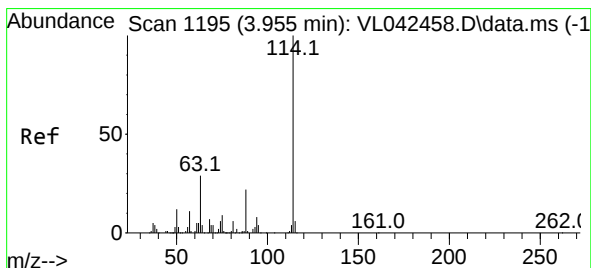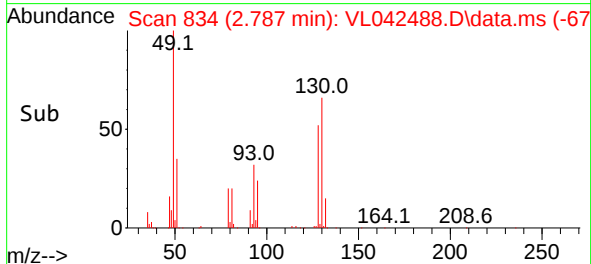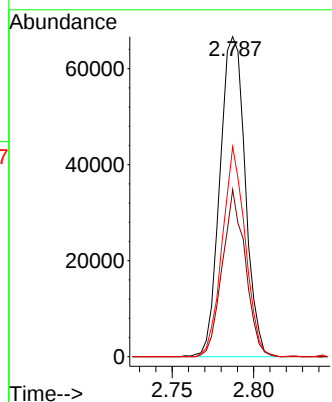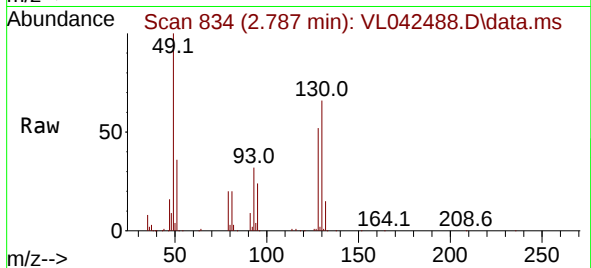

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.959 min Scan# 1196
Delta R.T. 0.003 min
Lab File: VL042488.D
Acq: 06 May 2025 09:49

Tgt Ion: 114 Resp: 194806
Ion Ratio Lower Upper
114 100
63 29.2 23.1 34.7
88 20.1 16.1 24.1

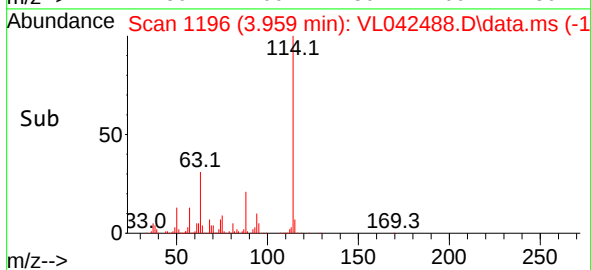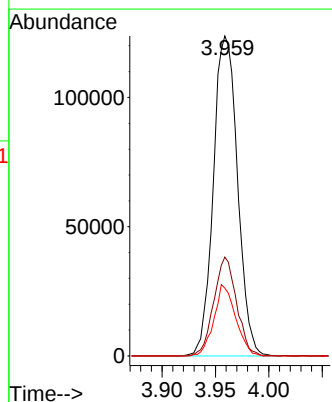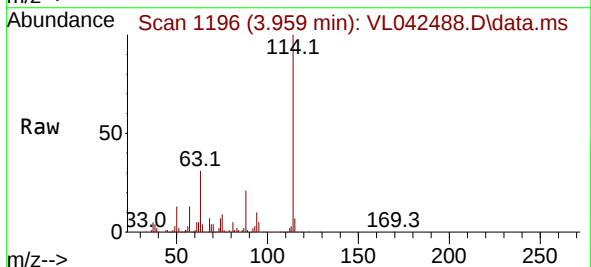

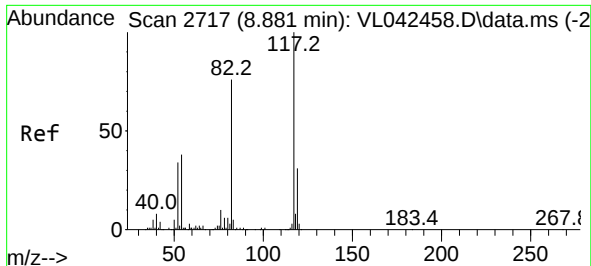

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 8.885 min Scan# 21

Delta R.T. 0.003 min

Lab File: VL042488.D

Acq: 06 May 2025 09:49

Instrument :

MSVOA_L

ClientSampleId :

VL0506ABL01





Tgt Ion:117 Resp: 158449

Ion Ratio Lower Upper

117 100

82 74.3 63.5 95.3

119 32.6 25.8 38.8

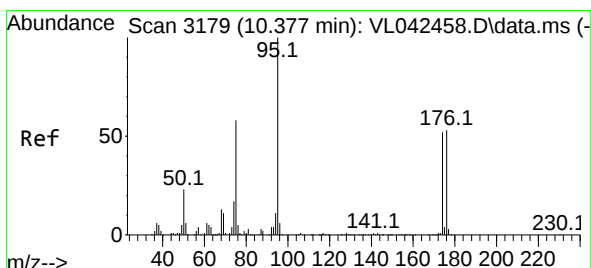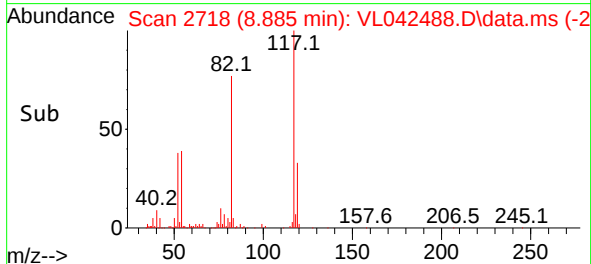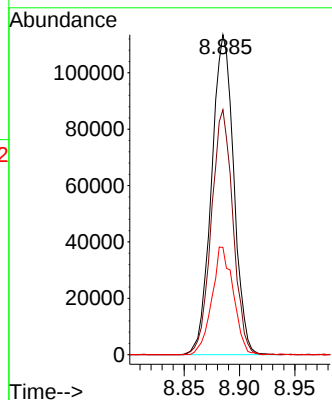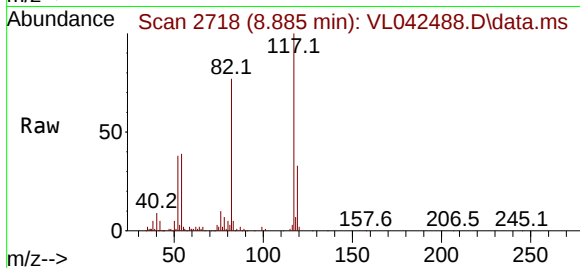

#68

1-Bromo-4-Fluorobenzene

Concen: 9.960 ppbv

RT: 10.380 min Scan# 3180

Delta R.T. 0.003 min

Lab File: VL042488.D

Acq: 06 May 2025 09:49

Tgt Ion: 95 Resp: 146316

Ion Ratio Lower Upper

95 100

174 51.1 42.7 64.1

175 3.8 3.6 5.4

