
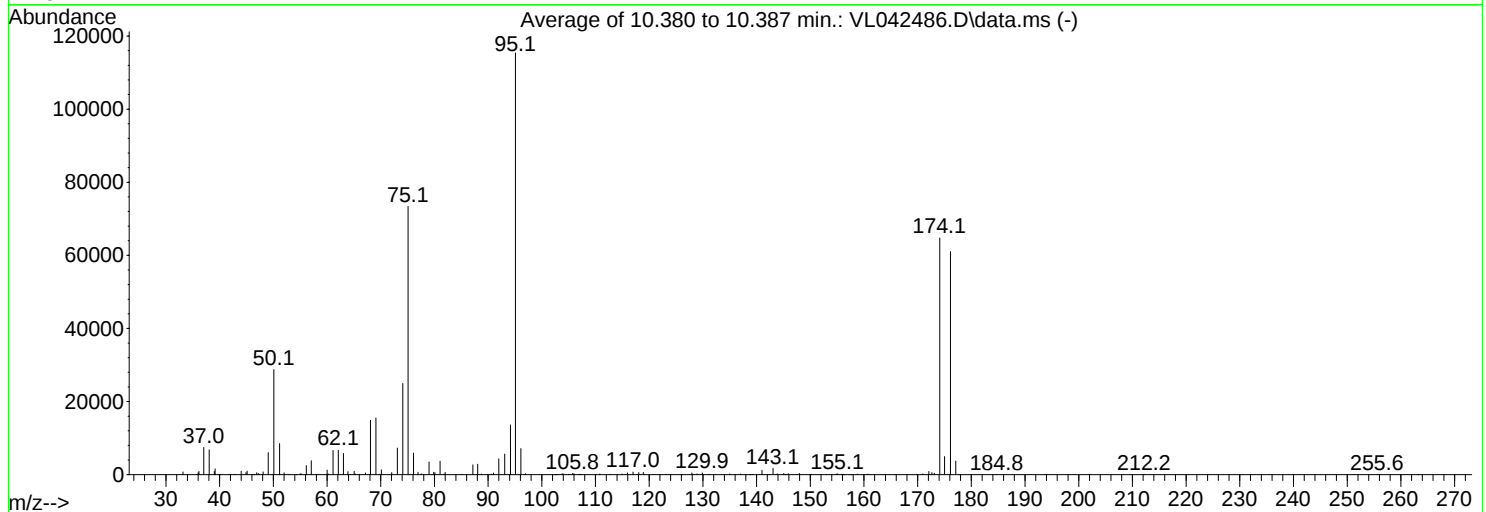


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050625\
Data File : VL042486.D
Acq On : 06 May 2025 08:16
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL050125AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 02 03:16:31 2025

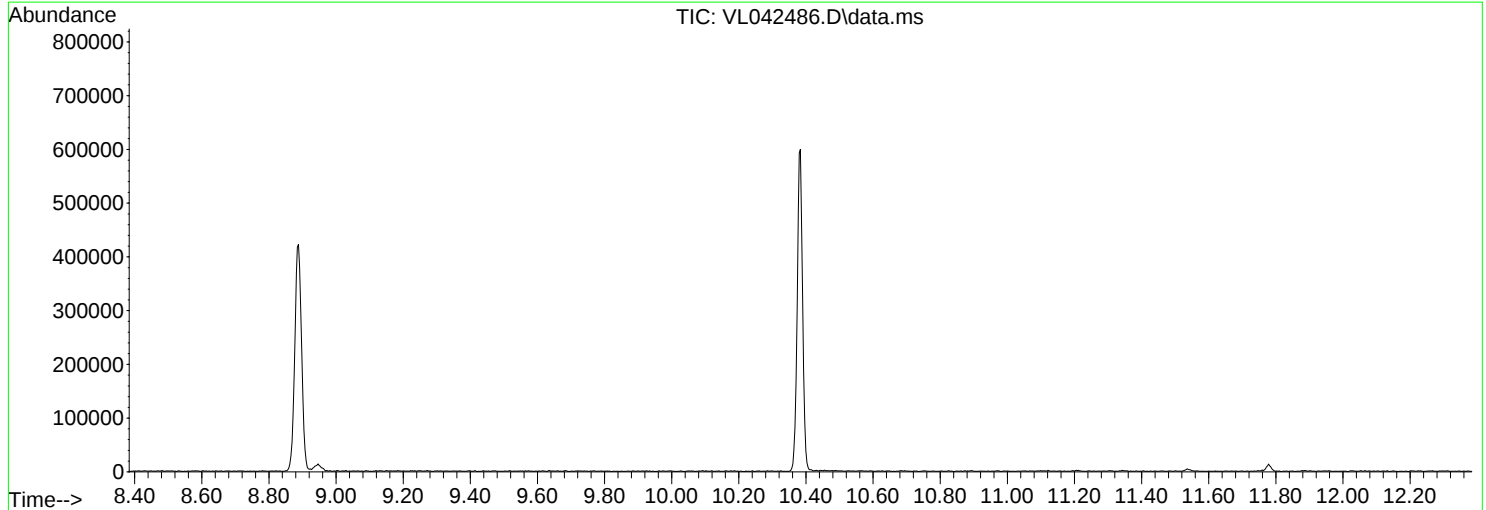

AutoFind: Scans 3180, 3181, 3182; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.9	28768	PASS
75	95	30	66	63.6	73411	PASS
95	95	100	100	100.0	115408	PASS
96	95	5	9	6.2	7151	PASS
173	174	0.00	2	0.6	392	PASS
174	95	50	120	56.1	64757	PASS
175	174	4	9	7.6	4952	PASS
176	174	93	101	94.3	61040	PASS
177	176	5	9	6.1	3717	PASS

Average of 10.380 to 10.387 min.: VL042486.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	747	44.90	582	52.20	94	61.10	660
36.00	545	45.10	985	52.95	69	62.10	665
36.15	878	46.30	22	53.85	41	63.05	578
37.05	7441	46.90	529	54.20	18	63.90	84
38.05	6773	47.20	308	55.00	259	64.30	110
39.00	897	47.40	72	55.20	175	65.05	918
39.15	1576	48.10	752	56.15	2518	65.30	159
39.85	23	49.05	6031	57.05	3793	66.00	34
40.20	61	50.10	28768	58.30	28	67.15	491
42.85	71	51.15	8478	60.00	1254	68.10	14901
44.00	958	52.00	525	60.20	226	69.10	15494

Average of 10.380 to 10.387 min.: VL042486.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
70.10	1325	80.10	556	93.10	5635	105.75	322
72.05	564	81.05	3686	94.15	13628	105.90	194
73.10	7278	81.80	196	95.10	115408	106.10	172
74.10	24939	82.00	613	96.10	7151	106.80	52
75.10	73411	84.95	66	96.95	257	107.10	128
76.10	5928	87.15	2690	102.50	22	107.30	42
76.95	655	88.05	2835	102.70	28	110.80	179
77.55	207	88.80	159	103.00	95	112.10	73
78.00	96	90.60	120	103.80	278	112.70	80
79.00	3478	91.00	425	104.10	183	114.20	69
79.85	642	92.00	4328	105.00	87	114.95	166

Average of 10.380 to 10.387 min.: VL042486.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
115.95	480	135.00	181	145.90	262	158.85	167
117.00	698	137.00	180	147.95	337	159.95	51
118.05	579	138.70	20	149.90	36	160.70	143
118.90	617	139.20	59	150.15	40	161.10	88
119.10	39	140.00	122	153.00	88	161.90	82
123.10	89	141.00	1204	154.85	173	165.70	24
126.15	49	142.30	55	155.10	201	169.85	126
127.95	479	143.05	1695	155.80	86	170.95	206
128.90	208	143.85	231	156.20	19	172.10	875
129.90	494	145.05	308	157.20	59	172.65	561
131.15	80	145.30	19	157.60	18	173.10	392

Average of 10.380 to 10.387 min.: VL042486.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.10	64757						
175.00	4952						
176.10	61040						
177.10	3717						
177.80	21						
184.75	55						
212.20	72						
251.20	54						
255.60	73						
263.20	21						

Instrument :

MSVOA_L

ClientSampleId :

BFB