


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL050720\
 Data File : VL034962.D
 Acq On : 7 May 2020 10:14
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050620AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed May 06 14:49:39 2020
 Last Update : Wed May 06 14:49:39 2020

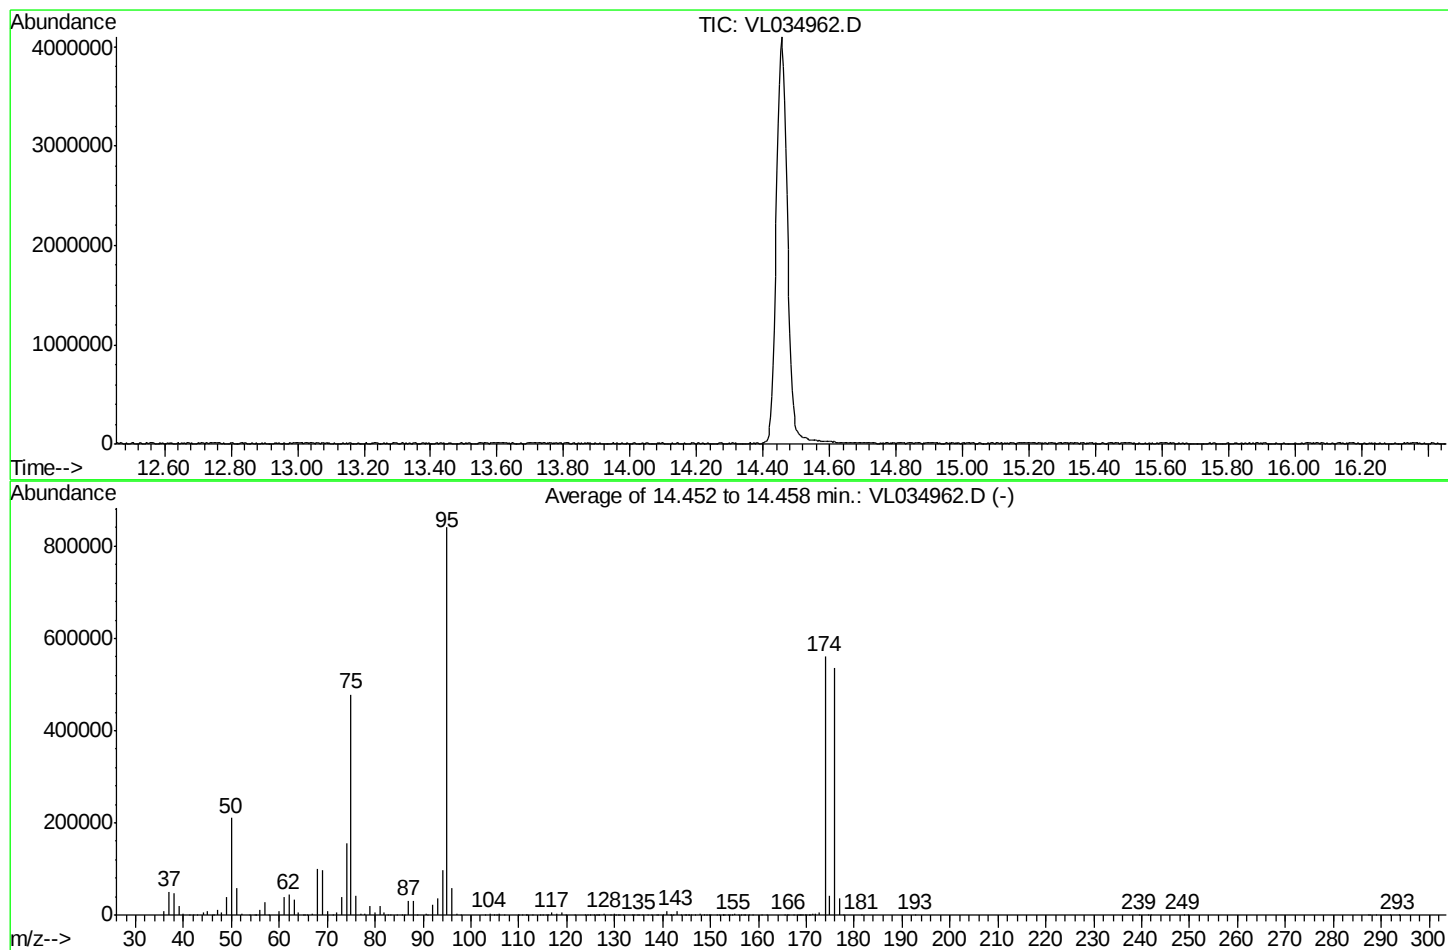

AutoFind: Scans 3628, 3629, 3630; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.0	209813	PASS
75	95	30	66	56.8	478037	PASS
95	95	100	100	100.0	840896	PASS
96	95	5	9	7.0	58544	PASS
173	174	0.00	2	0.8	4437	PASS
174	95	50	120	66.6	560170	PASS
175	174	4	9	7.4	41546	PASS
176	174	93	101	95.8	536768	PASS
177	176	5	9	6.7	35832	PASS