
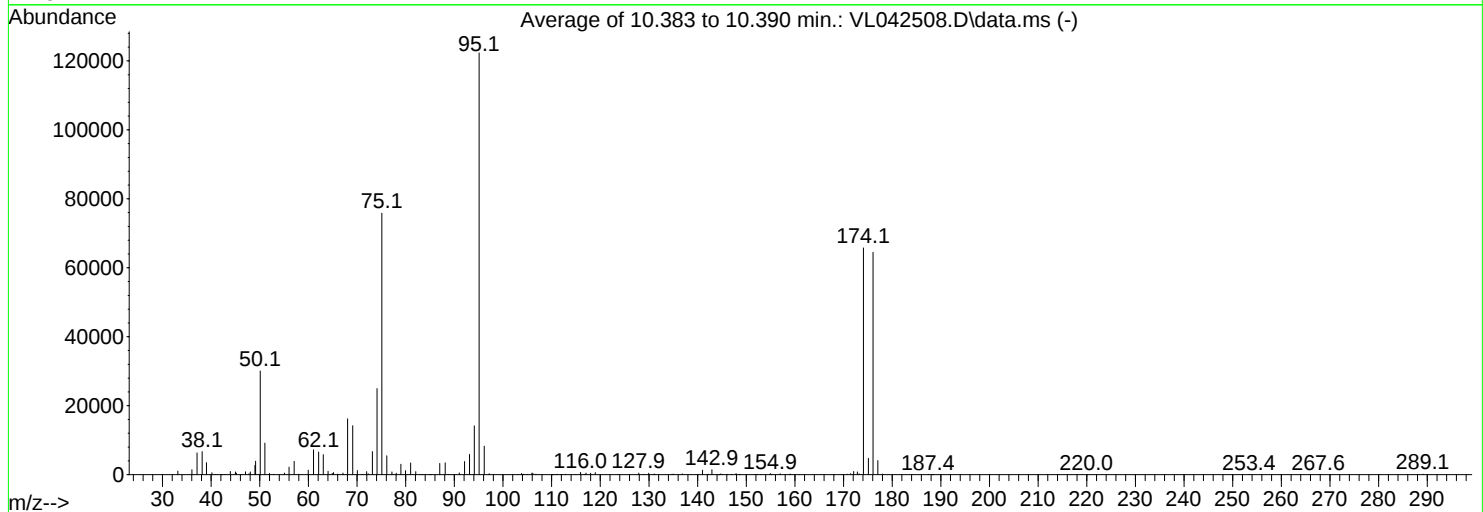


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050725\
Data File : VL042508.D
Acq On : 07 May 2025 07:53
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL050125AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 02 03:16:31 2025

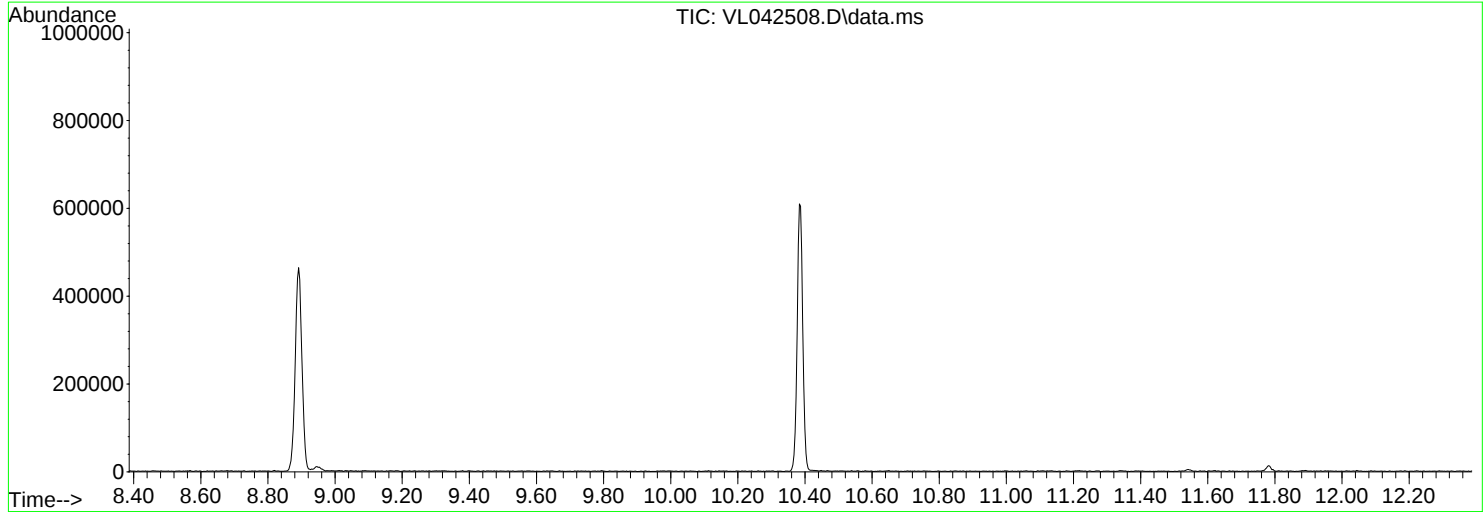

AutoFind: Scans 3181, 3182, 3183; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.6	30091	PASS
75	95	30	66	62.0	75856	PASS
95	95	100	100	100.0	122344	PASS
96	95	5	9	6.8	8282	PASS
173	174	0.00	2	1.2	792	PASS
174	95	50	120	53.7	65757	PASS
175	174	4	9	7.2	4721	PASS
176	174	93	101	98.1	64517	PASS
177	176	5	9	6.3	4092	PASS

Average of 10.383 to 10.390 min.: VL042508.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	1042	45.20	407	55.05	454	66.00	14
36.05	1453	46.30	56	56.00	2201	67.10	49
37.10	6305	47.05	856	57.05	3876	68.05	1620
38.15	6670	47.80	274	58.00	142	69.10	1421
39.05	3477	48.05	776	59.95	1317	70.05	1229
40.15	558	49.00	2690	61.05	7215	71.00	40
40.95	68	49.15	3885	62.10	6535	71.95	866
42.10	23	50.10	30091	63.05	5810	72.30	236
42.90	62	51.05	9134	64.05	991	73.15	6695
43.95	936	51.95	358	64.90	373	74.10	24995
45.00	774	52.85	77	65.15	614	75.10	75856

Average of 10.383 to 10.390 min.: VL042508.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.10	5486	87.00	3234	103.00	49	112.10	54
77.15	804	88.10	3442	103.80	338	112.85	115
78.05	429	88.85	44	104.20	149	115.00	35
79.00	3006	89.90	17	104.95	91	115.95	628
79.95	1185	91.00	502	105.95	451	116.80	115
81.00	3390	92.10	3784	106.15	414	117.05	476
82.05	869	93.10	5831	106.75	156	118.00	425
83.10	98	94.10	14139	110.10	23	118.95	613
83.50	54	95.10	122344	110.70	51	123.65	117
84.05	99	96.15	8282	111.10	123	127.90	480
85.00	17	97.15	297	111.90	60	128.90	119

Average of 10.383 to 10.390 min.: VL042508.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.95	403	144.80	242	155.20	77	172.10	924
131.00	119	145.10	46	157.00	267	172.85	792
131.20	176	146.10	112	158.80	103	173.20	218
134.75	156	146.95	105	159.05	200	174.10	65757
135.10	161	147.90	306	159.90	54	175.10	4721
136.85	215	148.60	24	161.00	71	176.05	64517
140.10	88	150.00	73	167.90	18	177.05	4092
141.00	1321	151.80	35	169.65	57	178.05	183
142.20	122	152.30	95	169.90	31	187.40	82
142.95	1426	153.00	31	170.75	150	188.30	23
144.30	26	154.95	333	171.45	273	220.00	17

Average of 10.383 to 10.390 min.: VL042508.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
253.40	31						
267.65	50						
289.15	140						

Instrument :

MSVOA_L

ClientSampleId :

BFB