


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050924\
Data File : VL041248.D
Acq On : 9 May 2024 8:07
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 10 01:23:08 2024

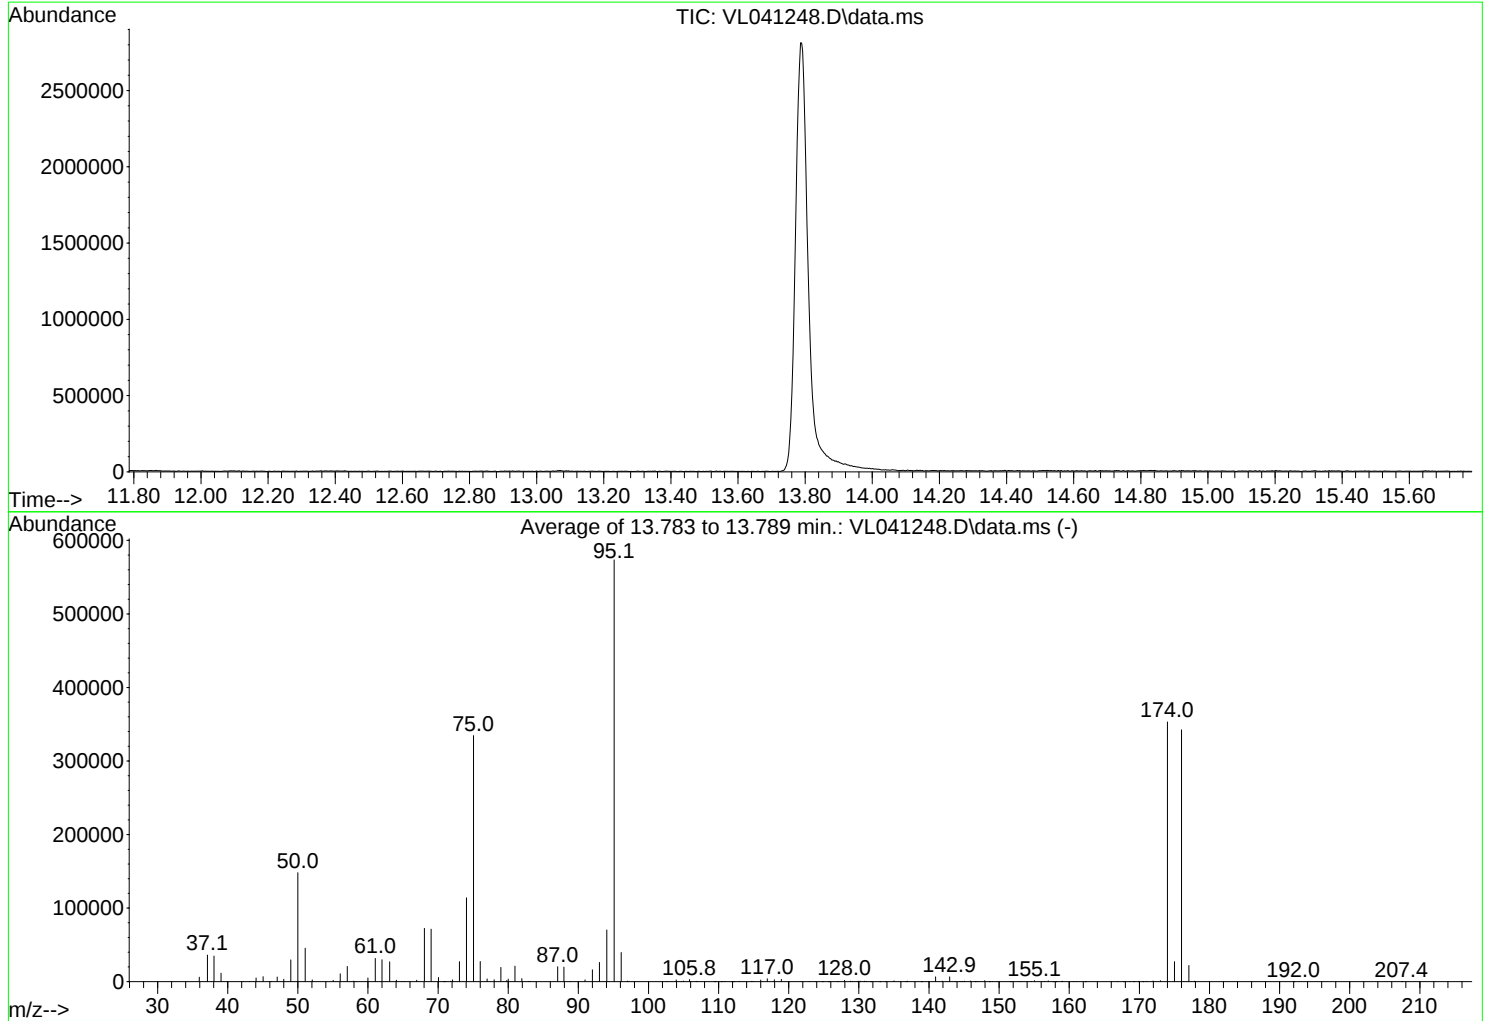

AutoFind: Scans 3477, 3478, 3479; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.8	148160	PASS
75	95	30	66	58.3	334549	PASS
95	95	100	100	100.0	573589	PASS
96	95	5	9	6.9	39600	PASS
173	174	0.00	2	0.4	1397	PASS
174	95	50	120	61.6	353216	PASS
175	174	4	9	7.7	27243	PASS
176	174	93	101	97.0	342443	PASS
177	176	5	9	6.5	22107	PASS

Average of 13.783 to 13.789 min.: VL041248.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	6016	47.05	6268	60.00	5068	70.80	71
37.10	36245	48.00	3270	61.05	31611	71.05	230
38.05	34907	49.00	29536	62.00	29864	71.80	75
39.05	11591	50.00	148160	63.10	26979	72.05	241
39.90	233	51.05	45387	64.05	1996	73.05	27144
42.20	159	52.05	2409	64.85	298	74.05	114096
43.10	206	55.05	1714	65.20	148	75.05	334549
44.05	5062	56.05	10650	66.95	2040	76.00	27349
45.05	6844	57.05	20595	68.05	72536	77.00	3825
45.95	336	57.95	635	69.00	71352	78.00	2675
46.20	214	58.30	202	70.05	5597	78.95	19467

Average of 13.783 to 13.789 min.: VL041248.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.80	1642	92.00	16086	105.85	2846	114.70	372
80.00	3403	93.00	26075	106.80	509	114.90	386
80.95	21227	94.05	70248	107.00	313	116.00	2228
81.95	4068	95.10	573589	109.40	51	116.95	3947
82.90	324	96.10	39600	109.60	422	117.95	2597
83.10	384	97.00	801	110.00	136	118.95	3116
86.00	527	97.20	290	110.40	66	119.90	68
87.05	20275	102.65	199	110.90	564	121.75	210
87.95	19773	103.95	2325	111.90	350	122.95	152
88.85	265	104.70	184	112.10	102	123.85	237
90.95	2491	105.00	956	112.95	517	124.80	51

Average of 13.783 to 13.789 min.: VL041248.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.70	65	131.70	59	140.95	6500	147.95	1313
126.90	141	133.00	59	141.90	727	148.60	75
127.10	152	133.80	71	142.95	6647	149.05	214
127.95	1768	135.00	1138	143.75	412	149.70	143
128.80	717	135.95	255	144.40	163	150.10	299
129.10	190	136.70	200	144.60	142	151.60	67
129.80	444	136.80	316	144.80	295	151.95	271
130.00	797	136.95	742	145.05	616	152.85	181
130.20	730	138.90	75	145.95	846	153.15	202
130.80	608	139.10	149	146.60	110	154.00	132
131.10	362	139.95	490	147.05	209	154.60	334

Average of 13.783 to 13.789 min.: VL041248.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.05	1412	167.70	56	177.05	22107		
156.50	167	168.65	256	177.85	590		
157.00	1212	169.20	57	192.00	56		
157.70	105	169.90	359	207.40	65		
158.10	103	170.50	96				
158.90	233	171.05	533				
159.05	763	171.95	932				
160.60	282	173.00	1397				
161.10	340	174.00	353216				
162.30	52	175.00	27243				
166.90	167	176.00	342443				