


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL051122\
 Data File : VL039020.D
 Acq On : 11 May 2022 14:17
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 05 10:12:15 2022
 Last Update : Thu May 05 10:12:15 2022

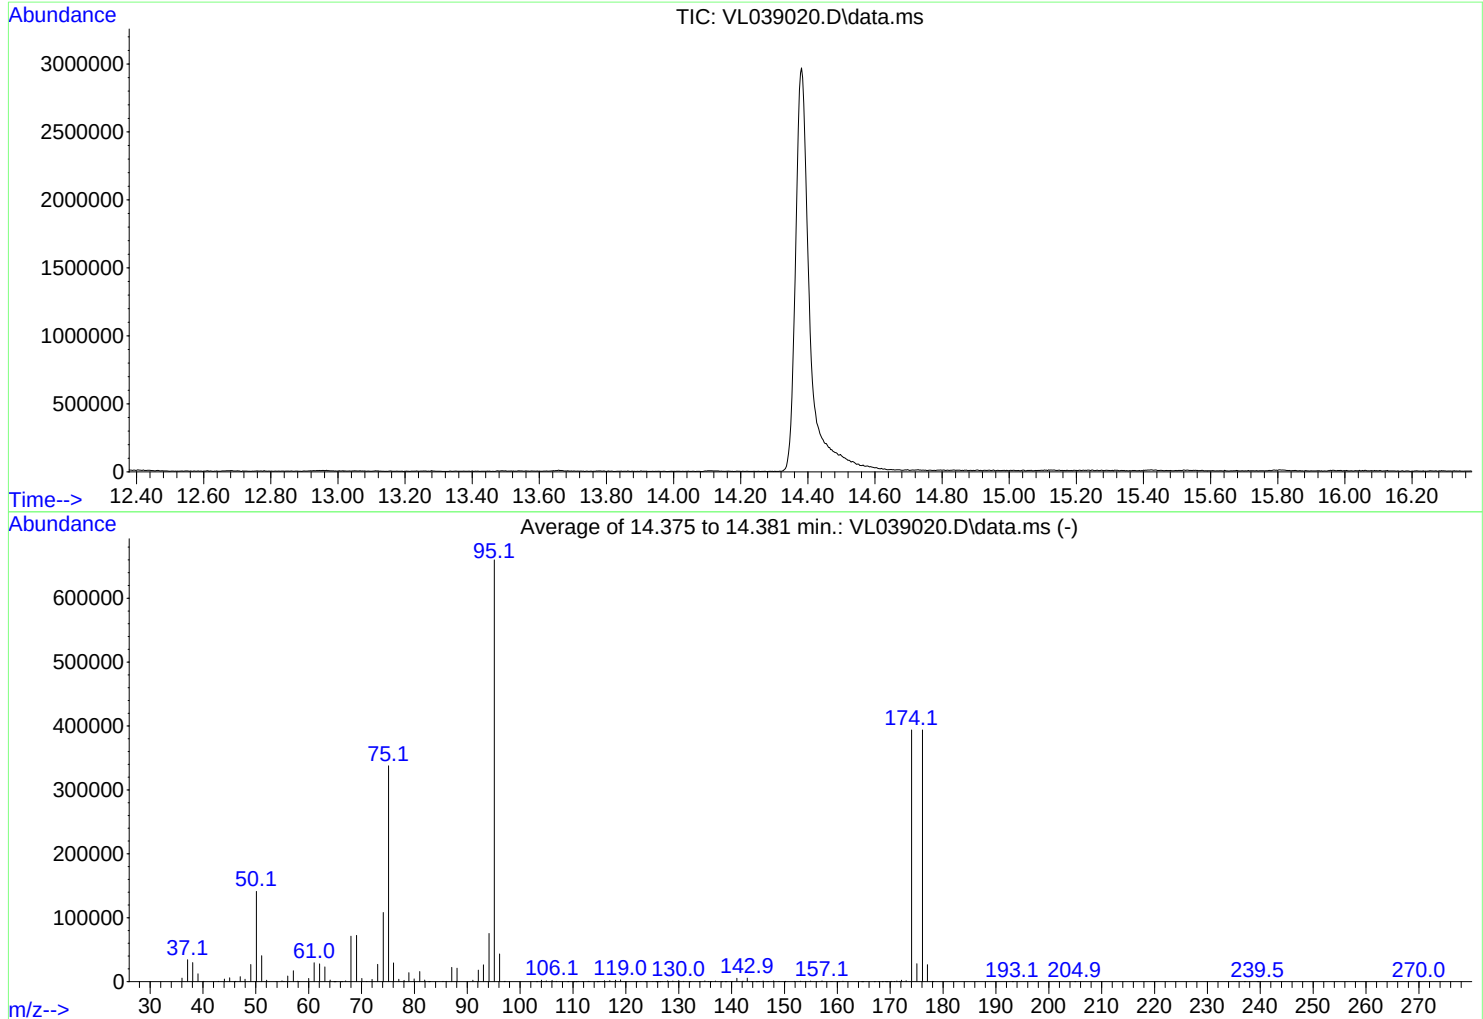

AutoFind: Scans 3604, 3605, 3606; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.4	141291	PASS
75	95	30	66	51.2	337728	PASS
95	95	100	100	100.0	660075	PASS
96	95	5	9	6.6	43336	PASS
173	174	0.00	2	0.4	1506	PASS
174	95	50	120	59.7	393963	PASS
175	174	4	9	7.1	28085	PASS
176	174	93	101	100.0	393792	PASS
177	176	5	9	6.7	26533	PASS

Average of 14.375 to 14.381 min.: VL039020.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	5463	47.95	3662	58.20	180	69.05	7225
37.10	34245	49.05	26725	60.00	4909	70.05	4931
38.05	29723	50.10	141291	61.05	29520	71.00	17
39.05	12293	51.10	40485	62.05	27819	72.00	342
40.15	467	52.05	2284	63.05	23040	73.05	27157
42.90	453	53.85	180	64.05	2525	74.10	108069
44.05	3965	54.95	1278	64.80	127	75.10	337728
45.05	5949	55.30	393	65.00	97	76.05	29331
45.90	142	56.05	8749	66.20	71	77.05	3700
46.20	404	57.10	17178	67.00	1385	78.05	2028
47.05	7664	57.95	698	68.00	71120	78.95	13928

Average of 14.375 to 14.381 min.: VL039020.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	4284	93.05	26395	109.00	61	115.70	325
81.00	15903	94.10	75280	110.20	141	115.95	1539
81.95	2593	95.10	660075	110.60	64	116.95	1877
82.70	153	96.10	43336	111.10	523	118.05	2238
83.00	233	97.00	507	111.85	217	119.00	2830
85.40	388	97.15	608	112.85	485	120.05	175
86.00	556	103.10	104	113.00	496	122.00	136
87.05	22195	104.05	2210	113.20	227	122.85	204
88.05	20981	104.95	1300	114.60	115	123.70	136
91.05	2217	106.05	2093	114.90	377	123.95	181
92.10	18107	106.90	638	115.10	298	125.10	199

Average of 14.375 to 14.381 min.: VL039020.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.70	102	134.95	1312	142.95	5434	150.00	91
126.00	141	135.65	218	143.80	219	150.15	391
126.40	139	136.00	78	144.00	165	151.90	485
126.85	185	136.95	1079	144.70	128	153.00	647
127.90	1203	138.10	154	145.10	331	154.00	455
128.10	487	138.80	53	145.30	208	154.95	897
128.90	899	139.10	348	145.95	907	156.10	202
130.00	1819	139.90	371	146.70	311	157.10	1241
130.95	464	140.10	162	147.00	172	158.80	354
132.10	98	141.00	5253	147.95	1196	159.00	242
133.90	105	142.15	772	148.95	532	160.20	62

Average of 14.375 to 14.381 min.: VL039020.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
161.05	663	171.25	906	204.90	65		
164.60	102	171.80	495	237.00	58		
164.80	85	172.15	2224	239.50	98		
167.00	115	173.00	1506	270.00	88		
167.85	181	174.05	393963				
168.50	124	175.05	28085				
169.10	223	176.10	393792				
169.30	94	177.05	26533				
169.60	187	178.00	530				
170.20	469	178.20	210				
170.80	305	193.10	91				

Instrument :

MSVOA_L

ClientSampleId :

BFB