


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL051123\
Data File : VL040399.D
Acq On : 11 May 2023 12:00
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041323AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Apr 13 14:37:02 2023

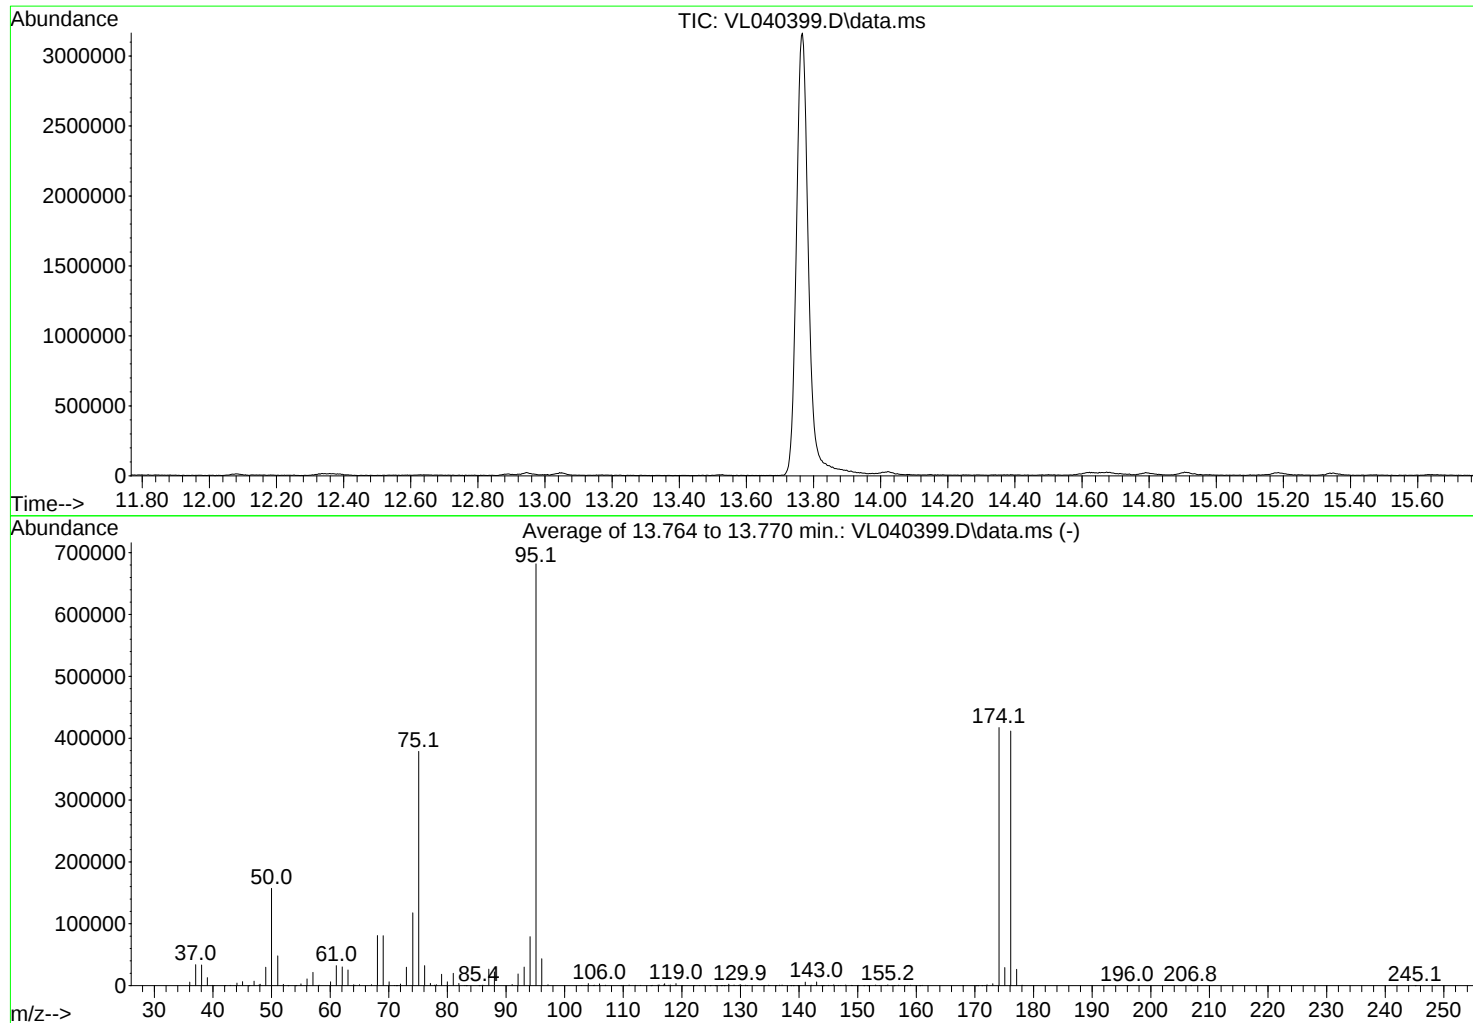

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3447

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.1	157269	PASS
75	95	30	66	55.5	378688	PASS
95	95	100	100	100.0	681920	PASS
96	95	5	9	6.4	43613	PASS
173	174	0.00	2	0.8	3209	PASS
174	95	50	120	61.2	417280	PASS
175	174	4	9	7.0	29344	PASS
176	174	93	101	98.6	411541	PASS
177	176	5	9	6.4	26435	PASS

Average of 13.764 to 13.770 min.: VL040399.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	5682	46.25	238	56.05	10933	68.05	8086
37.05	33928	47.00	7238	57.05	21400	69.05	8067
38.05	33349	47.90	1341	58.10	845	70.05	612
39.05	12941	48.05	2409	60.05	6180	70.95	20
39.95	425	49.00	29632	61.05	32467	71.30	136
40.20	284	50.00	157269	62.05	30419	72.00	2749
42.00	85	51.05	48248	63.05	25436	73.00	29723
42.95	461	52.00	2181	64.00	1327	74.10	117853
44.10	4273	52.80	156	64.20	725	75.10	378688
45.05	6425	54.10	112	65.00	1518	76.10	32437
46.10	155	55.00	2767	67.05	1645	77.10	3647

Average of 13.764 to 13.770 min.: VL040399.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.80	844	88.00	22269	105.05	882	116.10	1280
78.10	1512	91.05	1712	105.95	2860	116.90	1003
79.00	18485	92.05	18891	106.95	925	117.05	3226
80.00	6272	93.10	29976	109.60	85	117.80	803
81.00	19933	94.10	79147	110.05	536	118.05	1175
81.95	3769	95.10	681920	111.00	1068	119.00	3349
82.95	388	96.10	43613	112.10	451	120.00	151
83.20	95	97.15	1531	112.95	447	122.00	54
85.40	117	102.90	205	114.70	99	123.00	165
86.05	784	104.05	3463	114.95	575	123.80	495
87.05	26528	104.90	305	115.90	691	124.80	124

Average of 13.764 to 13.770 min.: VL040399.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.70	142	131.20	182	139.80	77	148.90	478
125.95	163	132.10	228	141.05	5651	149.10	160
126.70	98	133.65	173	142.05	711	150.05	599
126.95	165	134.05	133	143.00	5928	151.05	116
127.20	121	134.80	842	143.85	183	151.70	100
128.00	2485	135.00	320	144.10	130	152.05	391
128.90	1176	136.00	65	145.05	566	153.05	928
129.70	519	136.65	707	145.90	1231	153.75	340
129.95	1946	137.10	1045	146.70	245	154.00	382
130.20	657	138.60	102	147.10	200	154.80	321
130.90	677	139.00	143	147.95	1074	155.15	1226

Average of 13.764 to 13.770 min.: VL040399.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.85	180	171.20	109	245.10	69		
156.20	55	171.70	358				
157.00	872	172.05	1194				
158.00	50	173.05	3209				
158.50	214	174.10	417280				
159.05	735	175.10	29344				
160.60	152	176.10	411541				
161.00	510	177.10	26435				
167.90	72	178.05	872				
170.20	132	196.00	94				
170.50	124	206.80	135				