


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL051223\
Data File : VL040418.D
Acq On : 12 May 2023 14:50
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041323AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Apr 13 14:37:02 2023

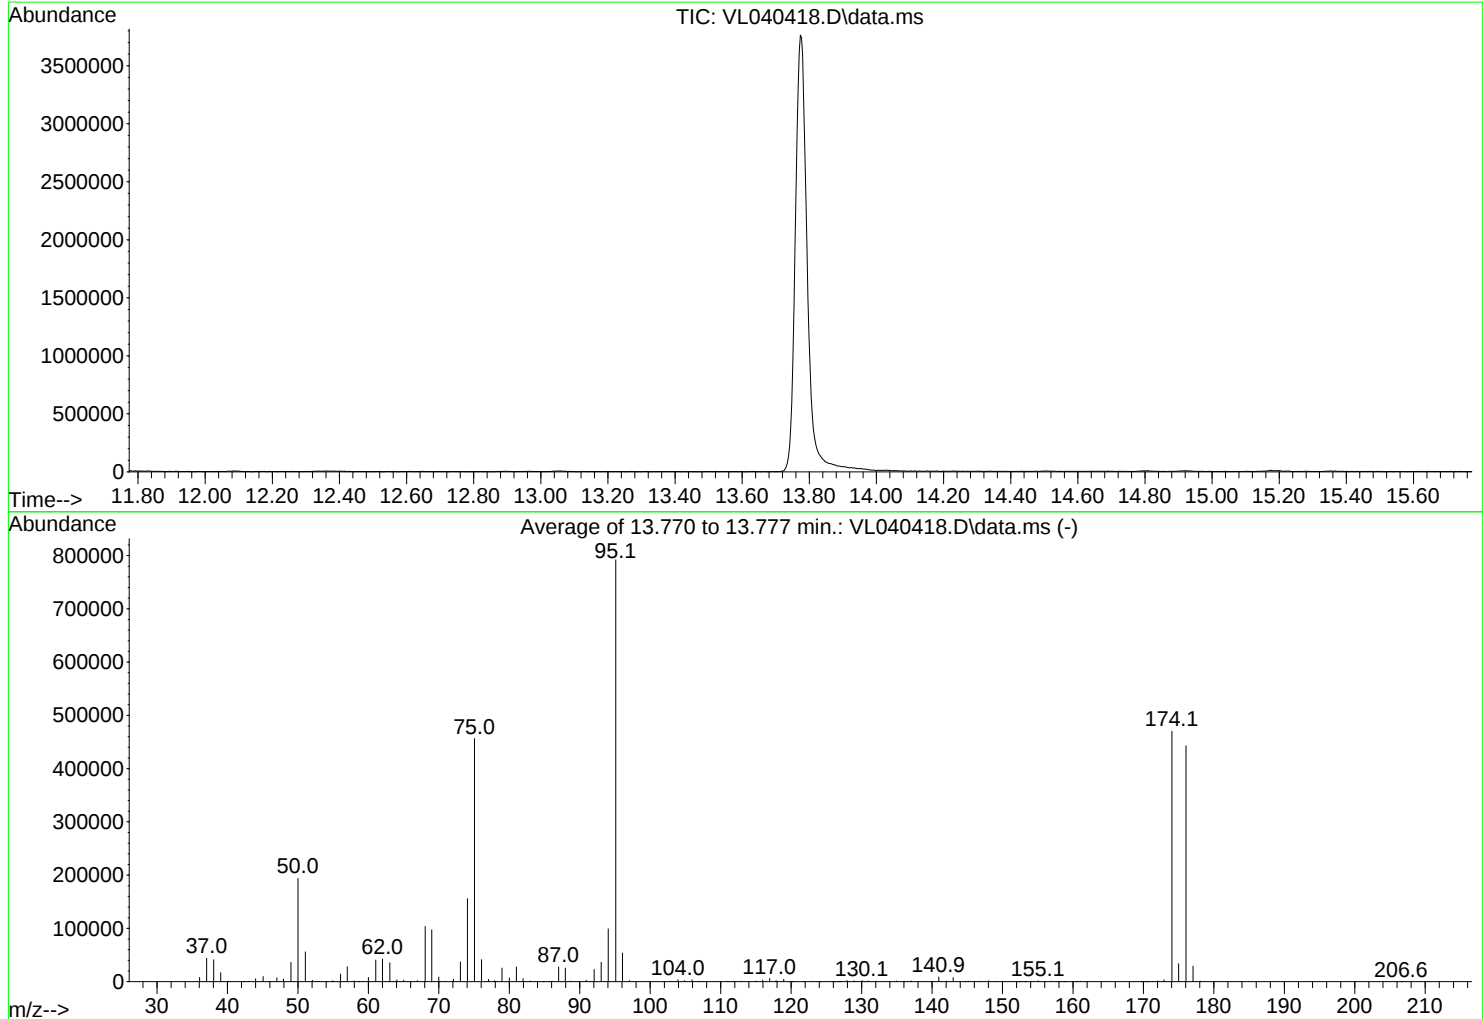

AutoFind: Scans 3473, 3474, 3475; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.5	193792	PASS
75	95	30	66	57.6	456448	PASS
95	95	100	100	100.0	792000	PASS
96	95	5	9	6.8	53811	PASS
173	174	0.00	2	0.7	3257	PASS
174	95	50	120	59.4	470208	PASS
175	174	4	9	7.2	33661	PASS
176	174	93	101	94.2	442752	PASS
177	176	5	9	6.6	29213	PASS

Average of 13.770 to 13.777 min.: VL040418.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7836	47.00	7304	57.00	27872	66.95	190
37.05	44013	47.95	4996	58.00	1588	68.05	10369
38.05	41261	49.00	36045	58.60	74	69.00	9721
39.05	16716	50.00	193792	60.00	7777	70.00	860
40.15	1066	51.05	55955	61.05	40611	70.95	508
42.30	101	52.05	2561	62.00	42365	72.05	4840
42.95	554	52.90	377	63.05	35429	73.05	36893
44.00	5452	54.00	72	63.90	914	74.05	155541
45.05	9659	54.90	1428	64.05	3034	75.05	456448
45.80	251	55.10	543	65.00	2678	76.05	41173
46.10	464	56.05	14063	66.10	432	77.05	4298

Average of 13.770 to 13.777 min.: VL040418.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.90	1724	86.05	840	102.85	547	112.10	400
78.10	524	87.00	27739	103.95	3491	112.90	958
78.95	25595	87.95	25445	104.85	1743	115.00	1111
80.00	7184	88.70	956	105.95	3468	115.95	2907
81.00	27677	90.90	2608	106.80	324	116.95	5903
81.95	5492	92.05	22904	106.95	639	117.85	1915
82.95	1115	93.05	36224	109.75	297	118.10	902
84.00	231	94.05	99043	110.00	201	118.95	4509
84.80	70	95.10	792000	110.90	576	120.10	109
85.60	97	96.05	53811	111.15	349	121.80	79
85.90	336	97.05	1686	111.80	545	121.95	160

Average of 13.770 to 13.777 min.: VL040418.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.05	225	130.60	166	142.05	1334	152.00	65
123.65	343	130.95	1196	143.00	7411	152.40	142
124.10	138	132.05	337	144.05	492	152.75	301
124.95	232	133.95	265	144.70	128	153.20	67
125.85	312	134.95	1340	145.15	768	154.05	571
126.10	65	135.95	108	146.00	1034	155.05	1599
126.70	82	136.90	342	146.90	604	155.95	133
126.95	155	137.05	1198	148.05	1847	156.90	867
127.95	2116	139.05	250	148.90	245	157.80	120
128.95	1414	139.95	1080	149.15	250	158.00	59
130.05	2252	140.95	8683	150.00	873	158.70	72

Average of 13.770 to 13.777 min.: VL040418.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
159.00	709	172.90	3257				
160.50	155	174.05	470208				
161.00	639	175.00	33661				
168.70	199	176.05	442752				
169.70	78	177.05	29213				
170.10	213	178.05	975				
170.40	88	206.60	87				
170.70	246						
171.25	420						
172.00	1761						
172.20	667						