

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL051322\
Data File : VL039037.D
Acq On : 13 May 2022 14:21
Operator : SY/AP
Sample : VL0513ABL03
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0513ABL03

Quant Time: May 14 01:09:17 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL050522AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu May 05 10:12:15 2022
QLast Update : Thu May 05 10:12:15 2022
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.65	49	895624	10.00	ppbv	-0.02
33) 1,4-Difluorobenzene	7.15	114	2216766	10.00	ppbv	-0.02
55) Chlorobenzene-d5	12.06	117	1805132	10.00	ppbv	-0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.38	95	1415344	9.90	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.00%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL051322\
Data File : VL039037.D
Acq On : 13 May 2022 14:21
Operator : SY/AP
Sample : VL0513ABL03
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0513ABL03

Quant Time: May 14 01:09:17 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL050522AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 05 10:12:15 2022
QLast Update : Thu May 05 10:12:15 2022
Response via : Initial Calibration

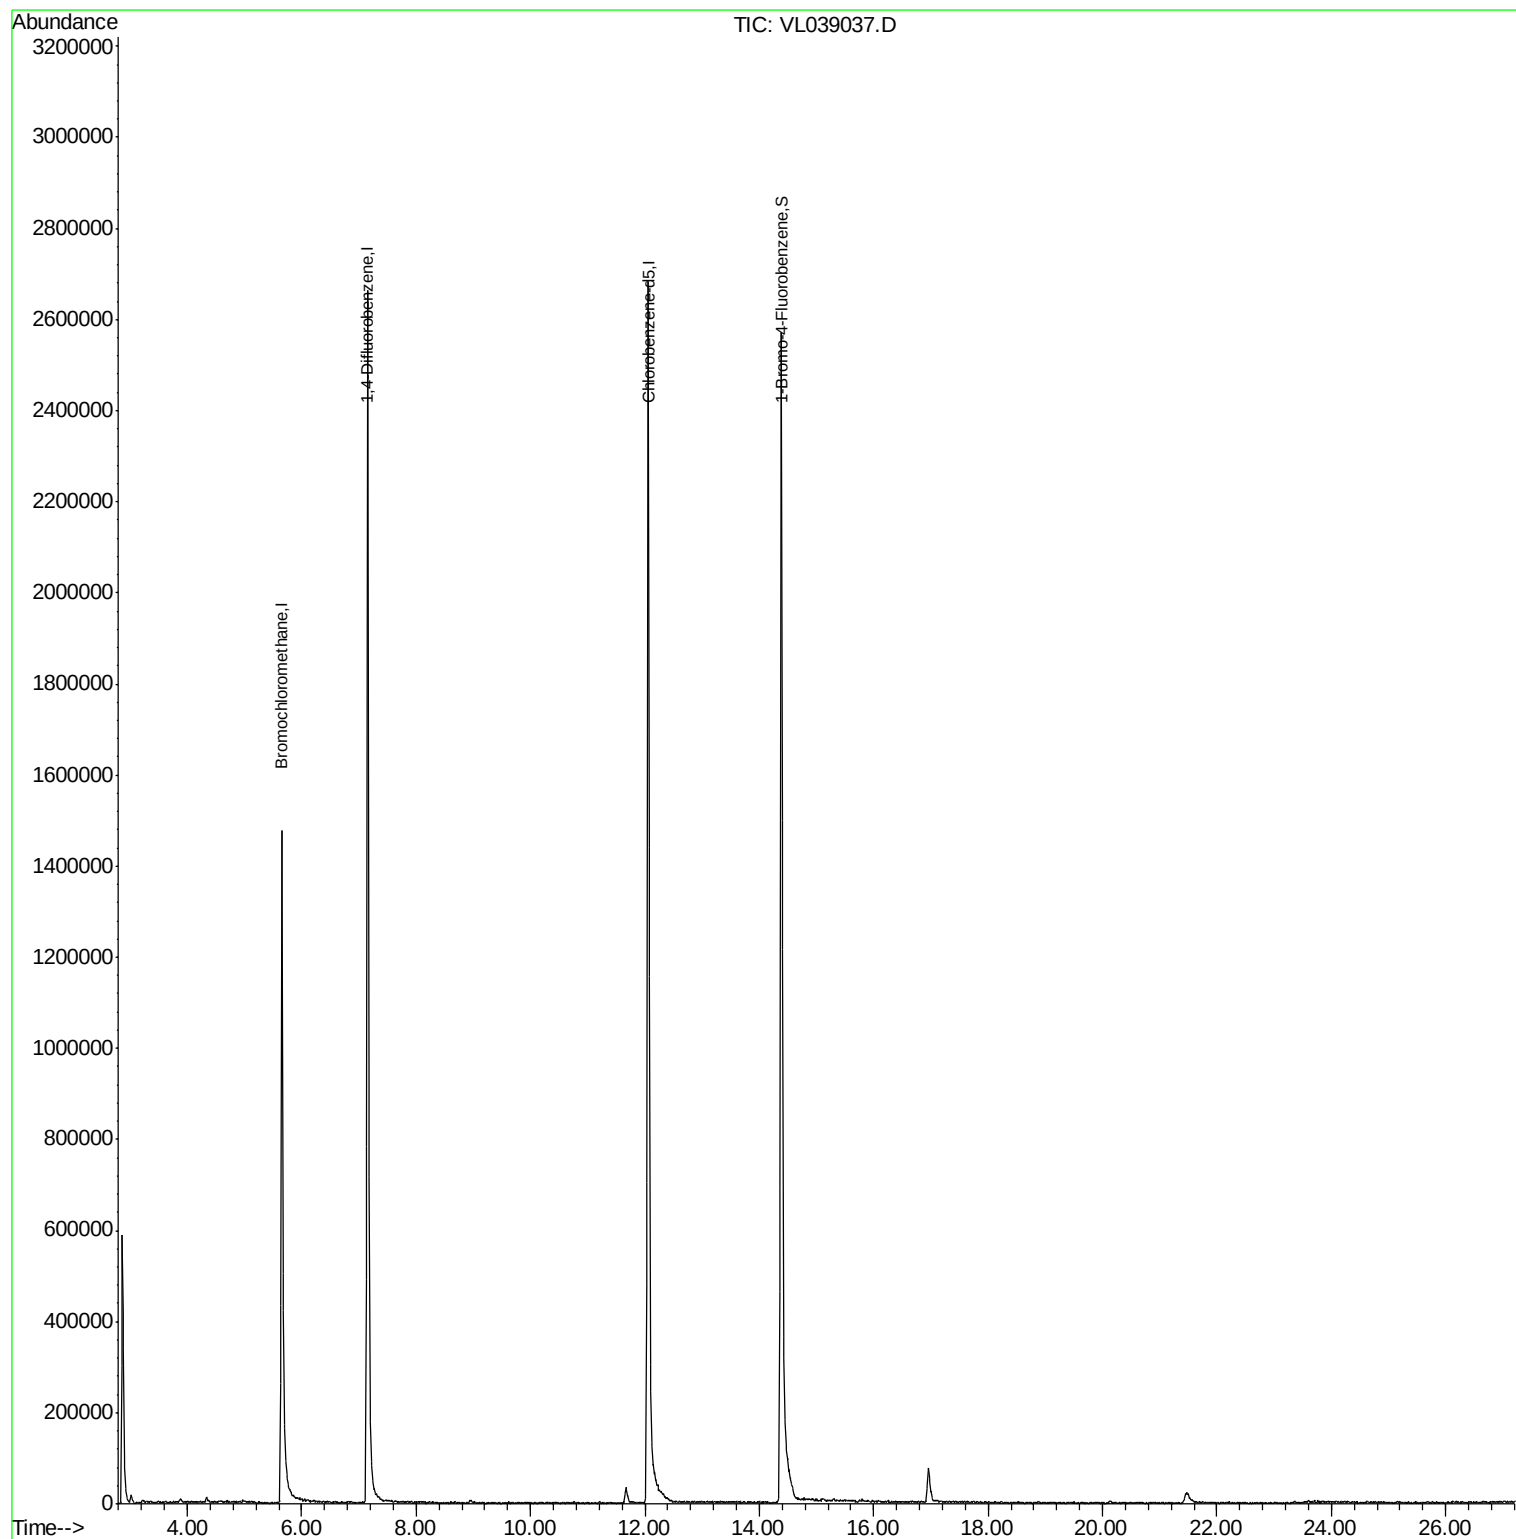

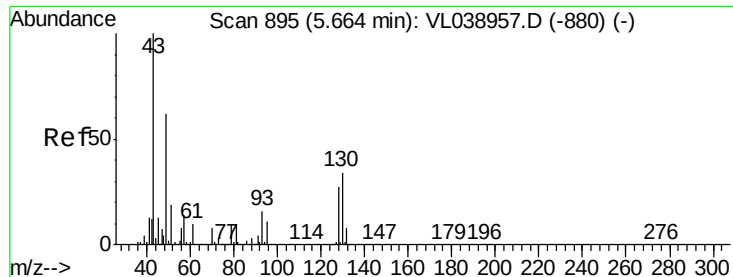

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.65

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

VL0513ABL03

Acq: 13 May 2022 14:21


Tot Ion: 49 Resp: 895624

Ion Ratio Lower Upper

49 100

128 49.5 23.3 69.8




130 62.1 29.8 89.3

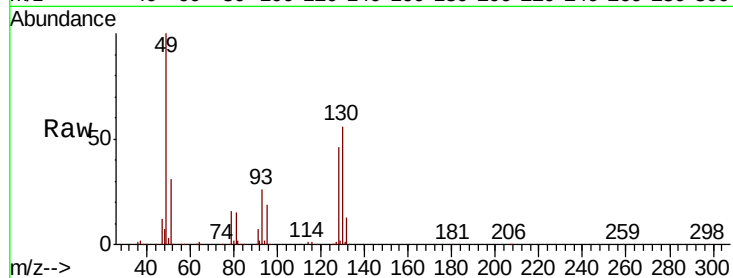

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

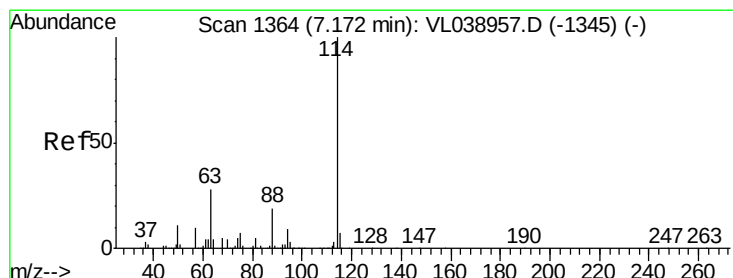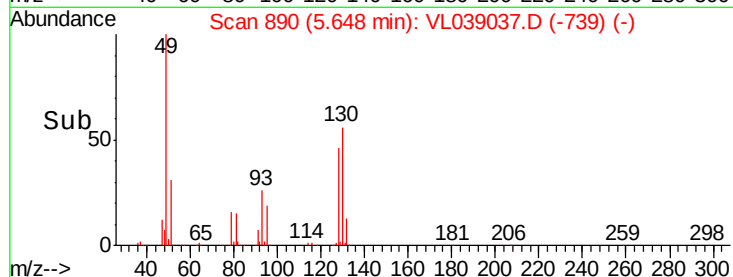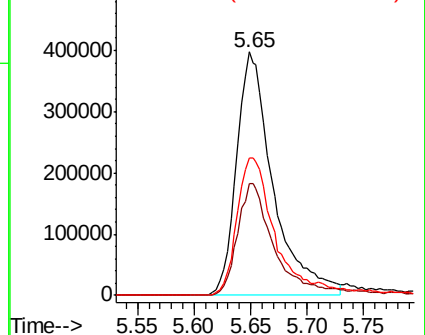

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.15 min Scan# 1358

Delta R.T. -0.02 min

Lab File: VL039037.D

Acq: 13 May 2022 14:21


Tgt Ion:114 Resp: 2216766

Ion Ratio Lower Upper

114 100

63 27.5 22.6 33.8



88 19.1 15.4 23.0

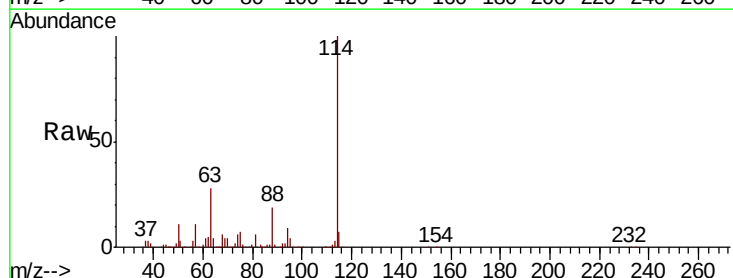


Abundance Ion 114.10 (113.80 to 114.80): V

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



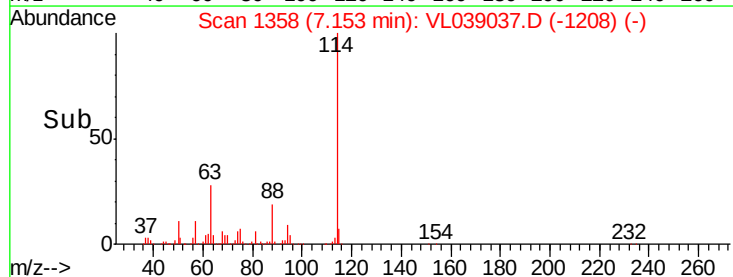
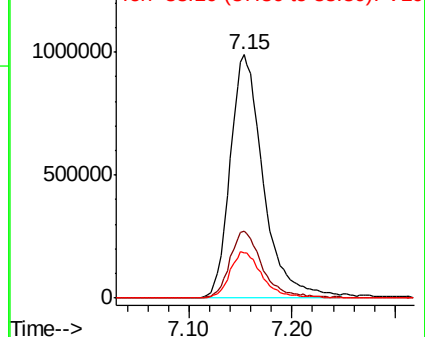


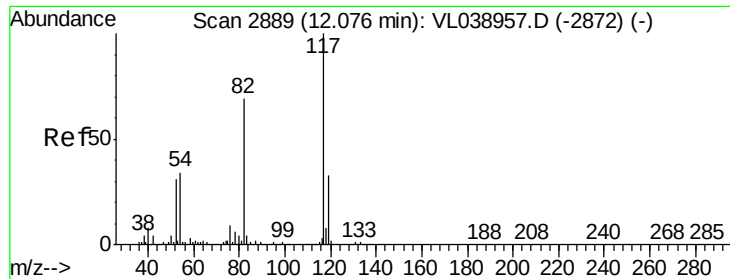

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.06 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId : VL0513ABL03
Acq: 13 May 2022 14:21

Tot Ion:117 Resp: 1805132

Ion	Ratio	Lower	Upper
117	100		
82	75.5	57.0	85.6
119	34.4	27.2	40.8

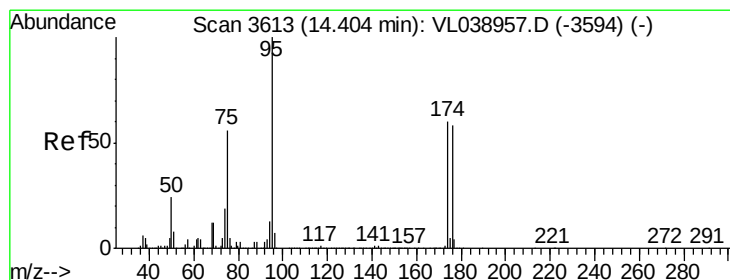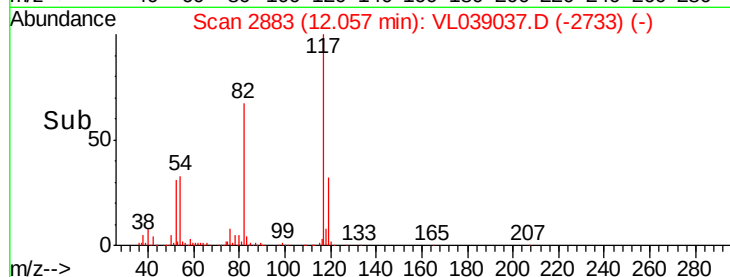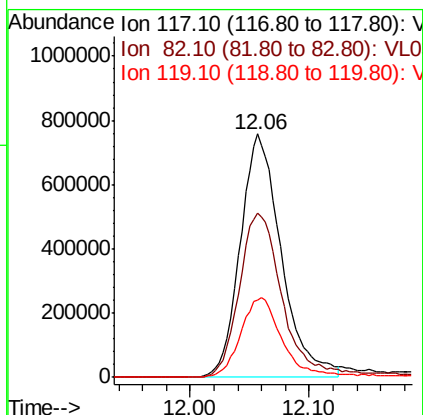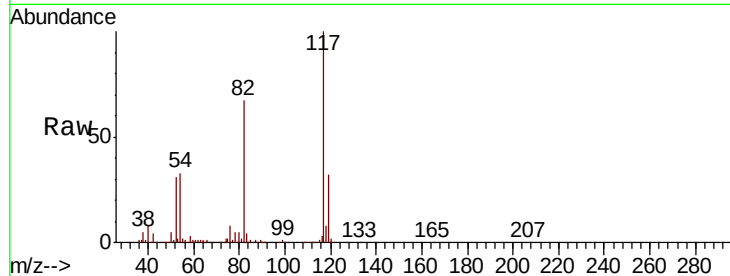

#68
1-Bromo-4-Fluorobenzene
Concen: 9.900 ppbv
RT: 14.38 min Scan# 3607
Delta R.T.: -0.02 min
Lab File: VL039037.D
Acq: 13 May 2022 14:21

Tgt Ion: 95 Resp: 1415344

Ion	Ratio	Lower	Upper
95	100		
174	65.7	50.8	76.2
175	4.7	3.8	5.6

