


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL051322\
 Data File : VL039033.D
 Acq On : 13 May 2022 11:50
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu May 05 10:12:15 2022
 Last Update : Thu May 05 10:12:15 2022

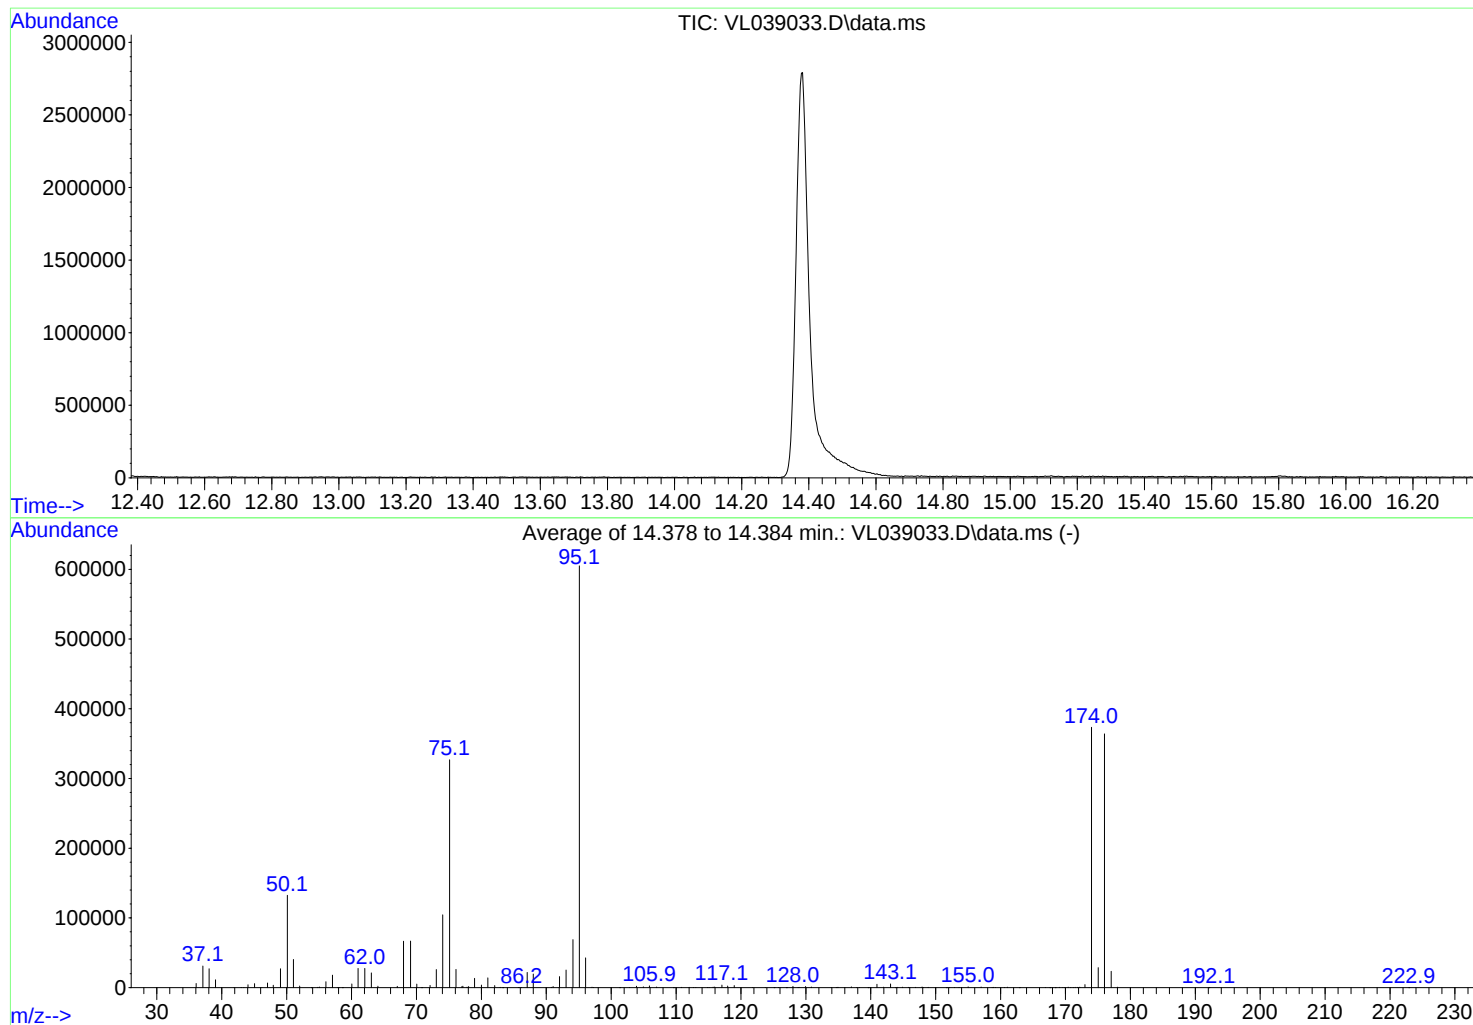

AutoFind: Scans 3605, 3606, 3607; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.9	132339	PASS
75	95	30	66	54.0	326763	PASS
95	95	100	100	100.0	605013	PASS
96	95	5	9	7.1	42744	PASS
173	174	0.00	2	1.2	4346	PASS
174	95	50	120	61.7	373312	PASS
175	174	4	9	7.7	28731	PASS
176	174	93	101	97.5	363947	PASS
177	176	5	9	6.4	23376	PASS

Average of 14.378 to 14.384 min.: VL039033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6047	47.05	6763	57.90	258	70.05	516
37.10	30947	47.95	3363	58.10	311	70.80	61
38.05	27107	49.05	27187	58.60	87	72.10	322
39.05	11309	50.10	132339	60.05	5387	73.05	2586
41.90	262	51.05	40344	61.00	27456	74.05	104501
43.00	139	52.00	2212	62.05	27485	75.10	326763
43.40	154	53.80	56	63.05	21195	76.10	26267
44.05	4088	54.80	424	64.05	2085	77.00	1650
45.05	5663	55.05	937	67.05	1913	77.15	2054
45.95	268	56.05	8602	68.00	66544	77.80	655
46.20	254	57.05	17965	69.10	66761	78.05	1523

Average of 14.378 to 14.384 min.: VL039033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	13416	90.80	592	103.90	2123	115.10	149
80.00	3611	91.05	1532	104.95	1071	115.70	614
81.00	14065	92.05	15745	105.90	2533	115.95	1017
82.05	3022	93.05	25339	107.00	869	117.05	3650
82.90	362	94.10	68947	109.60	86	117.95	2241
83.30	98	95.10	605013	110.00	280	118.95	2906
85.70	175	96.05	42744	110.85	393	121.80	337
85.90	254	97.05	822	112.00	390	123.75	134
86.20	318	97.30	231	112.70	264	125.10	114
87.05	21843	101.30	95	113.05	226	125.80	128
88.00	19461	102.85	294	114.85	277	127.00	86

Average of 14.378 to 14.384 min.: VL039033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.00	1825	137.85	140	146.00	239	155.00	1184
128.80	218	138.25	229	146.90	413	157.00	947
128.95	527	139.60	81	147.90	940	158.70	134
129.95	1709	140.00	181	148.10	313	158.90	468
130.85	938	140.95	4796	148.85	584	159.20	195
133.90	139	141.95	771	150.00	346	160.60	151
134.70	183	143.05	5197	151.65	123	161.05	608
134.80	367	143.80	114	152.15	225	162.90	69
134.95	563	144.15	376	152.90	340	166.90	226
136.00	215	144.90	747	153.60	190	167.60	124
137.00	1080	145.80	580	154.00	206	168.05	220

Average of 14.378 to 14.384 min.: VL039033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
168.40	92	174.00	373312				
169.05	370	175.05	28731				
169.60	259	176.00	363947				
169.90	216	177.05	23376				
170.40	694	178.05	628				
170.80	219	192.10	55				
171.20	202	222.90	53				
171.50	469						
171.85	492						
172.20	629						
173.00	4346						