

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL051623\
 Data File : VL040443.D
 Acq On : 16 May 2023 18:24
 Operator : SY/MD
 Sample : 02793-02 8X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SG-2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2023
 Supervised By :Mahesh Dadoda 05/17/2023

Quant Time: May 17 05:16:06 2023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL051623AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Wed May 17 05:12:40 2023

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.208	49	1016107	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.671	114	2525813	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.491	117	2311290	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.806	95	1867460	10.048	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.500%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.732	85	24814	0.124	ppbv	99
3) Chlorodifluoromethane	2.677	51	14723m	0.112	ppbv	
4) Chloromethane	2.816	50	11826	0.145	ppbv #	84
9) Propene	2.700	41	80710	1.581	ppbv	90
10) Heptane	7.600	43	518845	4.398	ppbv	100
13) Ethanol	3.240	45	654286	169.110	ppbv	94
15) Acetone	3.478	43	457111m	3.556	ppbv	
19) Isopropyl Alcohol	3.591	45	52108m	0.832	ppbv	
20) Methylene Chloride	3.941	84	3015925	52.668	ppbv	97
26) Hexane	5.230	57	3376418	33.645	ppbv #	35
30) Cyclohexane	6.619	84	401825m	4.922	ppbv	
34) 2-Butanone	4.803	43	57265m	0.426	ppbv	
35) Carbon Tetrachloride	6.510	117	5571m	0.031	ppbv	
36) Benzene	6.391	78	463925	2.261	ppbv	98
41) Tetrahydrofuran	5.587	42	24171	0.324	ppbv #	87
44) 2,2,4-Trimethylpentane	7.349	57	499059	1.470	ppbv #	25
52) Tetrachloroethene	10.645	164	3587m	0.051	ppbv	
53) Toluene	9.246	91	2288528	10.562	ppbv	100
58) Ethyl Benzene	12.114	91	946298	3.235	ppbv	96
59) m/p-Xylene	12.372	91	2907676	10.899	ppbv	96
60) o-Xylene	13.085	91	1224278	4.822	ppbv	100
62) Isopropylbenzene	14.056	105	216711	0.584	ppbv	99
64) n-propylbenzene	14.947	120	113730	1.242	ppbv	79
67) sec-Butylbenzene	16.661	105	193674	0.413	ppbv	98
69) p-Isopropyltoluene	17.021	119	100420	0.273	ppbv	94
70) n-Butylbenzene	17.915	91	273140	0.666	ppbv #	62
72) 4-Ethyltoluene	15.220	105	599301	2.082	ppbv	97
73) 1,3,5-Trimethylbenzene	15.378	105	592751	2.243	ppbv	94
74) 1,2,4-Trimethylbenzene	16.133	105	1712774	5.632	ppbv #	71
79) Naphthalene	21.426	128	42645m	0.232	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL051623\
Data File : VL040443.D
Acq On : 16 May 2023 18:24
Operator : SY/MD
Sample : 02793-02 8X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SG-2

Quant Time: May 17 05:16:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL051623AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Wed May 17 05:12:40 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 05/17/2023
Supervised By : Mahesh Dadoda 05/17/2023

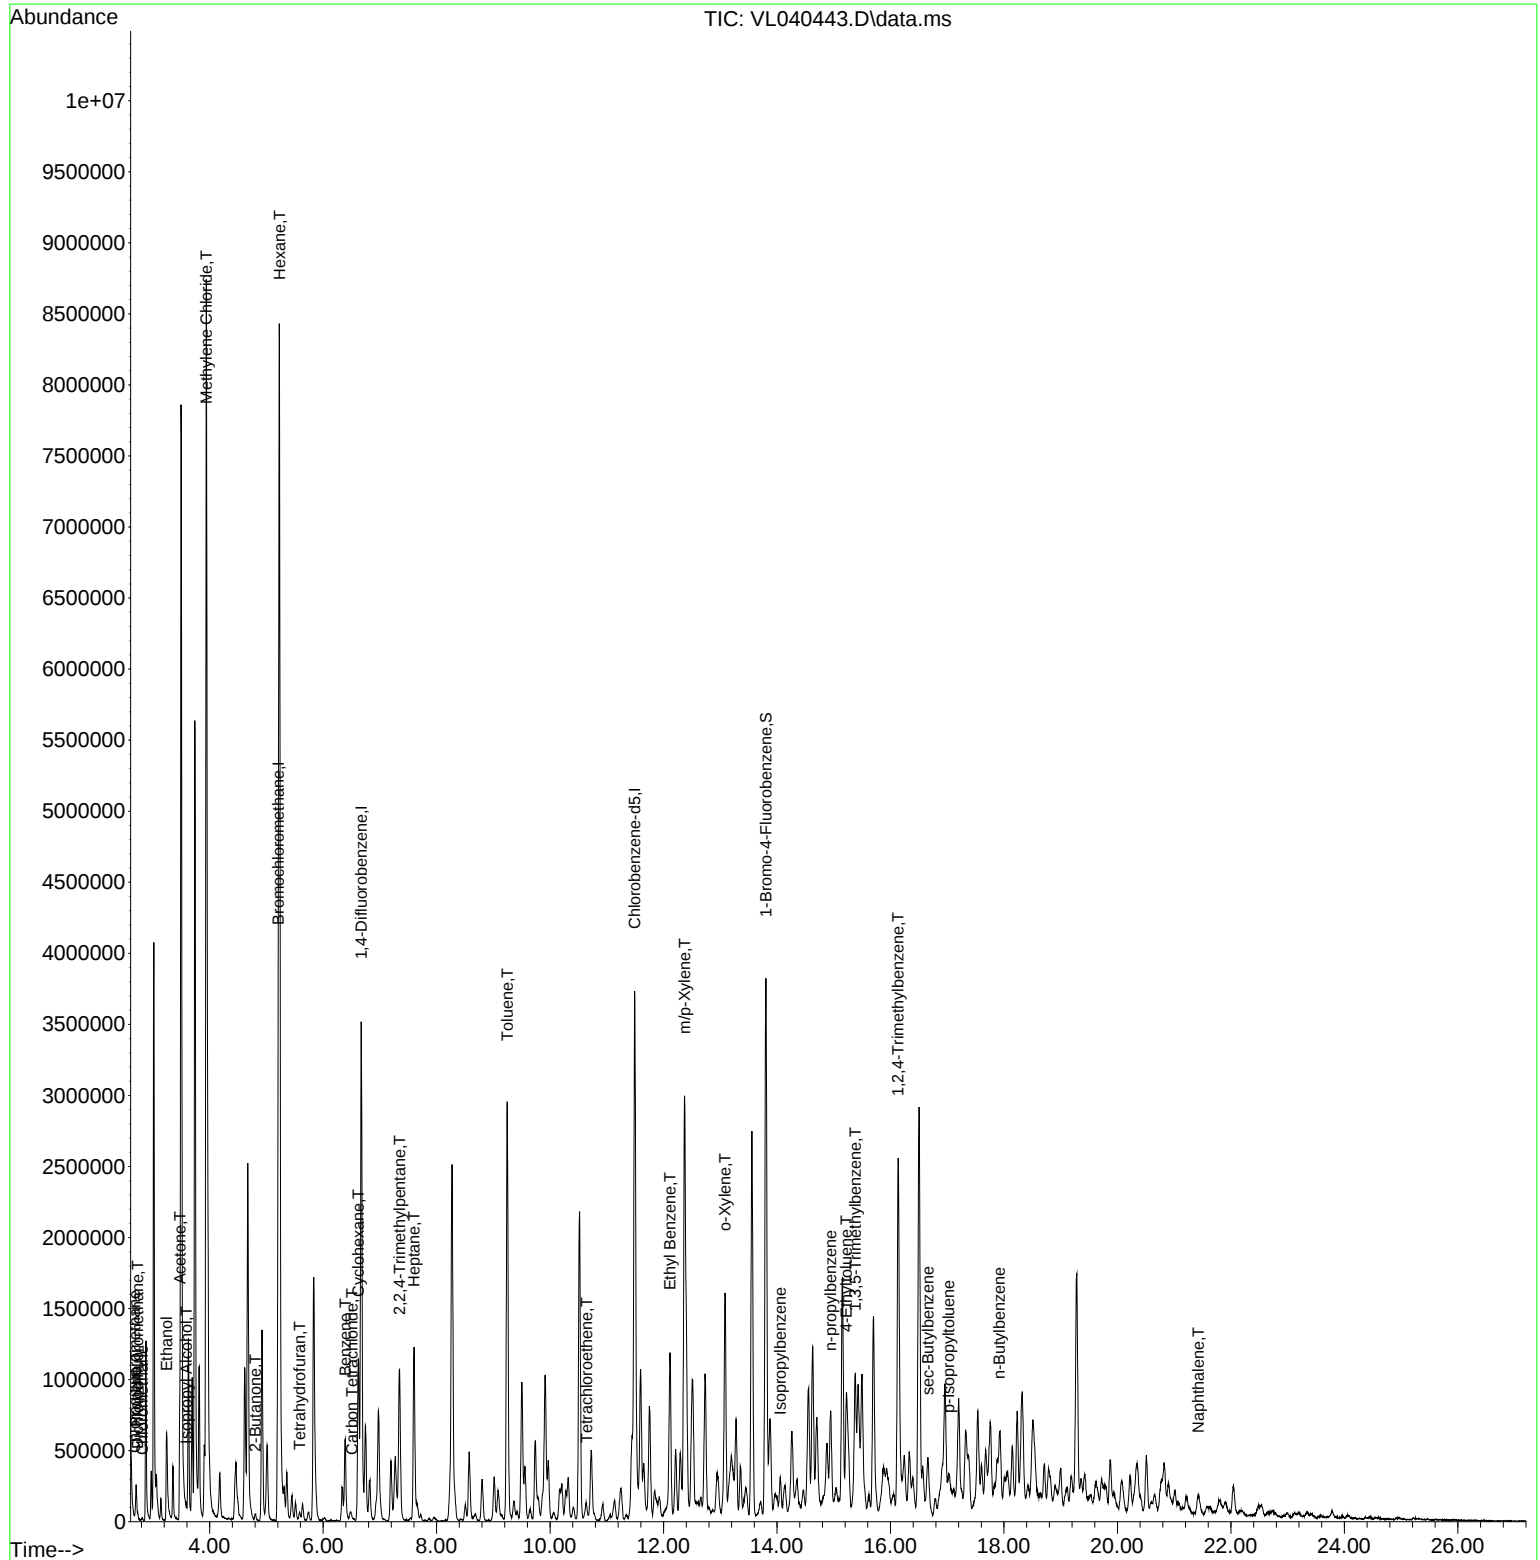



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.208 min Scan# 81
Delta R.T. 0.003 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24




Instrument :
MSVOA_L
ClientSampleId :
SG-2




Tgt Ion: 49 Resp: 101610
Ion Ratio Lower Upper
49 100
128 47.7 24.3 72.8
130 60.4 30.2 90.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023




#2
Dichlorodifluoromethane
Concen: 0.124 ppbv
RT: 2.732 min Scan# 40
Delta R.T. 0.003 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24




Tgt Ion: 85 Resp: 24814
Ion Ratio Lower Upper
85 100
87 34.7 27.4 41.0

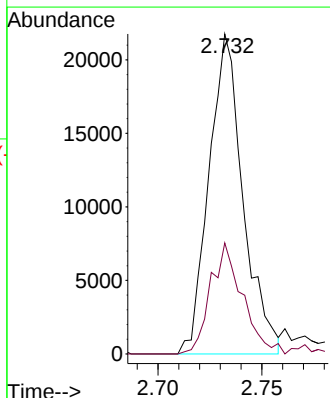

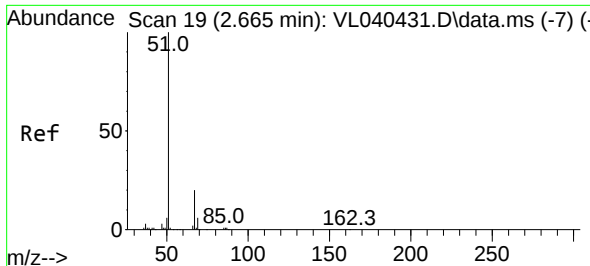

#3
Chlorodifluoromethane
Concen: 0.112 ppbv m
RT: 2.677 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24




Instrument :
MSVOA_L
ClientSampleId :
SG-2

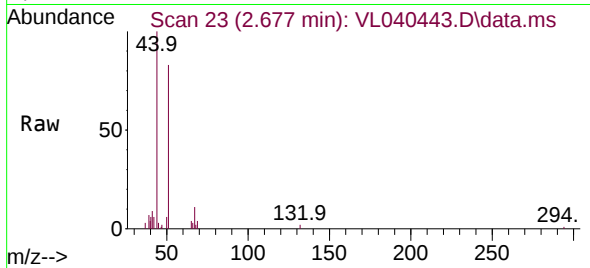


Tgt Ion: 51 Resp: 1472
Ion Ratio Lower Upper
51 100
67 16.7 15.8 23.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

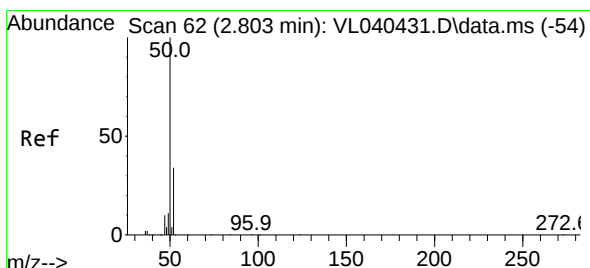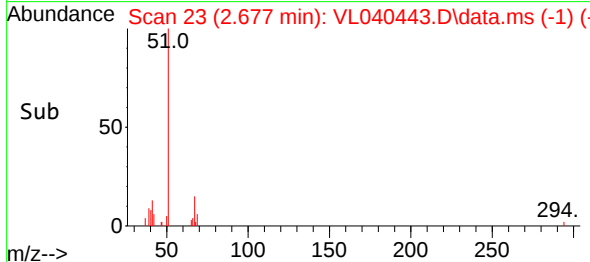


#4
Chloromethane
Concen: 0.145 ppbv
RT: 2.816 min Scan# 66
Delta R.T. 0.003 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24

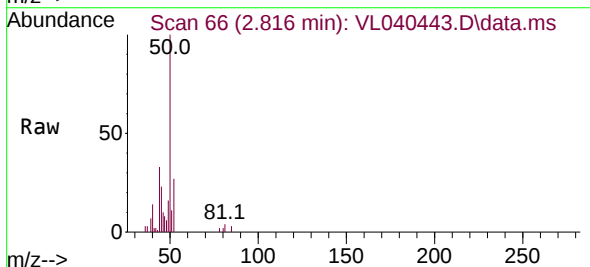

Tgt Ion: 50 Resp: 11826
Ion Ratio Lower Upper
50 100
52 25.4 27.6 41.4#

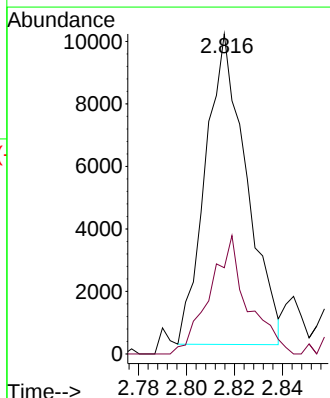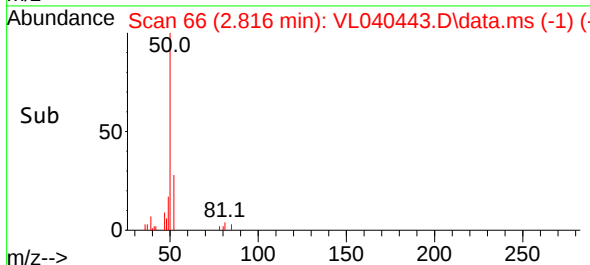

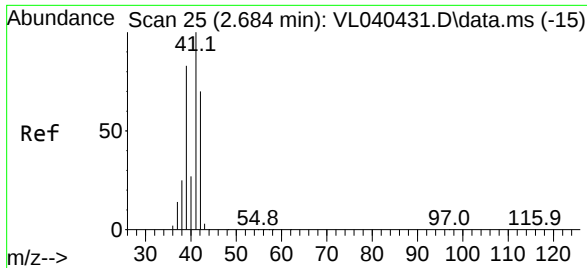

#9

Propene

Concen: 1.581 ppbv

RT: 2.700 min Scan# 30

Delta R.T. 0.007 min

Lab File: VL040443.D

Acq: 16 May 2023 18:24

Instrument :

MSVOA_L

ClientSampleId :

SG-2

Tgt Ion: 41 Resp: 80710

Ion Ratio Lower Upper

41 100





42 62.5 56.6 84.8

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2023

Supervised By :Mahesh Dadoda 05/17/2023

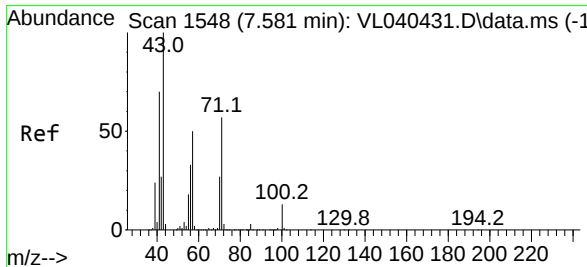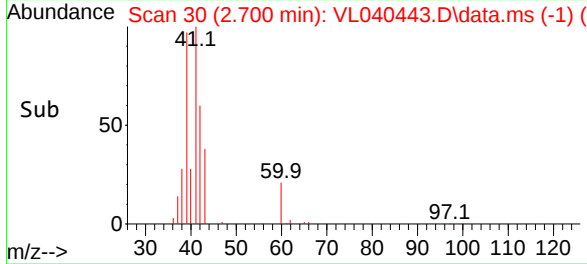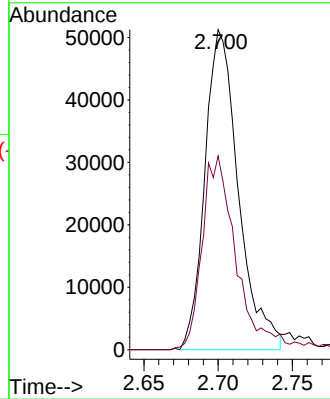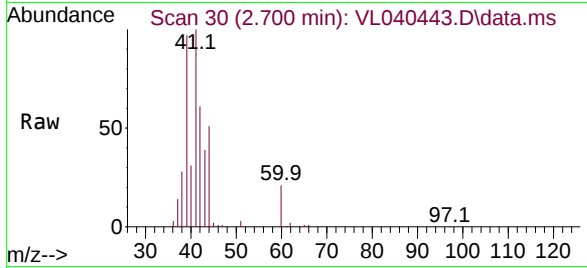

#10

Heptane

Concen: 4.398 ppbv

RT: 7.600 min Scan# 1554

Delta R.T. 0.003 min

Lab File: VL040443.D




Acq: 16 May 2023 18:24


Tgt Ion: 43 Resp: 518845

Ion Ratio Lower Upper

43 100

57 52.5 42.2 63.2

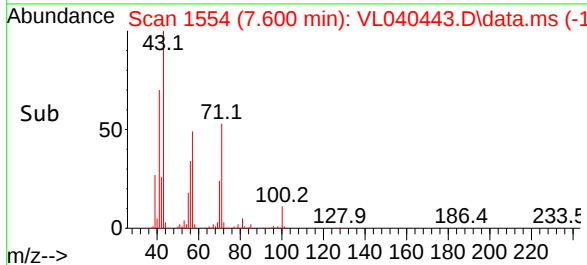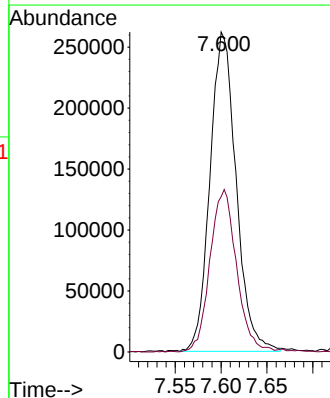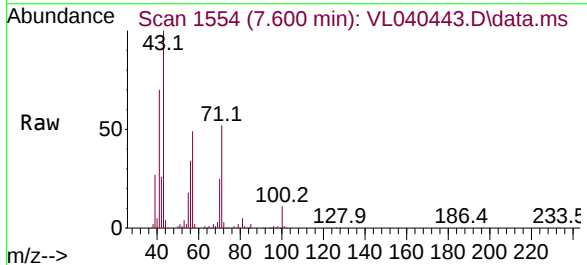







#13
Ethanol
Concen: 169.110 ppbv
RT: 3.240 min Scan# 197
Delta R.T. -0.010 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24

Instrument :
MSVOA_L
ClientSampleId :
SG-2

Tgt Ion: 45 Resp: 654280
Ion Ratio Lower Upper
45 100
46 36.6 13.2 52.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

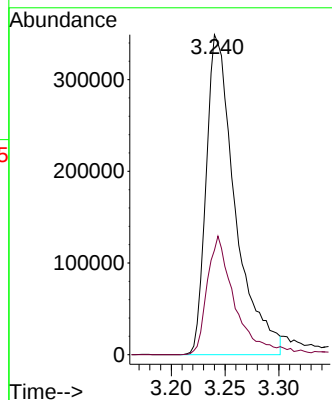

#15
Acetone
Concen: 3.556 ppbv m
RT: 3.478 min Scan# 272
Delta R.T. 0.010 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24


Tgt Ion: 43 Resp: 457111
Ion Ratio Lower Upper
43 100
58 63.9 22.2 33.4#

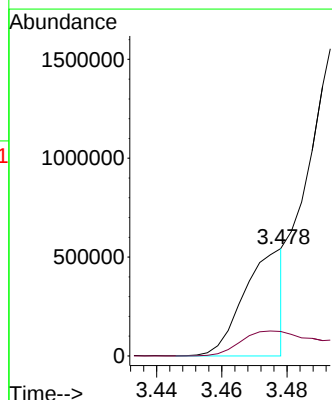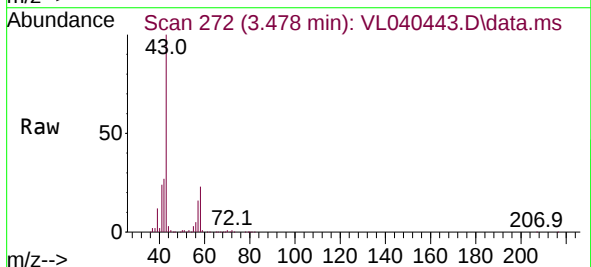



#19
Isopropyl Alcohol
Concen: 0.832 ppbv m
RT: 3.591 min Scan# 307
Delta R.T. 0.013 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24




Instrument :
MSVOA_L
ClientSampleId :
SG-2

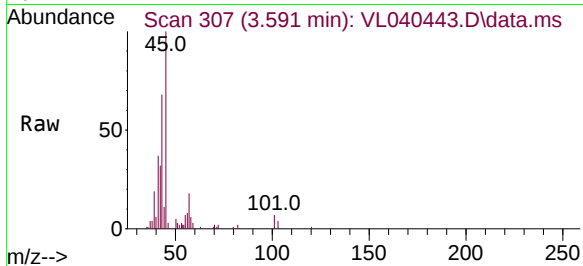

Tgt Ion: 45 Resp: 52108
Ion Ratio Lower Upper
45 100
58 567.6 2.1 3.1




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023



#20
Methylene Chloride
Concen: 52.668 ppbv
RT: 3.941 min Scan# 416
Delta R.T. 0.003 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24


Tgt Ion: 84 Resp: 3015925
Ion Ratio Lower Upper
84 100
49 148.2 123.7 185.5
51 49.0 38.6 57.8
86 65.8 53.2 79.8

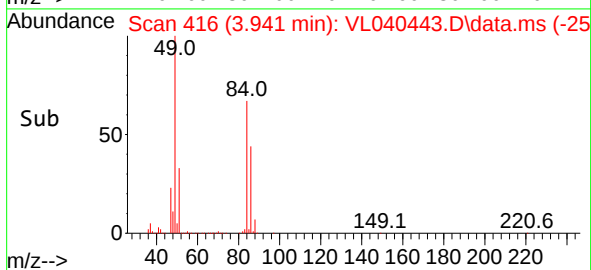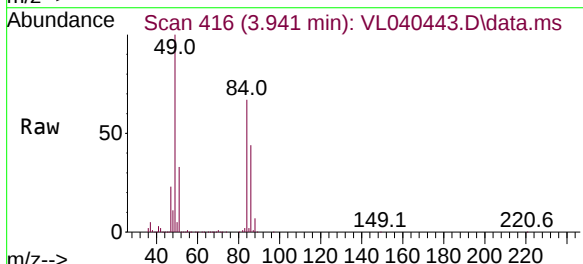



#26
Hexane
Concen: 33.645 ppbv
RT: 5.230 min Scan# 810
Delta R.T. 0.007 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24




Instrument :
MSVOA_L
ClientSampleId :
SG-2

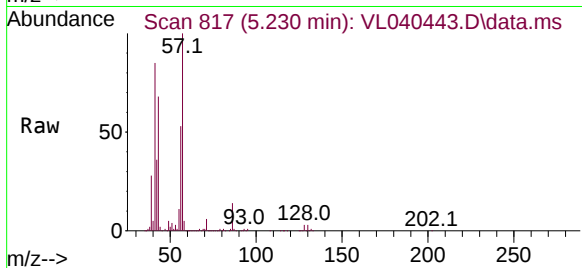

Tgt Ion: 57 Resp: 3376418
Ion Ratio Lower Upper
57 100
41 88.8 75.1 112.7
43 69.2 194.4 291.6
56 54.7 42.7 64.1




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

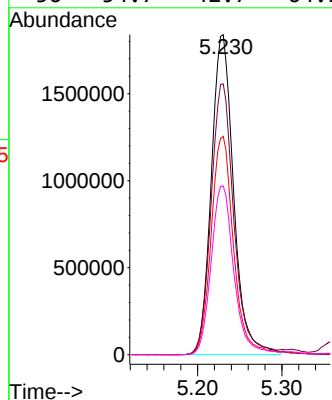

#30
Cyclohexane
Concen: 4.922 ppbv m
RT: 6.619 min Scan# 1249
Delta R.T. 0.003 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24

Tgt Ion: 84 Resp: 401825
Ion Ratio Lower Upper
84 100
56 0.0 108.2 162.4#
41 88.7 66.9 100.3

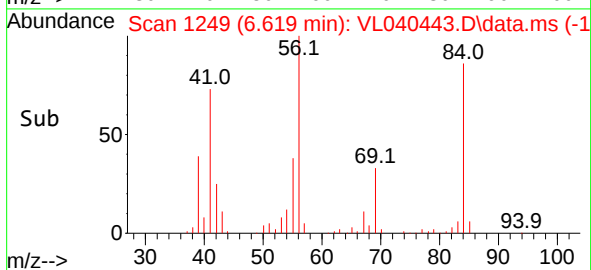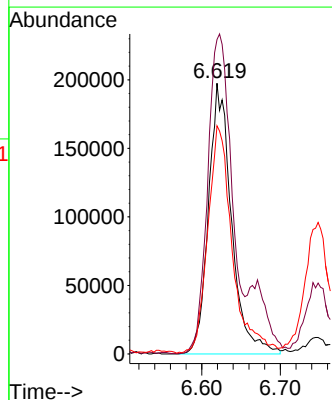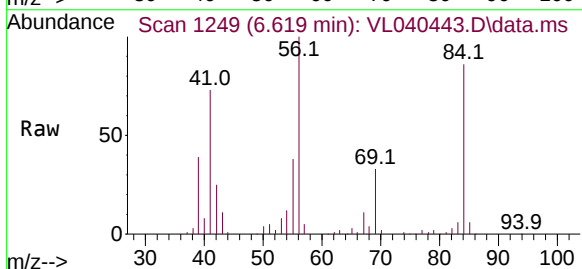



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 6.671 min Scan# 114

Delta R.T. 0.000 min

Lab File: VL040443.D

Acq: 16 May 2023 18:24

Instrument :

MSVOA_L

ClientSampleId :

SG-2

Tgt Ion:114 Resp: 252581

Ion Ratio Lower Upper

114 100

63 26.6 21.0 31.6





88 18.2 14.6 22.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2023

Supervised By :Mahesh Dadoda 05/17/2023

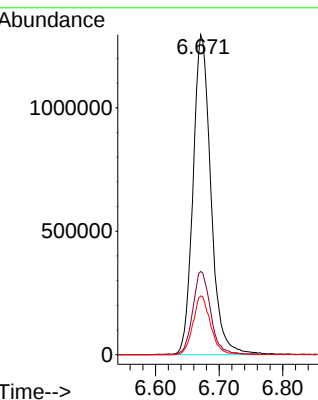

#34

2-Butanone

Concen: 0.426 ppbv m

RT: 4.803 min Scan# 684

Delta R.T. 0.007 min

Lab File: VL040443.D




Acq: 16 May 2023 18:24


Tgt Ion: 43 Resp: 57265

Ion Ratio Lower Upper

43 100

72 20.3 18.3 27.5

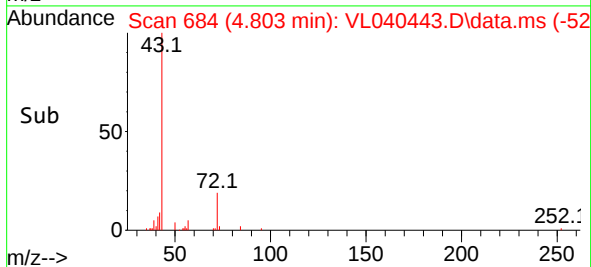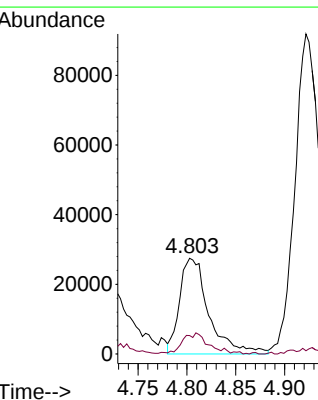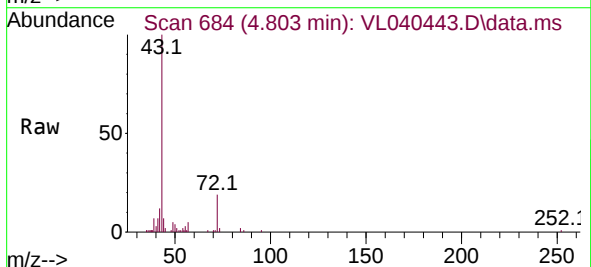







#35
Carbon Tetrachloride
Concen: 0.031 ppbv m
RT: 6.510 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24

Instrument :
MSVOA_L
ClientSampleId :
SG-2

Tgt Ion: 117 Resp: 557
Ion Ratio Lower Upper
117 100
119 63.9 78.0 117.0
121 16.9 25.2 37.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023



#36
Benzene
Concen: 2.261 ppbv
RT: 6.391 min Scan# 1178
Delta R.T. 0.007 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24

Tgt Ion: 78 Resp: 463925
Ion Ratio Lower Upper
78 100
77 23.5 17.7 26.5
50 20.4 15.8 23.8

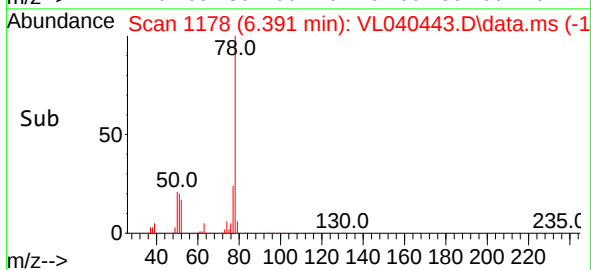



#41

Tetrahydrofuran

Concen: 0.324 ppbv

RT: 5.587 min Scan# 918

Delta R.T. 0.019 min

Lab File: VL040443.D

Acq: 16 May 2023 18:24

Instrument :

MSVOA_L

ClientSampleId :





SG-2

Tgt Ion: 42	Resp: 2417
Ion Ratio	Lower Upper
42	100
72	50.6 33.0 49.4
71	47.4 32.2 48.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

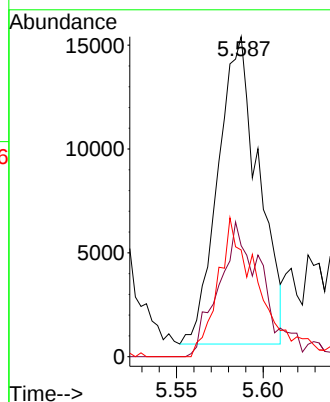

#44

2,2,4-Trimethylpentane

Concen: 1.470 ppbv




RT: 7.349 min Scan# 1476


Delta R.T. 0.007 min

Lab File: VL040443.D

Acq: 16 May 2023 18:24

Tgt Ion: 57	Resp: 499059
Ion Ratio	Lower Upper
57	100
41	70.6 27.0 40.4
56	78.2 25.0 37.4

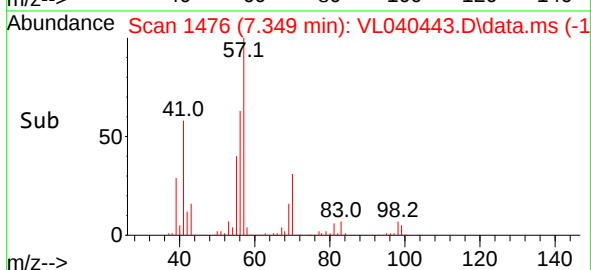



#52

Tetrachloroethene

Concen: 0.051 ppbv m

RT: 10.645 min Scan# 2065

Delta R.T. 0.007 min

Lab File: VL040443.D


Acq: 16 May 2023 18:24

Instrument :

MSVOA_L

ClientSampleId :

SG-2






Tgt Ion:	164	Resp:	358
Ion	Ratio	Lower	Upper
164	100		
166	106.5	97.8	146.6
129	59.4	88.4	132.6
131	63.3	86.1	129.1

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

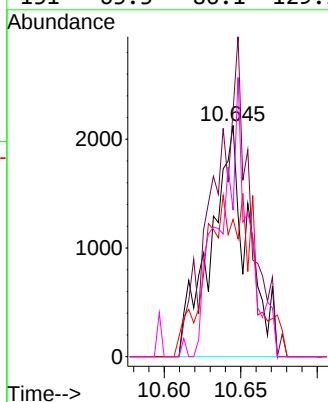

#53

Toluene

Concen: 10.562 ppbv

RT: 9.246 min Scan# 2066

Delta R.T. 0.003 min

Lab File: VL040443.D




Acq: 16 May 2023 18:24


Tgt Ion: 91 Resp: 2288528

Ion Ratio Lower Upper

91 100


92 61.5 49.1 73.7

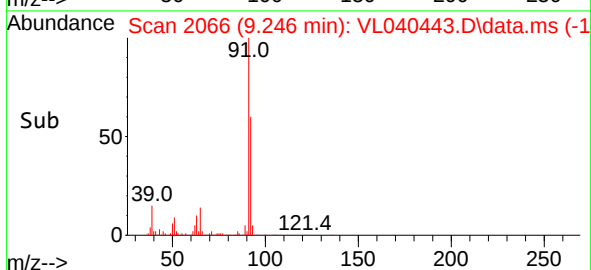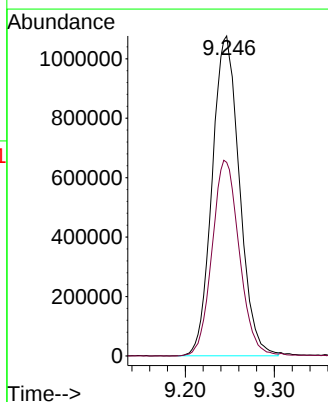

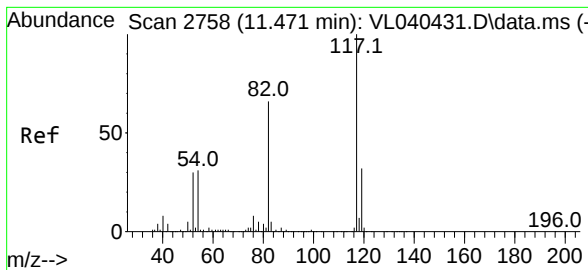

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.491 min Scan# 21
Delta R.T. 0.000 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24




Instrument :
MSVOA_L
ClientSampleId :
SG-2

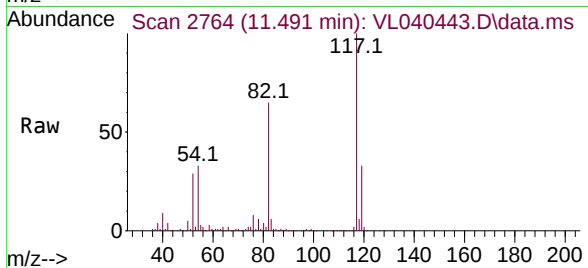

Tgt Ion:117 Resp: 2311290
Ion Ratio Lower Upper
117 100
82 67.0 52.5 78.7
119 33.0 24.0 36.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

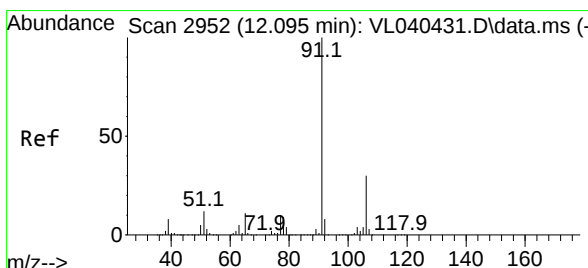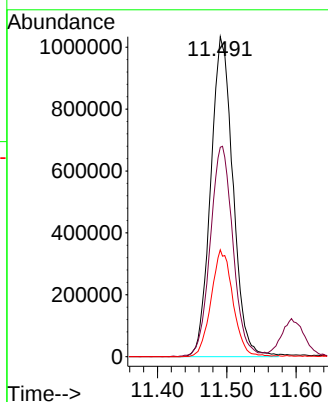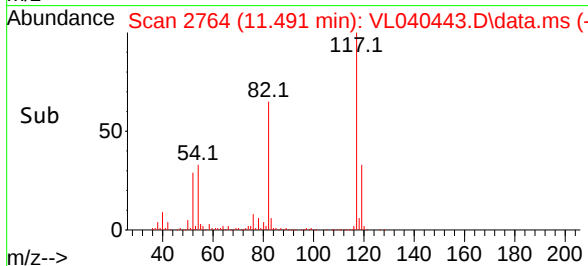

#58
Ethyl Benzene
Concen: 3.235 ppbv
RT: 12.114 min Scan# 2958
Delta R.T. 0.003 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24

Tgt Ion: 91 Resp: 946298
Ion Ratio Lower Upper
91 100
106 27.7 23.8 35.8

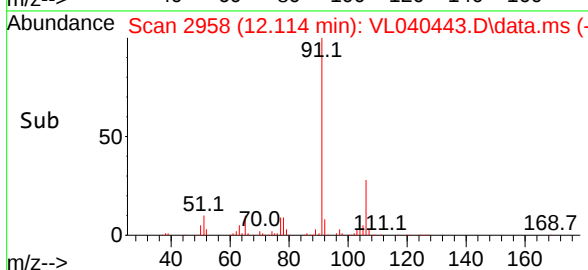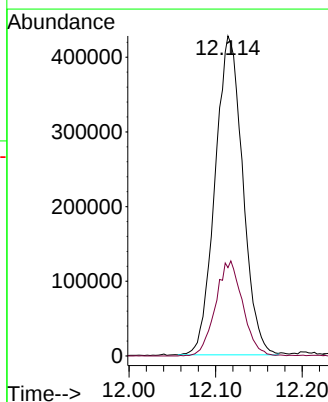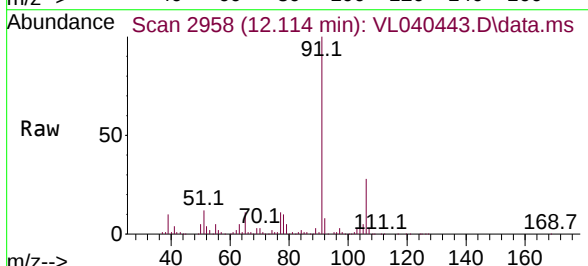



#59

m/p-Xylene

Concen: 10.899 ppbv

RT: 12.372 min Scan# 3041

Delta R.T. -0.026 min

Lab File: VL040443.D

Acq: 16 May 2023 18:24

Instrument :

MSVOA_L

ClientSampleId :

SG-2

Tgt Ion: 91 Resp: 2907670

Ion Ratio Lower Upper

91 100





106 46.5 34.9 52.3

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2023

Supervised By :Mahesh Dadoda 05/17/2023



#60

o-Xylene

Concen: 4.822 ppbv

RT: 13.085 min Scan# 3260

Delta R.T. 0.003 min

Lab File: VL040443.D




Acq: 16 May 2023 18:24


Tgt Ion: 91 Resp: 1224278

Ion Ratio Lower Upper

91 100


106 43.7 21.8 65.4

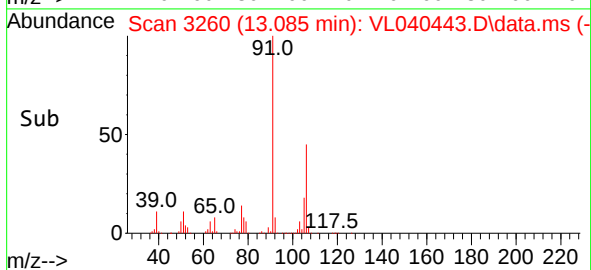

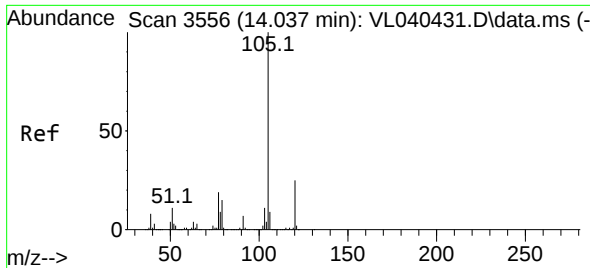

#62
Isopropylbenzene
Concen: 0.584 ppbv
RT: 14.056 min Scan# 31
Delta R.T. 0.000 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24




Instrument :
MSVOA_L
ClientSampleId :
SG-2

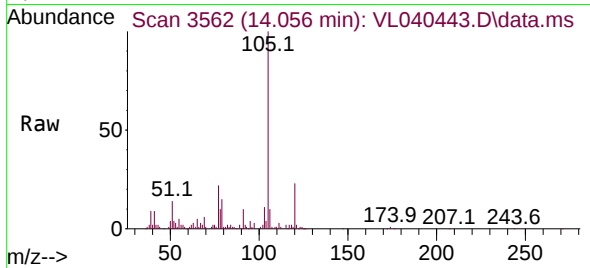

Tgt Ion:105 Resp: 21671
Ion Ratio Lower Upper
105 100
120 24.3 20.0 30.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

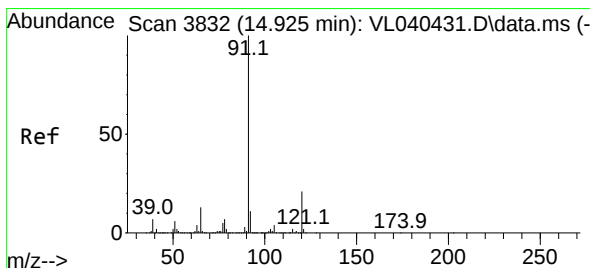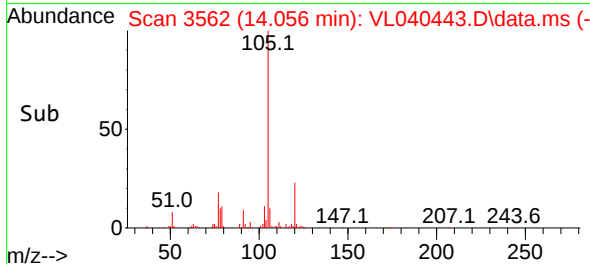

#64
n-propylbenzene
Concen: 1.242 ppbv
RT: 14.947 min Scan# 3839
Delta R.T. 0.003 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24


Tgt Ion:120 Resp: 113730
Ion Ratio Lower Upper
120 100
91 549.8 393.2 589.8

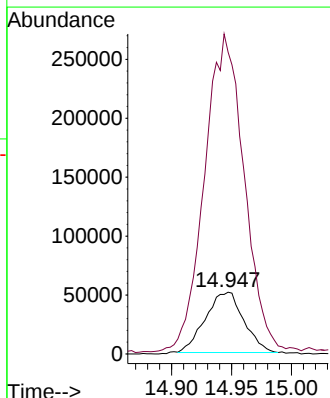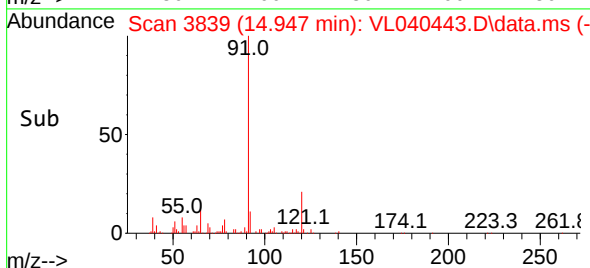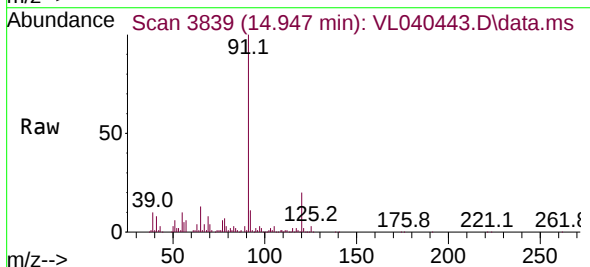

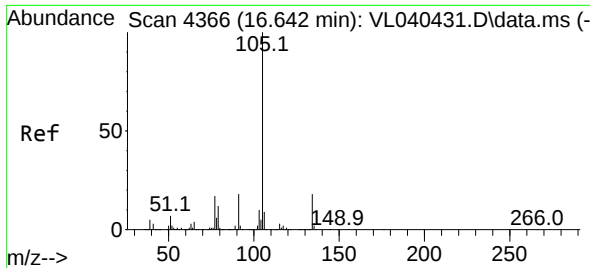

#67
 sec-Butylbenzene
 Concen: 0.413 ppbv
 RT: 16.661 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: VL040443.D
 Acq: 16 May 2023 18:24




Instrument :
 MSVOA_L
 ClientSampleId :
 SG-2

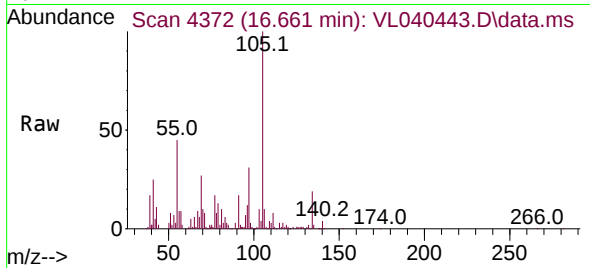


Tgt Ion:105 Resp: 193674
 Ion Ratio Lower Upper
 105 100
 134 18.3 14.1 21.1

Manual Integrations
 APPROVED



Reviewed By :Semsettin Yesilyurt 05/17/2023
 Supervised By :Mahesh Dadoda 05/17/2023

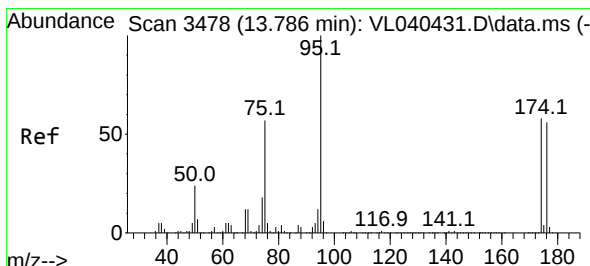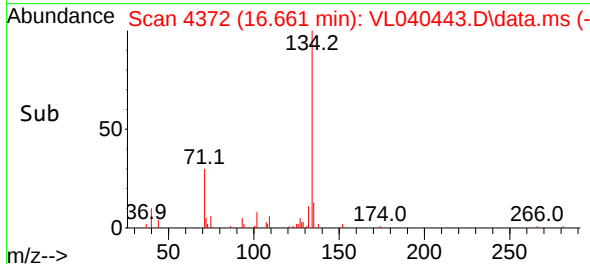


#68
 1-Bromo-4-Fluorobenzene
 Concen: 10.048 ppbv
 RT: 13.806 min Scan# 3484
 Delta R.T. 0.007 min
 Lab File: VL040443.D
 Acq: 16 May 2023 18:24

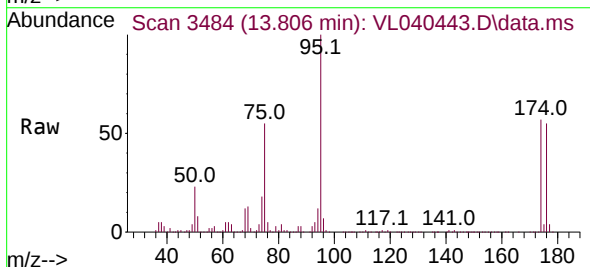


Tgt Ion: 95 Resp: 1867460
 Ion Ratio Lower Upper
 95 100
 174 59.3 47.0 70.6
 175 4.1 3.4 5.0

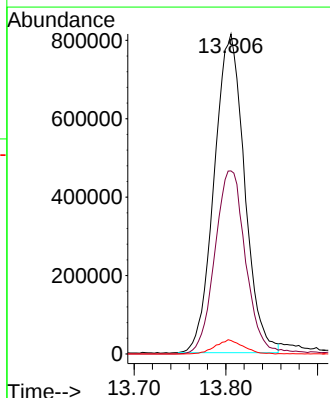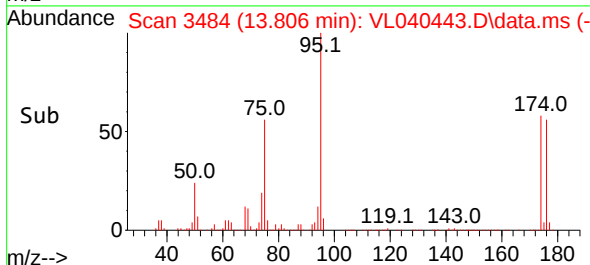



#69
p-Isopropyltoluene
Concen: 0.273 ppbv
RT: 17.021 min Scan# 4479
Delta R.T. 0.000 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24




Instrument :
MSVOA_L
ClientSampleId :
SG-2

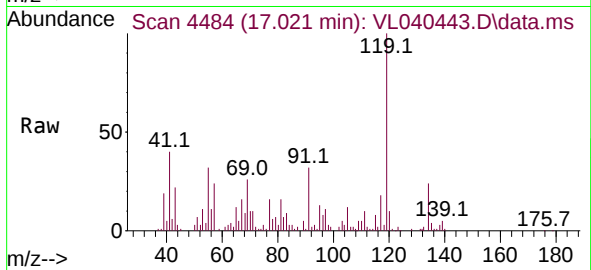


Tgt Ion: 119 Resp: 100420
Ion Ratio Lower Upper
119 100
134 26.5 20.2 30.4
91 36.2 25.4 38.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

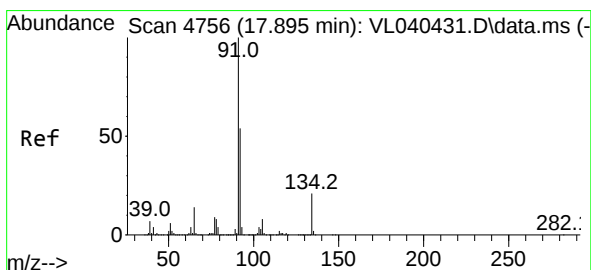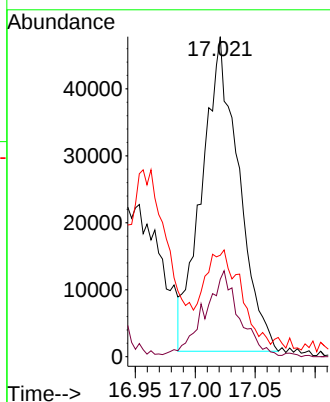


#70
n-Butylbenzene
Concen: 0.666 ppbv
RT: 17.915 min Scan# 4762
Delta R.T. 0.003 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24

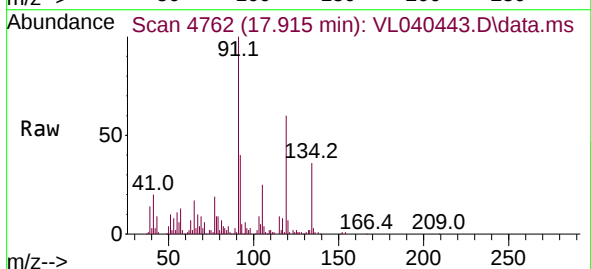


Tgt Ion: 91 Resp: 273140
Ion Ratio Lower Upper
91 100
92 40.0 43.2 64.8#
134 61.7 16.9 25.3#



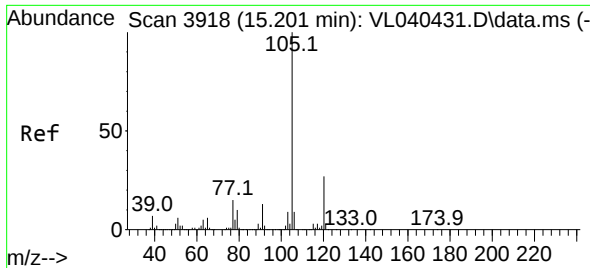

#72
4-Ethyltoluene
Concen: 2.082 ppbv
RT: 15.220 min Scan# 3924
Delta R.T. 0.000 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24




Instrument :
MSVOA_L
ClientSampleId :
SG-2

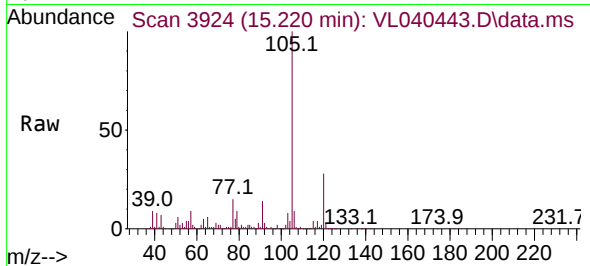

Tgt Ion:105 Resp: 59930
Ion Ratio Lower Upper
105 100
120 27.3 23.8 35.8
91 14.0 11.0 16.4
77 16.4 12.2 18.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

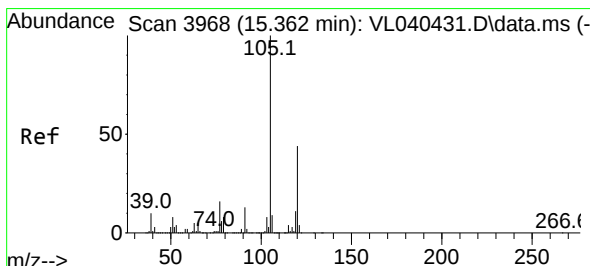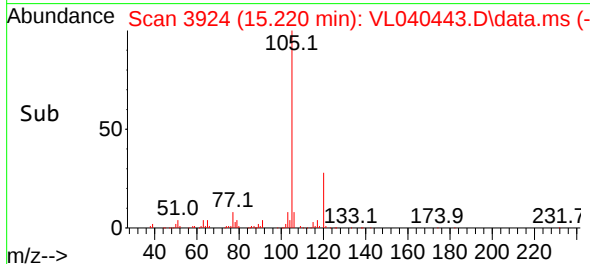

#73
1,3,5-Trimethylbenzene
Concen: 2.243 ppbv
RT: 15.378 min Scan# 3973
Delta R.T. 0.003 min
Lab File: VL040443.D
Acq: 16 May 2023 18:24

Tgt Ion:105 Resp: 592751
Ion Ratio Lower Upper
105 100
120 40.3 35.2 52.8

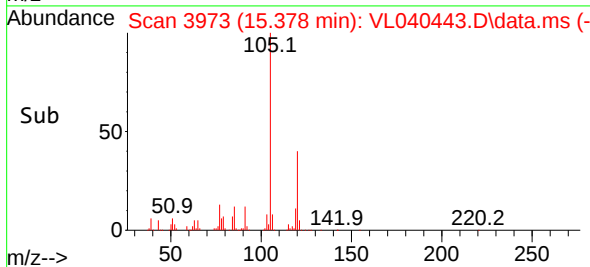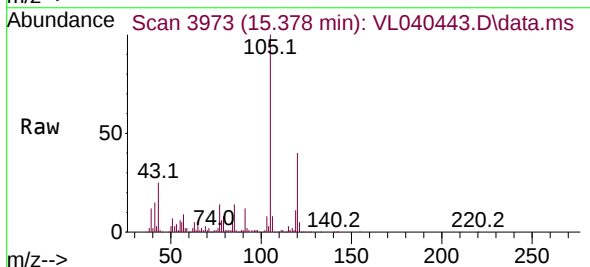



#74

1,2,4-Trimethylbenzene

Concen: 5.632 ppbv

RT: 16.133 min Scan# 41

Delta R.T. 0.000 min

Lab File: VL040443.D

Acq: 16 May 2023 18:24

Instrument :

MSVOA_L

ClientSampleId :

SG-2

Tgt Ion:105 Resp: 1712774

Ion Ratio Lower Upper

105 100

120 42.2 38.1 57.1

91 12.0 40.2 60.2





77 16.2 19.0 28.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2023

Supervised By :Mahesh Dadoda 05/17/2023

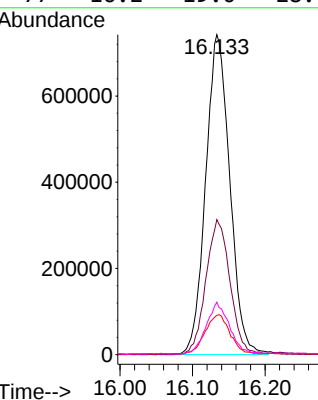

#79

Naphthalene

Concen: 0.232 ppbv m

RT: 21.426 min Scan# 5854

Delta R.T. 0.010 min

Lab File: VL040443.D

Acq: 16 May 2023 18:24

Tgt Ion:128 Resp: 42645

Ion Ratio Lower Upper

128 100

127 8.6 10.3 15.5

129 18.1 9.0 13.6

