


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL051623\
 Data File : VL040429.D
 Acq On : 16 May 2023 8:16
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL051623AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Wed May 17 05:12:40 2023

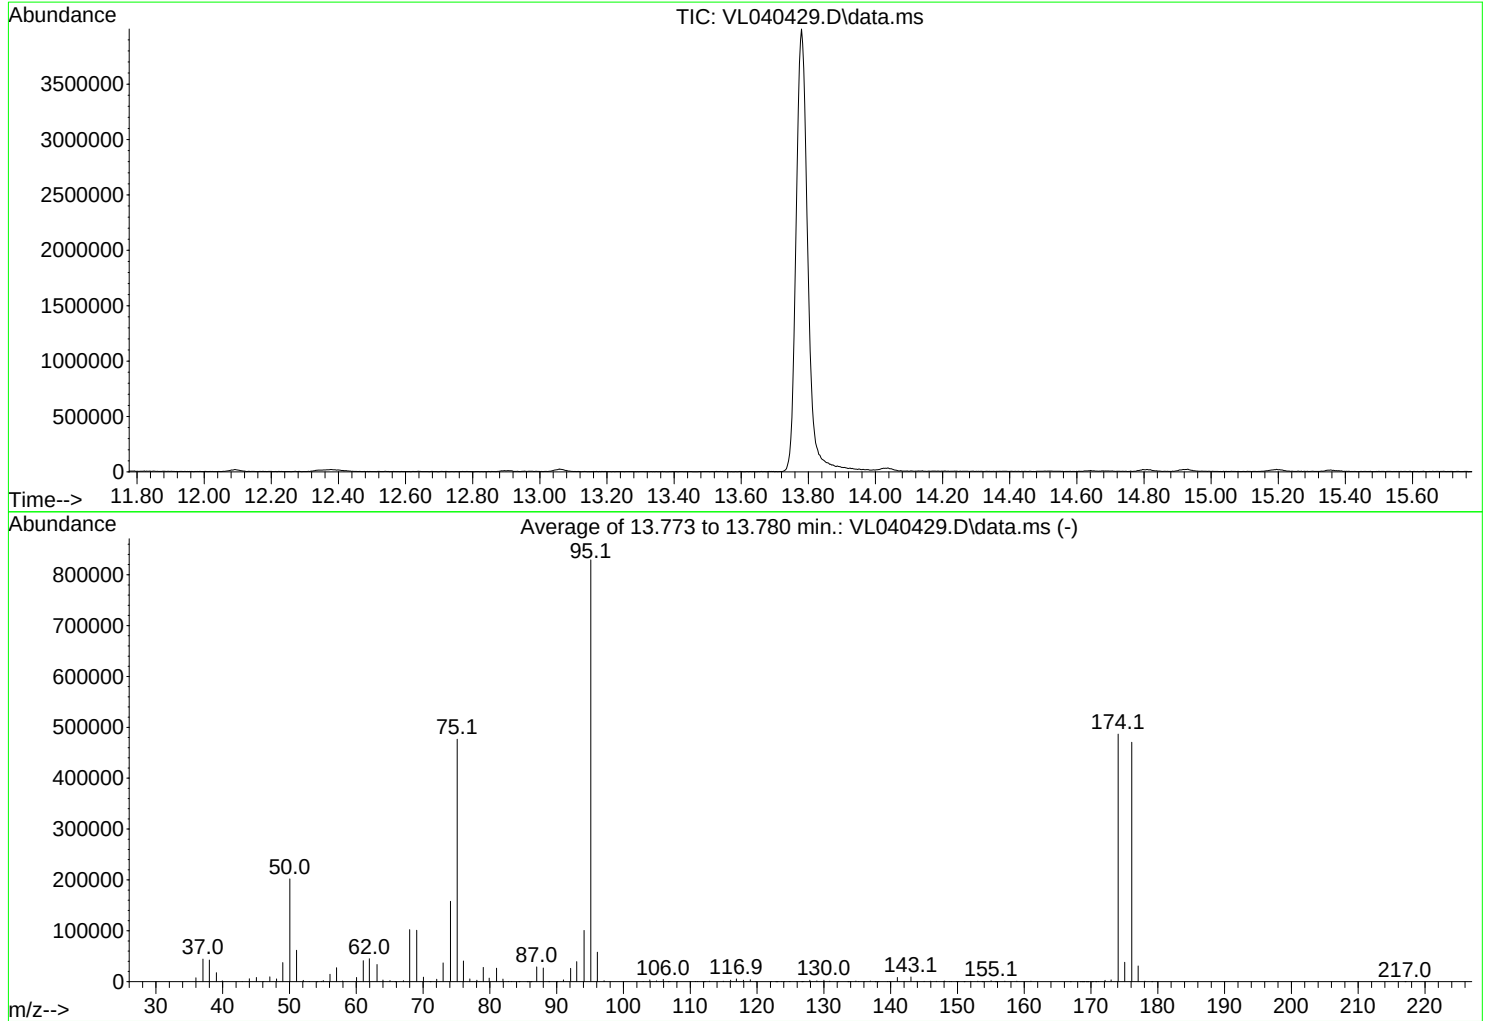

AutoFind: Scans 3474, 3475, 3476; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	201835	PASS
75	95	30	66	57.5	476757	PASS
95	95	100	100	100.0	829291	PASS
96	95	5	9	7.0	57989	PASS
173	174	0.00	2	0.7	3567	PASS
174	95	50	120	58.7	486741	PASS
175	174	4	9	7.8	38005	PASS
176	174	93	101	96.7	470549	PASS
177	176	5	9	6.5	30733	PASS

Average of 13.773 to 13.780 min.: VL040429.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7438	49.00	37541	60.05	8038	71.05	181
37.05	44341	50.05	201835	61.05	41288	72.05	460
38.00	42584	51.05	61851	61.95	45006	73.00	3695
39.05	17629	52.05	2613	63.10	33653	74.10	15788
39.95	1451	52.95	239	64.00	3220	75.10	476757
42.90	374	54.10	69	65.05	2327	76.05	40685
44.00	5829	54.80	540	65.80	86	77.00	5305
45.05	8060	55.05	2140	67.05	2064	78.05	2820
46.15	497	56.05	14462	68.00	102205	79.00	27957
47.05	9401	57.05	27429	69.05	100965	79.90	6882
48.05	5262	57.95	1160	70.05	8703	81.00	26456

Average of 13.773 to 13.780 min.: VL040429.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.95	5200	91.00	3541	106.70	151	116.90	5270
82.80	404	92.10	26157	107.00	239	117.95	2847
83.25	455	93.00	39496	108.00	90	119.00	3827
84.35	144	94.10	100664	110.00	347	119.80	82
85.60	166	95.10	829291	110.80	483	122.15	217
85.85	510	96.10	57989	111.10	296	122.80	87
86.15	189	97.10	1985	111.90	341	123.00	60
87.00	28808	102.95	362	112.10	137	123.70	289
88.00	26880	103.95	3490	112.90	942	124.10	310
88.80	155	104.95	1658	114.95	960	124.80	211
90.00	79	105.95	4300	116.05	2881	124.95	228

Average of 13.773 to 13.780 min.: VL040429.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.95	373	135.20	425	145.00	583	153.05	850
126.70	107	136.05	219	145.95	875	153.70	74
127.00	309	136.95	1326	146.85	712	153.95	364
127.90	2921	137.70	52	147.90	601	155.05	1769
128.95	1755	138.10	70	148.10	1360	155.70	103
130.00	2937	139.55	214	148.85	309	155.90	143
130.90	1084	139.80	314	149.10	220	157.10	1035
132.10	133	141.00	8058	149.90	268	158.90	1096
133.60	183	142.00	624	150.15	424	161.00	842
133.90	79	143.05	9295	151.00	171	166.90	54
134.80	1131	143.95	598	152.00	631	168.40	60

Average of 13.773 to 13.780 min.: VL040429.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
168.70	144	176.10	470549				
168.90	129	177.05	30733				
169.30	92	178.05	806				
169.50	75	179.10	50				
170.20	170	217.00	61				
170.70	172						
171.10	433						
172.10	2628						
173.00	3567						
174.05	486741						
175.05	38005						