


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL051719\
 Data File : VL033699.D
 Acq On : 17 May 2019 1:21
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL051719AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri May 17 08:15:41 2019
 Last Update : Fri May 17 08:15:41 2019

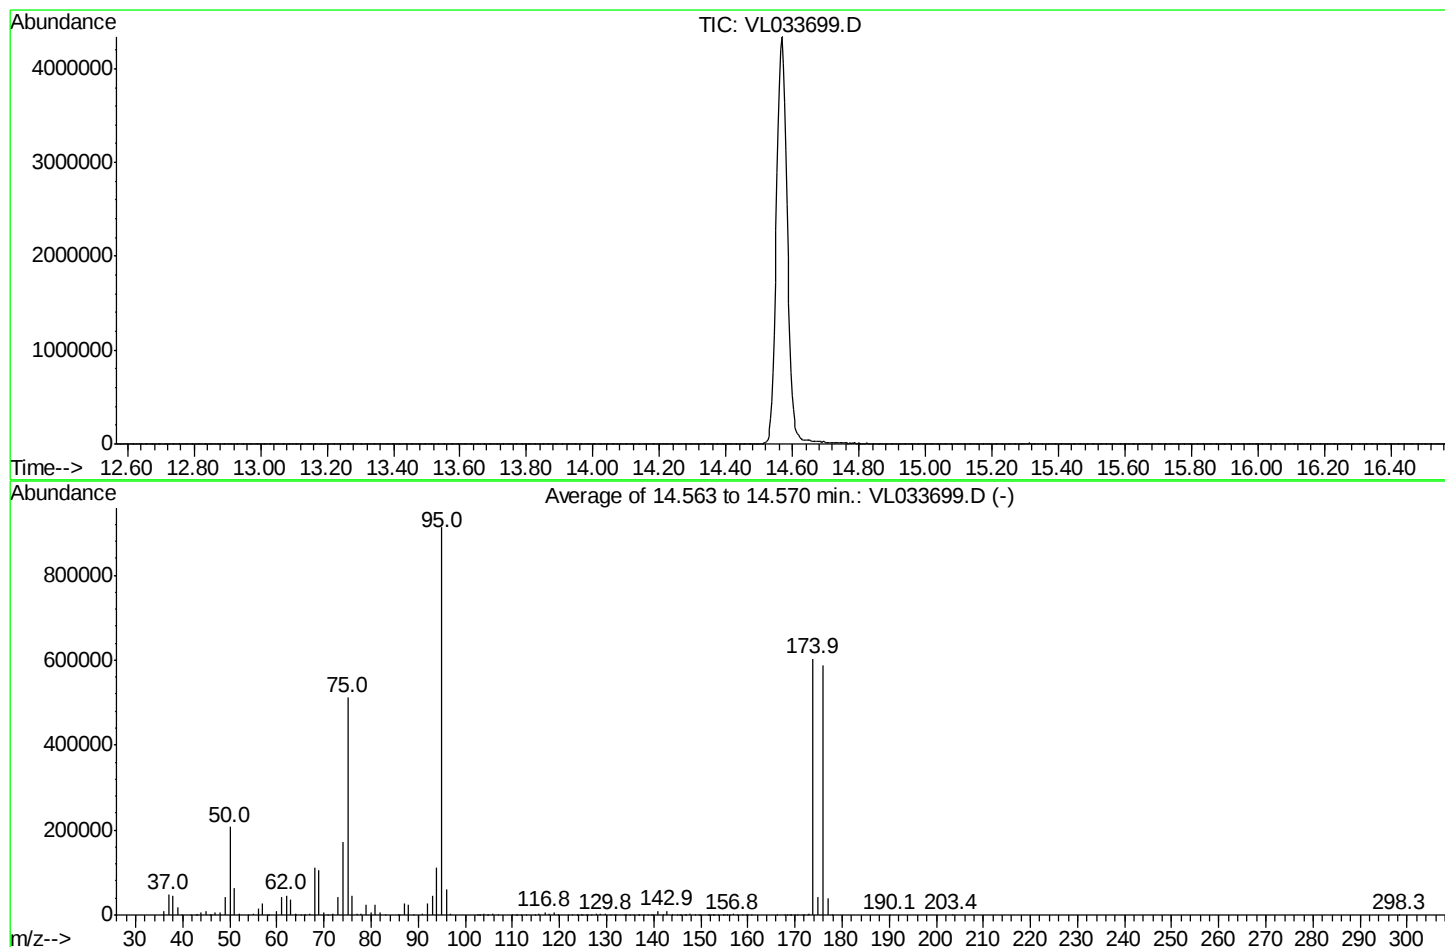

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.7	207338	PASS
75	95	30	66	56.0	511573	PASS
95	95	100	100	100.0	912768	PASS
96	95	5	9	6.5	59365	PASS
173	174	0.00	2	0.6	3769	PASS
174	95	50	120	66.2	603946	PASS
175	174	4	9	7.0	42018	PASS
176	174	93	101	97.3	587541	PASS
177	176	5	9	6.7	39098	PASS