


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL052019\
 Data File : VL033720.D
 Acq On : 20 May 2019 9:36
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL051719AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri May 17 08:15:41 2019
 Last Update : Fri May 17 08:15:41 2019

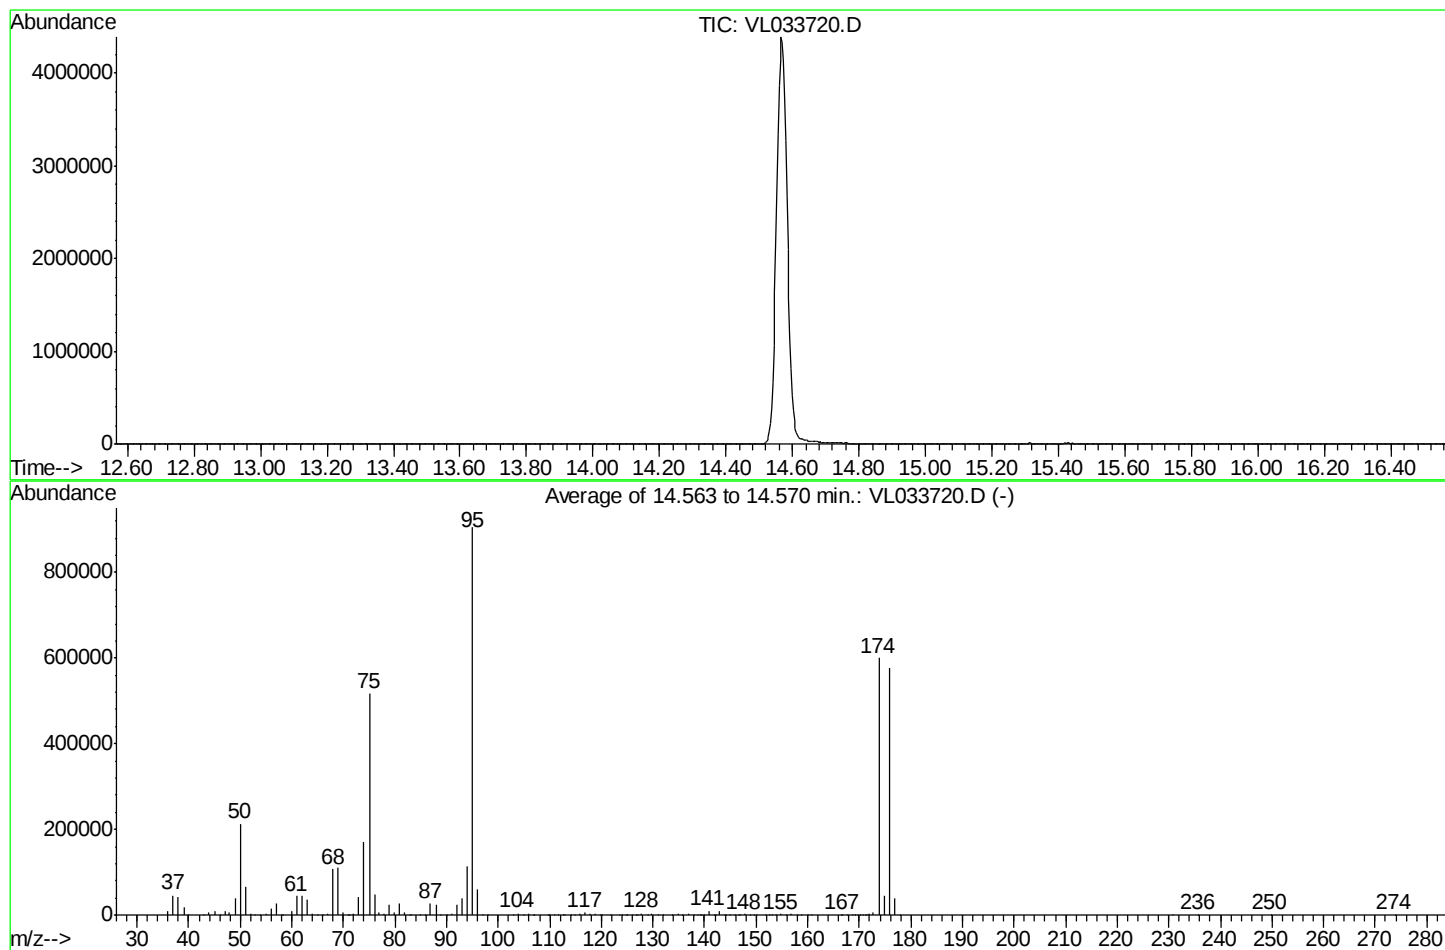

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	213290	PASS
75	95	30	66	57.1	516778	PASS
95	95	100	100	100.0	905429	PASS
96	95	5	9	6.6	59381	PASS
173	174	0.00	2	0.9	5151	PASS
174	95	50	120	66.3	600170	PASS
175	174	4	9	7.5	45130	PASS
176	174	93	101	96.0	575936	PASS
177	176	5	9	6.7	38666	PASS