
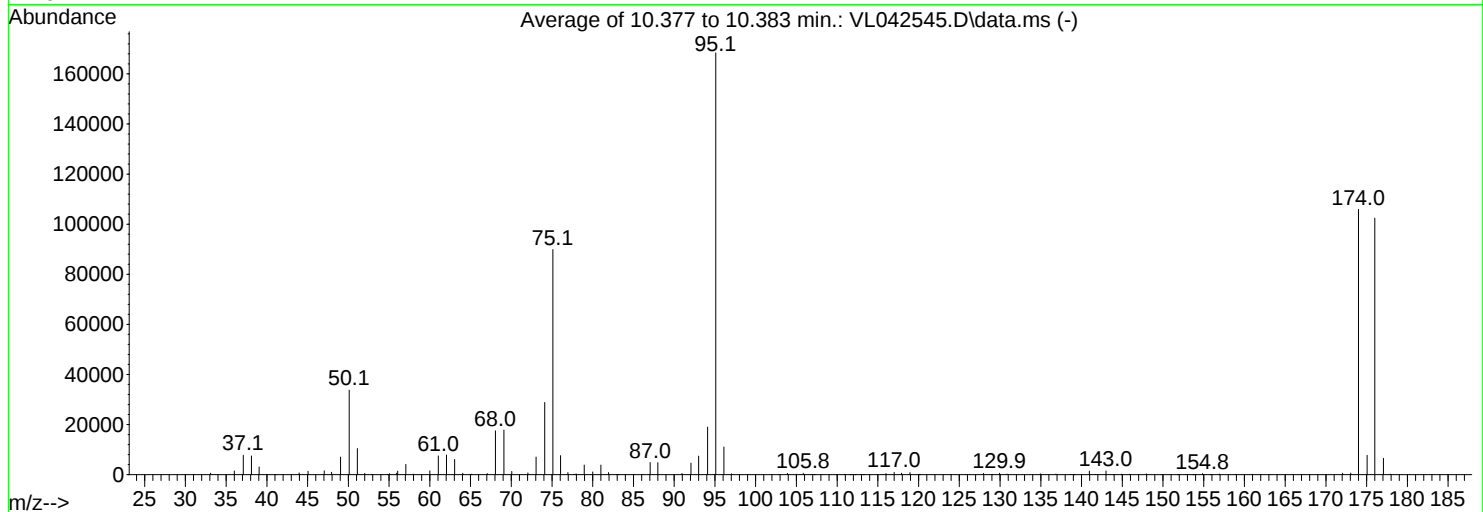


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052025\
Data File : VL042545.D
Acq On : 20 May 2025 08:27
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052025AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed May 21 00:21:29 2025

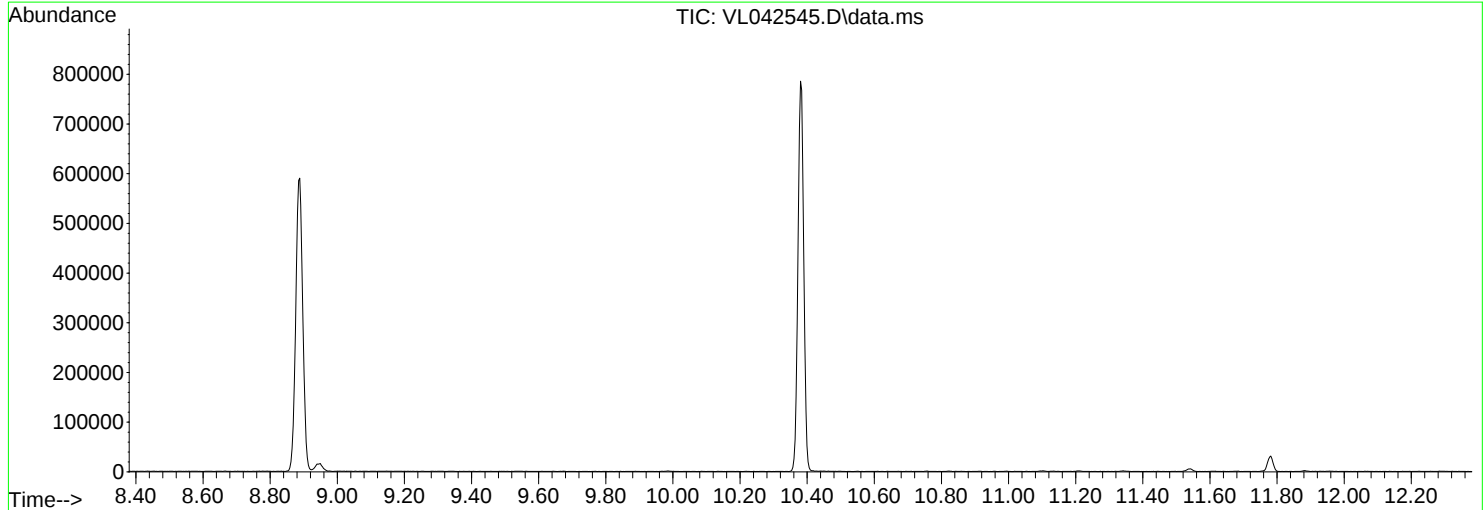

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	20.0	33723	PASS
75	95	30	66	53.4	89875	PASS
95	95	100	100	100.0	168405	PASS
96	95	5	9	6.6	11035	PASS
173	174	0.00	2	0.6	676	PASS
174	95	50	120	62.9	105904	PASS
175	174	4	9	7.3	7712	PASS
176	174	93	101	96.7	102381	PASS
177	176	5	9	6.4	6510	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	581	47.05	1567	57.05	4123	68.05	1753
36.00	1445	47.95	957	58.00	191	69.10	1781
37.10	7758	49.05	7048	60.00	1510	70.05	128
38.10	7454	50.10	33723	61.05	7478	71.00	5
39.05	3087	51.10	10435	62.05	7842	72.05	698
39.95	118	52.00	535	63.05	6050	73.05	7058
41.00	21	52.90	88	64.05	580	74.10	28797
43.05	91	54.80	92	65.00	142	75.10	89875
43.95	722	55.05	378	65.15	215	76.05	7599
45.05	1350	55.90	561	66.00	102	76.95	842
45.95	74	56.05	1421	67.05	447	77.70	120

Average of 10.377 to 10.383 min.: VL042545.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.95	320	92.05	4633	107.20	37	117.90	559
78.95	3808	93.00	7424	109.90	22	118.95	856
80.00	1113	94.10	18987	110.90	128	120.10	19
81.00	3859	95.10	168405	111.60	30	123.95	118
81.95	816	96.10	11035	112.00	55	125.80	49
82.90	53	97.05	358	112.20	33	127.95	494
83.10	23	102.85	54	112.85	87	128.90	92
86.05	64	103.90	490	113.20	22	129.05	162
87.05	4849	105.00	188	114.90	165	129.95	563
88.00	4800	105.85	552	116.00	462	130.85	262
90.95	526	106.80	136	117.00	923	134.95	313

Average of 10.377 to 10.383 min.: VL042545.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
136.85	258	145.90	178	156.90	264		
138.70	53	147.00	127	158.85	166		
139.10	28	147.95	300	160.95	188		
139.95	124	148.95	119	172.05	581		
140.95	1403	149.85	99	173.05	676		
141.75	134	151.80	32	174.00	105904		
142.00	52	152.80	47	175.05	7712		
143.00	1441	153.70	17	176.00	102381		
143.90	19	153.95	98	177.05	6510		
144.10	62	154.85	435	177.90	221		
144.90	198	155.80	37				

Instrument :

MSVOA_L

ClientSampleId :

BFB