

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052125\
 Data File : VL042564.D
 Acq On : 21 May 2025 14:14
 Operator : SY/MD
 Sample : QC051325 CAN 10331
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC051325 CAN 10331

Quant Time: May 21 22:55:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052025AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Wed May 21 00:21:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.794	49	104386	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.969	114	312149	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.888	117	265290	10.000	ppbv	0.00


System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.384	95	214186	10.088	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.900%

Target Compounds					Qvalue	
6) Bromomethane	1.661	94	46	0.012	ppbv #	3
7) Chloroethane	1.706	64	51	0.018	ppbv #	56
10) Heptane	4.580	43	53	0.004	ppbv #	24
14) Bromoethene	1.722	108	21	0.003	ppbv #	1
17) tert-Butyl alcohol	2.049	59	102	0.006	ppbv #	14
18) 1,1-Dichloroethene	1.988	96	56	0.008	ppbv #	1
21) Allyl Chloride	2.101	41	47	0.005	ppbv #	19
22) trans-1,2-Dichloroethene	2.315	96	24	0.003	ppbv #	1
23) Vinyl Acetate	2.473	43	25	0.002	ppbv #	1
24) 1,1-Dichloroethane	2.282	63	40	0.003	ppbv #	86
25) Ethyl Acetate	2.846	43	14	0.000	ppbv #	74
26) Hexane	2.412	57	25	0.002	ppbv #	1
27) Carbon Disulfide	2.156	76	64	0.003	ppbv #	1
29) Chloroform	2.852	83	27	0.001	ppbv	95
34) 2-Butanone	2.570	43	290	0.018	ppbv #	70
36) Benzene	3.674	78	25	0.001	ppbv #	56
41) Tetrahydrofuran	3.153	42	42	0.005	ppbv #	33
42) Bromodichloromethane	4.338	83	21	0.001	ppbv #	25
44) 2,2,4-Trimethylpentane	4.270	57	24	0.001	ppbv #	43
50) 4-Methyl-2-Pentanone	5.759	43	28	0.001	ppbv #	20
53) Toluene	6.946	91	30	0.001	ppbv #	21
57) Chlorobenzene	8.911	112	28	0.001	ppbv #	67
58) Ethyl Benzene	9.542	91	36	0.001	ppbv #	44
59) m/p-Xylene	9.542	91	36	0.001	ppbv #	30
60) o-Xylene	10.384	91	509	0.017	ppbv #	1
62) Isopropylbenzene	10.400	105	23	0.001	ppbv #	50
63) 1,1,2,2-Tetrachloroethane	10.387	83	224	0.011	ppbv #	1
65) tert-Butylbenzene	11.772	119	61	0.002	ppbv #	1
66) Benzyl Chloride	11.552	91	32	0.006	ppbv #	65
67) sec-Butylbenzene	11.879	105	49	0.001	ppbv #	1
69) p-Isopropyltoluene	11.785	119	126	0.003	ppbv #	48
72) 4-Ethyltoluene	11.131	105	66	0.002	ppbv #	56
73) 1,3,5-Trimethylbenzene	11.209	105	94	0.003	ppbv #	31
74) 1,2,4-Trimethylbenzene	11.539	105	247	0.007	ppbv #	48

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: May 21 22:55:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052025AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 26 06:05:16 2022
QLast Update : Wed May 21 00:21:29 2025
Response via : Initial Calibration









#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.794 min Scan# 81
Delta R.T. 0.004 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14




Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331


Tgt Ion: 49 Resp: 104386
Ion Ratio Lower Upper
49 100
128 54.2 28.6 85.8
130 69.7 36.6 109.8

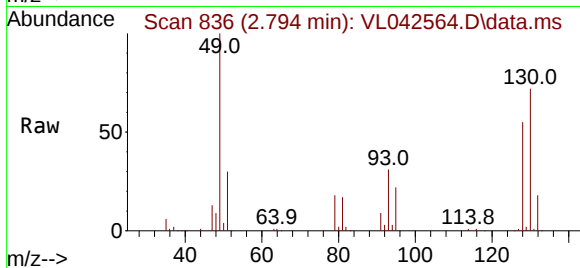

#6
Bromomethane
Concen: 0.012 ppbv
RT: 1.661 min Scan# 486
Delta R.T. -0.010 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Tgt Ion: 94 Resp: 46
Ion Ratio Lower Upper
94 100
96 0.0 74.9 112.3#


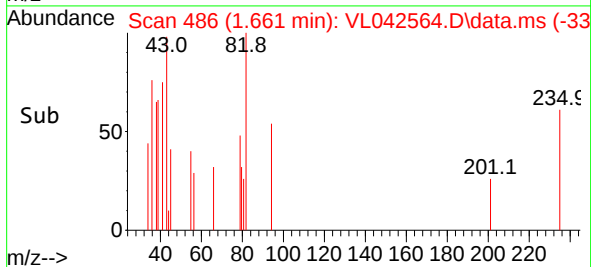

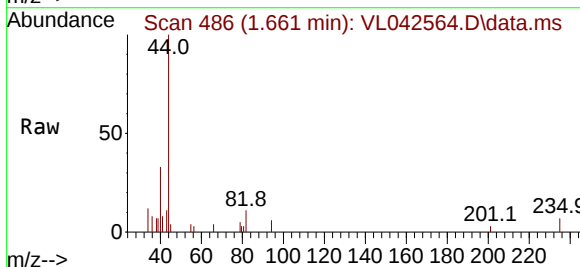




#7
Chloroethane
Concen: 0.018 ppbv
RT: 1.706 min Scan# 50
Delta R.T. 0.000 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14




Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331


Tgt Ion: 64 Resp: 51
Ion Ratio Lower Upper
64 100
66 54.3 24.4 36.6#

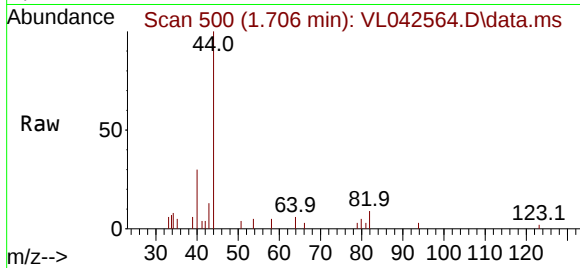

#10
Heptane
Concen: 0.004 ppbv
RT: 4.580 min Scan# 1388
Delta R.T. -0.408 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Tgt Ion: 43 Resp: 53
Ion Ratio Lower Upper
43 100
57 0.0 43.4 65.0#


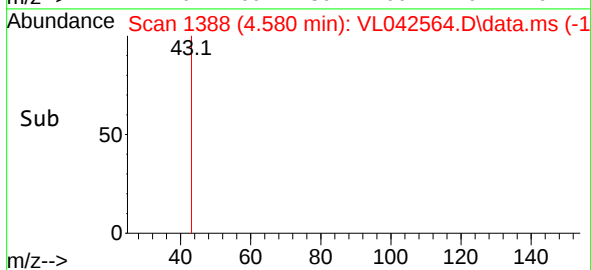

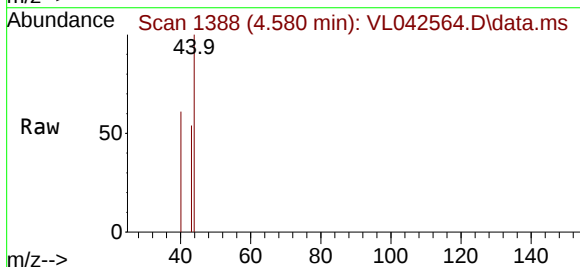




#14
Bromoethene
Concen: 0.003 ppbv
RT: 1.722 min Scan# 50
Delta R.T. -0.061 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14




Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331


Tgt Ion:108 Resp: 21
Ion Ratio Lower Upper
108 100
106 0.0 86.4 129.6#
79 661.9 11.9 17.9#



#17
tert-Butyl alcohol
Concen: 0.006 ppbv
RT: 2.049 min Scan# 606
Delta R.T. 0.007 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Tgt Ion: 59 Resp: 102
Ion Ratio Lower Upper
59 100
57 42.2 8.2 12.2#

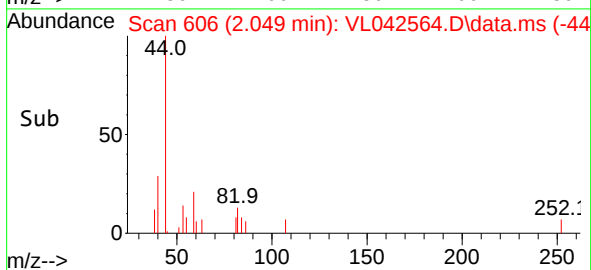



#18

1,1-Dichloroethene

Concen: 0.008 ppbv

RT: 1.988 min Scan# 51

Delta R.T. -0.048 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14

Instrument :

MSVOA_L

ClientSampleId :

QC051325 CAN 10331





Tgt Ion: 96 Resp: 56

Ion Ratio Lower Upper

96 100

61 0.0 137.5 206.3#

98 0.0 53.2 79.8#

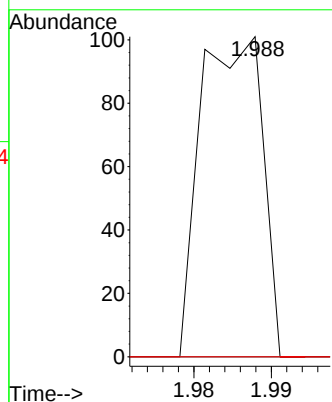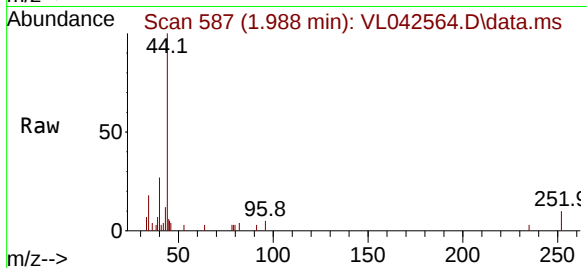

#21

Allyl Chloride

Concen: 0.005 ppbv

RT: 2.101 min Scan# 622

Delta R.T. 0.003 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14




Tgt Ion: 41 Resp: 47


Ion Ratio Lower Upper

41 100

76 0.0 30.2 45.4#

39 0.0 62.5 93.7#




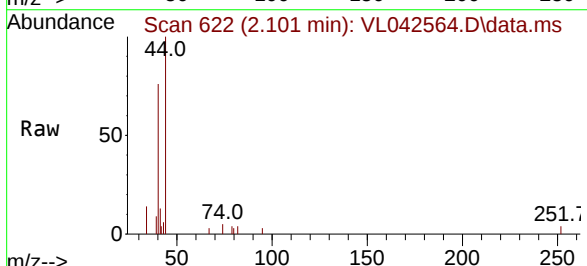




#22
trans-1,2-Dichloroethene
Concen: 0.003 ppbv
RT: 2.315 min Scan# 61
Delta R.T. -0.029 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14




Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331


Tgt Ion: 96 Resp: 24
Ion Ratio Lower Upper
96 100
61 0.0 112.5 168.7#
98 0.0 49.0 73.4#

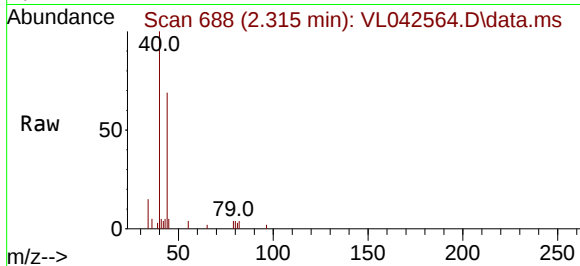

#23
Vinyl Acetate
Concen: 0.002 ppbv
RT: 2.473 min Scan# 737
Delta R.T. 0.007 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Tgt Ion: 43 Resp: 25
Ion Ratio Lower Upper
43 100
86 0.0 7.0 10.6#
42 100.0 7.4 11.2#
44 0.0 4.8 7.2#


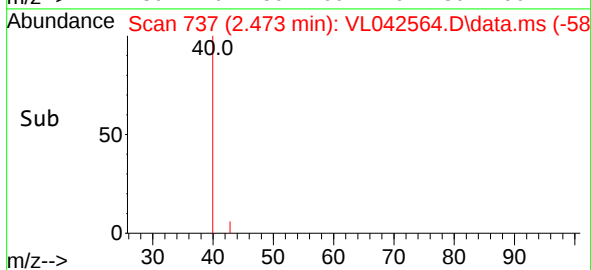

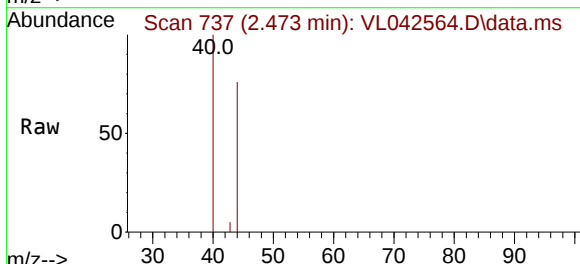




#24
1,1-Dichloroethane
Concen: 0.003 ppbv
RT: 2.282 min Scan# 61
Delta R.T. -0.129 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14




Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331


Tgt Ion: 63 Resp: 40
Ion Ratio Lower Upper
63 100
98 0.0 2.6 7.8#
100 0.0 1.8 5.3#

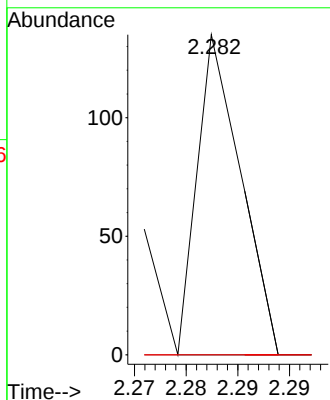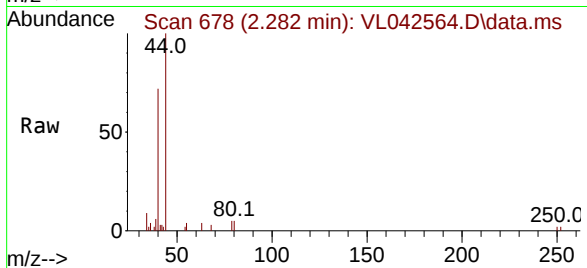

#25
Ethyl Acetate
Concen: 0.000 ppbv
RT: 2.846 min Scan# 852
Delta R.T. 0.007 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Tgt Ion: 43 Resp: 14
Ion Ratio Lower Upper
43 100
45 0.0 8.0 12.0#
61 0.0 7.5 11.3#
70 0.0 7.2 10.8#

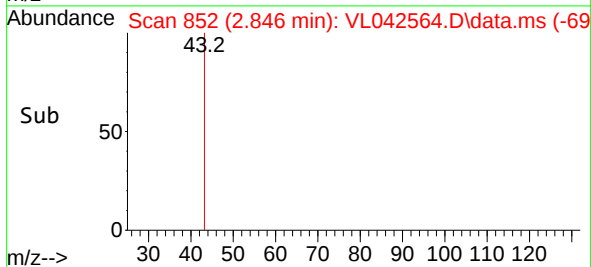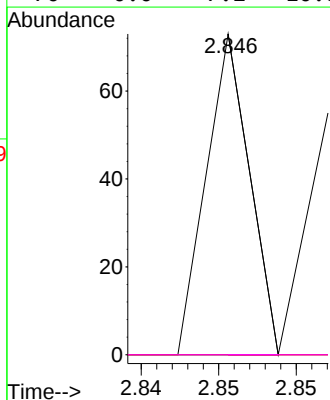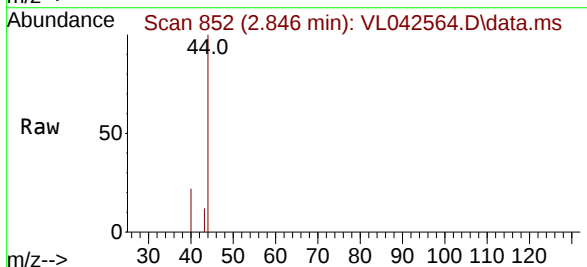



#26

Hexane

Concen: 0.002 ppbv

RT: 2.412 min Scan# 718

Delta R.T. -0.417 min

Lab File: VL042564.D


Acq: 21 May 2025 14:14

Instrument :




MSVOA_L

ClientSampleId :

QC051325 CAN 10331

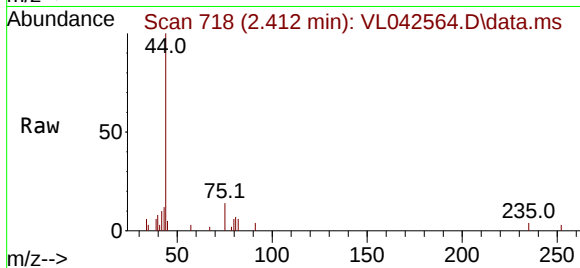

Tgt Ion:	57	Resp:	25
Ion	Ratio	Lower	Upper
57	100		
41	764.0	69.0	103.4#
43	1880.0	174.2	261.2#
56	356.0	44.1	66.1#

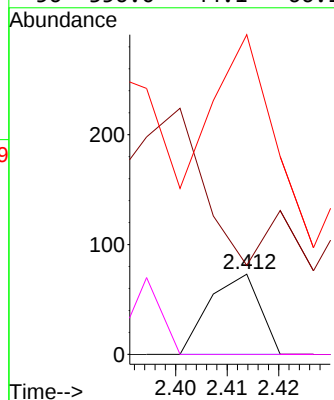

#27

Carbon Disulfide

Concen: 0.003 ppbv




RT: 2.156 min Scan# 639


Delta R.T. 0.003 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14

Tgt Ion:	76	Resp:	64
Ion	Ratio	Lower	Upper
76	100		
44	7781.3	14.0	21.0#
78	0.0	9.4	14.0#

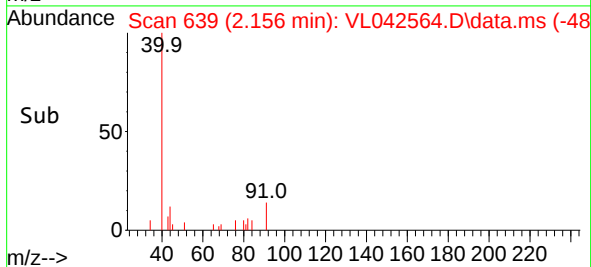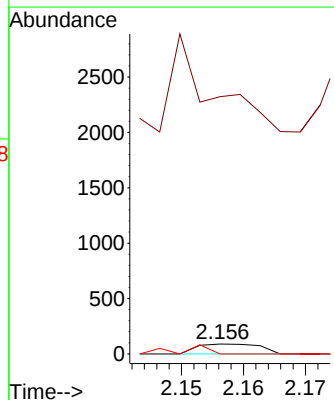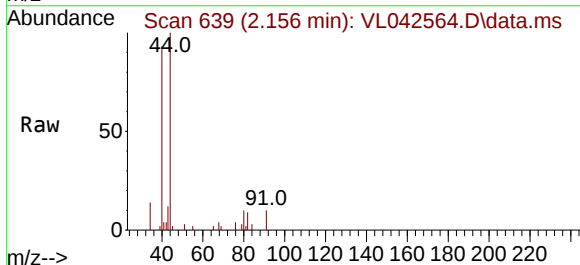



#29

Chloroform

Concen: 0.001 ppbv

RT: 2.852 min Scan# 854

Delta R.T. 0.000 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14

Instrument :

MSVOA_L

ClientSampleId :





QC051325 CAN 10331

Tgt Ion: 83 Resp: 27

Ion Ratio Lower Upper

83 100

85 68.3 51.6 77.4

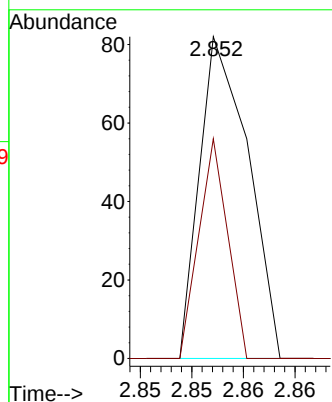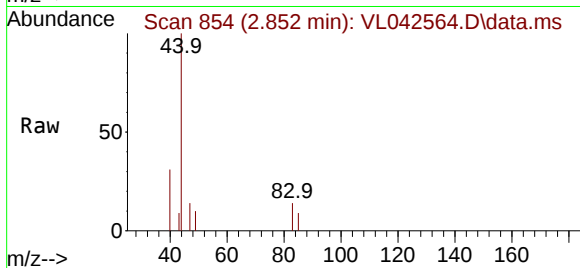

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 3.969 min Scan# 1199

Delta R.T. 0.003 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14




Tgt Ion: 114 Resp: 312149


Ion Ratio Lower Upper

114 100

63 23.9 18.4 27.6

88 17.2 14.0 21.0


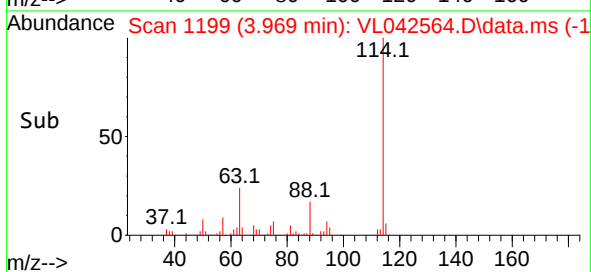
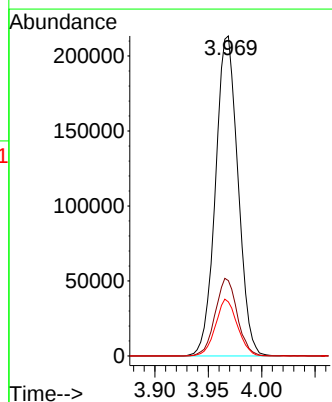
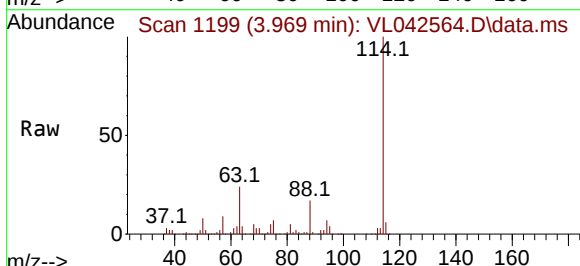




#34
2-Butanone
Concen: 0.018 ppbv
RT: 2.570 min Scan# 764
Delta R.T. 0.010 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14




Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331


Tgt Ion: 43 Resp: 290
Ion Ratio Lower Upper
43 100
72 10.3 20.5 30.7#



#36
Benzene
Concen: 0.001 ppbv
RT: 3.674 min Scan# 1108
Delta R.T. 0.013 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Tgt Ion: 78 Resp: 25
Ion Ratio Lower Upper
78 100
77 0.0 17.8 26.6#
50 0.0 14.0 21.0#


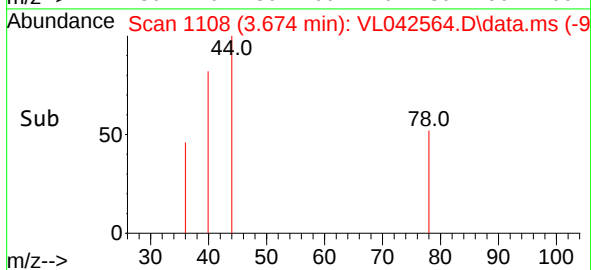






#41
Tetrahydrofuran
Concen: 0.005 ppbv
RT: 3.153 min Scan# 941
Delta R.T. 0.097 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14




Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331


Tgt Ion: 42 Resp: 42
Ion Ratio Lower Upper
42 100
72 0.0 34.8 52.2#
71 0.0 33.6 50.4#



#42
Bromodichloromethane
Concen: 0.001 ppbv
RT: 4.338 min Scan# 1313
Delta R.T. -0.158 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Tgt Ion: 83 Resp: 21
Ion Ratio Lower Upper
83 100
85 0.0 50.4 75.6#
127 0.0 6.5 9.7#


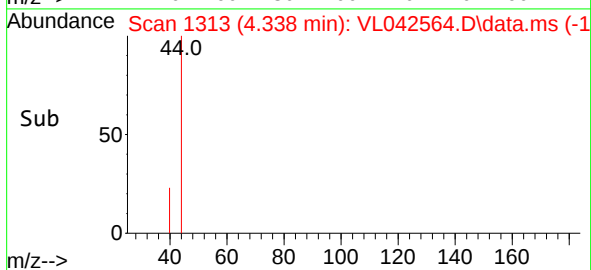






#44
2,2,4-Trimethylpentane
Concen: 0.001 ppbv
RT: 4.270 min Scan# 11
Delta R.T. -0.375 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14




Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331


Tgt Ion: 57 Resp: 24
Ion Ratio Lower Upper
57 100
41 0.0 25.0 37.4#
56 0.0 25.1 37.7#

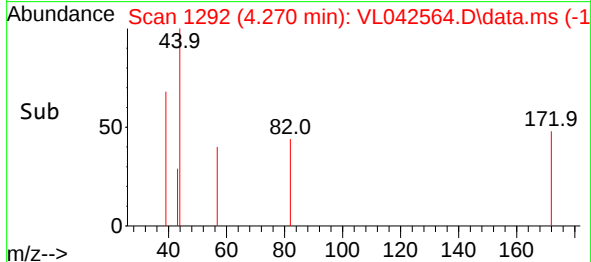

#50
4-Methyl-2-Pentanone
Concen: 0.001 ppbv
RT: 5.759 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Tgt Ion: 43 Resp: 28
Ion Ratio Lower Upper
43 100
58 85.7 30.0 45.0#

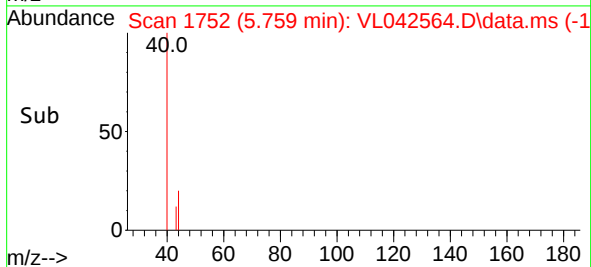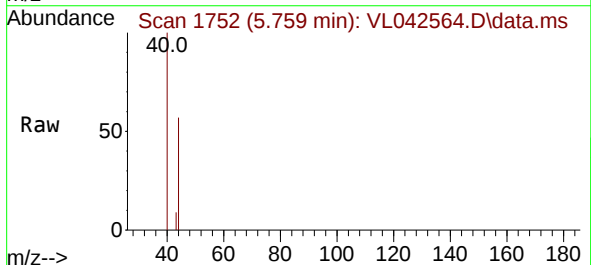



#53

Toluene

Concen: 0.001 ppbv

RT: 6.946 min Scan# 2118

Delta R.T. 0.003 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14

Instrument :

MSVOA_L

ClientSampleId :





QC051325 CAN 10331

Tgt Ion: 91 Resp: 30

Ion Ratio Lower Upper

91 100

92 0.0 47.8 71.8#

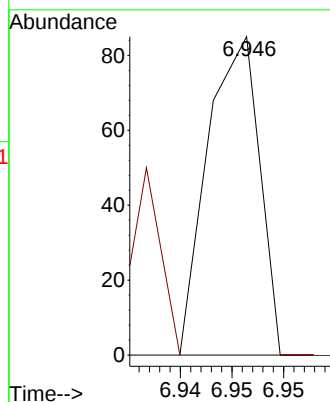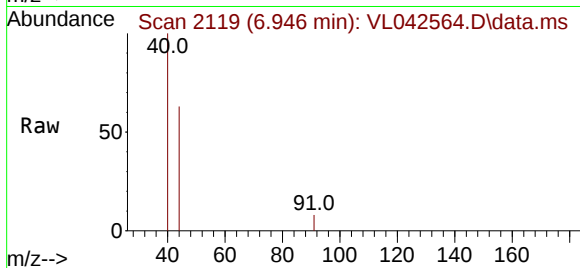

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 8.888 min Scan# 2719

Delta R.T. 0.000 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14




Tgt Ion: 117 Resp: 265290


Ion Ratio Lower Upper

117 100

82 63.3 51.0 76.4

119 32.3 27.0 40.4

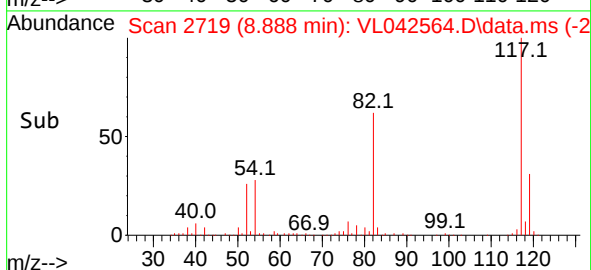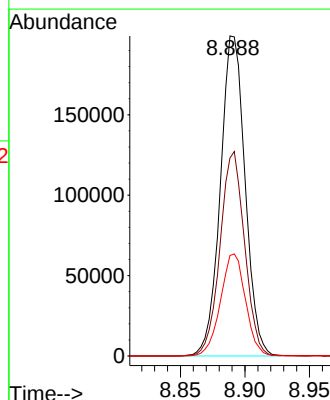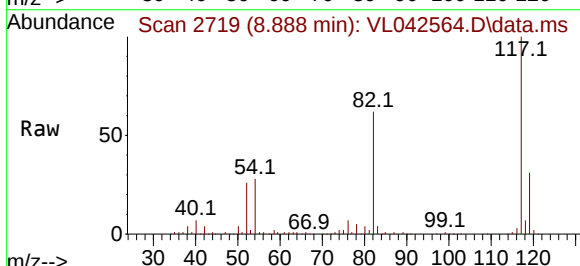



#57

Chlorobenzene

Concen: 0.001 ppbv

RT: 8.911 min Scan# 21

Delta R.T. -0.016 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14





Instrument :

MSVOA_L

ClientSampleId :

QC051325 CAN 10331

Tgt Ion:112	Resp:	28
Ion	Ratio	Lower Upper
112	100	
77	83.5	53.2 79.8#
114	0.0	28.4 34.8#

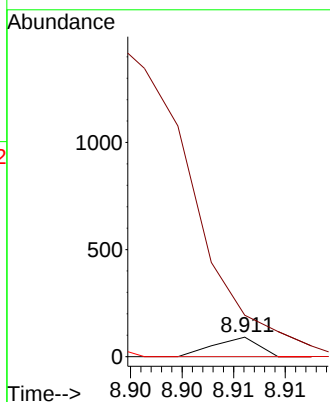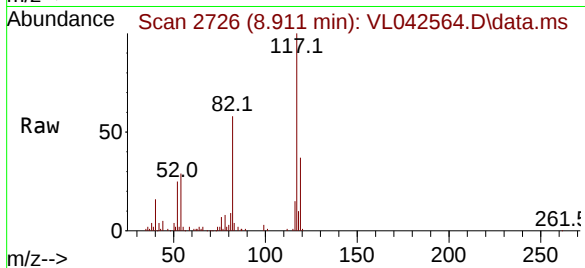

#58

Ethyl Benzene

Concen: 0.001 ppbv




RT: 9.542 min Scan# 2921


Delta R.T. 0.181 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14

Tgt Ion: 91	Resp:	36
Ion	Ratio	Lower Upper
91	100	
106	0.0	24.6 37.0#

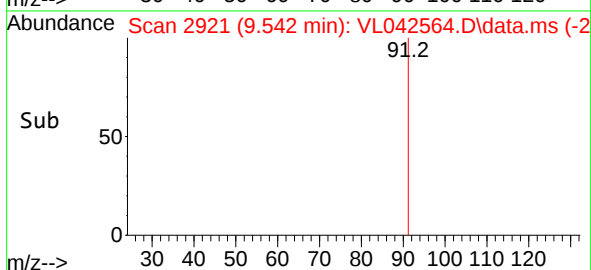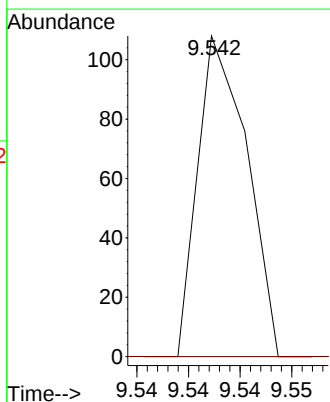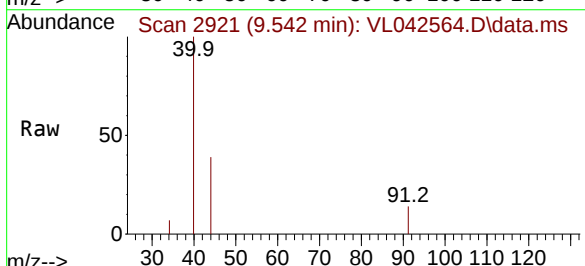



#59

m/p-Xylene

Concen: 0.001 ppbv

RT: 9.542 min Scan# 29

Delta R.T. -0.016 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14

Instrument :

MSVOA_L

ClientSampleId :





QC051325 CAN 10331

Tgt Ion: 91 Resp: 36

Ion Ratio Lower Upper

91 100

106 0.0 37.1 55.7#

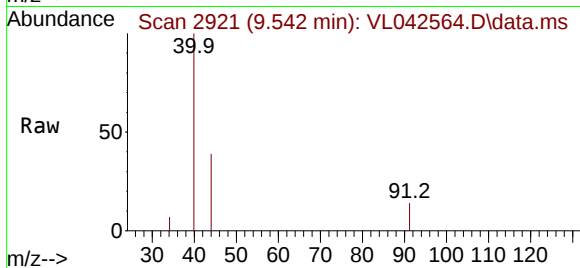

#60

o-Xylene

Concen: 0.017 ppbv

RT: 10.384 min Scan# 3181

Delta R.T. 0.414 min

Lab File: VL042564.D




Acq: 21 May 2025 14:14


Tgt Ion: 91 Resp: 509

Ion Ratio Lower Upper

91 100

106 199.0 21.6 64.8#


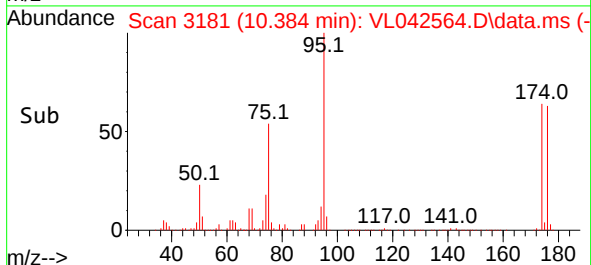
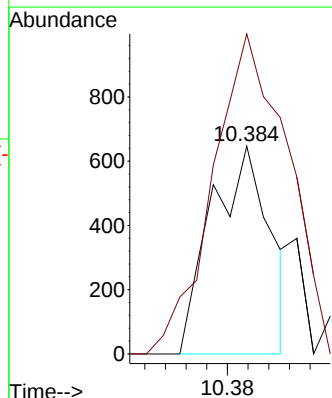
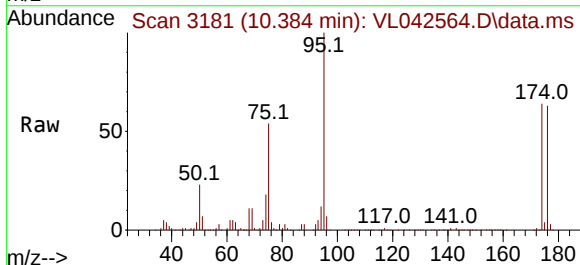




#62
Isopropylbenzene
Concen: 0.001 ppbv
RT: 10.400 min Scan# 3186
Delta R.T. -0.145 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14




Instrument :
MSVOA_1
ClientSampleId :
QC051325 CAN 10331


Tgt Ion:105 Resp: 23
Ion Ratio Lower Upper
105 100
120 0.0 20.0 30.0#

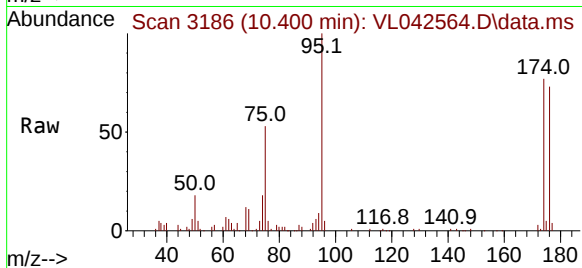

#63
1,1,2,2-Tetrachloroethane
Concen: 0.011 ppbv
RT: 10.387 min Scan# 3182
Delta R.T. 0.418 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14


Tgt Ion: 83 Resp: 224
Ion Ratio Lower Upper
83 100
131 147.8 5.1 15.3#
85 0.0 32.5 97.4#

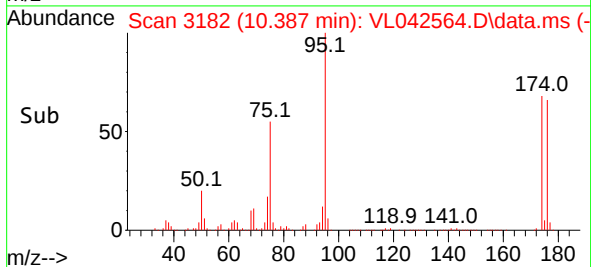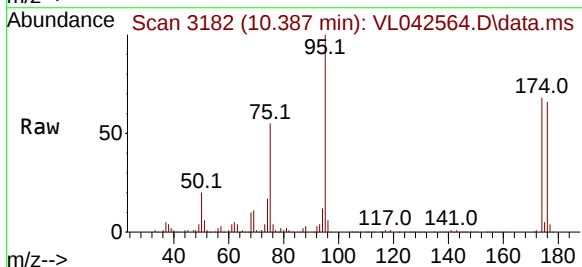






#65
tert-Butylbenzene
Concen: 0.002 ppbv
RT: 11.772 min Scan# 30
Delta R.T. 0.236 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14


Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331

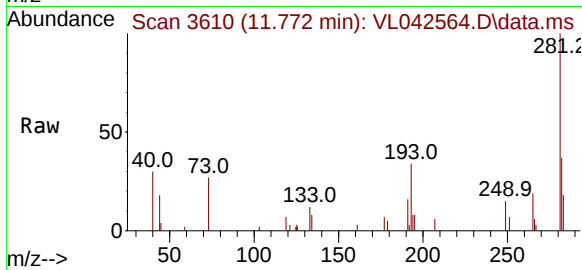



Tgt Ion:119 Resp: 61
Ion Ratio Lower Upper
119 100
91 0.0 62.7 94.1#
134 182.0 16.8 25.2#




#66
Benzyl Chloride
Concen: 0.006 ppbv
RT: 11.552 min Scan# 3542
Delta R.T. -0.068 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

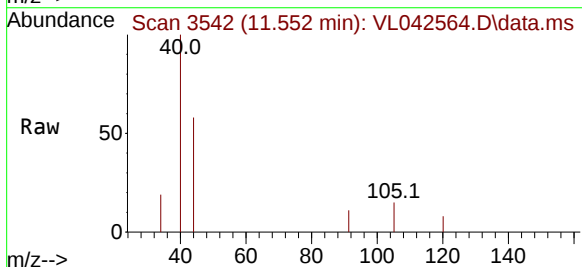

Tgt Ion: 91 Resp: 32
Ion Ratio Lower Upper
91 100
126 0.0 14.2 21.2#
128 0.0 4.6 6.8#

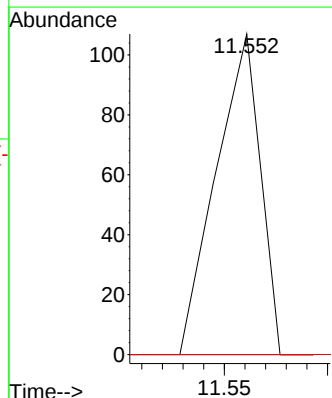

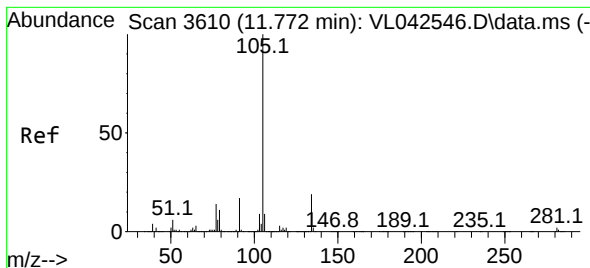

#67

sec-Butylbenzene

Concen: 0.001 ppbv

RT: 11.879 min Scan# 3610

Delta R.T. 0.107 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14

Instrument :

MSVOA_L

ClientSampleId :





QC051325 CAN 10331

Tgt Ion:105 Resp: 49

Ion Ratio Lower Upper

105 100

134 226.5 15.4 23.2#

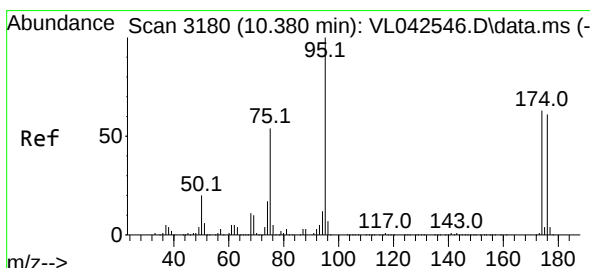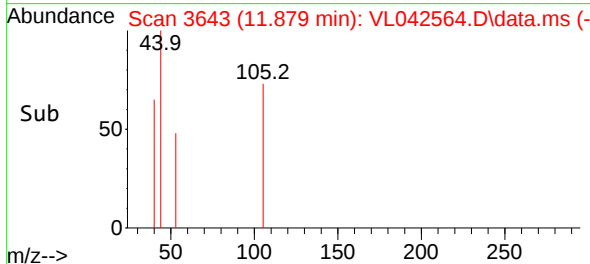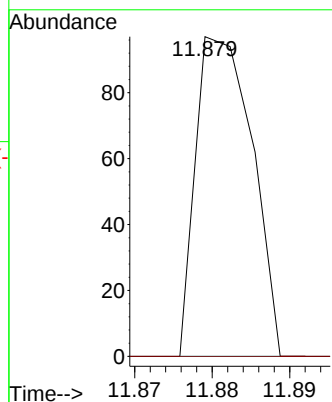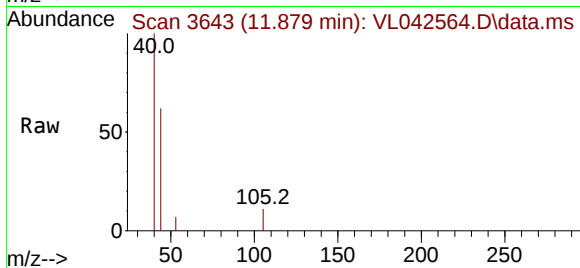

#68

1-Bromo-4-Fluorobenzene

Concen: 10.088 ppbv

RT: 10.384 min Scan# 3181

Delta R.T. 0.003 min

Lab File: VL042564.D

Acq: 21 May 2025 14:14




Tgt Ion: 95 Resp: 214186


Ion Ratio Lower Upper

95 100

174 65.0 52.0 78.0


175 4.5 3.8 5.6

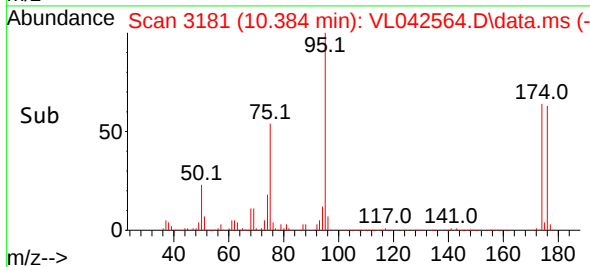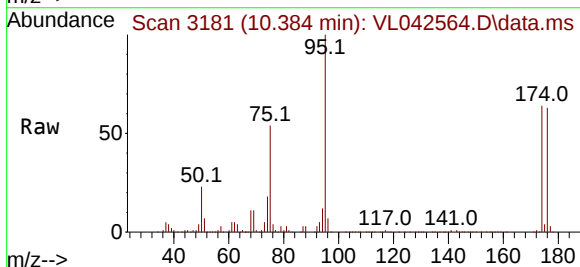






#69
p-Isopropyltoluene
Concen: 0.003 ppbv
RT: 11.785 min Scan# 3614
Delta R.T. -0.145 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331



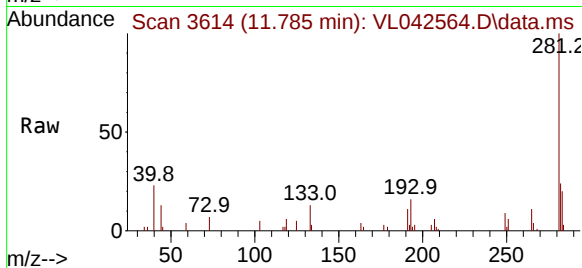



Tgt Ion:119 Resp: 126
Ion Ratio Lower Upper
119 100
134 0.0 20.1 30.1#
91 0.0 22.3 33.5#



#72
4-Ethyltoluene
Concen: 0.002 ppbv
RT: 11.131 min Scan# 3412
Delta R.T. 0.000 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Tgt Ion:105 Resp: 66
Ion Ratio Lower Upper
105 100
120 0.0 23.4 35.0#
91 0.0 10.2 15.4#
77 0.0 10.4 15.6#


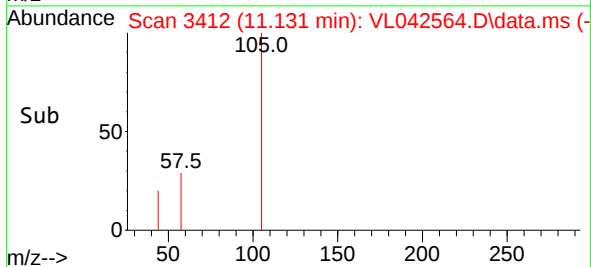

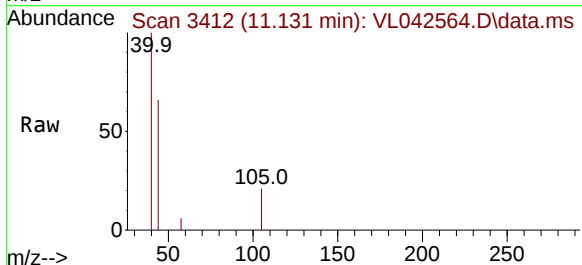




#73
1,3,5-Trimethylbenzene
Concen: 0.003 ppbv
RT: 11.209 min Scan# 3436
Delta R.T. 0.000 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Instrument :
MSVOA_L
ClientSampleId :
QC051325 CAN 10331

Tgt Ion:105 Resp: 94
Ion Ratio Lower Upper
105 100
120 0.0 36.5 54.7#

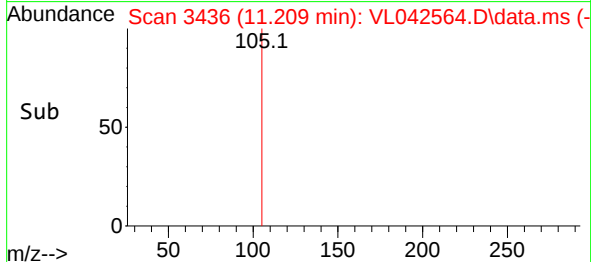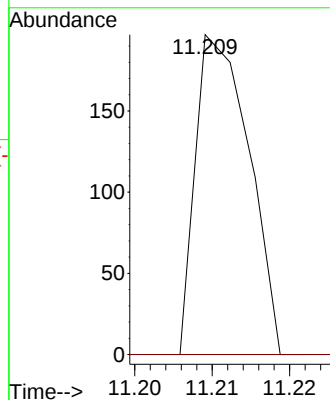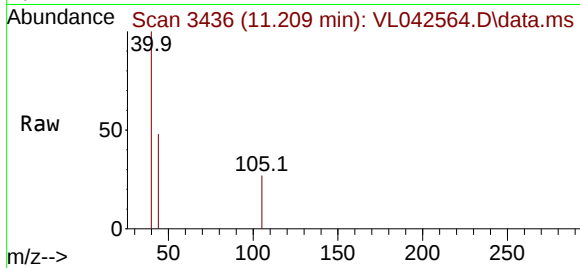

#74
1,2,4-Trimethylbenzene
Concen: 0.007 ppbv
RT: 11.539 min Scan# 3538
Delta R.T. -0.003 min
Lab File: VL042564.D
Acq: 21 May 2025 14:14

Tgt Ion:105 Resp: 247
Ion Ratio Lower Upper
105 100
120 68.6 39.4 59.0#
91 0.0 47.8 71.8#
77 37.0 17.8 26.6#

