
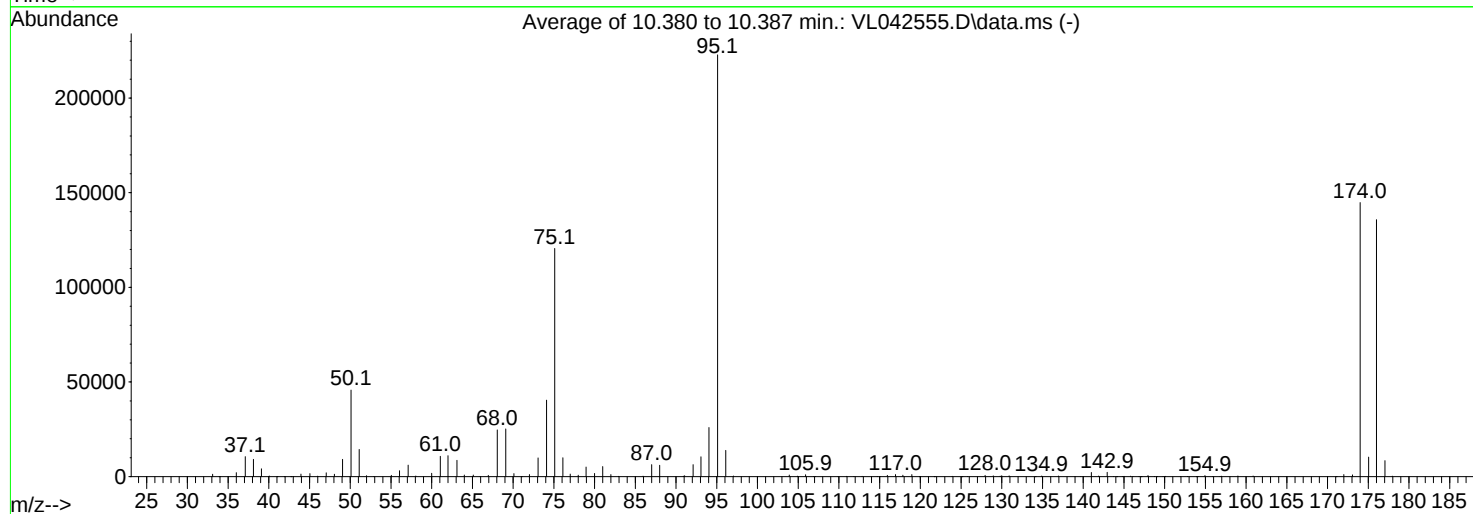


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052125\
Data File : VL042555.D
Acq On : 21 May 2025 07:53
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052025AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed May 21 00:21:29 2025

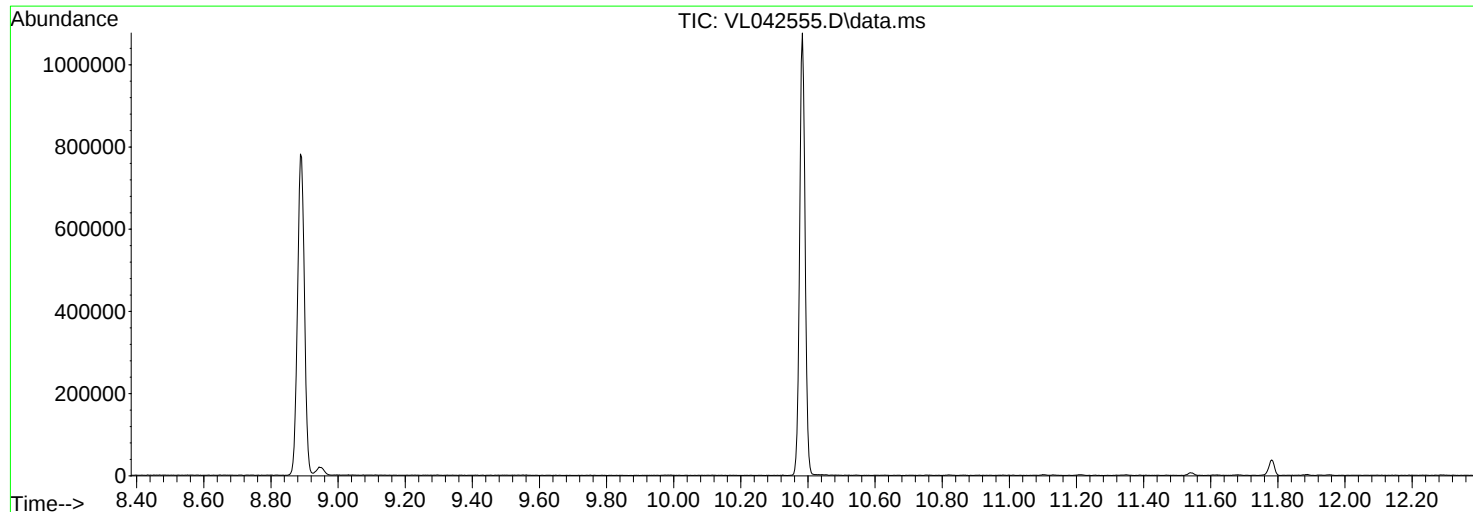

AutoFind: Scans 3180, 3181, 3182; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.5	45723	PASS
75	95	30	66	54.1	120509	PASS
95	95	100	100	100.0	222827	PASS
96	95	5	9	6.2	13845	PASS
173	174	0.00	2	0.7	967	PASS
174	95	50	120	65.0	144832	PASS
175	174	4	9	7.1	10294	PASS
176	174	93	101	93.7	135715	PASS
177	176	5	9	6.2	8472	PASS

Average of 10.380 to 10.387 min.: VL042555.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1249	43.95	1344	56.05	3174	68.05	2472
33.90	18	45.05	1596	57.10	6064	69.10	2515
36.00	2084	46.00	216	58.05	349	70.10	165
37.10	10609	47.05	1998	60.00	1744	71.00	1
38.10	9117	48.05	1240	61.05	10741	72.00	1080
39.10	4119	49.05	9155	62.00	11041	73.05	9921
40.05	322	50.10	45723	63.10	8655	74.10	40419
41.00	39	51.10	14339	64.00	869	75.10	120509
41.90	27	52.00	502	65.10	865	76.10	9991
42.70	26	52.90	94	65.95	85	77.00	1333
43.00	56	55.05	700	66.95	665	78.00	737

Average of 10.380 to 10.387 min.: VL042555.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	5087	93.05	10487	110.95	164	123.90	142
80.00	1681	94.05	25971	111.85	48	125.10	26
81.00	5310	95.10	222827	112.85	148	125.80	90
82.00	1072	96.10	13845	114.70	87	127.95	714
82.95	212	97.05	382	115.05	116	128.95	413
85.95	268	103.90	834	115.95	685	129.80	256
87.00	6332	104.90	272	116.95	1088	130.00	519
88.00	6002	105.90	1002	117.85	741	130.90	417
90.90	248	106.90	97	118.95	1088	134.10	17
91.05	543	107.10	71	119.90	24	134.90	375
92.10	6383	109.90	64	121.70	17	136.95	343

Average of 10.380 to 10.387 min.: VL042555.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
139.00	83	146.10	74	154.10	108	175.05	10294
139.70	50	146.85	117	154.95	627	176.00	135715
140.00	126	147.10	31	155.90	84	177.05	8472
141.00	2214	147.95	569	156.80	109	177.95	245
141.90	342	148.75	91	156.95	287		
142.95	2249	149.00	23	159.00	329		
143.75	96	149.80	65	160.85	309		
144.10	28	150.10	182	171.05	46		
144.80	96	151.95	107	172.00	1098		
145.00	158	152.80	131	173.05	967		
145.80	252	153.90	34	174.00	144832		