


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL052220\
 Data File : VL035077.D
 Acq On : 22 May 2020 9:08
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050620AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed May 06 14:49:39 2020
 Last Update : Wed May 06 14:49:39 2020

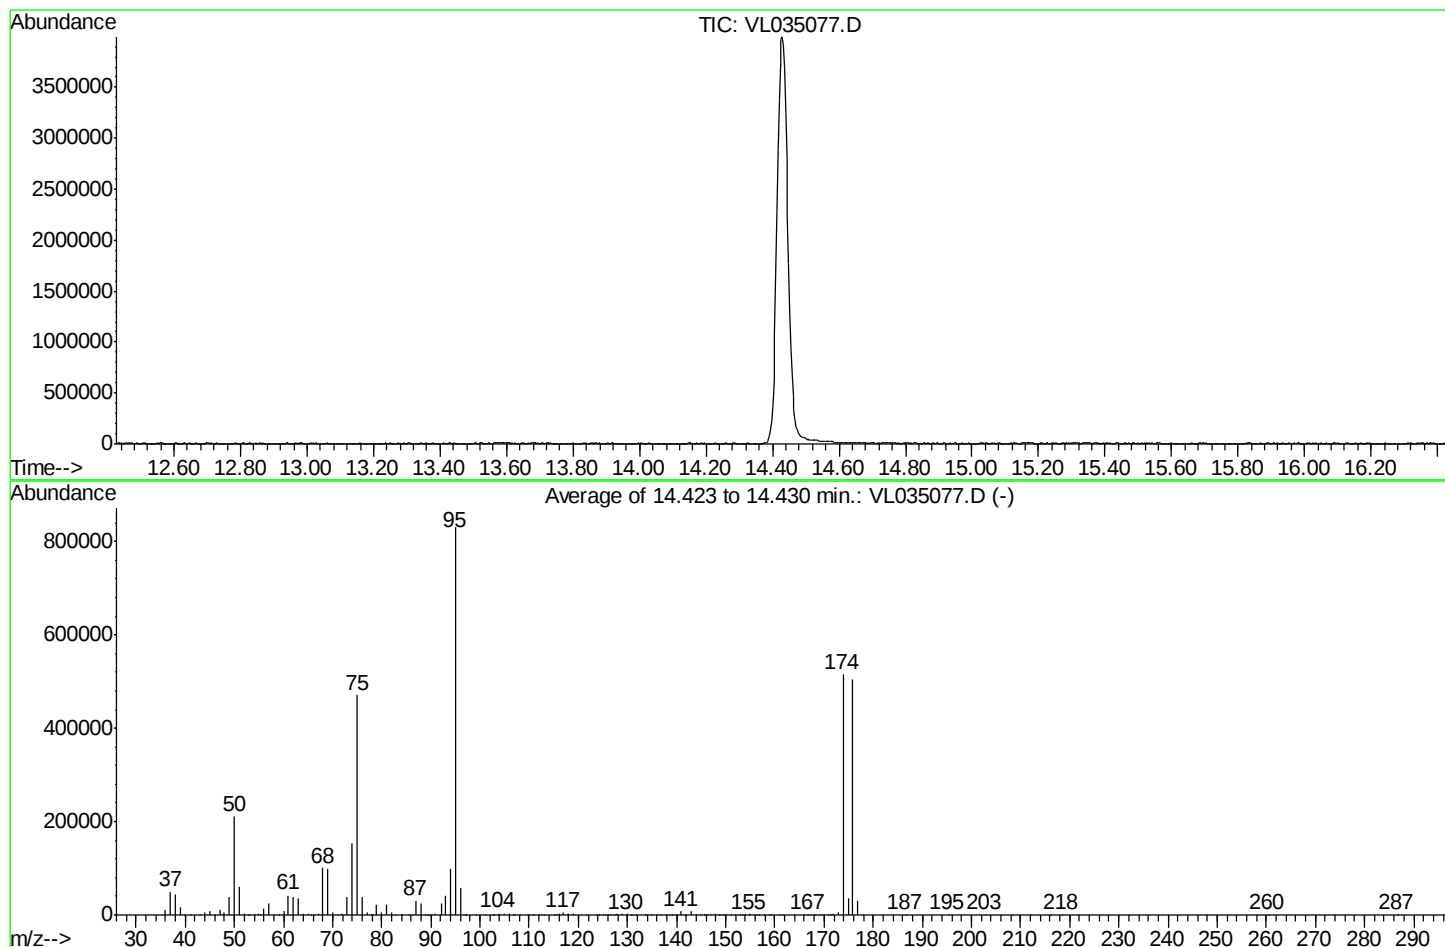

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.4	210901	PASS
75	95	30	66	56.8	471210	PASS
95	95	100	100	100.0	830250	PASS
96	95	5	9	7.1	58608	PASS
173	174	0.00	2	0.9	4631	PASS
174	95	50	120	62.0	514922	PASS
175	174	4	9	7.2	37101	PASS
176	174	93	101	98.2	505450	PASS
177	176	5	9	6.0	30416	PASS