

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052424\
 Data File : VL041286.D
 Acq On : 24 May 2024 11:42
 Operator : SY/MD
 Sample : P2599-01DUP 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Quant Time: May 24 23:19:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri May 24 23:11:50 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1)	Bromochloromethane	5.205	49	1057626	10.000	ppbv	0.00
33)	1,4-Difluorobenzene	6.661	114	2697279	10.000	ppbv	0.00
55)	Chlorobenzene-d5	11.471	117	2504616	10.000	ppbv	0.00
System Monitoring Compounds							
68)	1-Bromo-4-Fluorobenzene	13.783	95	1977567	10.459	ppbv	0.00
Spiked Amount 10.000		Range	65 - 135	Recovery	= 104.600%		
Target Compounds							Qvalue
2)	Dichlorodifluoromethane	2.751	85	18282	0.128	ppbv	# 61
3)	Chlorodifluoromethane	2.697	51	40875	0.254	ppbv	# 95
4)	Chloromethane	2.832	50	3847	0.061	ppbv	# 97
9)	Propene	2.716	41	221745	3.527	ppbv	# 94
10)	Heptane	7.587	43	61963	0.407	ppbv	# 88
11)	Trichlorofluoromethane	3.581	101	3688889	25.371	ppbv	# 96
13)	Ethanol	3.262	45	49502	3.513	ppbv	# 77
15)	Acetone	3.481	43	2236352	17.917	ppbv	# 91
16)	1,3-Butadiene	2.989	39	234530	3.722	ppbv	# 21
17)	tert-Butyl alcohol	3.902	59	29355	0.218	ppbv	# 72
19)	Isopropyl Alcohol	3.603	45	16582	0.202	ppbv	# 41
20)	Methylene Chloride	3.947	84	116237	2.678	ppbv	# 96
23)	Vinyl Acetate	4.626	43	49537	0.360	ppbv	# 11
25)	Ethyl Acetate	5.224	43	243842	0.979	ppbv	# 77
26)	Hexane	5.227	57	342455	3.080	ppbv	# 40
27)	Carbon Disulfide	4.140	76	171685	1.305	ppbv	# 94
29)	Chloroform	5.285	83	27982	0.182	ppbv	# 81
30)	Cyclohexane	6.606	84	18701	0.212	ppbv	# 1
34)	2-Butanone	4.796	43	2473069	18.014	ppbv	# 100
36)	Benzene	6.385	78	58487	0.258	ppbv	# 88
39)	1,2-Dichloropropane	6.664	63	690473	7.915	ppbv	# 24
44)	2,2,4-Trimethylpentane	7.333	57	125486	0.322	ppbv	# 55
51)	2-Hexanone	9.564	43	235836	1.290	ppbv	# 98
52)	Tetrachloroethene	10.626	164	360226	4.528	ppbv	# 98
53)	Toluene	9.230	91	318315	1.213	ppbv	# 99
58)	Ethyl Benzene	12.092	91	32749	0.095	ppbv	# 99
59)	m/p-Xylene	12.349	91	180113	0.624	ppbv	# 95
60)	o-Xylene	13.060	91	48732	0.180	ppbv	# 31
65)	tert-Butylbenzene	16.111	119	29575	0.082	ppbv	# 39
70)	n-Butylbenzene	17.892	91	14763	0.034	ppbv	# 1
72)	4-Ethyltoluene	15.198	105	48741	0.159	ppbv	# 80
73)	1,3,5-Trimethylbenzene	15.355	105	72344	0.261	ppbv	# 93
74)	1,2,4-Trimethylbenzene	16.108	105	301826	0.997	ppbv	# 67
79)	Naphthalene	21.390	128	11540	0.040	ppbv	# 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052424\
Data File : VL041286.D
Acq On : 24 May 2024 11:42
Operator : SY/MD
Sample : P2599-01DUP 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :

Quant Time: May 24 23:19:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri May 24 23:11:50 2024
Response via : Initial Calibration




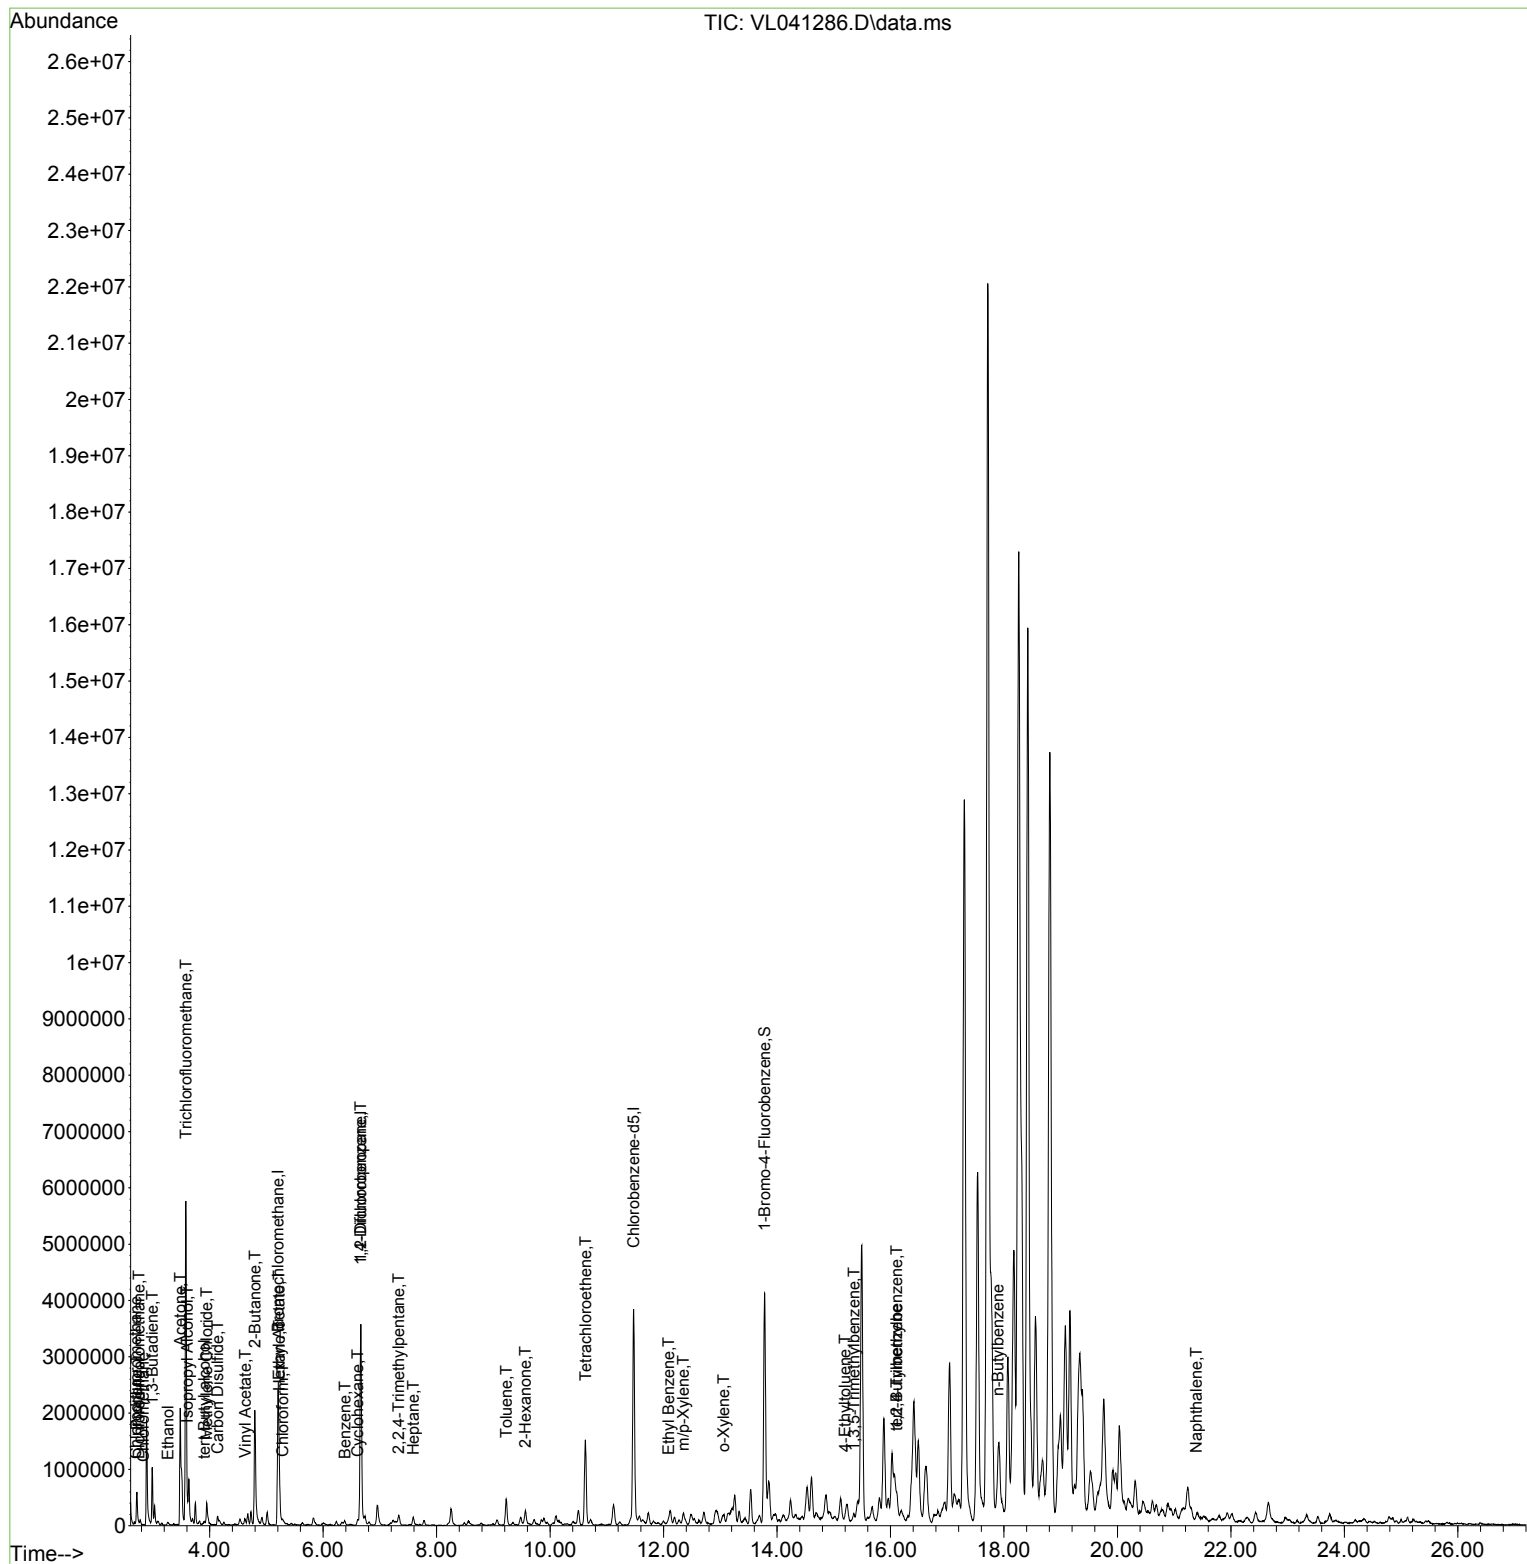




#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.205 min Scan# 80
Delta R.T. -0.003 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 49 Resp: 1057626
Ion Ratio Lower Upper
49 100
128 44.3 21.5 64.5
130 57.5 27.2 81.6

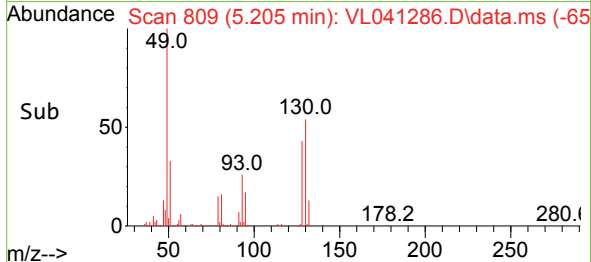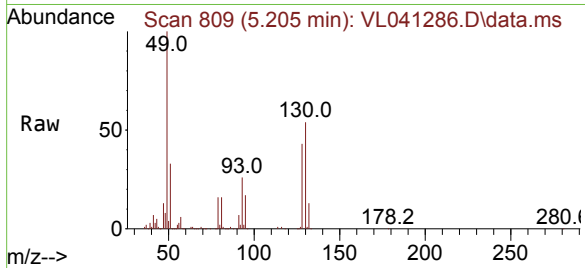

#2
Dichlorodifluoromethane
Concen: 0.128 ppbv
RT: 2.751 min Scan# 46
Delta R.T. -0.003 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 85 Resp: 18282
Ion Ratio Lower Upper
85 100
87 53.6 25.7 38.5#

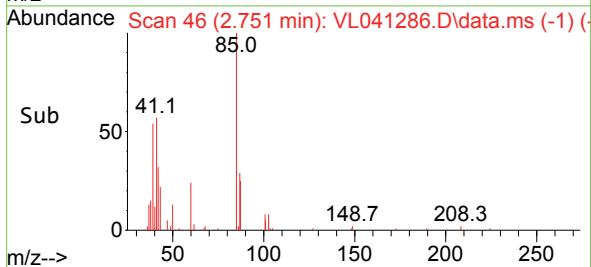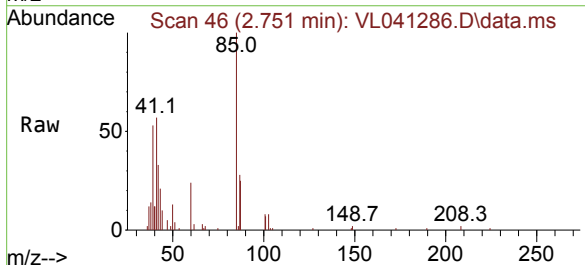

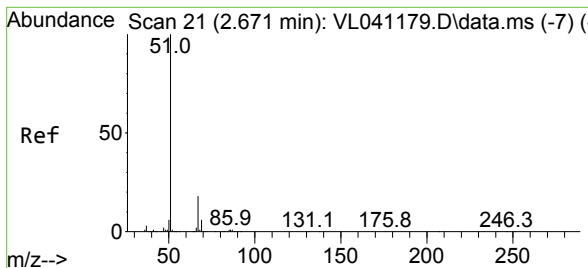

#3

Chlorodifluoromethane

Concen: 0.254 ppbv

RT: 2.697 min Scan# 21

Delta R.T. -0.003 min

Lab File: VL041286.D

Acq: 24 May 2024 11:42

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 51 Resp: 40875

Ion Ratio Lower Upper

51 100

67 15.3 14.0 21.0

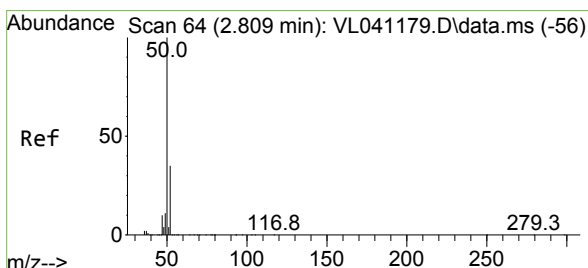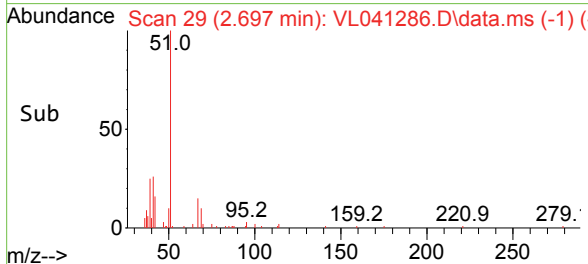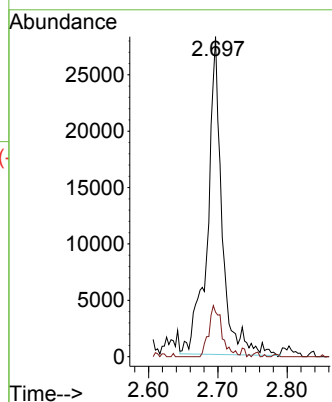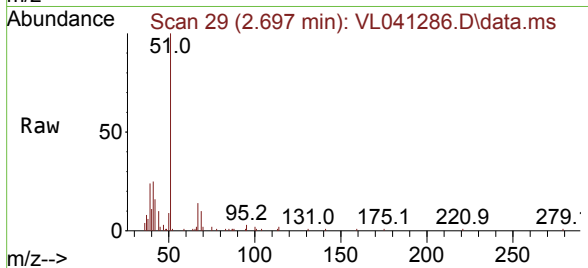

#4

Chloromethane

Concen: 0.061 ppbv

RT: 2.832 min Scan# 71

Delta R.T. -0.006 min

Lab File: VL041286.D




Acq: 24 May 2024 11:42


Tgt Ion: 50 Resp: 3847

Ion Ratio Lower Upper

50 100

52 33.8 28.3 42.5


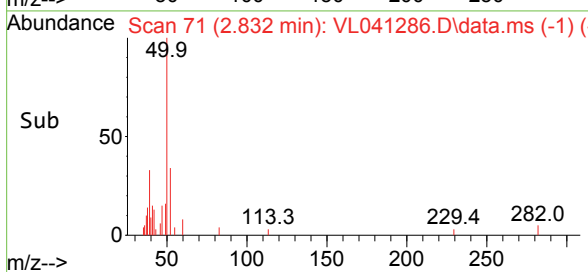
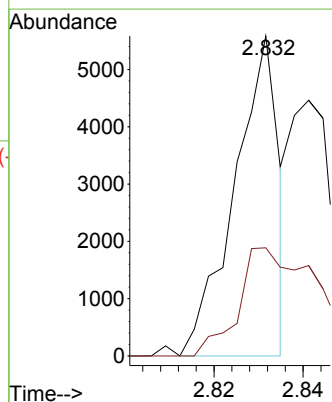
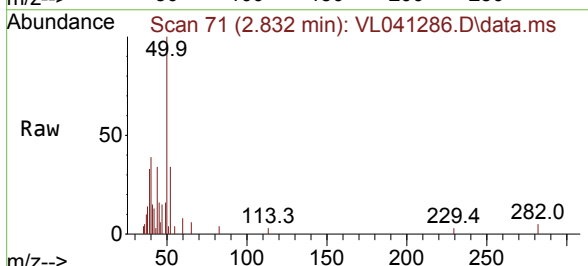


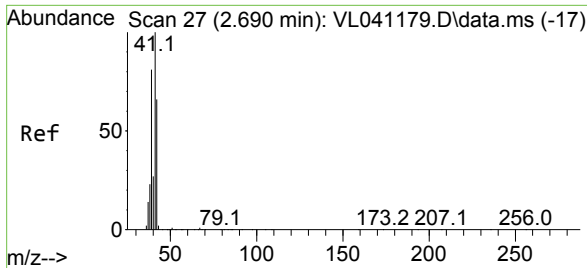

#9
 Propene
 Concen: 3.527 ppbv
 RT: 2.716 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VL041286.D
 Acq: 24 May 2024 11:42




Instrument :
 MSVOA_L
 ClientSampleId :


Tgt Ion: 41 Resp: 221745
 Ion Ratio Lower Upper
 41 100
 42 64.5 55.3 82.9

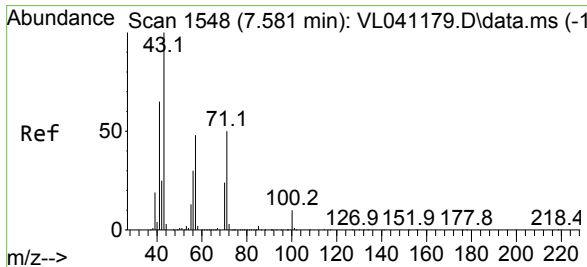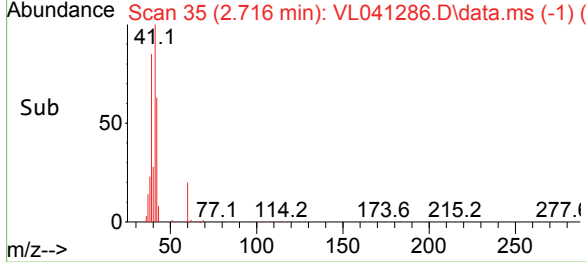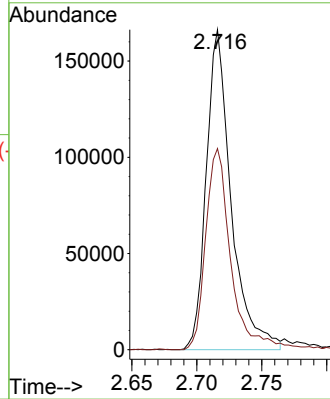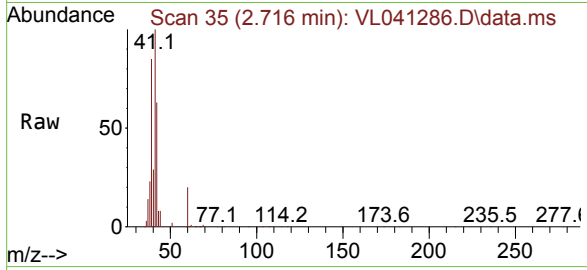

#10
 Heptane
 Concen: 0.407 ppbv
 RT: 7.587 min Scan# 1550
 Delta R.T. -0.003 min
 Lab File: VL041286.D
 Acq: 24 May 2024 11:42


Tgt Ion: 43 Resp: 61963
 Ion Ratio Lower Upper
 43 100
 57 56.3 38.7 58.1

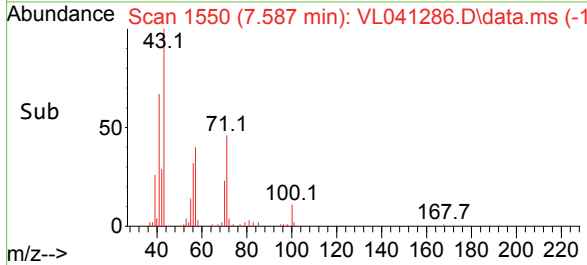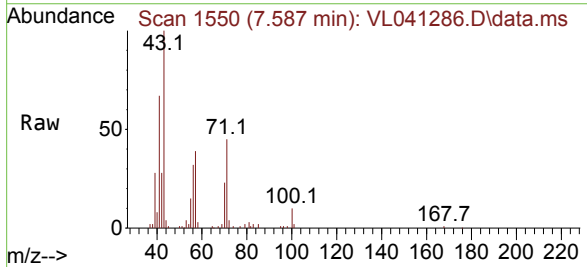






#11
 Trichlorofluoromethane
 Concen: 25.371 ppbv
 RT: 3.581 min Scan# 304
 Delta R.T. -0.003 min
 Lab File: VL041286.D
 Acq: 24 May 2024 11:42

Instrument :
 MSVOA_L
 ClientSampleId :







Tgt Ion:101 Resp: 3688889
 Ion Ratio Lower Upper
 101 100
 103 68.0 51.6 77.4



#13
 Ethanol
 Concen: 3.513 ppbv
 RT: 3.262 min Scan# 205
 Delta R.T. 0.003 min
 Lab File: VL041286.D
 Acq: 24 May 2024 11:42

Tgt Ion: 45 Resp: 49502
 Ion Ratio Lower Upper
 45 100
 46 50.6 14.8 59.0


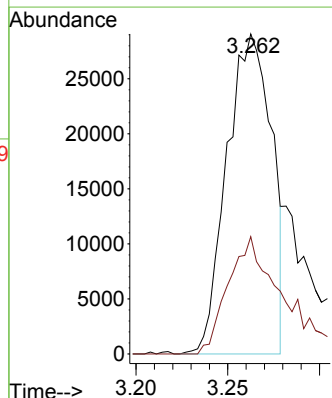
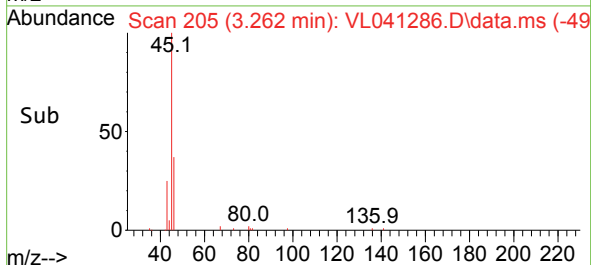
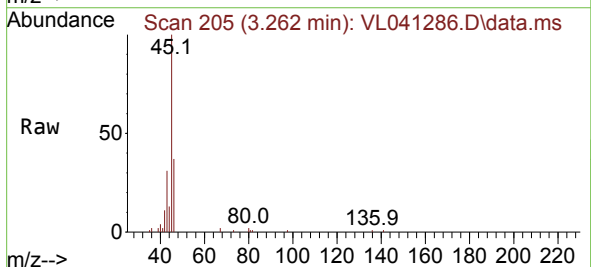




#15
Acetone
Concen: 17.917 ppbv
RT: 3.481 min Scan# 21
Delta R.T. -0.006 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 43 Resp: 2236352
Ion Ratio Lower Upper
43 100
58 31.4 21.4 32.0

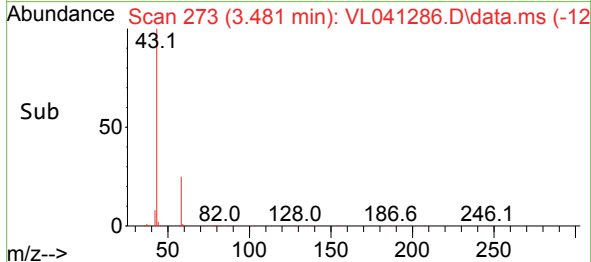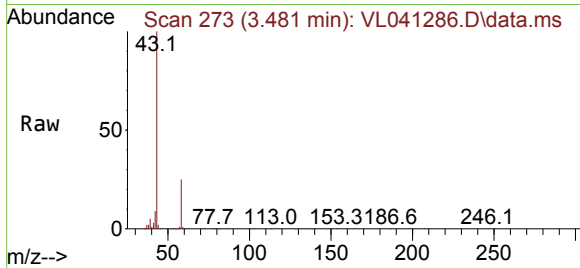

#16
1,3-Butadiene
Concen: 3.722 ppbv
RT: 2.989 min Scan# 120
Delta R.T. -0.019 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 39 Resp: 234530
Ion Ratio Lower Upper
39 100
54 9.2 62.2 93.4#

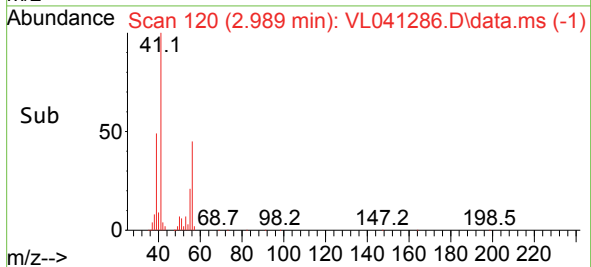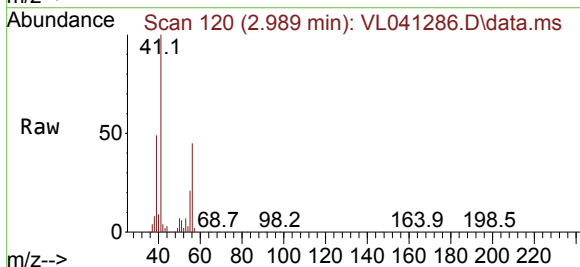



#17

tert-Butyl alcohol

Concen: 0.218 ppbv

RT: 3.902 min Scan# 404

Delta R.T. 0.006 min

Lab File: VL041286.D

Acq: 24 May 2024 11:42

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 59 Resp: 29355

Ion Ratio Lower Upper

59 100

57 0.0 8.4 12.6#

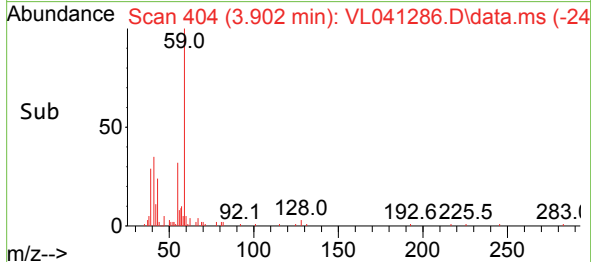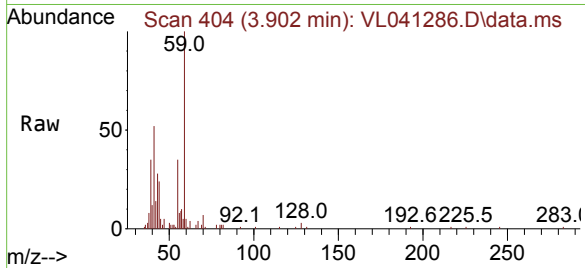

#19

Isopropyl Alcohol

Concen: 0.202 ppbv

RT: 3.603 min Scan# 311

Delta R.T. 0.010 min

Lab File: VL041286.D




Acq: 24 May 2024 11:42


Tgt Ion: 45 Resp: 16582

Ion Ratio Lower Upper

45 100


58 0.0 26.8 40.2#

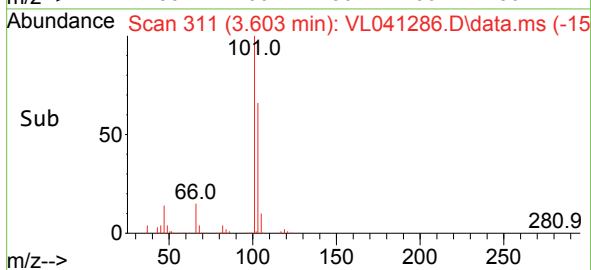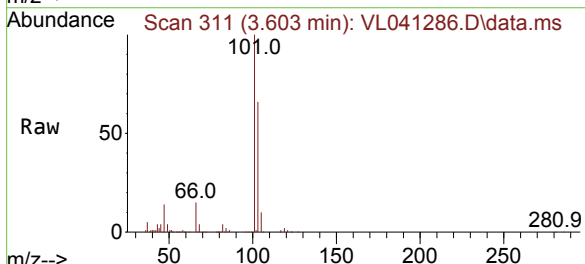






#20
Methylene Chloride
Concen: 2.678 ppbv
RT: 3.947 min Scan# 411
Delta R.T. -0.003 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Instrument :
MSVOA_L
ClientSampleId :



Tgt Ion: 84 Resp: 116237




Ion	Ratio	Lower	Upper
84	100		
49	163.1	130.4	195.6
51	43.4	38.0	57.0
86	54.1	50.3	75.5




#23
Vinyl Acetate
Concen: 0.360 ppbv
RT: 4.626 min Scan# 629
Delta R.T. -0.016 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 43 Resp: 49537


Ion	Ratio	Lower	Upper
43	100		
86	5.4	4.9	7.3
42	75.4	8.0	12.0#
44	9.4	3.7	5.5#

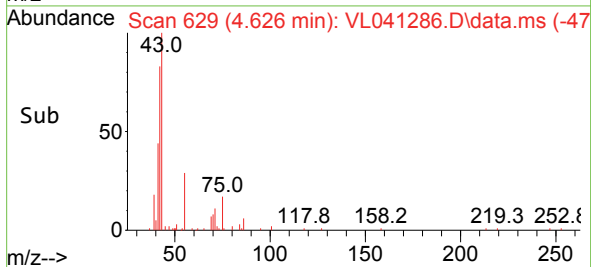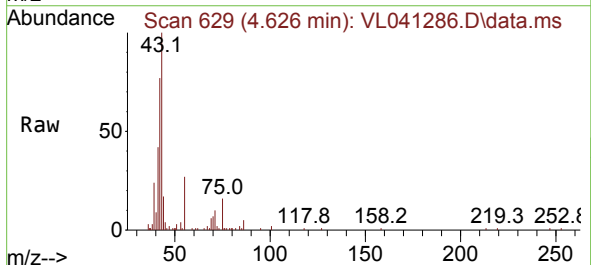






#25
Ethyl Acetate
Concen: 0.979 ppbv
RT: 5.224 min Scan# 815
Delta R.T. 0.006 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Instrument :
MSVOA_L
ClientSampleId :







Tgt Ion: 43 Resp: 243842
Ion Ratio Lower Upper
43 100
45 0.9 8.2 12.2#
61 0.1 7.7 11.5#
70 1.7 5.8 8.6#



#26
Hexane
Concen: 3.080 ppbv
RT: 5.227 min Scan# 816
Delta R.T. -0.000 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 57 Resp: 342455
Ion Ratio Lower Upper
57 100
41 100.2 75.8 113.8
43 73.0 187.0 280.4#
56 53.2 42.7 64.1


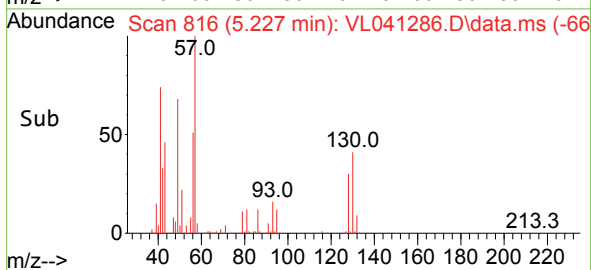
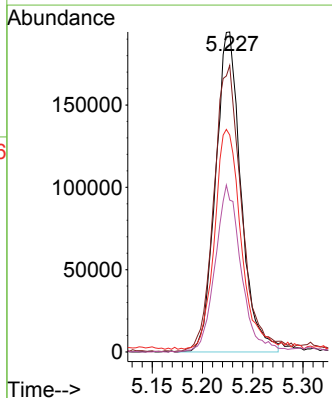





#27
Carbon Disulfide
Concen: 1.305 ppbv
RT: 4.140 min Scan# 41
Delta R.T. -0.003 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 76 Resp: 171685
Ion Ratio Lower Upper
76 100
44 24.2 16.3 24.5
78 9.9 7.3 10.9

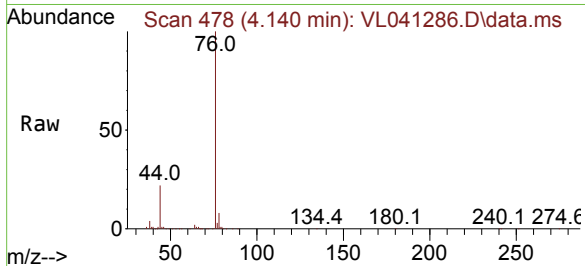

#29
Chloroform
Concen: 0.182 ppbv
RT: 5.285 min Scan# 834
Delta R.T. -0.007 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 83 Resp: 27982
Ion Ratio Lower Upper
83 100
85 49.4 51.7 77.5#


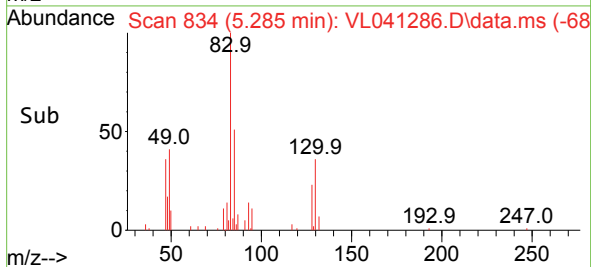

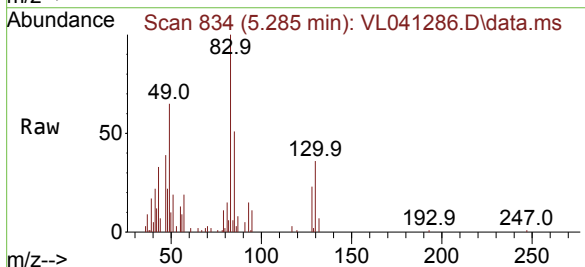




#30
Cyclohexane
Concen: 0.212 ppbv
RT: 6.606 min Scan# 11
Delta R.T. -0.006 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 84 Resp: 18701
Ion Ratio Lower Upper
84 100
56 0.0 116.8 175.2#
41 170.3 73.8 110.8#

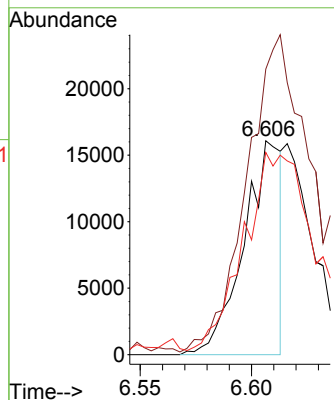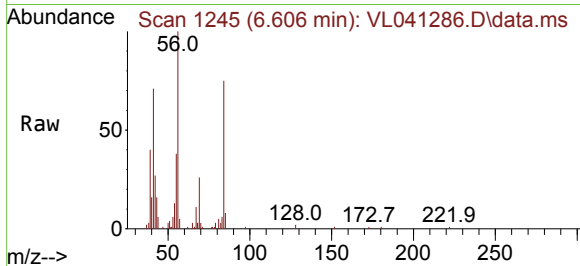

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.661 min Scan# 1262
Delta R.T. -0.007 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 114 Resp: 2697279
Ion Ratio Lower Upper
114 100
63 25.8 21.8 32.6
88 18.1 15.2 22.8


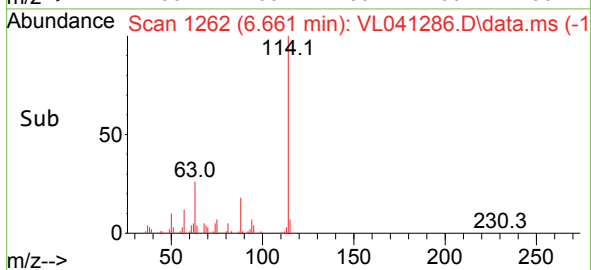
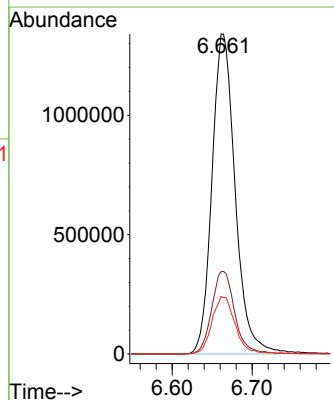
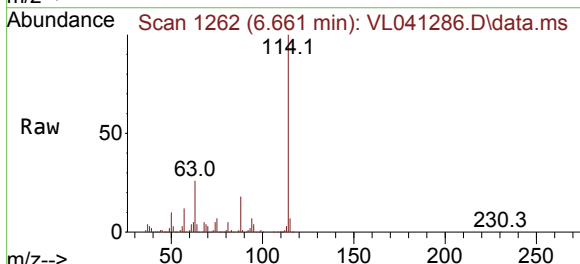




#34
2-Butanone
Concen: 18.014 ppbv
RT: 4.796 min Scan# 61
Delta R.T. -0.006 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 43 Resp: 2473069
Ion Ratio Lower Upper
43 100
72 21.7 17.3 25.9

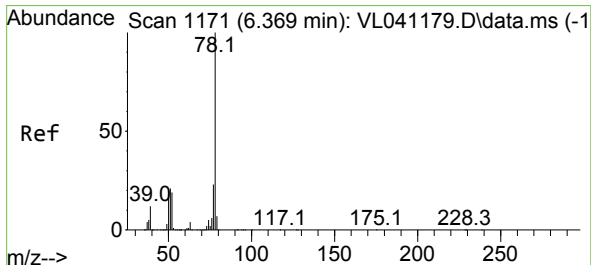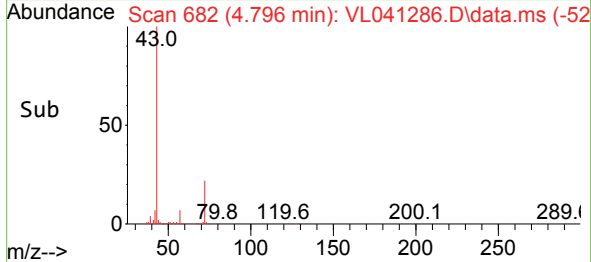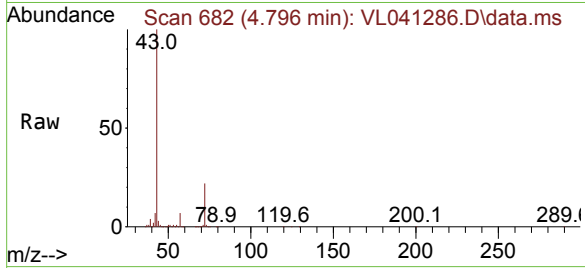

#36
Benzene
Concen: 0.258 ppbv
RT: 6.385 min Scan# 1176
Delta R.T. -0.000 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 78 Resp: 58487
Ion Ratio Lower Upper
78 100
77 16.1 18.3 27.5#
50 15.3 15.9 23.9#

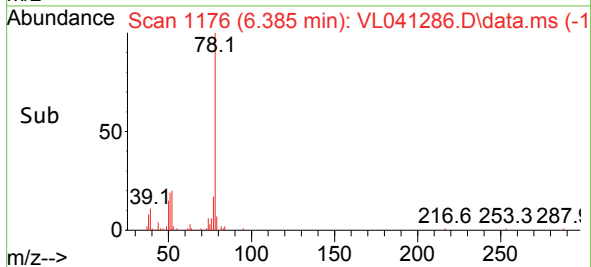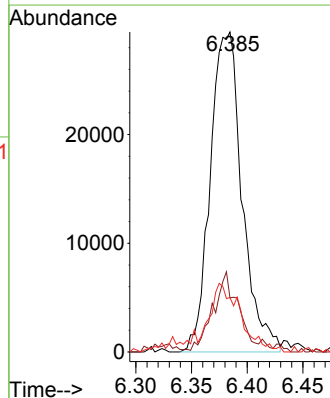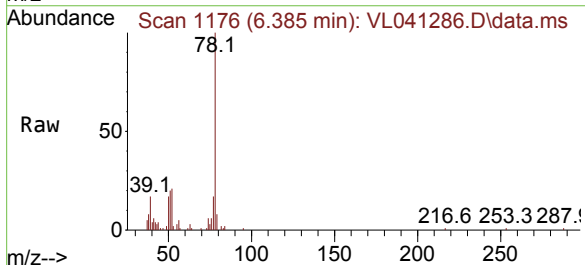



#39

1,2-Dichloropropane

Concen: 7.915 ppbv

RT: 6.664 min Scan# 11

Delta R.T. -0.421 min

Lab File: VL041286.D

Acq: 24 May 2024 11:42

Instrument :

MSVOA_L

ClientSampleId :





Tgt Ion: 63 Resp: 690473

Ion Ratio Lower Upper

63 100

41 0.0 59.4 89.0#

62 18.2 56.8 85.2#

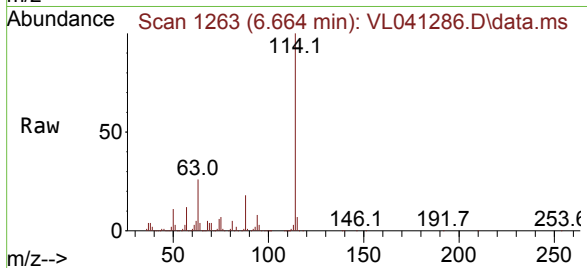

#44

2,2,4-Trimethylpentane

Concen: 0.322 ppbv

RT: 7.333 min Scan# 1471

Delta R.T. -0.003 min

Lab File: VL041286.D

Acq: 24 May 2024 11:42




Tgt Ion: 57 Resp: 125486


Ion Ratio Lower Upper

57 100

41 69.2 29.5 44.3#

56 50.7 25.3 37.9#


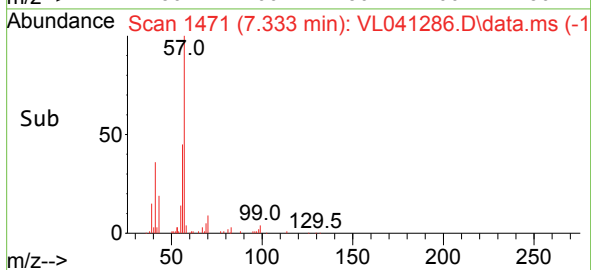

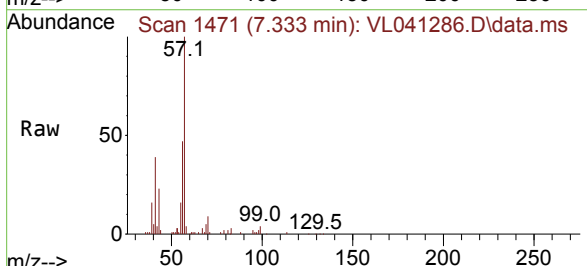




#51
2-Hexanone
Concen: 1.290 ppbv
RT: 9.564 min Scan# 2160
Delta R.T. 0.006 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 43 Resp: 235836
Ion Ratio Lower Upper
43 100
58 46.7 38.4 57.6
98 0.5 0.0 0.0#

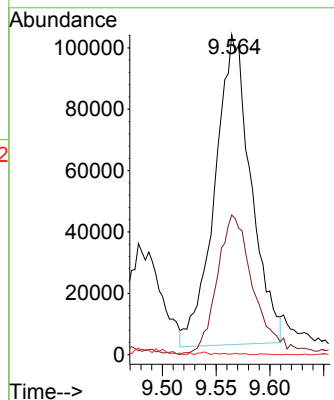

#52
Tetrachloroethene
Concen: 4.528 ppbv
RT: 10.626 min Scan# 2495
Delta R.T. 0.003 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 164 Resp: 360226
Ion Ratio Lower Upper
164 100
166 121.2 101.1 151.7
129 104.3 81.7 122.5
131 100.4 80.4 120.6


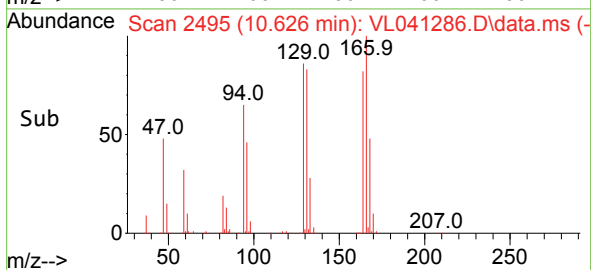
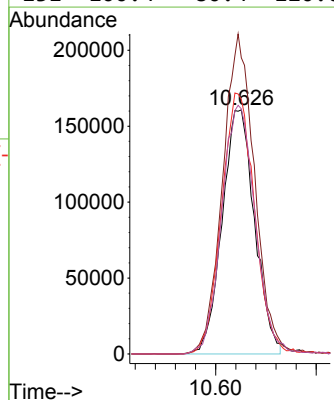





#53
Toluene
Concen: 1.213 ppbv
RT: 9.230 min Scan# 2058
Delta R.T. -0.000 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 91 Resp: 318315
Ion Ratio Lower Upper
91 100
92 60.9 48.2 72.4



#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.471 min Scan# 2758
Delta R.T. -0.000 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 117 Resp: 2504616
Ion Ratio Lower Upper
117 100
82 65.2 53.6 80.4
119 33.2 27.2 40.8


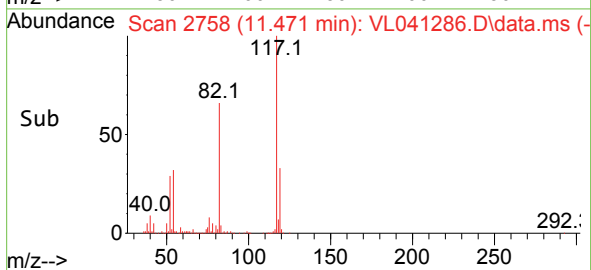

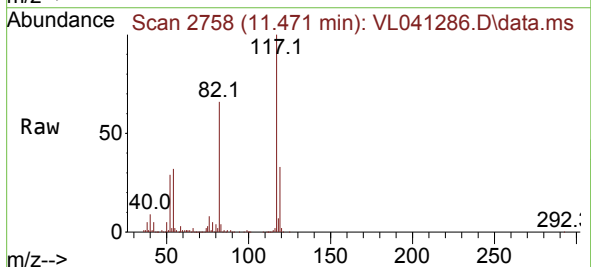


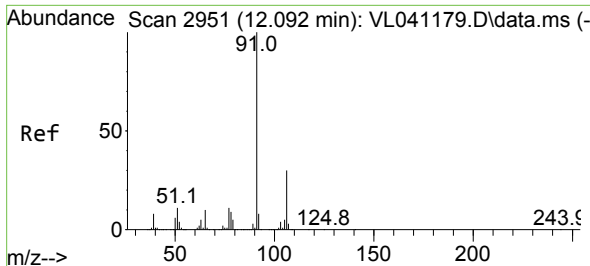

#58
Ethyl Benzene
Concen: 0.095 ppbv
RT: 12.092 min Scan# 2951
Delta R.T. -0.003 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 91 Resp: 32749
Ion Ratio Lower Upper
91 100
106 31.2 24.3 36.5

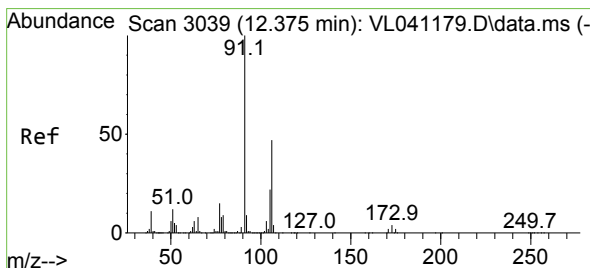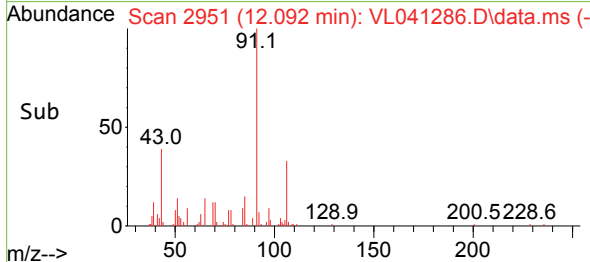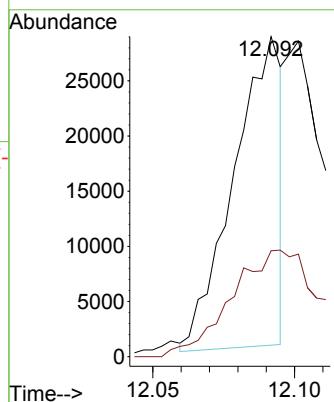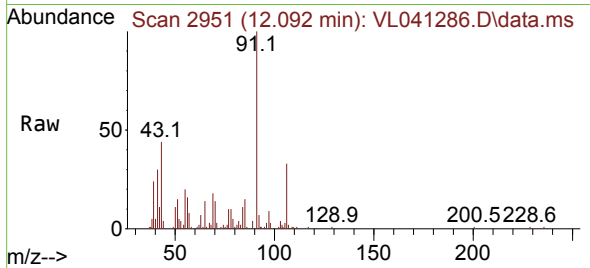

#59
m/p-Xylene
Concen: 0.624 ppbv
RT: 12.349 min Scan# 3031
Delta R.T. -0.029 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 91 Resp: 180113
Ion Ratio Lower Upper
91 100
106 47.6 35.7 53.5


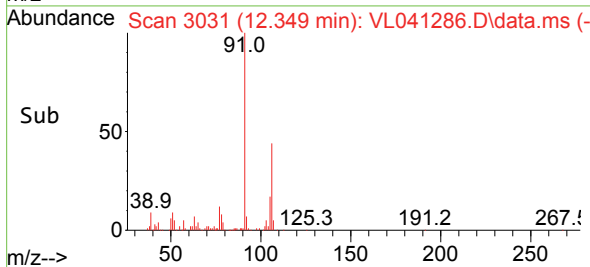
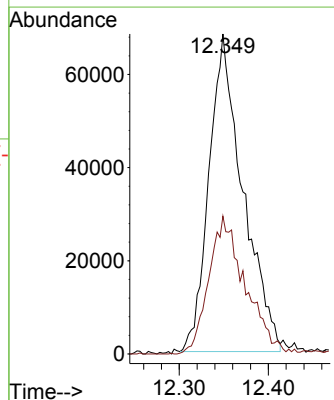
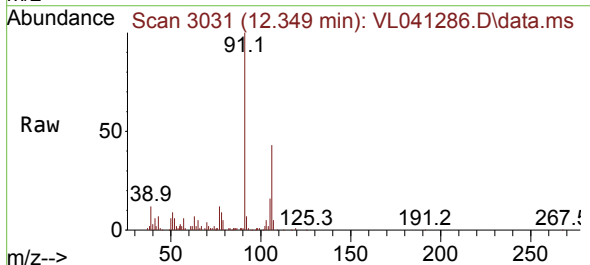




#60
o-Xylene
Concen: 0.180 ppbv
RT: 13.060 min Scan# 31
Delta R.T. -0.003 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 91 Resp: 48732
Ion Ratio Lower Upper
91 100
106 0.0 22.4 67.3#

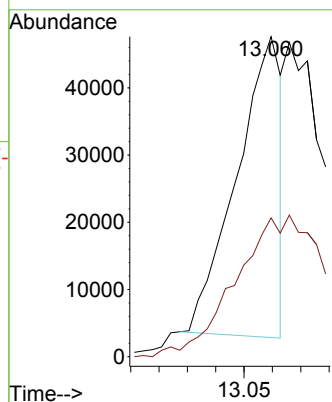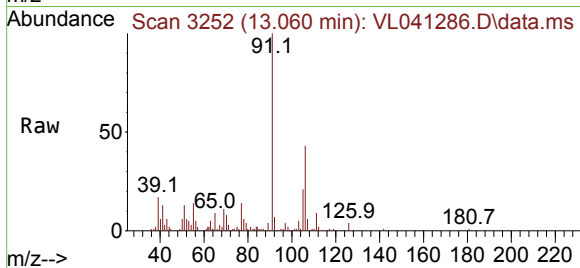

#65
tert-Butylbenzene
Concen: 0.082 ppbv
RT: 16.111 min Scan# 4201
Delta R.T. 0.019 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42

Tgt Ion: 119 Resp: 29575
Ion Ratio Lower Upper
119 100
91 142.6 67.0 100.4#
134 0.9 15.2 22.8#


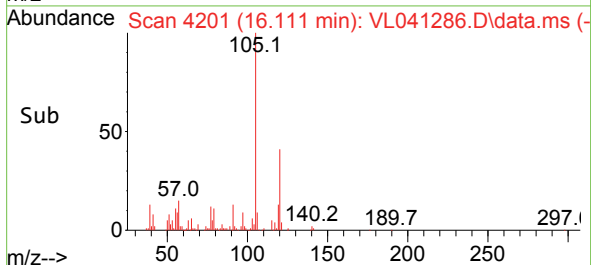

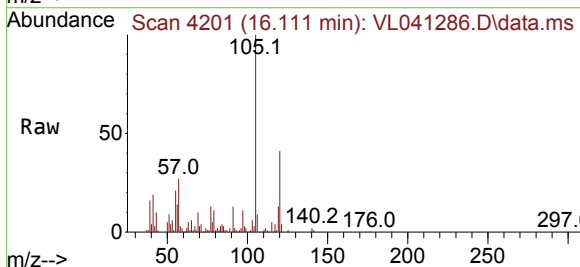


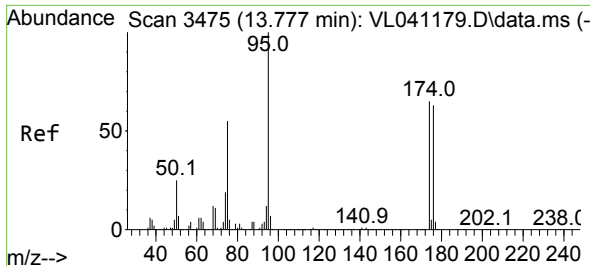

#68
1-Bromo-4-Fluorobenzene
Concen: 10.459 ppbv
RT: 13.783 min Scan# 3475
Delta R.T. 0.003 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 95 Resp: 1977567
Ion Ratio Lower Upper
95 100
174 66.2 53.6 80.4
175 4.9 4.2 6.4

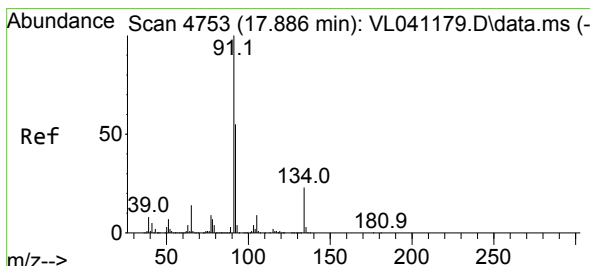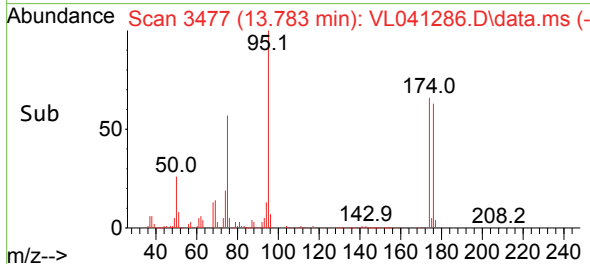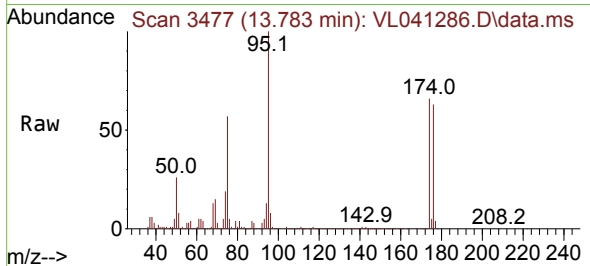

#70
n-Butylbenzene
Concen: 0.034 ppbv
RT: 17.892 min Scan# 4755
Delta R.T. 0.003 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42


Tgt Ion: 91 Resp: 14763
Ion Ratio Lower Upper
91 100
92 155.2 43.3 64.9#
134 0.0 17.8 26.8#

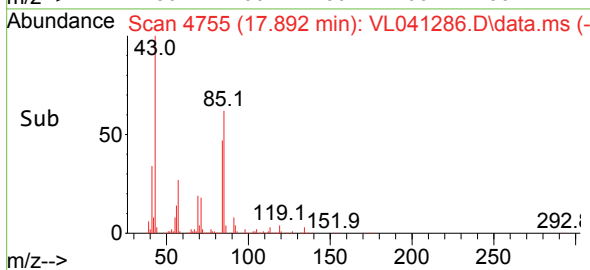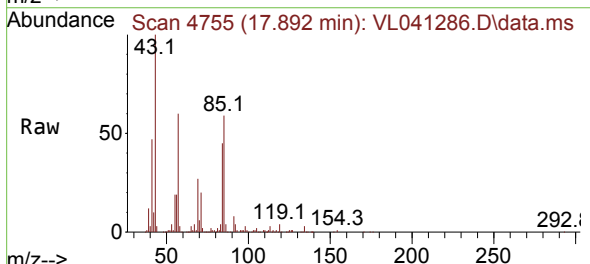






#72
4-Ethyltoluene
Concen: 0.159 ppbv
RT: 15.198 min Scan# 3917
Delta R.T. -0.000 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42


Instrument :
MSVOA_L
ClientSampleId :

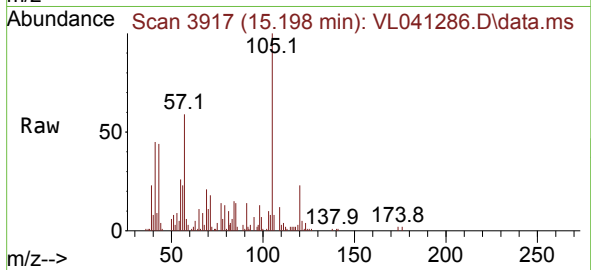



Tgt Ion:105 Resp: 48741
Ion Ratio Lower Upper
105 100
120 38.1 24.7 37.1#
91 24.7 10.3 15.5#
77 25.5 11.4 17.0#




#73
1,3,5-Trimethylbenzene
Concen: 0.261 ppbv
RT: 15.355 min Scan# 3966
Delta R.T. -0.000 min
Lab File: VL041286.D
Acq: 24 May 2024 11:42



Tgt Ion:105 Resp: 72344
Ion Ratio Lower Upper
105 100
120 51.1 37.0 55.4

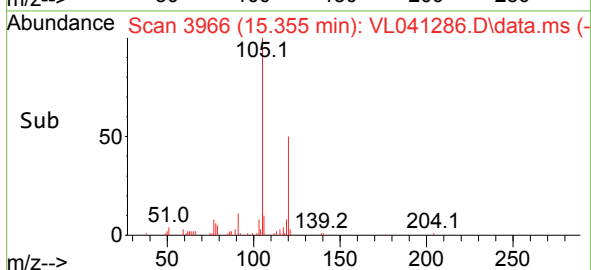

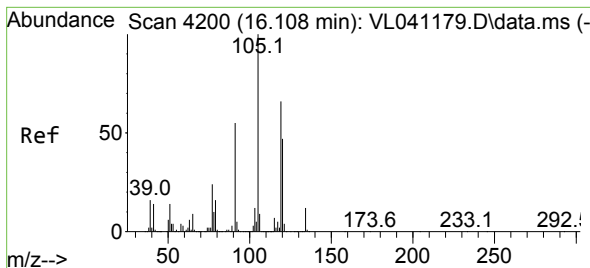

#74

1,2,4-Trimethylbenzene

Concen: 0.997 ppbv

RT: 16.108 min Scan# 41

Delta R.T. -0.003 min


Lab File: VL041286.D

Acq: 24 May 2024 11:42

Instrument :

MSVOA_L

ClientSampleId :

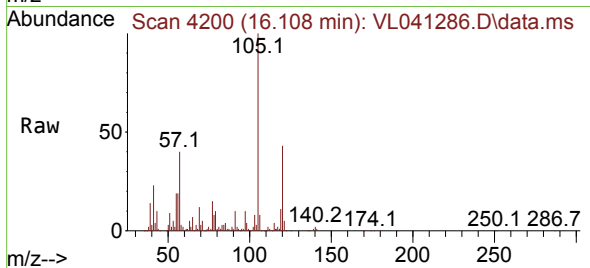

Tgt Ion:105 Resp: 301826




Ion Ratio Lower Upper

105 100

120 42.8 37.8 56.6

91 9.9 44.3 66.5#

77 14.6 19.0 28.4#

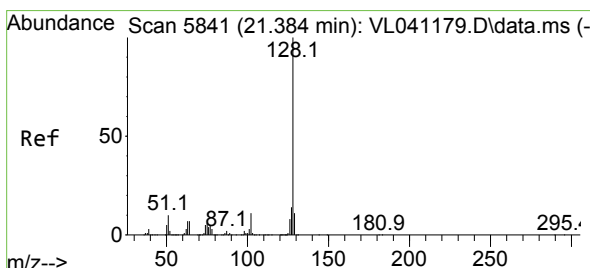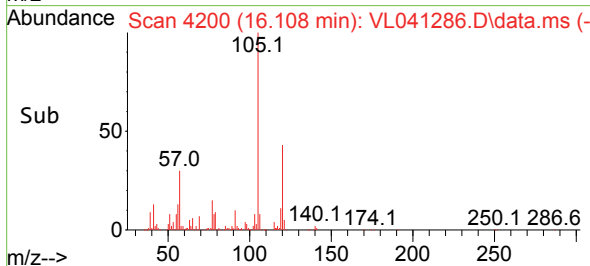

#79

Naphthalene

Concen: 0.040 ppbv

RT: 21.390 min Scan# 5843

Delta R.T. 0.006 min

Lab File: VL041286.D

Acq: 24 May 2024 11:42

Tgt Ion:128 Resp: 11540

Ion Ratio Lower Upper

128 100

127 2.4 10.8 16.2#

129 10.2 8.9 13.3

