
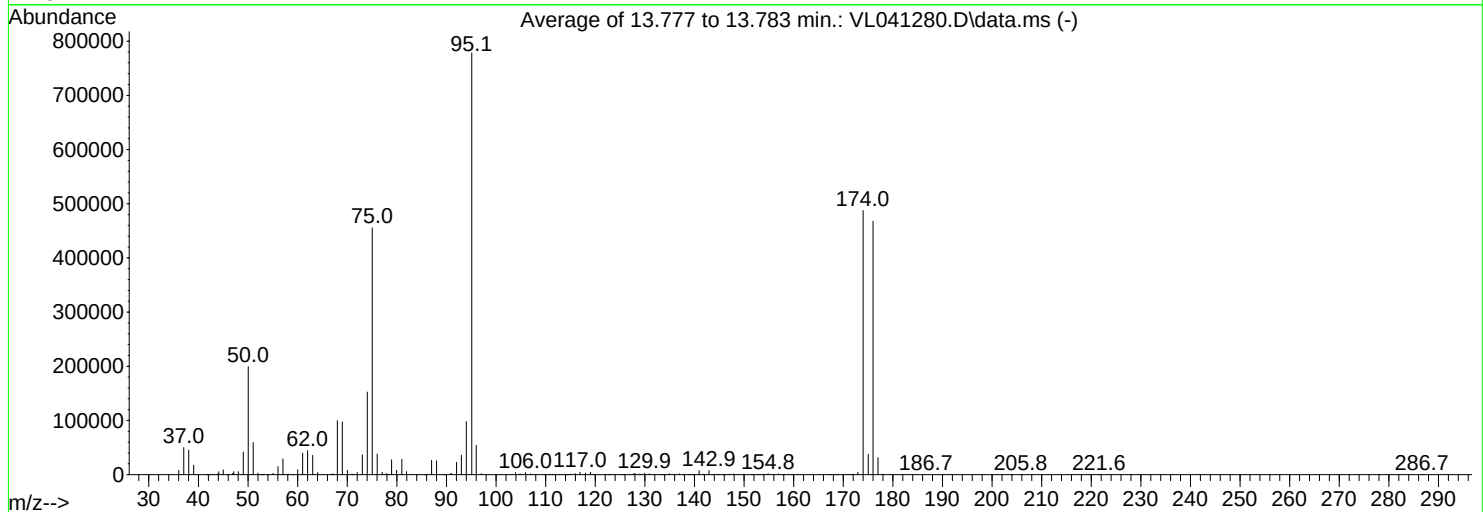


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052424\
Data File : VL041280.D
Acq On : 24 May 2024 7:45
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL042924AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 24 23:11:50 2024

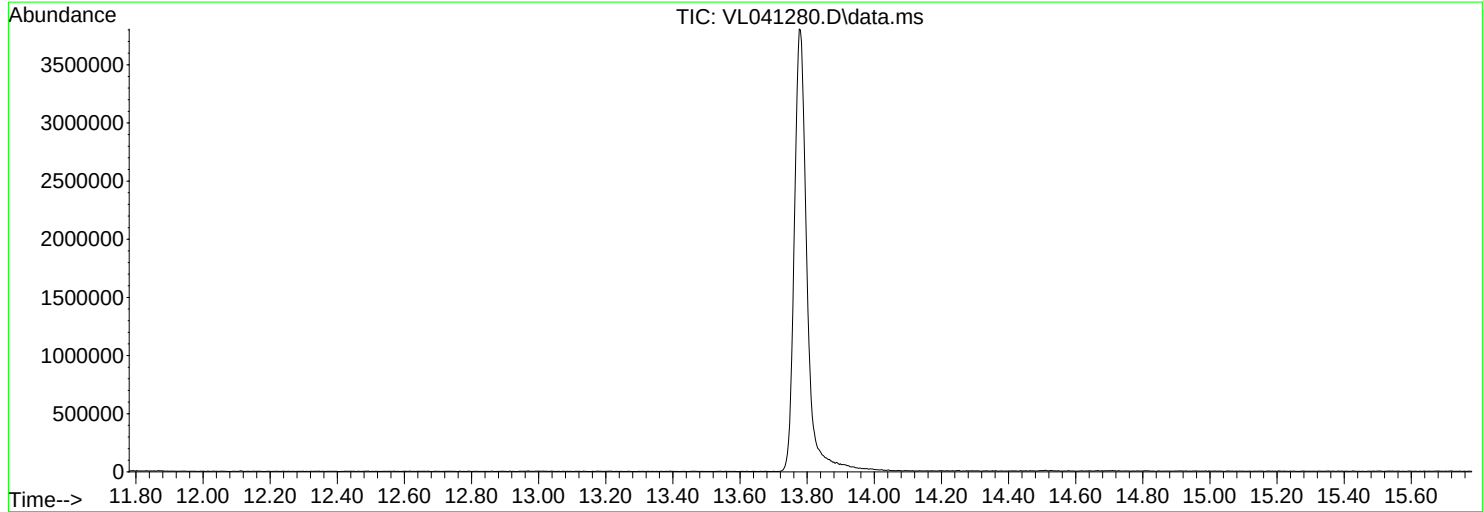

AutoFind: Scans 3475, 3476, 3477; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.6	199424	PASS
75	95	30	66	58.5	455509	PASS
95	95	100	100	100.0	778475	PASS
96	95	5	9	6.9	54093	PASS
173	174	0.00	2	0.8	4044	PASS
174	95	50	120	62.6	487595	PASS
175	174	4	9	7.7	37608	PASS
176	174	93	101	95.9	467797	PASS
177	176	5	9	6.7	31168	PASS

Average of 13.777 to 13.783 min.: VL041280.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8112	45.00	8997	53.00	118	63.05	3582
37.05	50019	45.90	543	53.90	79	64.05	384
38.05	45216	46.15	674	55.05	2258	64.95	46
39.05	17550	46.90	2469	56.05	14906	66.95	151
39.95	722	47.15	5648	57.05	28893	67.20	856
41.70	94	48.05	5251	57.90	759	68.00	99392
42.20	56	49.05	41731	58.15	996	69.00	97523
42.90	346	50.05	199424	59.00	83	70.05	8155
43.20	167	51.05	59240	60.00	8768	70.90	140
43.85	1609	52.00	2623	61.00	39525	71.25	383
44.10	5412	52.70	74	62.00	44405	72.00	4186

Average of 13.777 to 13.783 min.: VL041280.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.05	36579	82.80	288	92.05	22635	109.70	141
74.05	152384	83.05	734	93.00	35963	109.85	303
75.05	455509	83.90	61	94.00	98040	110.80	675
76.05	38085	85.60	149	95.10	778475	111.30	98
77.05	4513	85.80	191	96.00	54093	111.90	630
77.85	1805	86.10	207	97.00	1782	112.85	497
78.10	954	87.00	26341	102.95	644	113.10	395
78.95	27408	88.00	25429	103.95	3767	113.80	158
79.95	8096	89.50	62	104.85	1412	114.30	149
81.00	28453	90.80	1768	105.95	3732	114.70	324
81.95	5747	91.05	1992	106.95	1233	115.05	1022

Average of 13.777 to 13.783 min.: VL041280.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
115.80	1048	125.05	412	134.15	308	140.95	7429
116.00	1795	125.70	56	134.95	1778	141.80	820
116.95	4549	125.85	306	135.65	222	142.10	439
118.05	2785	126.90	241	135.90	55	142.95	7694
119.05	4488	127.70	1391	137.00	1441	143.70	211
119.95	174	128.00	2326	137.70	64	144.00	329
122.00	117	129.00	1322	138.80	209	144.60	249
122.60	87	129.95	2391	139.00	136	144.85	667
122.80	235	130.90	1534	139.60	84	145.10	195
123.10	171	133.40	65	139.90	142	145.75	519
123.90	440	133.90	131	140.20	276	145.90	320

Average of 13.777 to 13.783 min.: VL041280.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
146.10	136	154.85	1880	169.10	210	177.00	31168
147.05	570	156.00	315	169.85	170	178.00	999
147.90	1644	156.95	1082	170.35	762	186.70	165
148.90	203	157.70	94	170.90	271	190.00	83
150.00	819	158.00	115	171.35	417	203.90	52
151.50	57	158.95	937	171.70	265	205.80	83
151.95	328	159.60	78	172.00	874	221.60	116
152.70	126	160.90	819	172.95	4044	286.70	66
153.10	283	167.30	129	174.00	487595		
153.70	81	168.35	237	175.05	37608		
154.05	237	168.60	143	176.00	467797		