


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052522\
 Data File : VL039114.D
 Acq On : 25 May 2022 11:28
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050522AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu May 05 10:12:15 2022
 Last Update : Thu May 05 10:12:15 2022

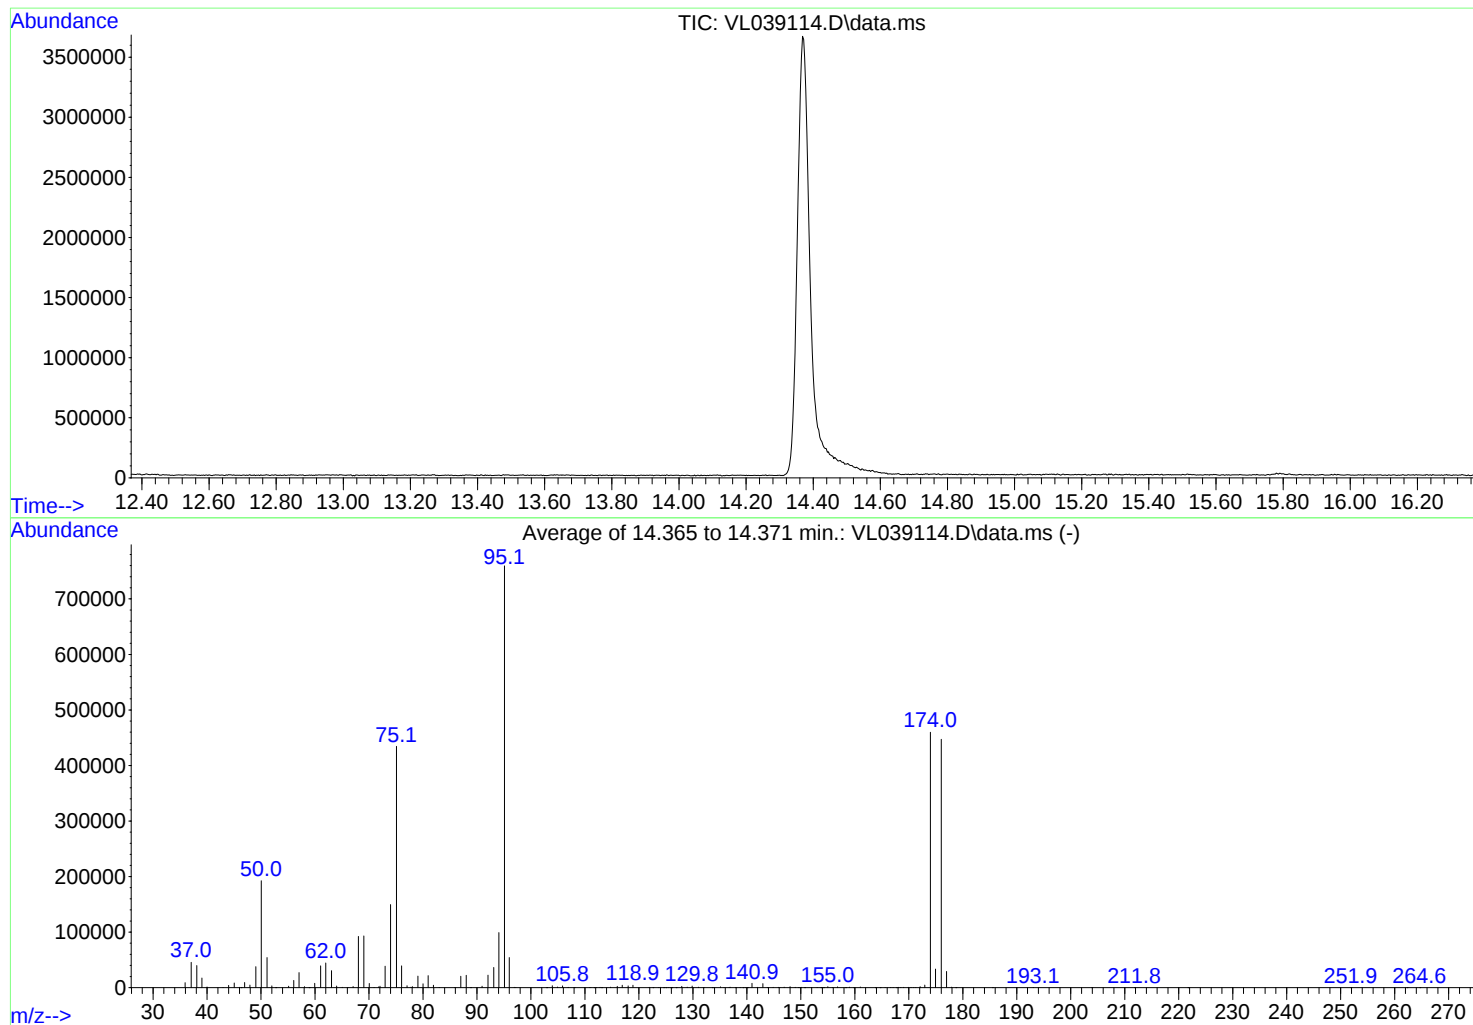

AutoFind: Scans 3601, 3602, 3603; Background Corrected with Scan 3576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.4	192597	PASS
75	95	30	66	57.2	434411	PASS
95	95	100	100	100.0	759531	PASS
96	95	5	9	7.1	54205	PASS
173	174	0.00	2	1.0	4653	PASS
174	95	50	120	60.5	459712	PASS
175	174	4	9	7.3	33571	PASS
176	174	93	101	97.3	447211	PASS
177	176	5	9	6.5	29272	PASS

Average of 14.365 to 14.371 min.: VL039114.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	8957	47.95	4554	59.95	7682	70.95	331
37.05	45667	49.05	37893	61.05	39277	71.80	133
38.10	39795	50.05	192597	62.00	44328	72.05	257
39.05	17435	51.10	54064	63.05	30533	73.00	3856
40.00	1258	52.00	3119	64.00	2878	74.00	149675
42.95	304	52.70	88	65.05	630	75.10	434411
44.00	3976	55.10	2465	66.10	318	76.05	39120
45.05	8428	56.05	13024	67.05	2170	77.05	3543
46.00	527	57.05	27176	68.05	92115	77.80	933
46.30	136	58.05	1630	69.05	93067	78.05	1848
46.95	9123	58.90	114	70.05	7469	79.05	20845

Average of 14.365 to 14.371 min.: VL039114.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.00	6938	93.10	36421	106.90	699	116.90	4353
80.95	21736	94.05	99235	108.00	60	118.00	3071
81.95	4332	95.10	759531	109.90	437	118.90	4380
83.00	327	96.00	54205	110.90	326	121.90	514
85.90	289	96.90	534	111.10	215	122.60	54
86.05	395	97.20	325	111.70	119	123.70	173
87.00	20453	102.90	72	112.10	299	124.00	490
88.00	22251	103.05	363	112.80	639	124.60	88
88.80	64	103.95	3608	113.10	157	125.00	84
90.95	2647	104.95	1244	114.75	780	125.55	168
92.05	22485	105.85	3147	116.00	2271	125.90	107

Average of 14.365 to 14.371 min.: VL039114.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.10	102	136.70	199	144.00	242	152.00	295
126.90	154	136.90	922	144.85	703	153.00	354
127.95	2459	137.90	105	145.85	655	153.70	126
128.95	768	138.75	378	146.10	185	153.95	403
129.85	2890	139.30	61	146.90	937	154.20	118
131.05	742	139.80	187	148.00	1745	155.00	1660
131.90	103	140.10	155	148.95	535	155.90	162
133.60	140	140.95	7787	149.60	229	156.80	1468
134.00	176	141.95	660	149.80	156	158.30	67
135.10	1499	142.95	7144	150.05	612	159.00	840
135.75	255	143.80	437	150.70	85	159.80	129

Average of 14.365 to 14.371 min.: VL039114.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
161.00	1167	170.40	254	185.50	120		
163.80	113	170.90	446	193.05	167		
164.70	81	171.30	424	203.90	57		
165.60	207	172.10	1816	211.80	66		
166.65	172	172.95	4653	221.70	58		
167.10	176	174.00	459712	251.90	97		
167.70	95	174.95	33571	262.30	73		
168.10	452	176.00	447211	264.65	129		
168.50	306	177.00	29272				
169.05	458	177.95	836				
169.90	583	178.70	79				