

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL052819\
Data File : VL033799.D
Acq On : 28 May 2019 10:28
Operator : SY/AP
Sample : VL0528ABL01
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0528ABL01

Quant Time: May 29 04:47:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL051719AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri May 17 08:15:41 2019
QLast Update : Fri May 17 08:15:41 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.75	49	899051	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.28	114	2141248	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.23	117	2090429	10.00	ppbv	-0.01

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.57	95	1761549	10.39	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	103.90%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL052819\
Data File : VL033799.D
Acq On : 28 May 2019 10:28
Operator : SY/AP
Sample : VL0528ABL01
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0528ABL01

Quant Time: May 29 04:47:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL051719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri May 17 08:15:41 2019
QLast Update : Fri May 17 08:15:41 2019
Response via : Initial Calibration

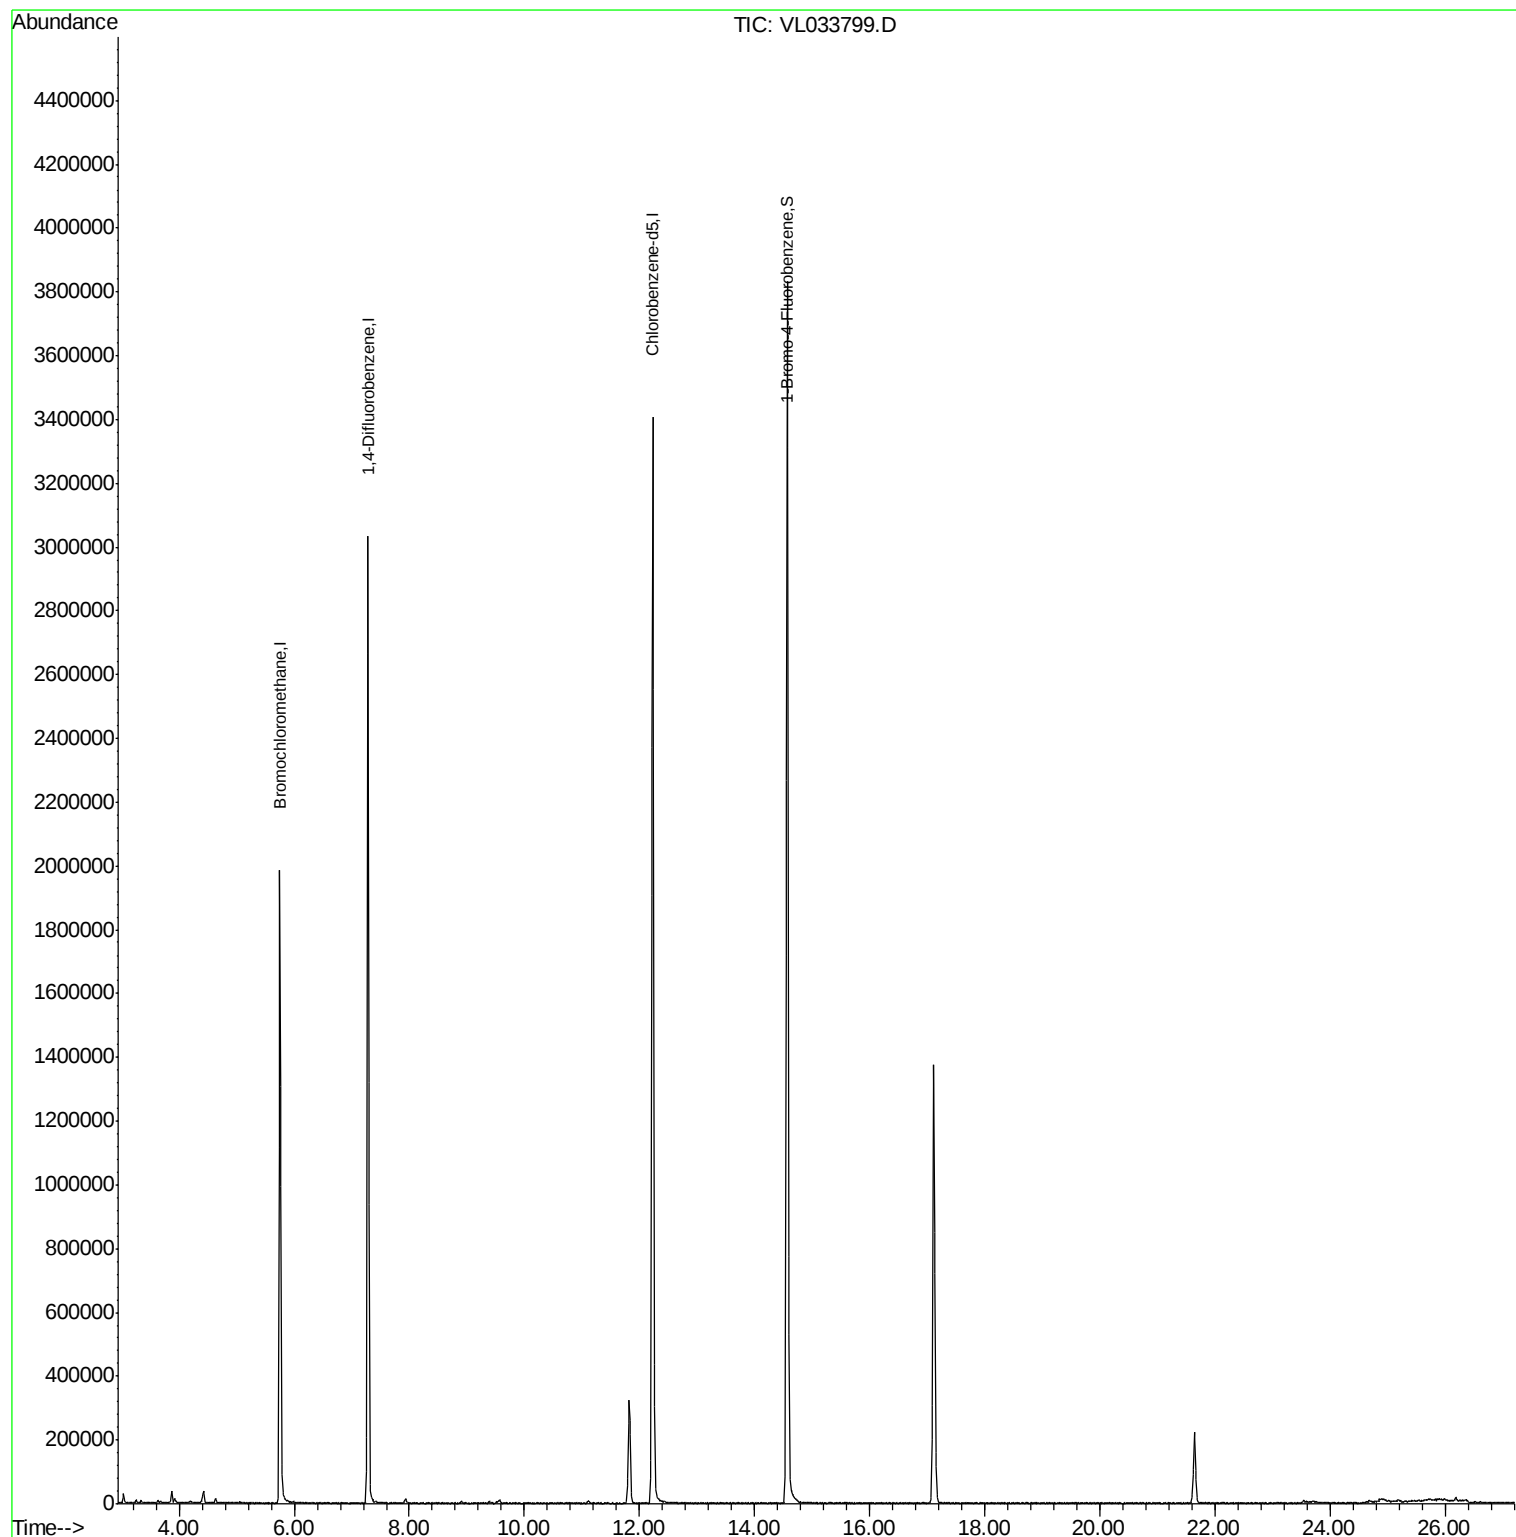

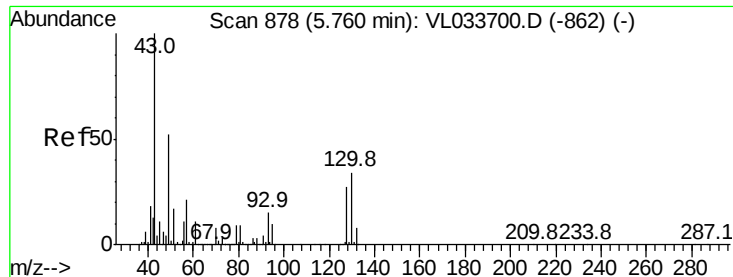

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.75 min Scan# 875

Delta R.T. -0.01 min

Lab File: VL033799.D

Acq: 28 May 2019 10:28

Instrument :

MSVOA_L

ClientSampleId :

VL0528ABL01


Tot Ion: 49 Resp: 899051

Ion Ratio Lower Upper

49 100

128 50.3 25.2 75.6




130 64.7 32.5 97.5

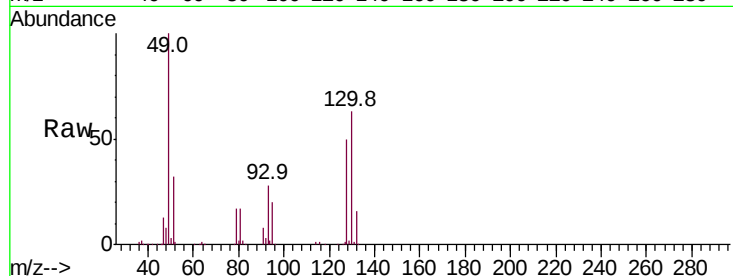

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

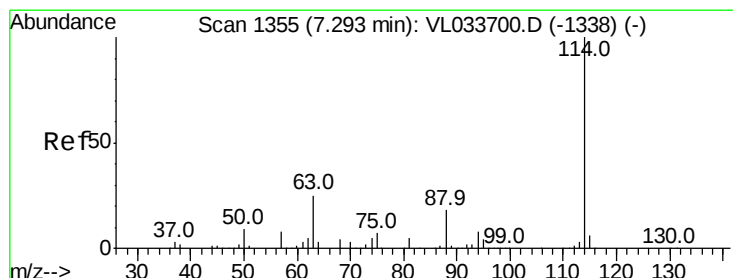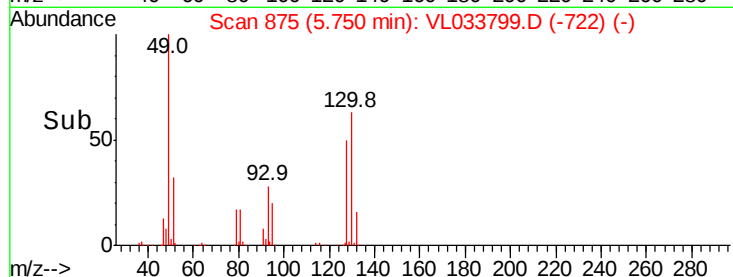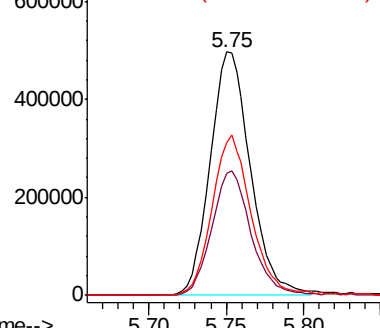

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.28 min Scan# 1352

Delta R.T. -0.01 min

Lab File: VL033799.D

Acq: 28 May 2019 10:28


Tgt Ion: 114 Resp: 2141248

Ion Ratio Lower Upper

114 100

63 25.8 20.9 31.3



88 17.8 14.3 21.5

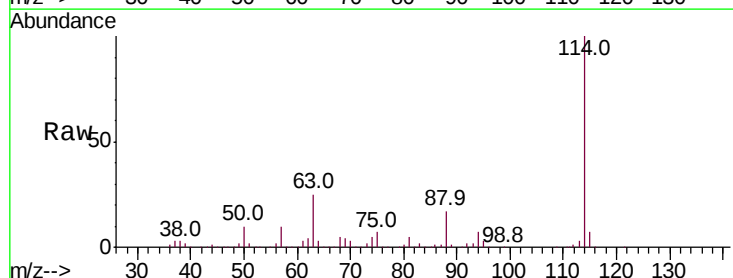


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



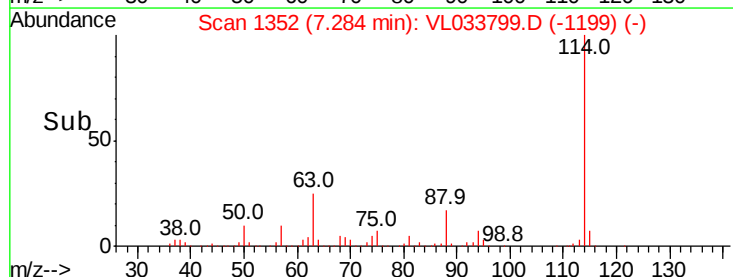
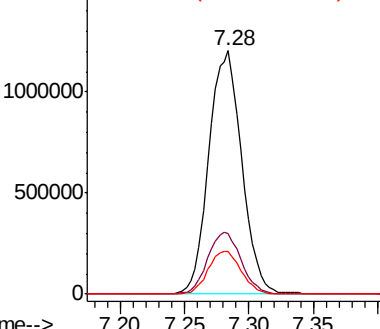


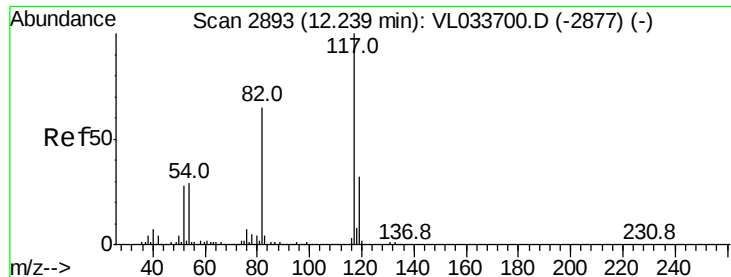

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.23 min Scan# 2889
Delta R.T. -0.01 min
Lab File: VL033799.D
Acq: 28 May 2019 10:28

Instrument :
MSVOA_L
ClientSampleId :
VL0528ABL01

Tot Ion:117 Resp: 2090429
Ion Ratio Lower Upper
117 100
82 66.5 49.4 74.0
119 32.8 24.9 37.3

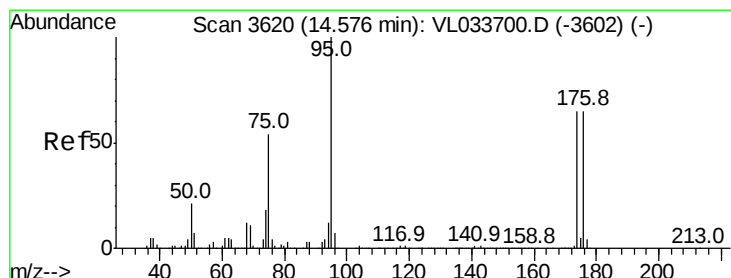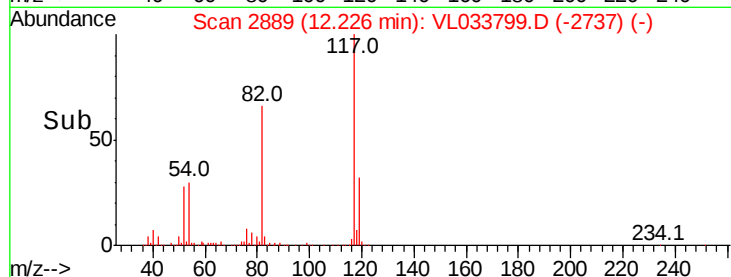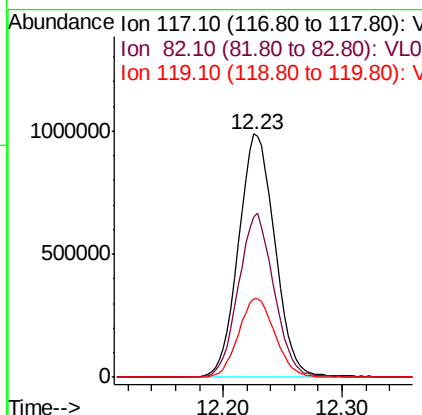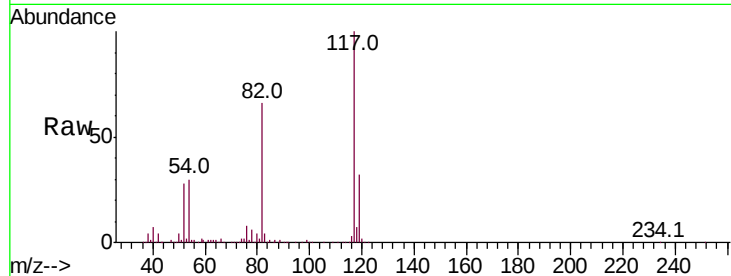

#68
1-Bromo-4-Fluorobenzene
Concen: 10.395 ppbv
RT: 14.57 min Scan# 3617
Delta R.T. -0.01 min
Lab File: VL033799.D
Acq: 28 May 2019 10:28

Tgt Ion: 95 Resp: 1761549
Ion Ratio Lower Upper
95 100
174 67.5 53.9 80.9
175 5.0 3.8 5.8

