


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL052819\
Data File : VL033797.D
Acq On : 28 May 2019 8:14
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL051719AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri May 17 08:15:41 2019
Last Update : Fri May 17 08:15:41 2019

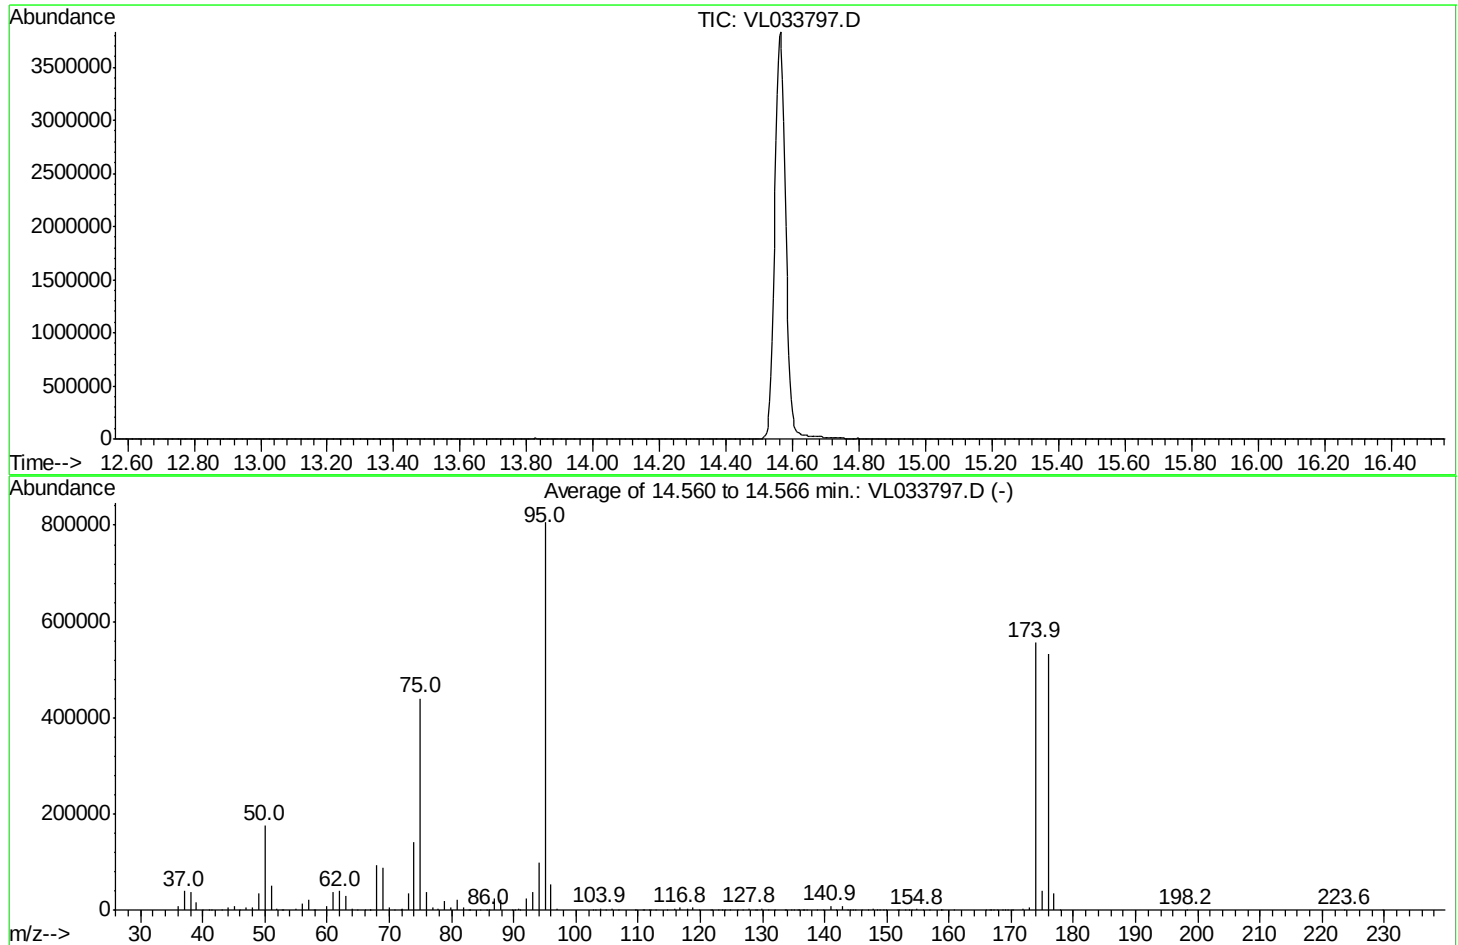

AutoFind: Scans 3615, 3616, 3617; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.7	174869	PASS
75	95	30	66	54.5	439722	PASS
95	95	100	100	100.0	806165	PASS
96	95	5	9	6.5	52680	PASS
173	174	0.00	2	0.8	4461	PASS
174	95	50	120	69.0	555989	PASS
175	174	4	9	7.2	40234	PASS
176	174	93	101	95.5	531200	PASS
177	176	5	9	6.5	34610	PASS