


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL053122\
 Data File : VL039132.D
 Acq On : 31 May 2022 15:33
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

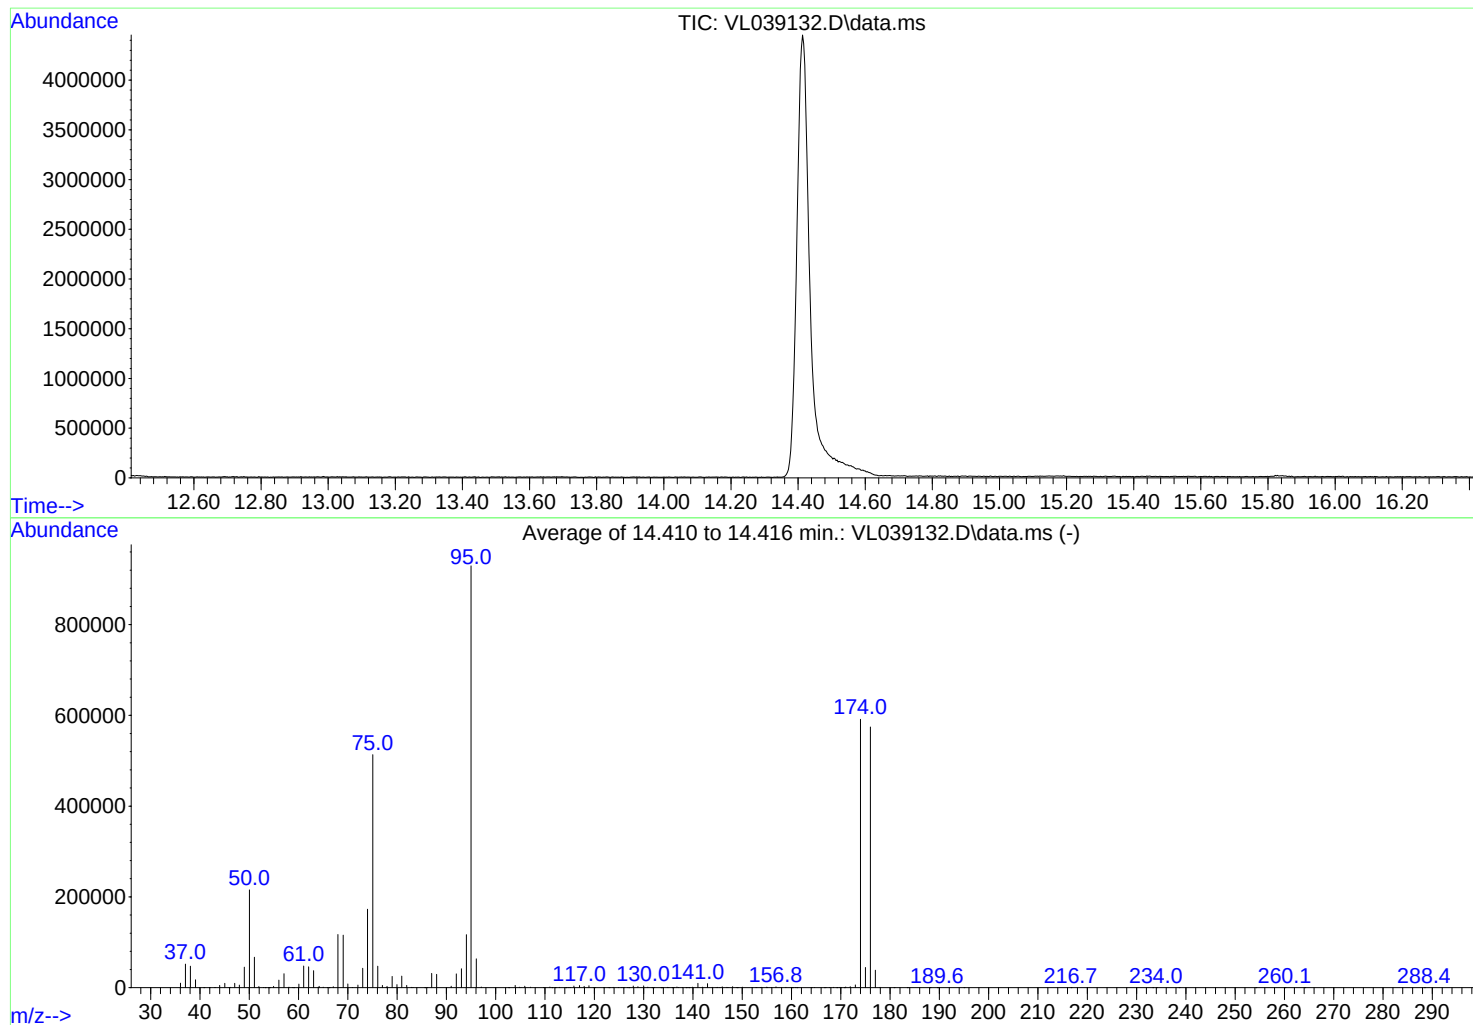

AutoFind: Scans 3615, 3616, 3617; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.2	215339	PASS
75	95	30	66	55.2	513280	PASS
95	95	100	100	100.0	929493	PASS
96	95	5	9	6.8	63571	PASS
173	174	0.00	2	1.0	6175	PASS
174	95	50	120	63.6	591381	PASS
175	174	4	9	7.5	44357	PASS
176	174	93	101	97.1	574443	PASS
177	176	5	9	6.7	38467	PASS

Average of 14.410 to 14.416 min.: VL039132.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9746	45.90	429	54.10	22	64.00	96
37.05	51888	46.15	808	54.95	2850	64.20	268
38.05	47405	47.05	9672	56.00	16634	65.00	92
39.10	17292	48.00	5761	57.05	30605	65.90	21
39.95	530	49.00	44993	58.05	1144	66.20	118
40.80	132	50.05	215339	58.75	278	67.05	2214
41.90	53	51.05	66955	59.00	163	68.00	117197
43.00	219	51.95	2573	60.05	7701	69.05	115781
43.20	196	52.90	258	61.05	47709	70.00	8169
44.00	4815	53.20	59	62.05	46003	70.95	453
45.05	9709	53.90	124	63.05	37517	72.05	5528

Average of 14.410 to 14.416 min.: VL039132.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.00	42565	82.95	714	95.00	929493	109.95	202
74.00	172928	83.20	195	96.05	63571	111.00	1413
75.05	513280	85.60	177	97.05	1444	111.40	174
76.05	47147	85.85	392	102.60	59	112.05	188
77.00	4964	86.20	489	102.75	248	112.90	696
77.80	526	87.00	31283	103.95	5072	114.20	177
77.95	2676	88.00	29368	104.80	1066	114.70	347
79.00	24813	90.95	3366	105.10	444	114.90	334
79.95	6606	92.00	30245	105.90	3292	115.15	510
80.95	25371	93.05	41587	107.05	1150	115.85	3437
81.95	4992	94.05	116589	109.70	238	117.00	4770

Average of 14.410 to 14.416 min.: VL039132.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.95	2786	126.75	397	134.80	792	141.00	9411
118.90	4362	127.00	131	135.10	428	141.95	1157
119.80	277	127.90	3587	135.80	135	142.95	8906
120.00	92	128.85	2096	136.00	155	143.95	561
121.90	130	130.00	4078	136.75	1581	144.70	214
122.80	333	130.85	1191	137.10	471	145.00	544
123.00	59	131.70	169	137.85	274	145.50	282
123.80	638	132.00	72	138.60	127	145.95	1714
124.90	215	133.50	51	139.00	219	146.90	701
125.60	292	133.70	141	139.20	190	147.10	197
125.90	68	134.05	337	139.95	1029	148.05	2090

Average of 14.410 to 14.416 min.: VL039132.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.80	433	156.85	1916	167.75	455	176.00	574443
149.00	175	158.85	749	168.55	548	177.00	38467
150.05	1116	159.90	89	169.20	100	177.95	741
152.00	315	160.20	122	169.85	581	180.80	58
152.80	372	160.75	471	170.10	395	183.50	131
152.95	529	160.90	523	170.70	186	188.10	56
153.70	222	161.10	166	171.00	1319	189.60	115
153.95	584	164.00	58	171.90	2106	195.00	103
154.90	1164	164.65	193	172.95	6175	216.70	150
155.10	609	166.70	116	174.00	591381	233.30	58
155.90	250	167.00	319	175.00	44357	234.00	61

Average of 14.410 to 14.416 min.: VL039132.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
238.60	55						
254.20	54						
260.10	102						
264.10	88						
288.40	102						