


Data Path : W:\HPCHEM1\MSVOA L\Data\VL060118\
 Data File : VL032024.D
 Acq On : 1 Jun 2018 15:18
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL053118AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jun 01 02:31:35 2018
 Last Update : Fri Jun 01 02:31:35 2018

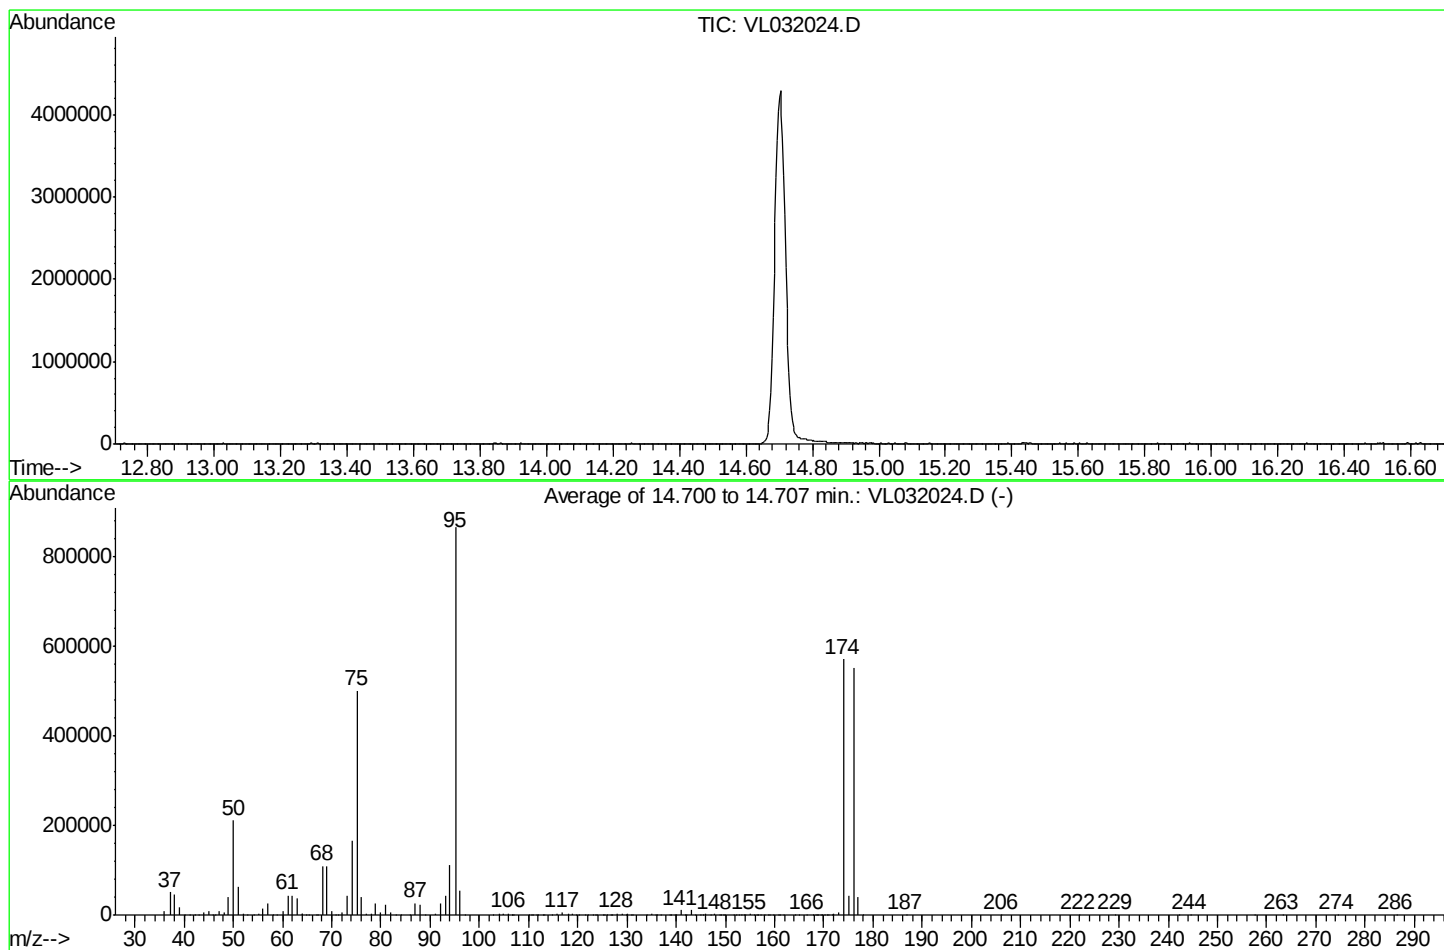

AutoFind: Scans 4234, 4235, 4236; Background Corrected with Scan 4212

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	210282	PASS
75	95	30	66	57.9	501461	PASS
95	95	100	100	100.0	865728	PASS
96	95	5	9	6.4	55226	PASS
173	174	0.00	2	1.1	6186	PASS
174	95	50	120	66.0	571008	PASS
175	174	4	9	7.6	43341	PASS
176	174	93	101	96.4	550677	PASS
177	176	5	9	7.1	38970	PASS