


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060122\
 Data File : VL039141.D
 Acq On : 1 Jun 2022 8:38
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

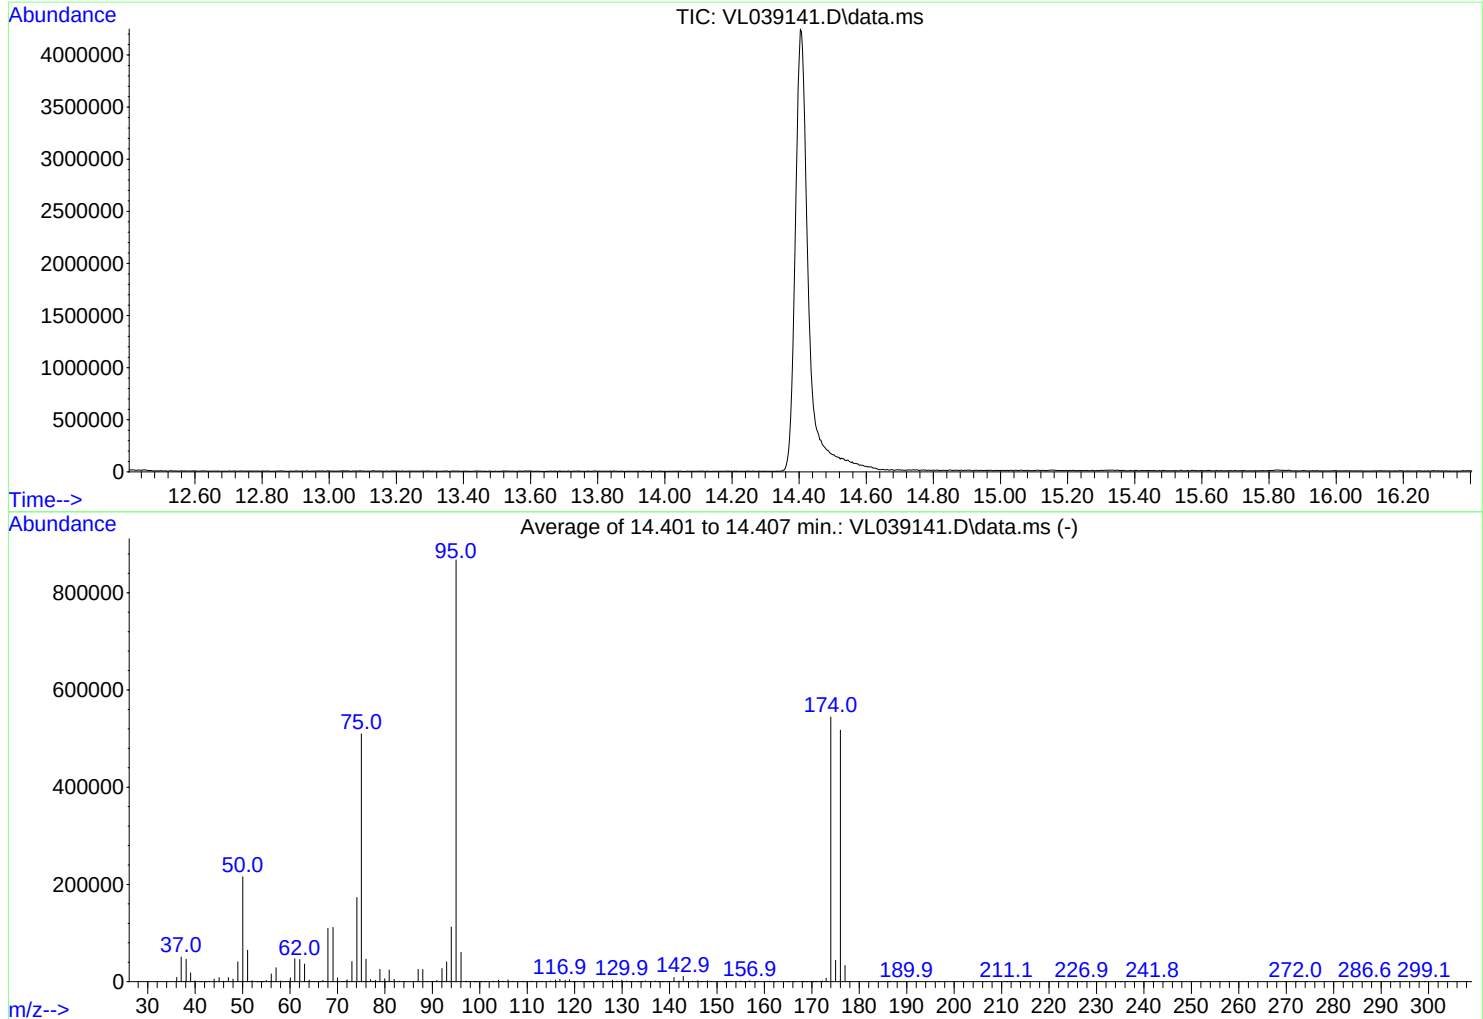

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.8	215509	PASS
75	95	30	66	58.7	509803	PASS
95	95	100	100	100.0	867840	PASS
96	95	5	9	6.9	60155	PASS
173	174	0.00	2	1.3	7153	PASS
174	95	50	120	62.8	544576	PASS
175	174	4	9	8.0	43773	PASS
176	174	93	101	95.1	517653	PASS
177	176	5	9	6.4	33293	PASS

Average of 14.401 to 14.407 min.: VL039141.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	8630	47.00	8180	57.05	28539	66.30	131
37.05	50605	48.00	5254	58.00	1477	66.95	268
38.10	45989	49.00	40763	59.00	237	68.00	10960
39.05	18265	50.05	215509	60.05	8052	69.05	11151
39.95	1684	51.05	64536	61.00	47003	70.00	8060
41.20	54	52.00	2077	62.05	45541	71.10	288
42.20	183	53.05	171	63.05	36339	71.30	216
43.05	674	53.80	80	64.05	3479	71.90	1426
44.00	5259	54.20	80	64.85	375	72.05	3679
45.05	8371	55.00	2547	65.15	333	73.05	41368
46.00	887	56.05	15988	65.95	226	74.10	173312

Average of 14.401 to 14.407 min.: VL039141.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.05	509803	86.05	1034	97.20	1108	105.95	3773
76.00	46267	87.00	25445	98.80	50	106.80	260
77.00	4433	88.00	25021	99.10	89	107.05	853
77.50	517	88.70	309	99.80	64	108.00	207
78.05	2766	90.95	2687	100.30	51	109.00	107
78.95	25429	92.05	27075	101.00	90	110.00	294
79.95	5948	93.00	40693	102.70	182	110.95	980
80.90	24131	94.00	112224	102.95	304	112.05	622
81.95	4901	95.00	867840	103.95	2880	112.90	550
83.00	919	96.05	60155	104.90	1162	114.95	1202
84.20	202	97.00	426	105.10	352	115.95	3261

Average of 14.401 to 14.407 min.: VL039141.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.90	4807	124.90	593	134.95	1644	142.00	1413
118.00	3102	125.90	515	135.80	261	142.90	10869
118.90	4094	126.95	442	137.00	1474	143.80	506
119.80	163	127.95	3015	137.60	63	144.10	388
121.75	137	128.90	1289	138.00	89	144.90	892
122.20	117	129.95	2950	138.50	152	145.95	1869
122.90	197	131.00	1329	138.95	440	146.60	183
123.10	83	131.70	59	139.50	107	146.80	485
123.60	93	131.90	63	139.90	362	148.00	2133
123.80	317	133.40	57	140.10	221	148.80	558
124.10	358	134.05	190	140.95	8620	149.80	348

Average of 14.401 to 14.407 min.: VL039141.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
150.05	613	157.90	151	170.70	173	178.05	540
151.60	179	158.10	164	171.00	571	186.30	53
152.15	290	158.80	877	171.50	458	189.95	314
152.70	284	161.10	1020	171.90	590	193.20	209
153.00	534	161.80	54	172.20	1762	196.70	51
153.95	538	165.00	61	173.00	7153	211.05	121
154.90	1262	166.20	71	174.00	544576	213.60	89
155.10	607	168.20	173	175.00	43773	214.60	64
155.70	97	168.90	44	176.00	517653	225.00	51
155.90	465	169.60	854	177.00	33293	226.90	130
156.95	1566	170.20	71	177.80	338	235.00	53

Average of 14.401 to 14.407 min.: VL039141.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
241.80	104						
272.00	94						
274.30	59						
286.60	115						
292.70	83						
299.10	64						