

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL060221\
 Data File : VL037106.D
 Acq On : 2 Jun 2021 17:53
 Operator : SY/AP
 Sample : M2548-10
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Quant Time: Jun 03 03:21:47 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL051821AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue May 18 12:00:15 2021
 QLast Update : Tue May 18 12:00:15 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.65	49	1324277	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.16	114	3929732	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.07	117	3584787	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.40	95	2712178	10.07	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.70%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.04	85	58026	0.258	ppbv	91
3) Chlorodifluoromethane	2.95	51	300617	1.239	ppbv #	68
4) Chloromethane	3.13	50	50300	0.609	ppbv	91
9) Propene	3.20	41	944389	10.871	ppbv	97
10) Heptane	8.11	43	17132	0.079	ppbv #	33
11) Trichlorofluoromethane	3.94	101	47494	0.228	ppbv	97
12) 1,1,2-Trichlorotrifluoroet	4.47	101	10387	0.070	ppbv	88
13) Ethanol	3.61	45	12595188	1086.618	ppbv	97
15) Acetone	3.84	43	1319683	9.729	ppbv #	75
16) 1,3-Butadiene	3.30	39	12506	0.148	ppbv #	10
17) tert-Butyl alcohol	3.97	59	662797	5.334	ppbv	97
19) Isopropyl Alcohol	3.97	45	15154433	207.840	ppbv #	33
20) Methylene Chloride	4.33	84	695038	9.559	ppbv	96
21) Allyl Chloride	4.17	41	48142	0.470	ppbv #	1
23) Vinyl Acetate	5.05	43	92079	0.428	ppbv #	53
25) Ethyl Acetate	5.67	43	725423	2.226	ppbv #	79
26) Hexane	5.67	57	1016027	6.102	ppbv #	47
29) Chloroform	5.74	83	126966	0.540	ppbv	92
30) Cyclohexane	7.11	84	5210	0.037	ppbv #	1
34) 2-Butanone	5.23	43	119356	0.834	ppbv	92
35) Carbon Tetrachloride	7.00	117	15418	0.059	ppbv #	84
36) Benzene	6.87	78	77284	0.228	ppbv	98
38) Trichloroethene	7.82	130	40121	0.277	ppbv	89
39) 1,2-Dichloropropane	7.16	63	914490	7.013	ppbv #	26
41) Tetrahydrofuran	5.67	42	373445	4.582	ppbv #	50
50) 4-Methyl-2-Pentanone	8.74	43	76917	0.326	ppbv	100
53) Toluene	9.79	91	1419498	3.524	ppbv	97
58) Ethyl Benzene	12.69	91	42759	0.085	ppbv	90
59) m/p-Xylene	12.98	91	12727	0.030	ppbv #	30
60) o-Xylene	13.68	91	17432	0.044	ppbv #	28
61) Styrene	13.51	104	28405	0.126	ppbv #	28
74) 1,2,4-Trimethylbenzene	16.75	105	25626	0.056	ppbv #	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.65 min Scan# 892

Delta R.T. 0.01 min


Lab File: VL037106.D

Acq: 2 Jun 2021 17:53

Instrument :
MSVOA_L
ClientSampleId :

Tot Ion: 49 Resp: 1324277


Ion	Ratio	Lower	Upper
49	100		
128	57.2	26.9	80.7
130	74.4	33.8	101.4

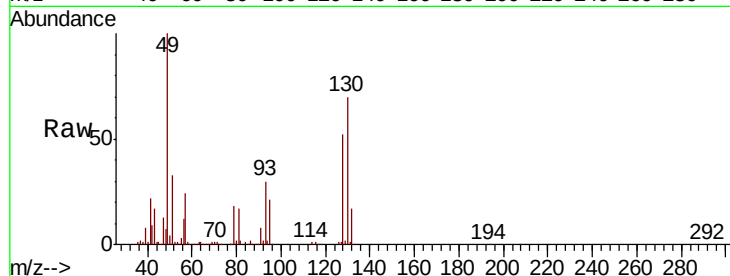


Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V



Time-->



#2

Dichlorodifluoromethane

Concen: 0.258 ppbv

RT: 3.04 min Scan# 78


Delta R.T. 0.00 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53


Tgt Ion: 85 Resp: 58026

Ion	Ratio	Lower	Upper
85	100		
87	38.4	26.6	39.8




Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0



Time-->

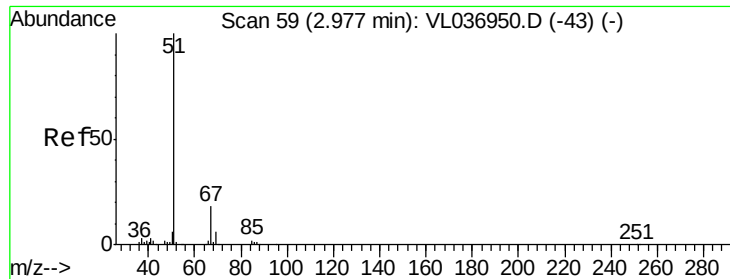

#3

Chlorodifluoromethane

Concen: 1.239 ppbv

RT: 2.95 min Scan# 52

Delta R.T. -0.02 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53

Instrument :

MSVOA_L


ClientSampled :

Tot Ion: 51 Resp: 300617

Ion Ratio Lower Upper

51 100

67 4.1 14.6 21.8#



Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

150000



100000

50000

0

2.80 2.90 3.00 3.10

Time-->



#4

Chloromethane

Concen: 0.609 ppbv

RT: 3.13 min Scan# 107

Delta R.T. 0.00 min

Lab File: VL037106.D


Acq: 2 Jun 2021 17:53

Tgt Ion: 50 Resp: 50300

Ion Ratio Lower Upper

50 100

52 27.7 26.1 39.1



Abundance Ion 50.10 (49.80 to 50.80): VL0

Ion 52.10 (51.80 to 52.80): VL0

30000


20000


10000

0

3.10 3.15

Time-->



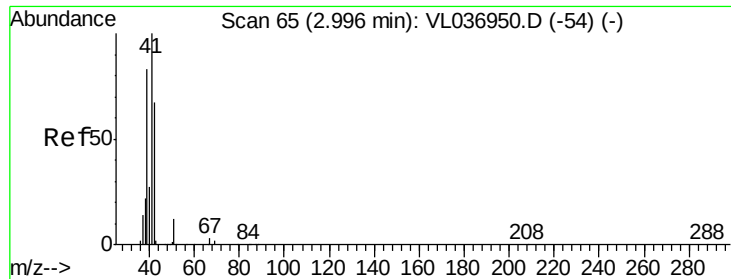

#9

Propene

Concen: 10.871 ppbv

RT: 3.20 min Scan# 127

Delta R.T. 0.20 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53

Instrument :

MSVOA_L





ClientSampleId :

Tot Ion: 41 Resp: 944389

Ion Ratio Lower Upper

41 100

42 64.7 53.9 80.9

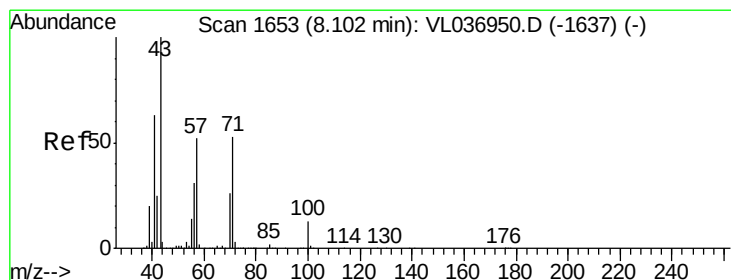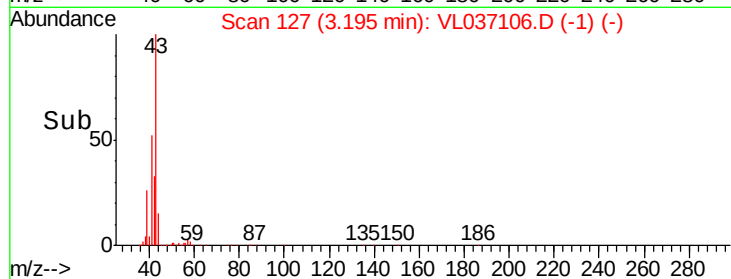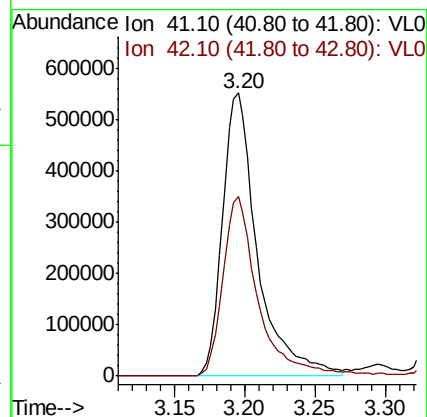

#10

Heptane

Concen: 0.079 ppbv

RT: 8.11 min Scan# 1655

Delta R.T. 0.01 min

Lab File: VL037106.D




Acq: 2 Jun 2021 17:53


Tgt Ion: 43 Resp: 17132

Ion Ratio Lower Upper

43 100

57 97.8 41.0 61.6#



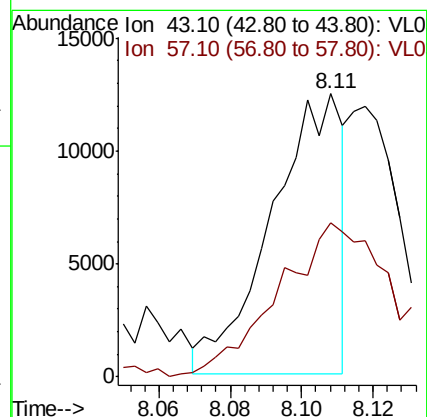
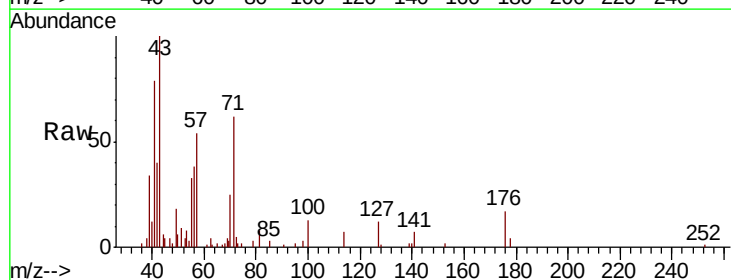




#11
 Trichlorofluoromethane
 Concen: 0.228 ppbv
 RT: 3.94 min Scan# 358
 Delta R.T. 0.00 min
 Lab File: VL037106.D
 Acq: 2 Jun 2021 17:53




Instrument :
 MSVOA_L
 ClientSampleId :


Tot Ion:101 Resp: 47494
 Ion Ratio Lower Upper
 101 100
 103 68.0 52.6 79.0

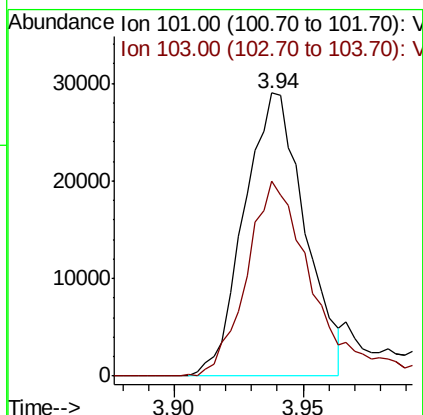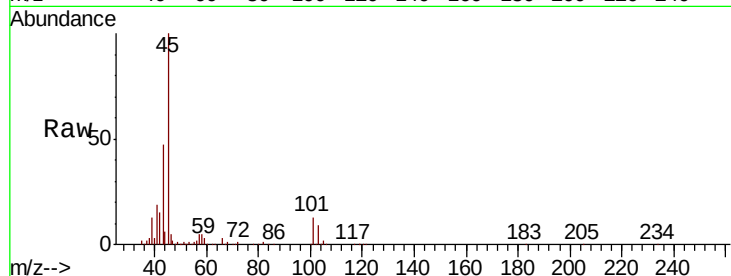

#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.070 ppbv
 RT: 4.47 min Scan# 525
 Delta R.T. 0.01 min
 Lab File: VL037106.D
 Acq: 2 Jun 2021 17:53

Tgt Ion:101 Resp: 10387
 Ion Ratio Lower Upper
 101 100
 151 82.3 57.7 86.5

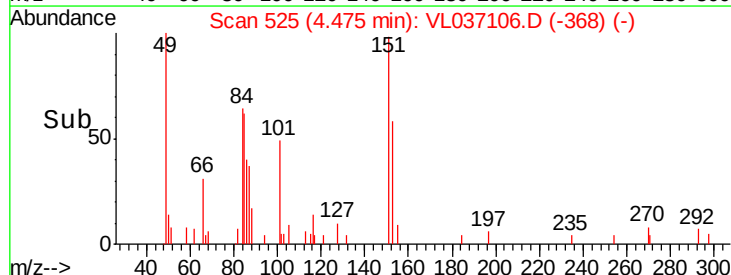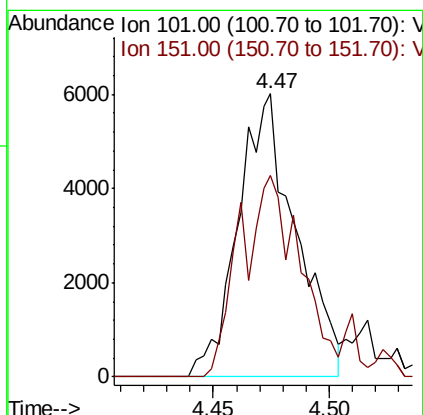

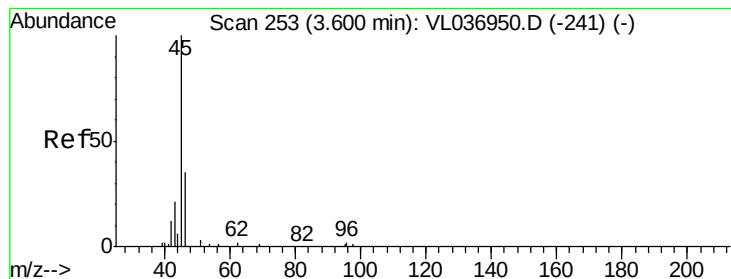

#13

Ethanol

Concen: 1086.618 ppbv

RT: 3.61 min Scan# 255

Delta R.T. 0.01 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53

Instrument :

MSVOA_L





ClientSampleId :

Tot Ion: 45 Resp:12595188

Ion Ratio Lower Upper

45 100

46 38.8 16.3 65.3

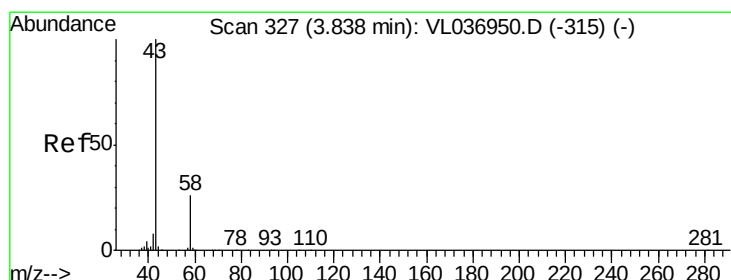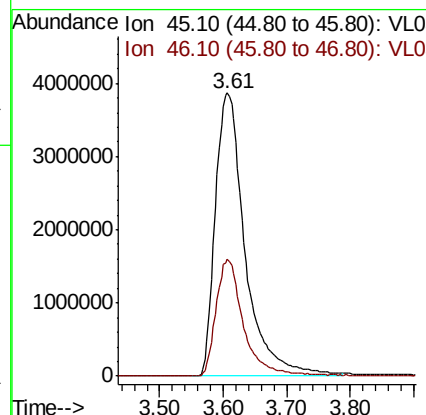

#15

Acetone

Concen: 9.729 ppbv

RT: 3.84 min Scan# 327

Delta R.T. -0.00 min

Lab File: VL037106.D




Acq: 2 Jun 2021 17:53


Tgt Ion: 43 Resp: 1319683

Ion Ratio Lower Upper

43 100

58 43.3 24.0 36.0#


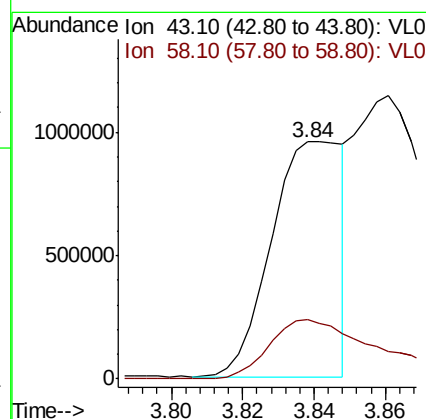






#16
 1,3-Butadiene
 Concen: 0.148 ppbv
 RT: 3.30 min Scan# 159
 Delta R.T. -0.02 min
 Lab File: VL037106.D
 Acq: 2 Jun 2021 17:53




Instrument :
 MSVOA_L
 ClientSampleId :


Tot Ion: 39 Resp: 12506
 Ion Ratio Lower Upper
 39 100
 54 0.0 63.2 94.8#

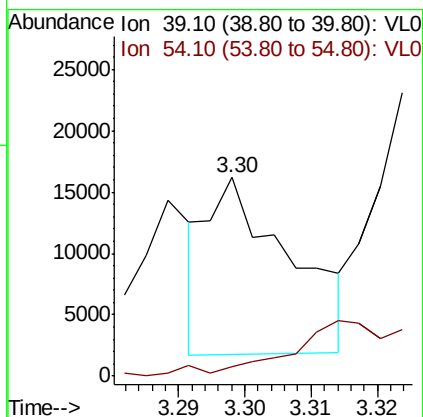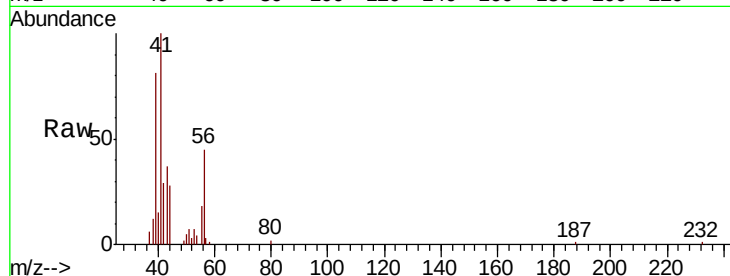

#17
 tert-Butyl alcohol
 Concen: 5.334 ppbv
 RT: 3.97 min Scan# 369
 Delta R.T. -0.30 min
 Lab File: VL037106.D
 Acq: 2 Jun 2021 17:53

Tgt Ion: 59 Resp: 662797
 Ion Ratio Lower Upper
 59 100
 57 11.6 8.3 12.5



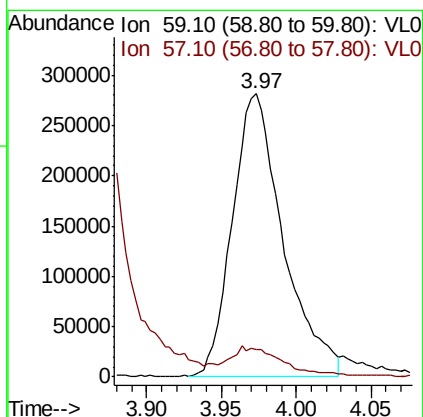





#19
Isopropyl Alcohol
Concen: 207.840 ppbv
RT: 3.97 min Scan# 369
Delta R.T. 0.02 min
Lab File: VL037106.D
Acq: 2 Jun 2021 17:53




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 45 Resp:15154433
Ion Ratio Lower Upper
45 100
58 1.7 37.2 55.8#

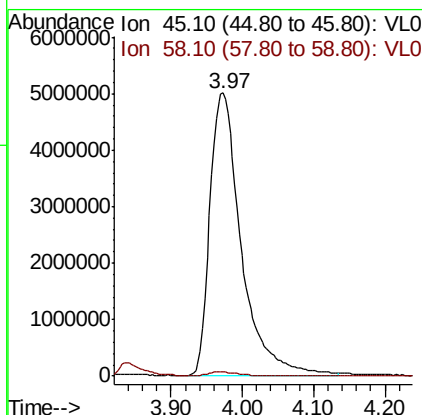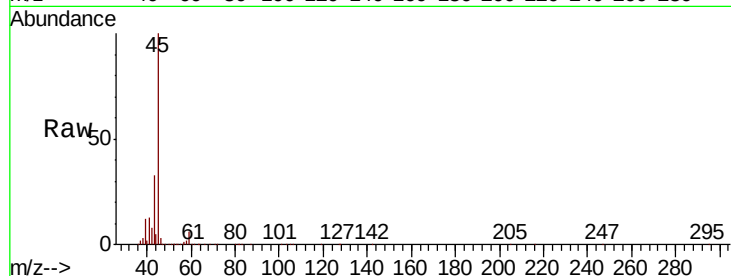

#20
Methylene Chloride
Concen: 9.559 ppbv
RT: 4.33 min Scan# 481
Delta R.T. 0.01 min
Lab File: VL037106.D
Acq: 2 Jun 2021 17:53

Tgt Ion: 84 Resp: 695038
Ion Ratio Lower Upper
84 100
49 143.9 119.8 179.6
51 43.2 35.1 52.7
86 59.2 50.9 76.3

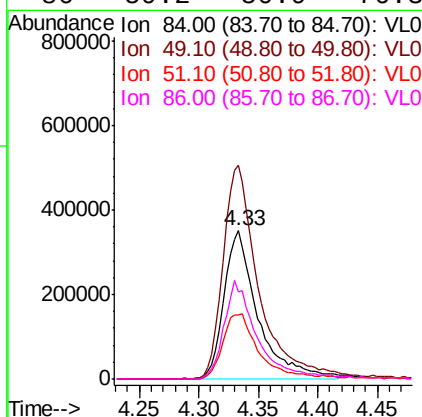



#21

Allvl Chloride

Concen: 0.470 ppbv

RT: 4.17 min Scan# 431

Delta R.T. -0.22 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53

Instrument :

MSVOA_L

ClientSampleId :


Tot Ion: 41 Resp: 48142

Ion Ratio Lower Upper




41 100

76 14.5 24.9 37.3#

39 210.7 63.7 95.5#

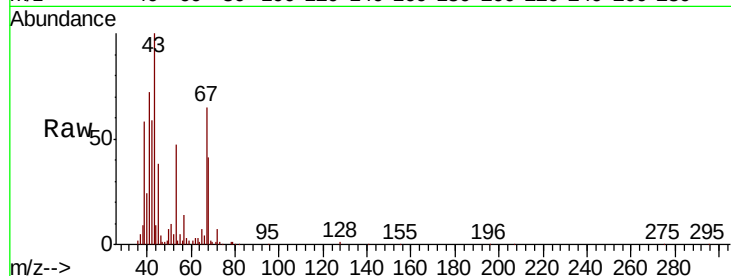

Abundance Ion 41.10 (40.80 to 41.80): VL0
Ion 76.10 (75.80 to 76.80): VL0
Ion 39.10 (38.80 to 39.80): VL0

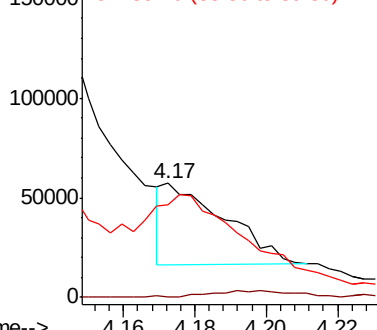

#23

Vinyl Acetate

Concen: 0.428 ppbv

RT: 5.05 min Scan# 704

Delta R.T. -0.01 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53

Tgt Ion: 43 Resp: 92079


Ion Ratio Lower Upper

43 100



86 9.9 5.8 8.8#


42 43.3 7.4 11.2#

44 0.0 3.3 4.9#



Abundance Ion 43.10 (42.80 to 43.80): VL0
Ion 86.10 (85.80 to 86.80): VL0
Ion 42.10 (41.80 to 42.80): VL0
Ion 44.10 (43.80 to 44.80): VL0



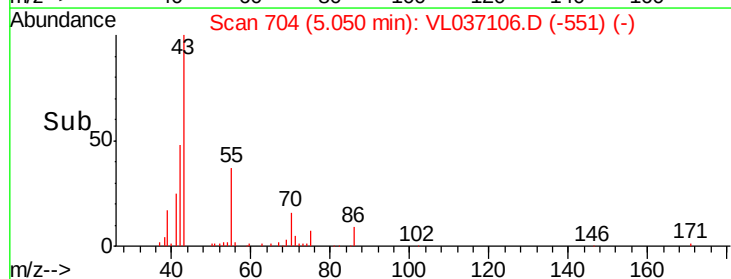
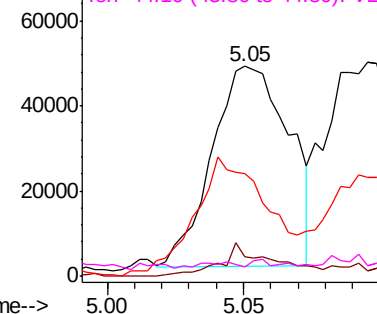




#25
Ethyl Acetate
Concen: 2.226 ppbv
RT: 5.67 min Scan# 898
Delta R.T. 0.01 min
Lab File: VL037106.D
Acq: 2 Jun 2021 17:53




Instrument :
MSVOA_L
ClientSampled :


Tot Ion:	43	Resp:	725423
Ion	Ratio	Lower	Upper
43	100		
45	1.3	7.8	11.8#
61	0.7	7.8	11.8#
70	1.9	5.6	8.4#

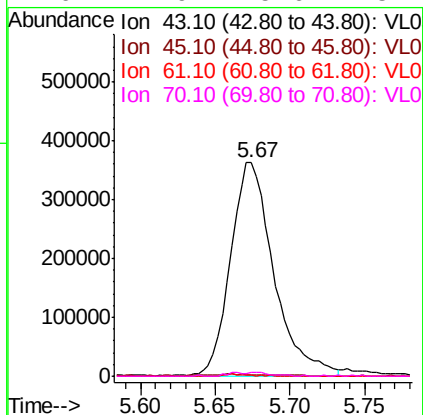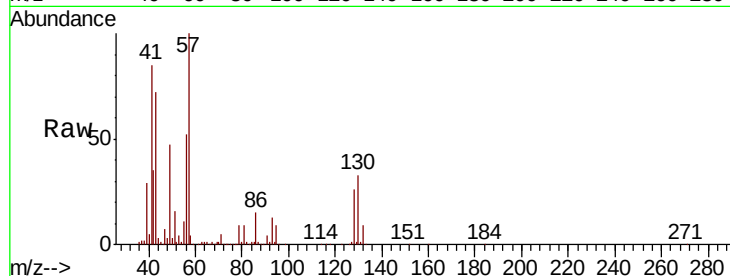

#26
Hexane
Concen: 6.102 ppbv
RT: 5.67 min Scan# 898
Delta R.T. 0.01 min
Lab File: VL037106.D
Acq: 2 Jun 2021 17:53

Tgt Ion:	57	Resp:	1016027
Ion	Ratio	Lower	Upper
57	100		
41	93.7	70.5	105.7
43	73.6	165.8	248.8#
56	53.8	42.2	63.4



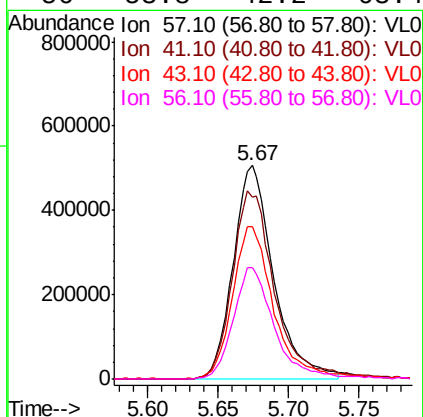



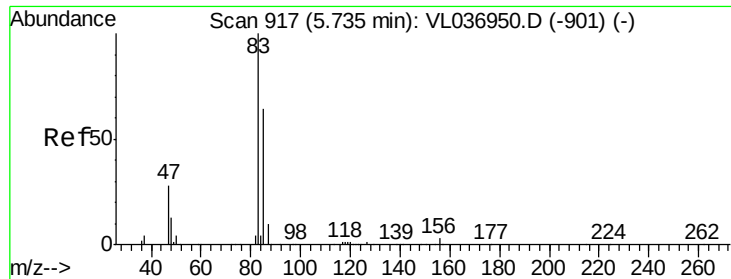

#29
Chloroform
Concen: 0.540 ppbv
RT: 5.74 min Scan# 918
Delta R.T. 0.00 min
Lab File: VL037106.D
Acq: 2 Jun 2021 17:53




Instrument :
MSVOA_L
ClientSampled :


Tot Ion: 83 Resp: 126966
Ion Ratio Lower Upper
83 100
85 57.9 51.1 76.7

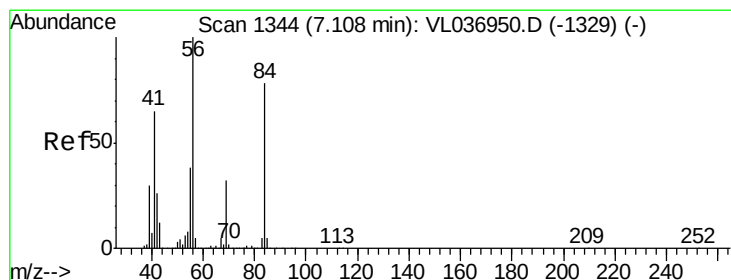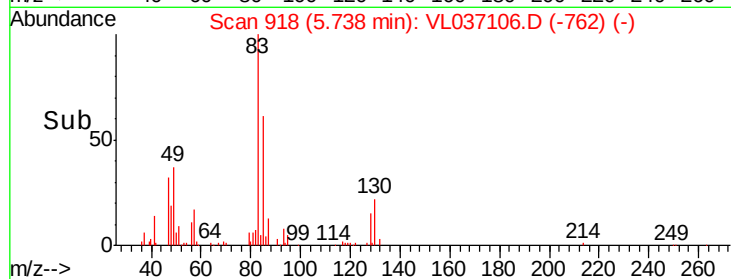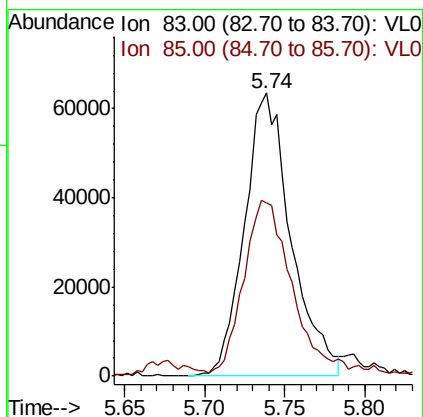

#30
Cyclohexane
Concen: 0.037 ppbv
RT: 7.11 min Scan# 1346
Delta R.T. 0.01 min
Lab File: VL037106.D
Acq: 2 Jun 2021 17:53

Tgt Ion: 84 Resp: 5210
Ion Ratio Lower Upper
84 100
56 0.0 107.9 161.9#
41 267.9 65.5 98.3#



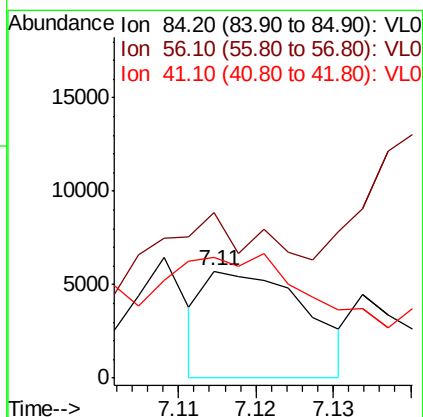
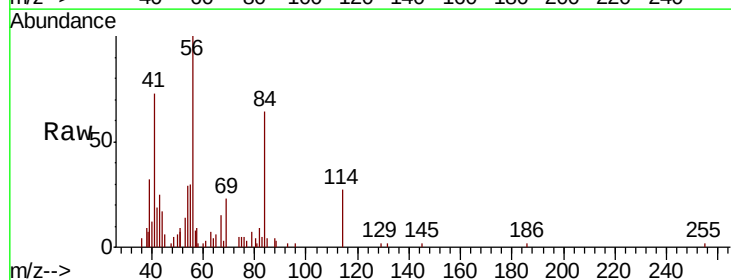




#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.16 min Scan# 1360
 Delta R.T. 0.00 min
 Lab File: VL037106.D
 Acq: 2 Jun 2021 17:53




Instrument :
 MSVOA_L
 ClientSampleId :


Tot Ion:114 Resp: 3929732
 Ion Ratio Lower Upper
 114 100
 63 24.1 19.6 29.4
 88 17.9 14.6 21.8

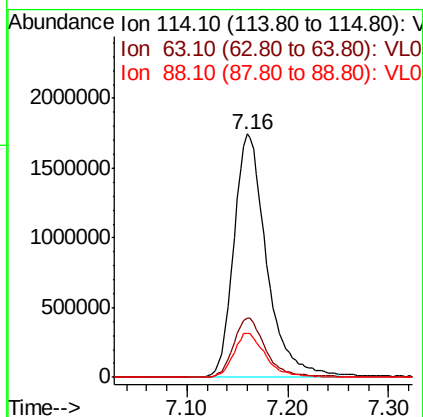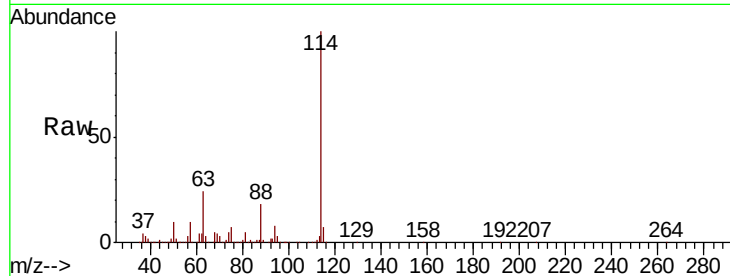

#34
 2-Butanone
 Concen: 0.834 ppbv
 RT: 5.23 min Scan# 761
 Delta R.T. 0.00 min
 Lab File: VL037106.D
 Acq: 2 Jun 2021 17:53

Tgt Ion: 43 Resp: 119356
 Ion Ratio Lower Upper
 43 100
 72 27.6 19.0 28.4

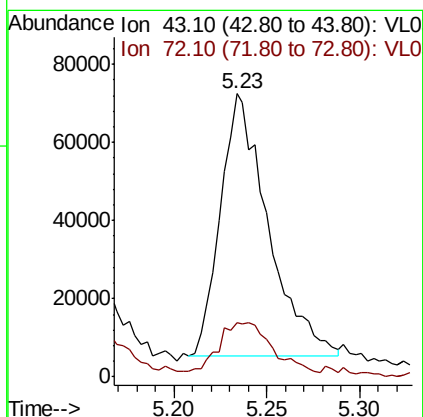



#35

Carbon Tetrachloride

Concen: 0.059 ppbv

RT: 7.00 min Scan# 1309

Delta R.T. -0.00 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53

Instrument :

MSVOA_L

ClientSampleId :


Tot Ion:117 Resp: 15418

Ion Ratio Lower Upper




117 100

119 76.3 76.6 114.8#

121 35.3 25.8 38.6



Abundance Ion 117.00 (116.70 to 117.70): V
Ion 119.00 (118.70 to 119.70): V
Ion 121.00 (120.70 to 121.70): V

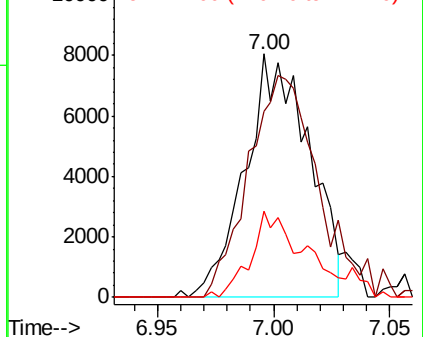

#36

Benzene

Concen: 0.228 ppbv

RT: 6.87 min Scan# 1271

Delta R.T. 0.00 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53


Tgt Ion: 78 Resp: 77284

Ion Ratio Lower Upper



78 100


77 22.9 18.6 28.0

50 17.2 15.0 22.4



Abundance Ion 78.10 (77.80 to 78.80): VL0
Ion 77.10 (76.80 to 77.80): VL0
Ion 50.10 (49.80 to 50.80): VL0

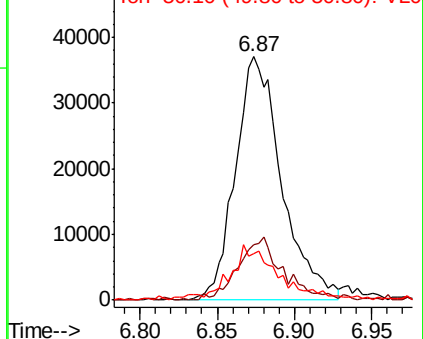



#38

Trichloroethene

Concen: 0.277 ppbv

RT: 7.82 min Scan# 1565

Delta R.T. 0.01 min

Lab File: VL037106.D


Acq: 2 Jun 2021 17:53

Instrument :

MSVOA_L

ClientSampleId :

Tot Ion:130	Resp:	40121
Ion Ratio	Lower	Upper
130	100	
95	98.0	86.9 130.3
132	112.5	78.4 117.6
97	75.5	55.0 82.6



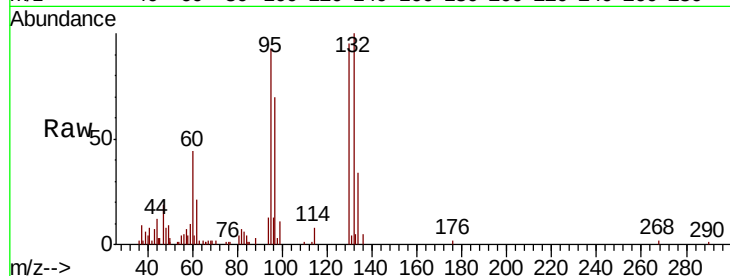


Abundance Ion 130.00 (129.70 to 130.70): V

Ion 95.00 (94.70 to 95.70): VL0

Ion 132.00 (131.70 to 132.70): V

Ion 97.00 (96.70 to 97.70): VL0

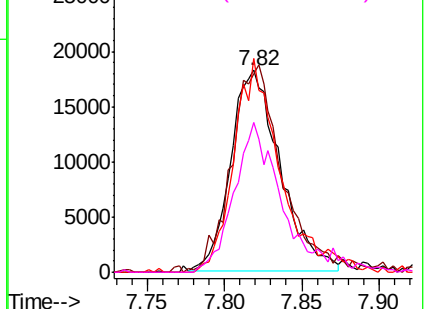

#39

1,2-Dichloropropane

Concen: 7.013 ppbv


RT: 7.16 min Scan# 1361

Delta R.T. -0.43 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53



Tgt Ion: 63	Resp:	914490
Ion Ratio	Lower	Upper
63	100	
41	0.0	55.7 83.5#
62	18.5	56.2 84.4#




Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 62.10 (61.80 to 62.80): VL0



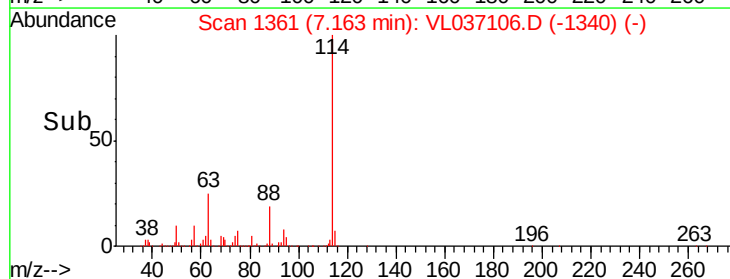
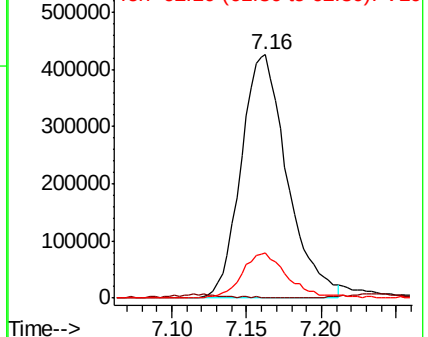




#41
Tetrahydrofuran
Concen: 4.582 ppbv
RT: 5.67 min Scan# 897
Delta R.T. -0.36 min
Lab File: VL037106.D
Acq: 2 Jun 2021 17:53




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 42 Resp: 373445
Ion Ratio Lower Upper
42 100
72 1.2 31.4 47.2#
71 15.9 30.4 45.6#

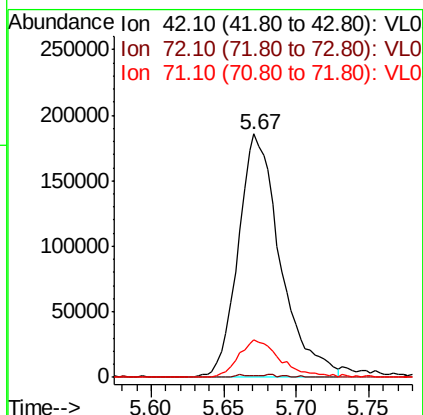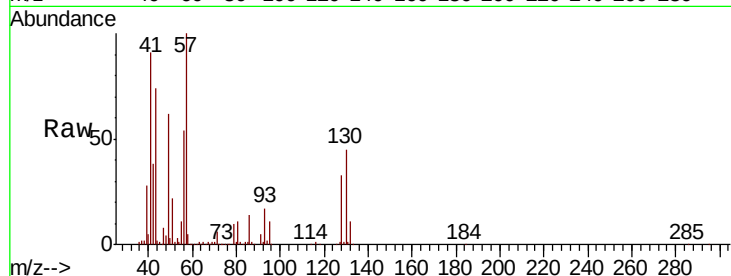

#50
4-Methyl-2-Pentanone
Concen: 0.326 ppbv
RT: 8.74 min Scan# 1850
Delta R.T. 0.01 min
Lab File: VL037106.D
Acq: 2 Jun 2021 17:53

Tgt Ion: 43 Resp: 76917
Ion Ratio Lower Upper
43 100
58 37.0 29.4 44.2

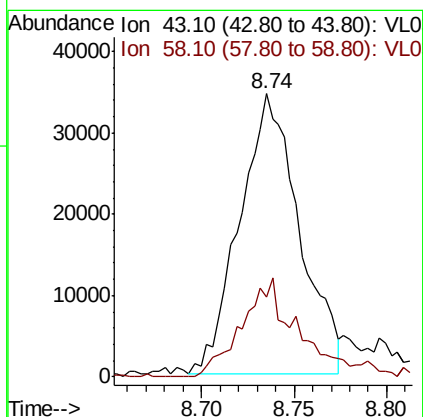



#53

Toluene

Concen: 3.524 ppbv

RT: 9.79 min Scan# 2178

Delta R.T. 0.01 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53

Instrument :

MSVOA_L


ClientSampleId :

Tot Ion: 91 Resp: 1419498

Ion Ratio Lower Upper


91 100

92 59.6 49.5 74.3





Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 92.10 (91.80 to 92.80): VL0

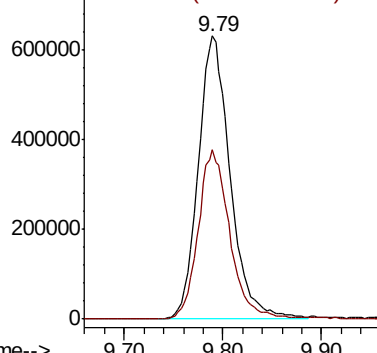

Time-->

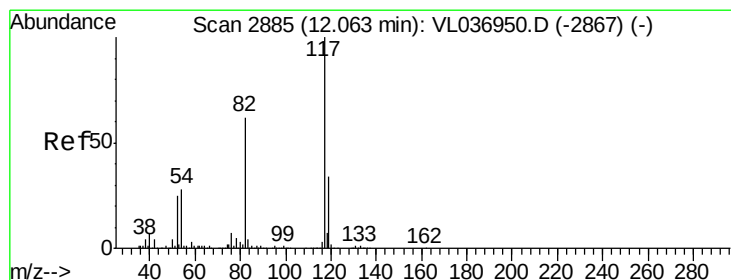

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.07 min Scan# 2887

Delta R.T. 0.01 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53


Tgt Ion: 117 Resp: 3584787

Ion Ratio Lower Upper

117 100

82 63.1 52.6 79.0


119 34.3 46.6 70.0#




Abundance Ion 117.10 (116.80 to 117.80): V


Ion 82.10 (81.80 to 82.80): VL0

Ion 119.10 (118.80 to 119.80): V

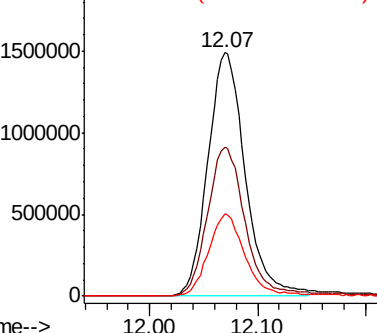

Time-->





#58

Ethyl Benzene

Concen: 0.085 ppbv

RT: 12.69 min Scan# 3080

Delta R.T. 0.00 min

Lab File: VL037106.D

Acq: 2 Jun 2021 17:53

Instrument :

MSVOA_L





ClientSampleId :

Tot Ion: 91 Resp: 42759

Ion Ratio Lower Upper

91 100

106 26.4 25.6 38.4

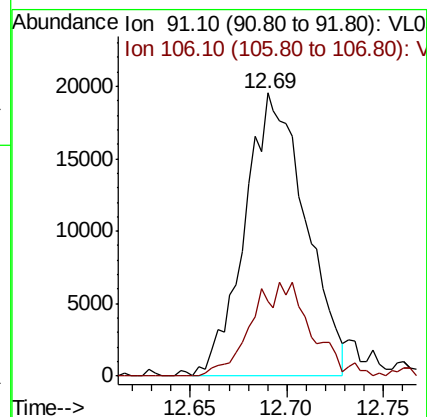

#59

m/p-Xylene

Concen: 0.030 ppbv

RT: 12.98 min Scan# 3170

Delta R.T. 0.01 min

Lab File: VL037106.D




Acq: 2 Jun 2021 17:53


Tgt Ion: 91 Resp: 12727

Ion Ratio Lower Upper

91 100

106 0.0 37.4 56.2#



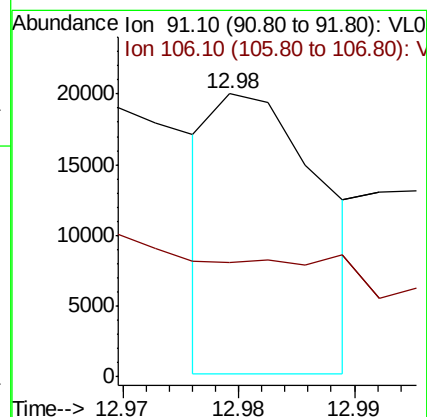



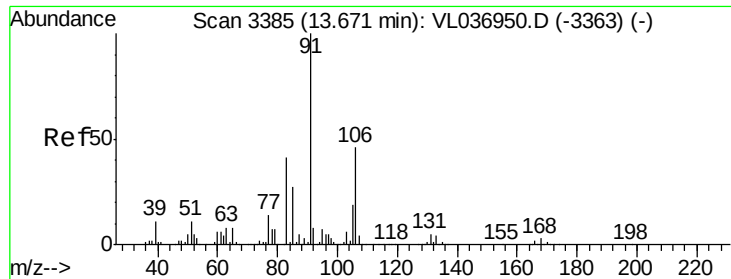

#60
o-Xylene
Concen: 0.044 ppbv
RT: 13.68 min Scan# 3387
Delta R.T. 0.01 min
Lab File: VL037106.D
Acq: 2 Jun 2021 17:53




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 91 Resp: 17432
Ion Ratio Lower Upper
91 100
106 95.2 23.4 70.3#

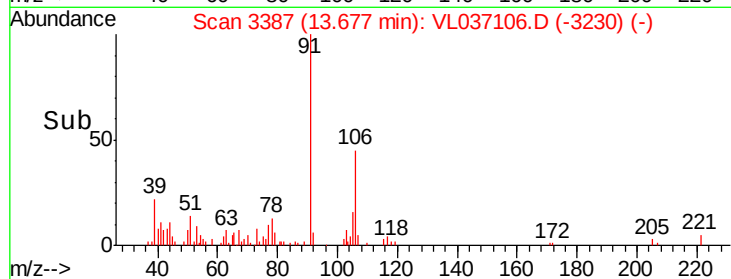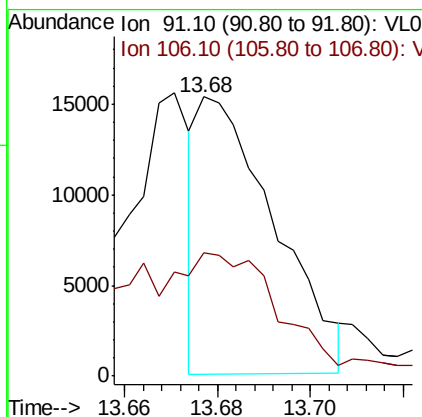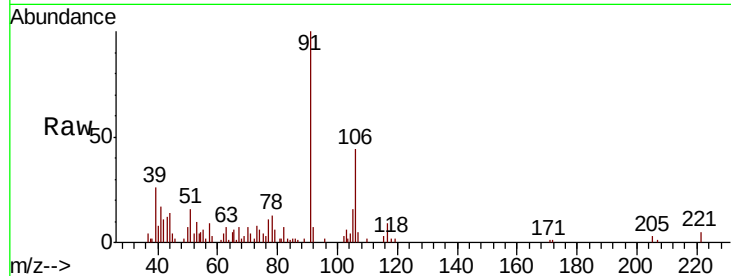

#61
Styrene
Concen: 0.126 ppbv
RT: 13.51 min Scan# 3336
Delta R.T. 0.01 min
Lab File: VL037106.D
Acq: 2 Jun 2021 17:53

Tgt Ion:104 Resp: 28405
Ion Ratio Lower Upper
104 100
78 102.6 39.0 58.6#
103 91.6 38.0 57.0#



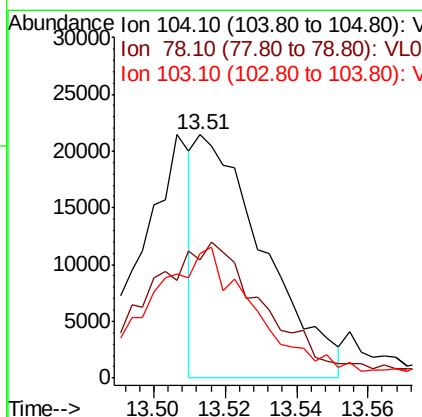



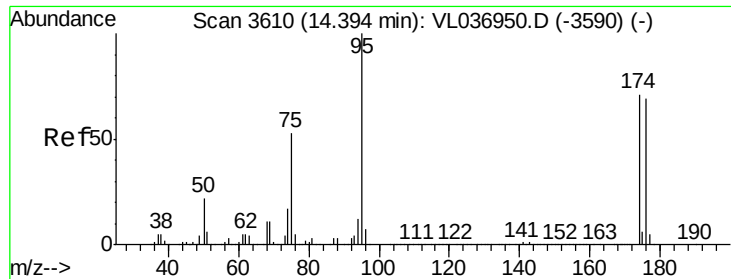

#68
 1-Bromo-4-Fluorobenzene
 Concen: 10.071 ppbv
 RT: 14.40 min Scan# 3612
 Delta R.T. 0.01 min
 Lab File: VL037106.D
 Acq: 2 Jun 2021 17:53

Instrument :
 MSVOA_L
 ClientSampled :

Tot Ion: 95 Resp: 2712178
 Ion Ratio Lower Upper
 95 100
 174 73.2 58.4 87.6
 175 5.5 4.4 6.6

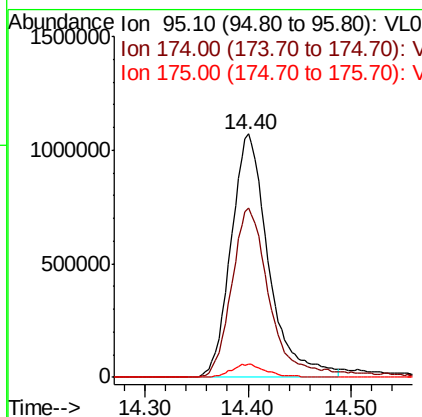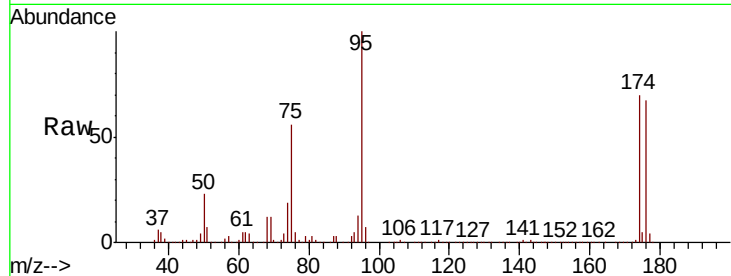

#74
 1,2,4-Trimethylbenzene
 Concen: 0.056 ppbv
 RT: 16.75 min Scan# 4342
 Delta R.T. 0.01 min
 Lab File: VL037106.D
 Acq: 2 Jun 2021 17:53

Tgt Ion:105 Resp: 25626
 Ion Ratio Lower Upper
 105 100
 120 44.9 40.6 61.0
 91 11.8 37.4 56.0#
 77 11.1 16.2 24.4#

