


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060322\
 Data File : VL039153.D
 Acq On : 3 Jun 2022 14:31
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

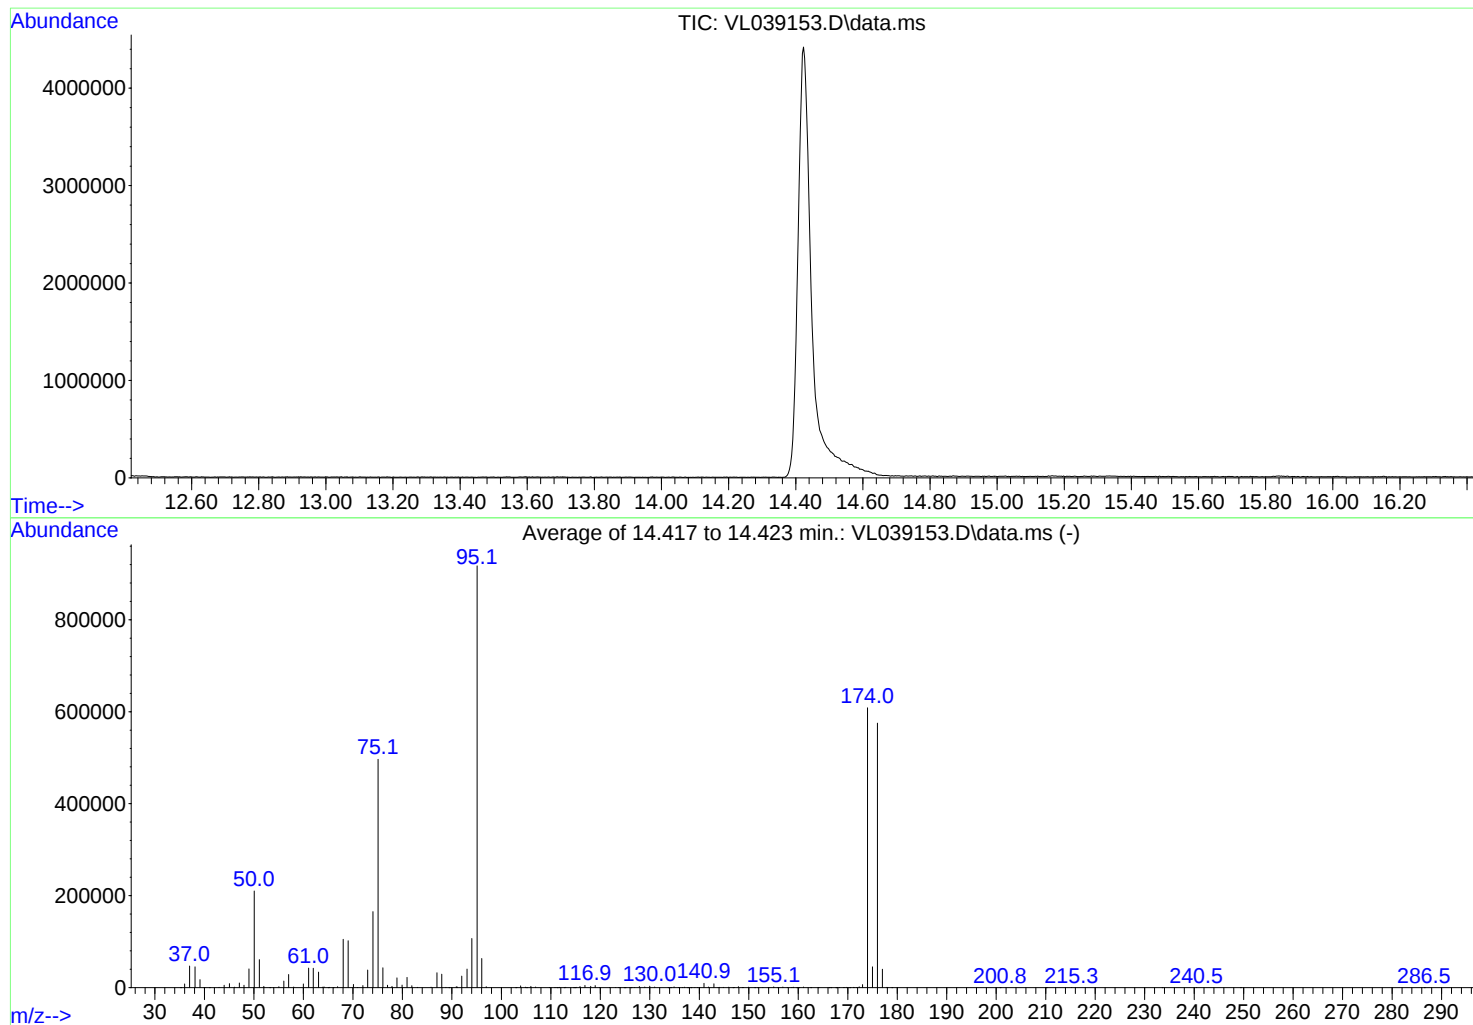

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.9	210325	PASS
75	95	30	66	54.1	496533	PASS
95	95	100	100	100.0	917227	PASS
96	95	5	9	6.9	63467	PASS
173	174	0.00	2	1.1	6634	PASS
174	95	50	120	66.3	608427	PASS
175	174	4	9	7.5	45333	PASS
176	174	93	101	94.5	575211	PASS
177	176	5	9	7.0	40032	PASS

Average of 14.417 to 14.423 min.: VL039153.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.20	115	47.05	9973	58.05	1453	68.05	10497
36.00	8057	48.00	5207	60.00	7994	69.05	10212
37.00	47115	49.00	40763	61.05	42320	70.10	709
38.10	45136	50.05	210325	62.00	42176	70.95	31
39.10	17383	51.10	61008	63.05	33603	72.00	4527
39.90	142	52.00	2901	63.90	1119	73.00	38309
41.00	164	53.20	50	64.15	1863	74.05	165227
42.95	680	53.95	226	65.00	147	75.10	496533
44.00	5165	55.05	2181	65.25	827	76.05	43307
45.05	8764	56.05	14364	66.00	81	77.00	5086
46.10	1097	57.00	28533	66.90	2033	77.90	2930

Average of 14.417 to 14.423 min.: VL039153.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	21421	91.10	1288	105.10	163	114.90	163
79.95	5669	92.00	25061	105.95	2857	115.10	620
80.95	22341	93.05	40552	106.95	1278	115.90	2396
81.90	4350	94.05	106824	109.70	288	116.90	4896
83.05	594	95.10	917227	110.80	260	118.05	2795
85.80	1052	96.05	63467	111.05	298	118.95	4551
87.00	32483	96.95	1964	111.30	157	119.85	197
87.95	29104	102.90	156	111.80	604	121.85	319
88.80	616	103.15	396	112.70	135	123.10	260
89.40	59	103.90	3976	113.00	893	123.70	224
90.90	2006	104.85	1167	114.60	163	123.90	187

Average of 14.417 to 14.423 min.: VL039153.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.80	77	134.90	1656	141.85	1281	148.95	297
125.00	114	135.80	228	142.95	8401	149.95	1125
126.00	353	136.00	224	143.80	203	151.20	81
126.20	180	136.60	465	144.05	637	151.80	160
126.90	342	137.00	1218	144.85	696	152.85	198
127.90	2581	137.65	133	145.95	974	153.90	180
129.00	1463	138.30	94	146.80	171	155.05	1931
130.00	3079	139.10	325	147.10	379	155.85	161
131.00	1485	139.70	263	147.90	1966	156.90	1487
133.70	115	140.05	508	148.70	247	157.80	202
134.20	131	140.95	9457	148.80	431	158.70	244

Average of 14.417 to 14.423 min.: VL039153.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
159.00	1025	169.10	295	175.00	45333	249.35	160
159.70	128	169.30	229	176.00	575211	286.50	88
160.10	116	169.70	611	177.00	40032		
161.05	1294	170.00	324	177.90	728		
162.50	72	170.40	171	178.10	343		
164.00	188	171.15	810	178.90	59		
166.20	82	171.40	515	200.80	73		
166.60	79	171.80	488	210.10	54		
167.60	68	172.30	1813	215.25	210		
167.80	139	173.00	6634	233.50	115		
168.35	306	174.00	608427	240.50	268		