
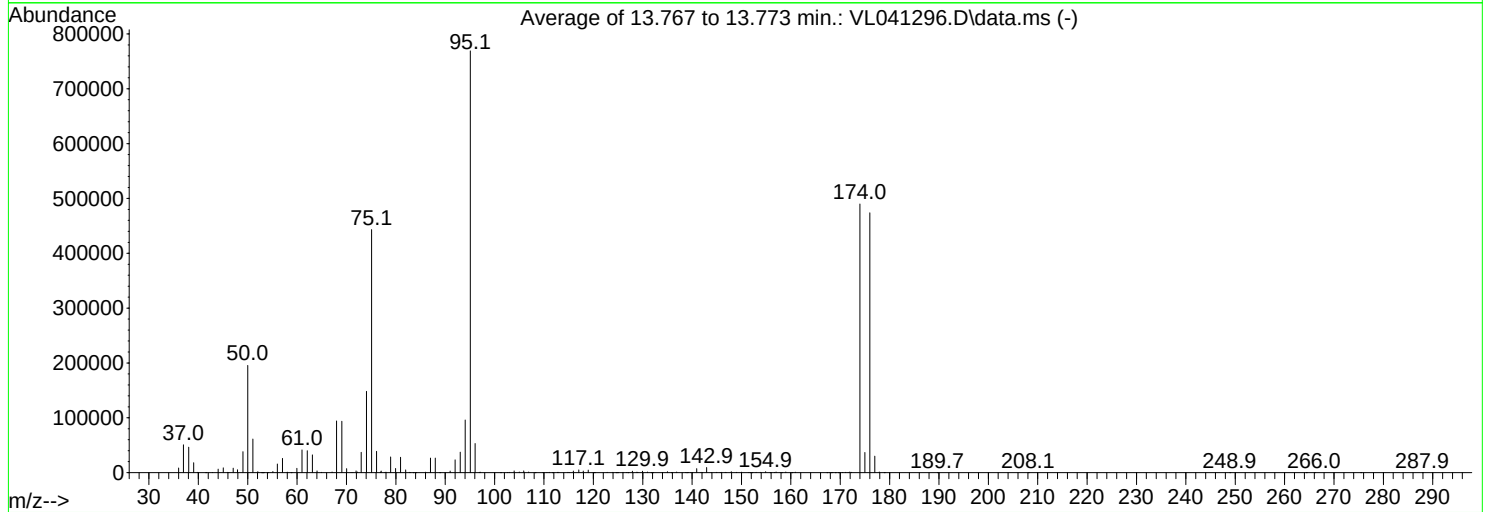


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060424\
Data File : VL041296.D
Acq On : 4 Jun 2024 7:53
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060424AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Jun 05 04:42:10 2024

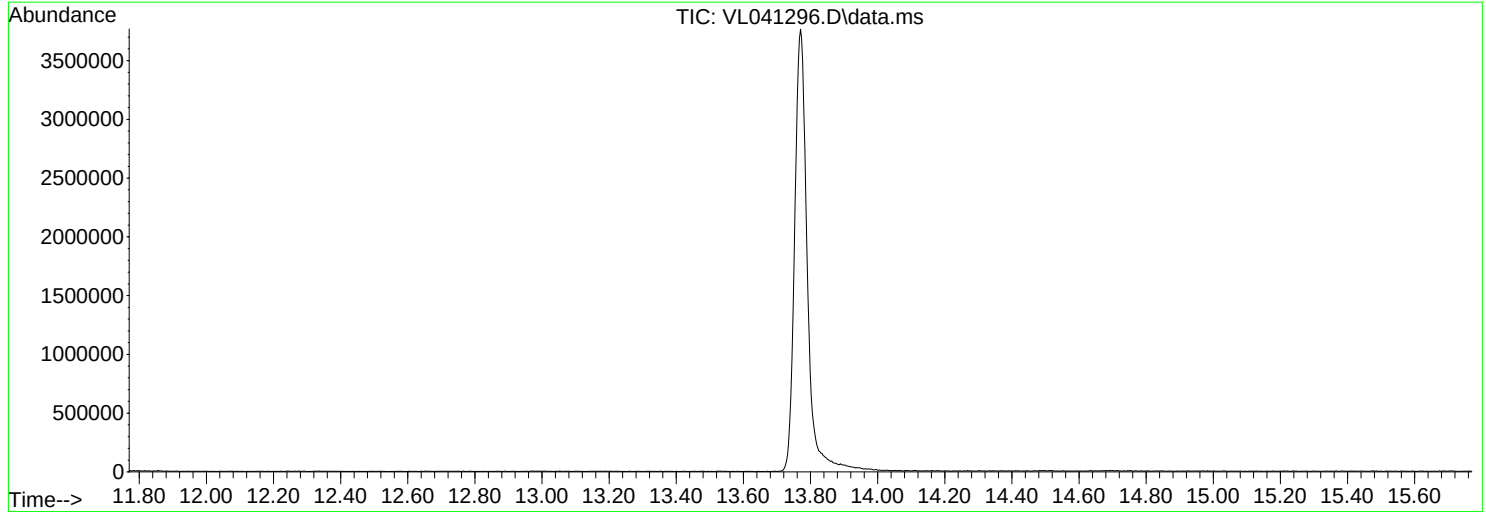

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.4	195499	PASS
75	95	30	66	57.6	443157	PASS
95	95	100	100	100.0	769173	PASS
96	95	5	9	6.9	53109	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.7	489877	PASS
175	174	4	9	7.5	36667	PASS
176	174	93	101	96.7	473835	PASS
177	176	5	9	6.3	30056	PASS

Average of 13.767 to 13.773 min.: VL041296.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8638	47.05	8195	56.00	15855	68.00	9414
37.00	50709	47.95	5141	57.05	26075	69.05	9356
38.05	46451	49.05	38168	58.00	978	70.05	733
39.05	18016	50.00	195499	58.80	96	70.95	24
39.90	473	51.05	61216	59.95	7945	71.30	262
41.50	117	52.05	1752	61.00	41499	71.95	3374
42.85	377	52.80	61	62.05	40013	72.20	1058
44.00	6445	53.00	64	63.10	32280	73.00	37085
45.05	8710	53.20	79	64.05	3157	74.05	148352
45.95	490	54.00	114	64.95	523	75.10	443157
46.20	281	55.10	2199	67.10	1115	76.10	38955

Average of 13.767 to 13.773 min.: VL041296.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.90	1107	84.00	63	96.90	734	109.95	312
77.05	3054	86.05	1029	97.10	951	110.60	199
77.80	750	87.00	26469	101.20	88	111.05	725
78.00	831	88.00	26533	102.60	249	111.70	107
78.95	28595	88.90	134	102.95	513	111.95	390
79.95	7502	91.00	2791	103.95	3268	112.75	692
80.95	28133	92.00	23459	105.00	1093	113.00	461
82.00	5035	93.05	37411	105.90	3362	114.85	582
82.75	584	94.05	96080	106.90	1115	115.10	339
83.00	271	95.10	769173	108.20	83	115.95	2861
83.50	143	96.05	53109	109.80	173	117.05	4980

Average of 13.767 to 13.773 min.: VL041296.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.95	3031	128.80	778	138.90	132	146.00	720
118.95	4575	129.00	696	139.25	201	146.70	520
120.20	56	129.95	2616	139.75	286	146.90	279
122.80	490	130.95	1122	140.10	425	147.95	1673
123.95	470	131.70	93	140.95	7449	149.00	448
124.60	62	132.00	107	141.80	647	150.00	777
124.90	80	134.00	194	142.10	364	151.50	228
126.00	534	135.00	1703	142.95	9399	151.75	133
126.75	207	135.80	68	143.90	431	152.10	61
127.00	65	136.90	1341	145.00	693	152.95	470
127.90	2582	138.70	264	145.70	337	153.90	479

Average of 13.767 to 13.773 min.: VL041296.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.90	1879	167.90	217	174.00	489877	275.40	63
155.80	121	168.20	92	175.00	36667	287.90	144
155.95	246	168.50	203	176.00	473835		
156.70	369	169.00	65	177.00	30056		
157.00	1088	169.60	108	177.90	1076		
157.85	174	169.90	431	178.90	51		
158.10	53	170.50	447	189.70	74		
159.00	1087	171.10	535	208.10	62		
160.20	64	171.60	376	248.90	88		
160.90	875	171.95	1128	264.40	50		
167.30	84	172.30	496	266.00	75		