
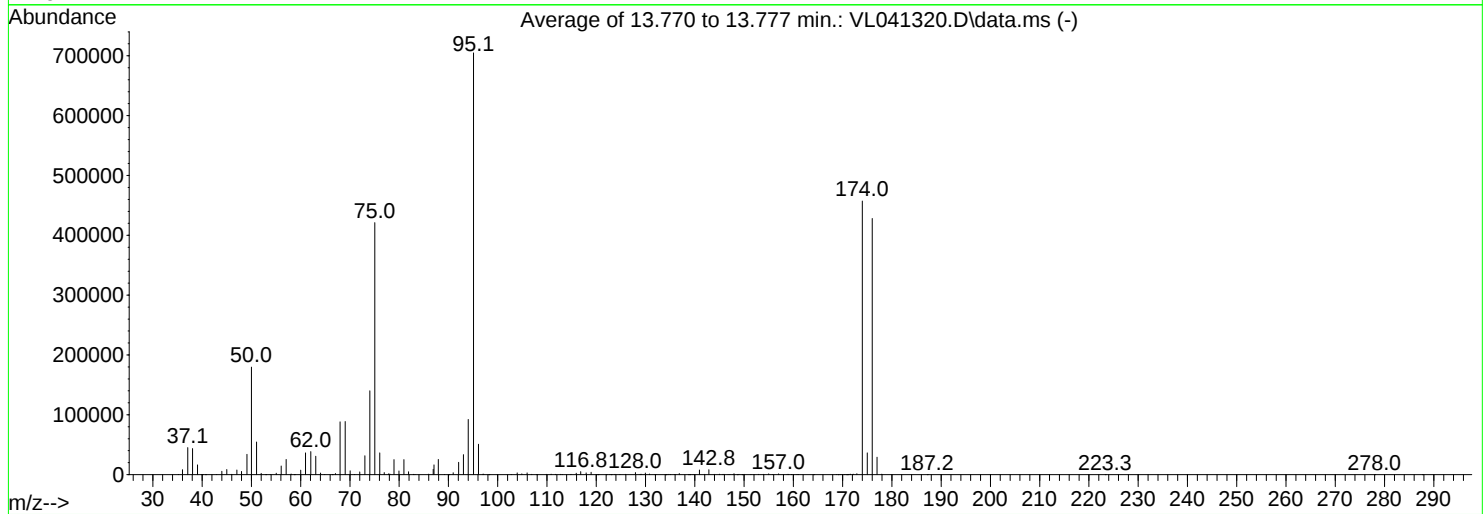


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060524\
Data File : VL041320.D
Acq On : 5 Jun 2024 8:49
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060424AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Jun 05 04:42:10 2024

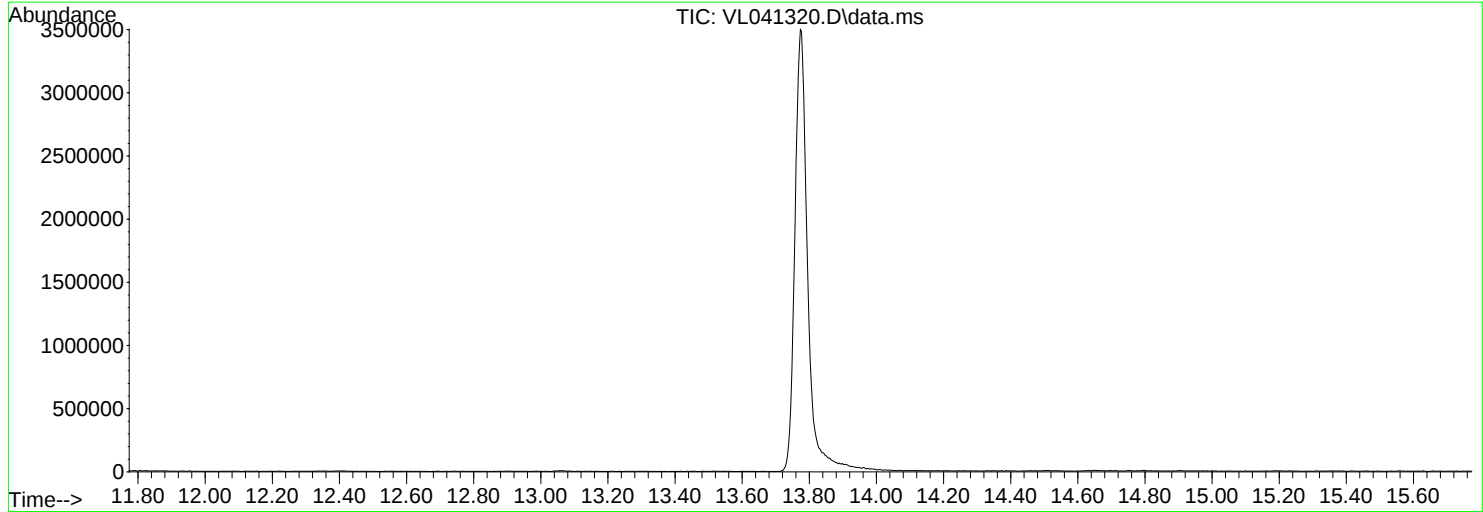

AutoFind: Scans 3473, 3474, 3475; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.5	179819	PASS
75	95	30	66	59.8	421269	PASS
95	95	100	100	100.0	704917	PASS
96	95	5	9	7.2	50835	PASS
173	174	0.00	2	0.4	1662	PASS
174	95	50	120	64.9	457195	PASS
175	174	4	9	8.0	36389	PASS
176	174	93	101	93.7	428245	PASS
177	176	5	9	6.8	29120	PASS

Average of 13.770 to 13.777 min.: VL041320.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.20	160	46.00	428	57.05	25472	68.00	8817
36.00	8431	47.05	7797	58.05	981	69.05	8876
37.10	45107	48.00	5300	58.70	51	70.05	646
38.05	43613	49.10	33981	60.00	7638	70.95	29
39.05	16308	50.00	179819	61.00	36400	72.00	4602
39.90	153	51.05	54672	62.05	38445	73.05	31584
40.20	388	52.00	2190	63.05	30883	74.05	140096
40.70	54	52.90	99	64.05	2601	75.05	421269
42.95	350	53.85	249	64.90	179	76.05	36432
44.00	5726	55.05	2393	66.40	106	76.95	3645
45.00	8622	56.05	14496	67.05	1804	77.85	1390

Average of 13.770 to 13.777 min.: VL041320.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.10	982	89.20	243	102.75	226	114.85	583
78.95	25165	90.10	86	103.95	2887	115.95	2488
79.95	6146	90.95	3195	104.90	1279	116.85	5137
80.95	25128	92.05	20597	105.95	3030	117.95	3073
81.90	4893	93.05	33365	106.90	587	118.95	4116
82.90	551	94.00	92272	107.90	103	120.00	153
83.20	291	95.10	704917	109.85	558	120.40	128
86.00	705	96.10	50835	110.85	923	122.00	127
86.90	8712	97.00	805	111.70	643	122.75	277
87.05	16456	97.15	858	112.80	513	123.00	90
87.95	25336	98.20	74	113.10	270	123.80	435

Average of 13.770 to 13.777 min.: VL041320.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.80	302	135.10	232	143.95	592	150.00	585
125.95	473	135.85	208	145.00	712	151.40	233
127.95	3504	136.10	181	145.70	649	152.00	233
128.90	328	136.85	1947	145.95	517	152.95	467
129.10	853	138.70	147	146.75	194	153.95	446
129.95	2747	139.00	81	147.10	311	155.00	1429
130.80	1150	139.65	337	147.80	309	155.85	254
131.90	89	140.00	226	147.95	1743	157.00	1443
134.00	155	140.95	7686	148.60	127	158.05	292
134.20	98	142.00	536	148.95	439	158.75	557
134.75	623	142.85	8212	149.60	153	159.05	634

Average of 13.770 to 13.777 min.: VL041320.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
159.65	252	171.30	610	278.00	54		
160.75	350	171.60	801	287.70	51		
161.00	164	172.15	861				
164.10	91	172.90	1662				
168.75	295	174.00	457195				
169.10	140	175.00	36389				
169.65	274	176.00	428245				
170.30	380	177.00	29120				
170.50	264	177.95	945				
170.80	136	187.20	51				
171.00	147	223.30	61				