

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060525\
 Data File : VL042615.D
 Acq On : 05 Jun 2025 10:12
 Operator : SY/MD
 Sample : VL0605ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0605ABL01

Quant Time: Jun 06 01:37:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052925AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri May 30 02:01:56 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	100644	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.965	114	264126	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.888	117	238873	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.383	95	179494	10.024	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060525\
Data File : VL042615.D
Acq On : 05 Jun 2025 10:12
Operator : SY/MD
Sample : VL0605ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0605ABL01

Quant Time: Jun 06 01:37:14 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052925AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri May 30 02:01:56 2025
Response via : Initial Calibration




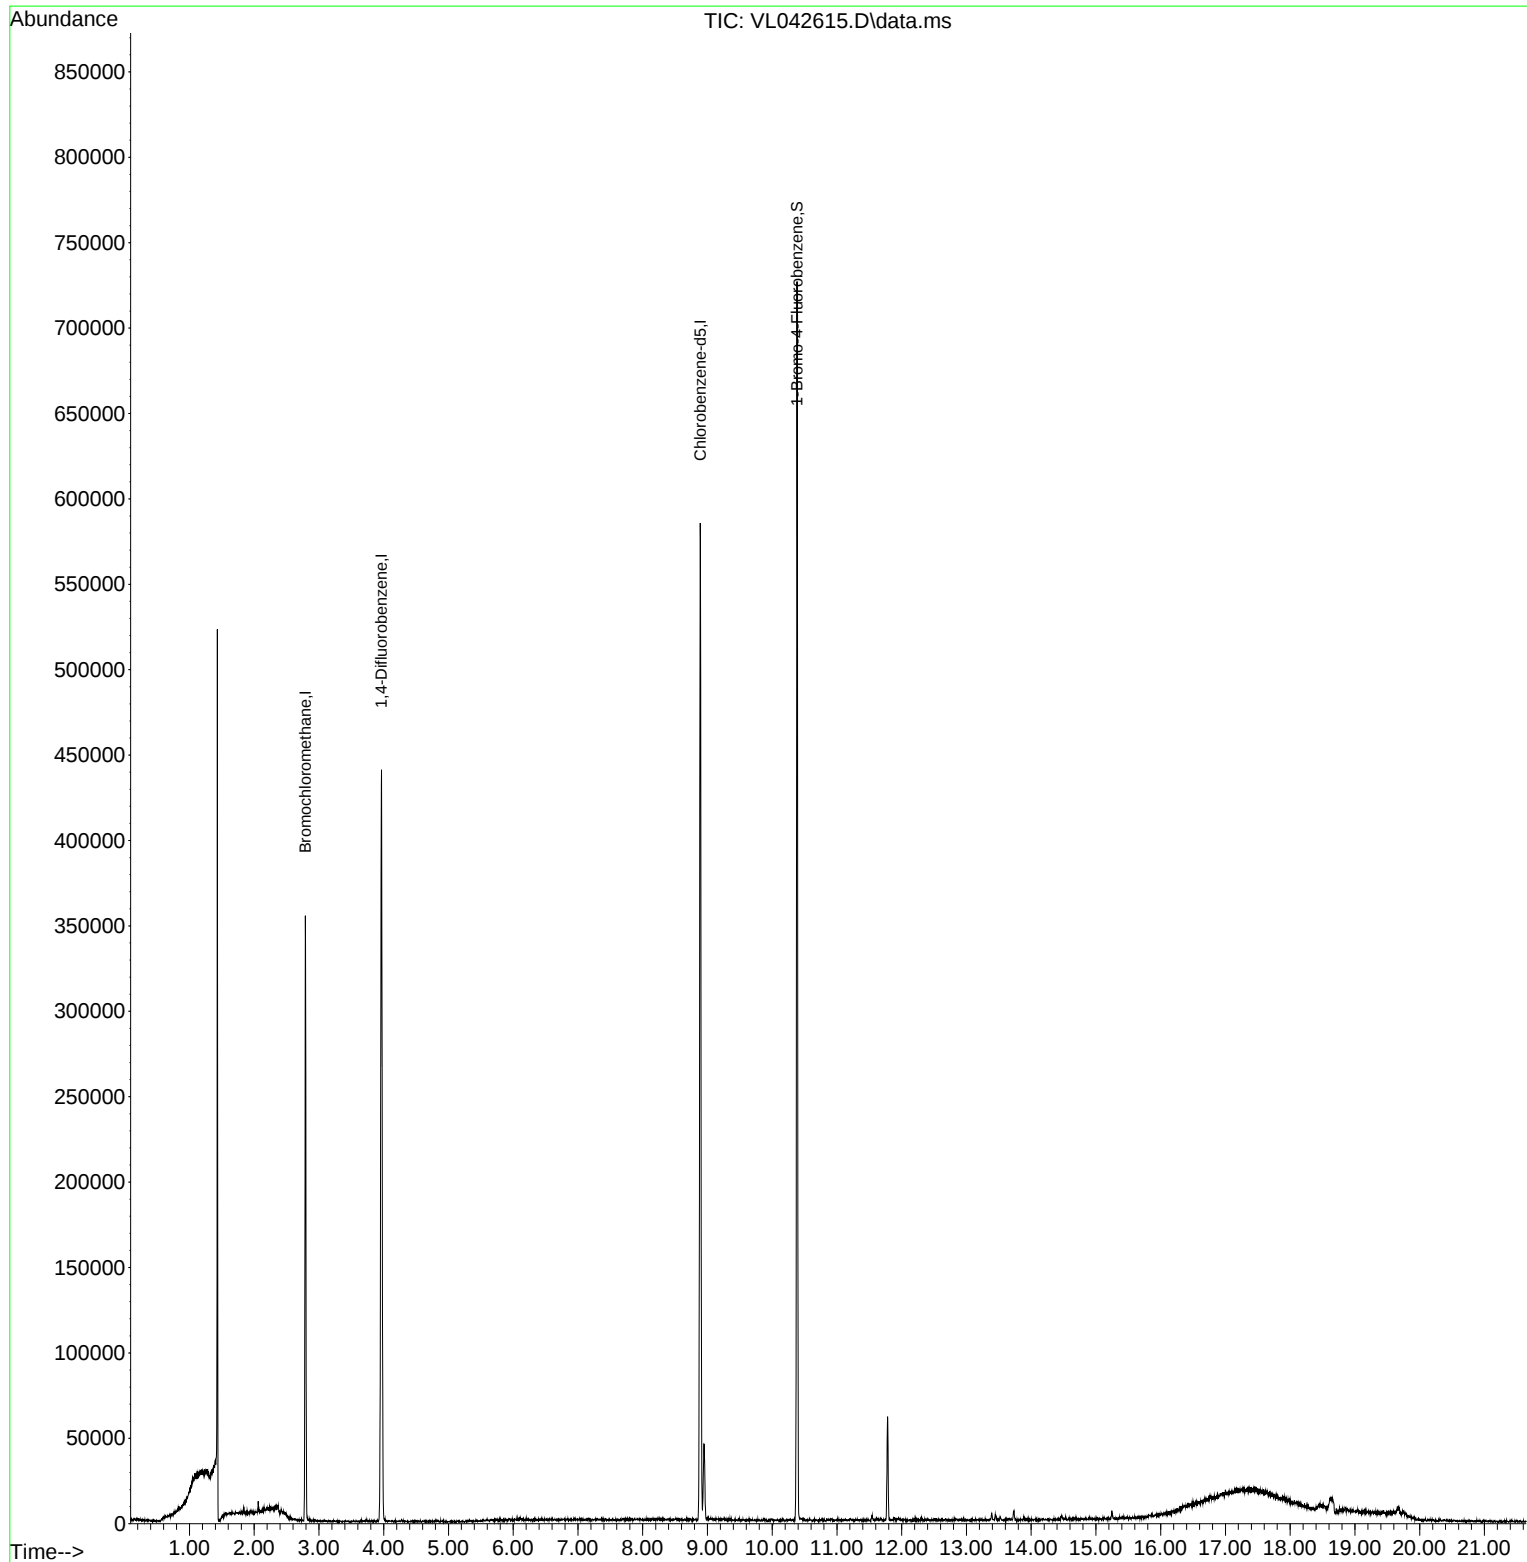


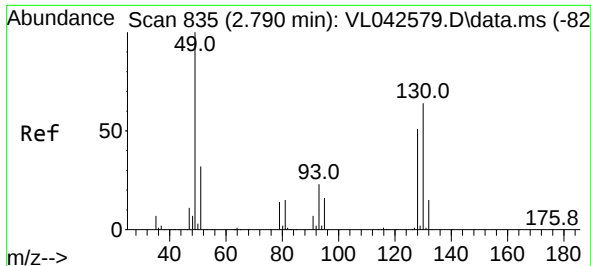

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.790 min Scan# 81
Delta R.T. 0.000 min
Lab File: VL042615.D
Acq: 05 Jun 2025 10:12




Instrument :
MSVOA_L
ClientSampleId :
VL0605ABL01


Tgt Ion: 49 Resp: 100644
Ion Ratio Lower Upper
49 100
128 45.1 24.2 72.6
130 57.3 30.4 91.2

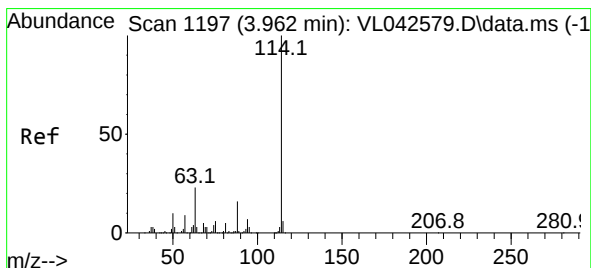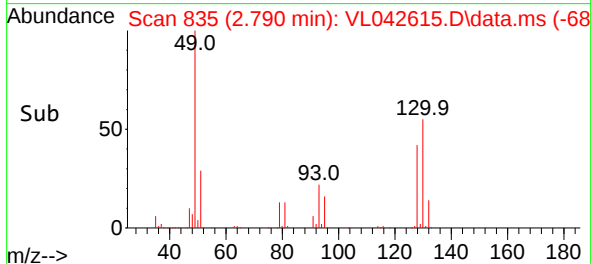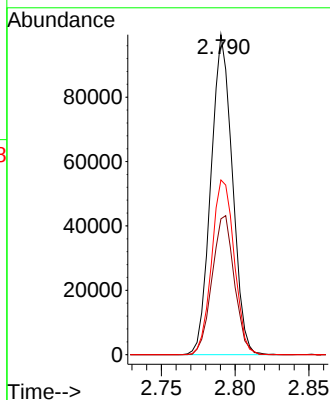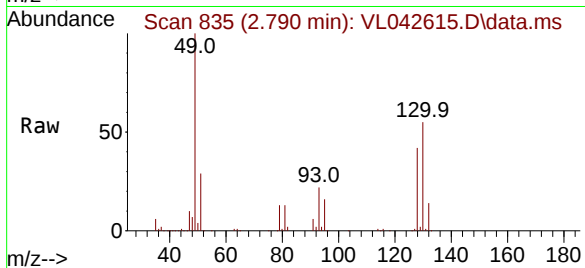

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.965 min Scan# 1198
Delta R.T. 0.003 min
Lab File: VL042615.D
Acq: 05 Jun 2025 10:12

Tgt Ion: 114 Resp: 264126
Ion Ratio Lower Upper
114 100
63 25.5 19.0 28.6
88 17.5 13.6 20.4

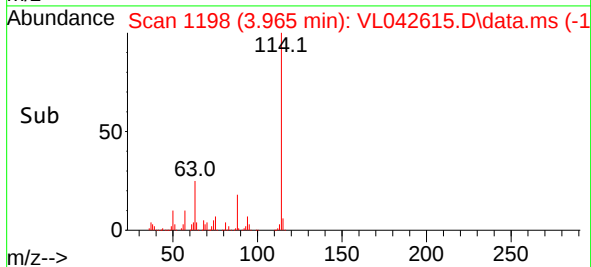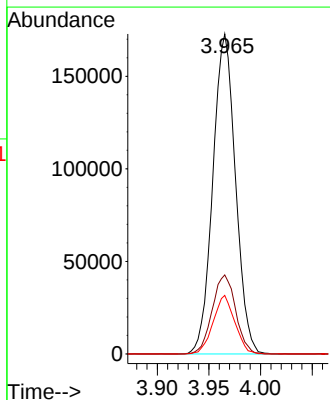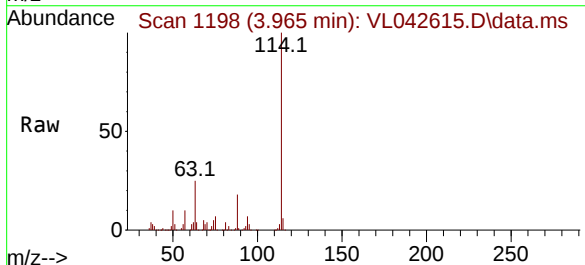

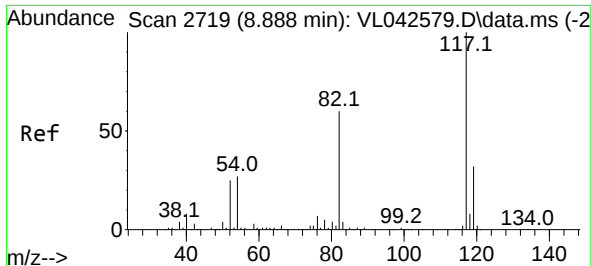

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 8.888 min Scan# 21

Delta R.T. 0.000 min

Lab File: VL042615.D

Acq: 05 Jun 2025 10:12

Instrument :

MSVOA_L

ClientSampleId :

VL0605ABL01





Tgt Ion:117 Resp: 238873

Ion Ratio Lower Upper

117 100

82 63.7 51.2 76.8

119 31.3 26.3 39.5

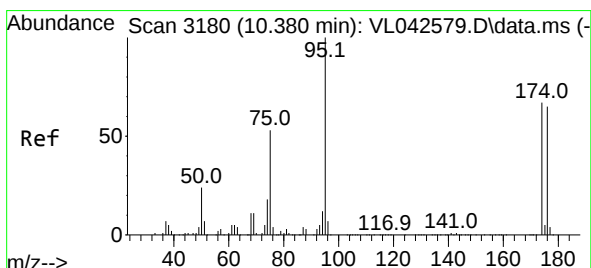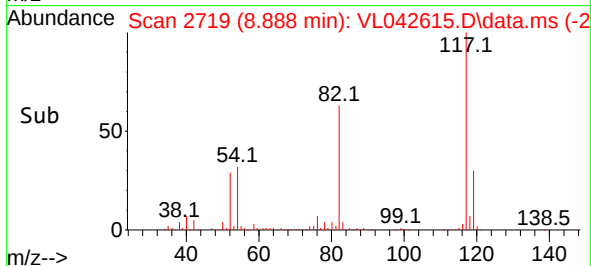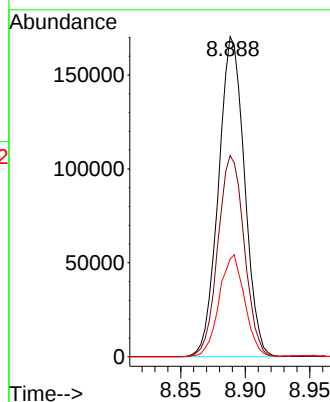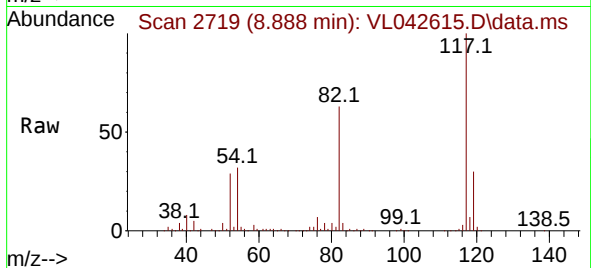

#68

1-Bromo-4-Fluorobenzene

Concen: 10.024 ppbv

RT: 10.383 min Scan# 3181

Delta R.T. 0.003 min

Lab File: VL042615.D

Acq: 05 Jun 2025 10:12

Tgt Ion: 95 Resp: 179494

Ion Ratio Lower Upper

95 100

174 63.1 53.1 79.7

175 4.9 4.2 6.2

