


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060525\
Data File : VL042613.D
Acq On : 05 Jun 2025 07:59
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052925AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 30 02:01:56 2025

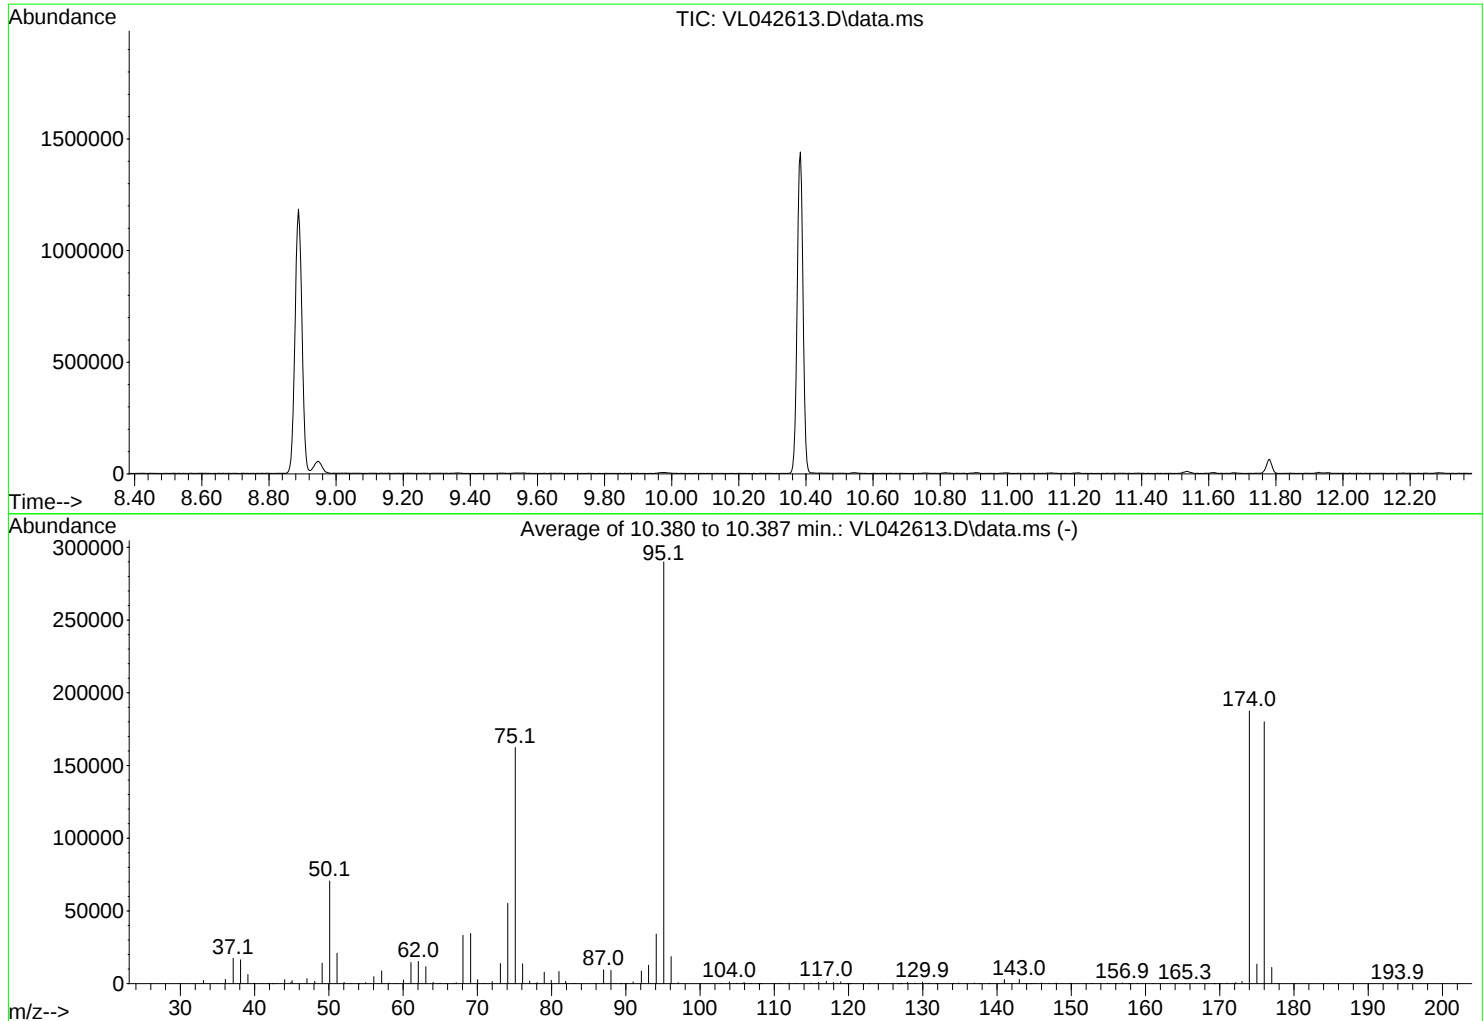

AutoFind: Scans 3180, 3181, 3182; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.3	70608	PASS
75	95	30	66	56.0	162389	PASS
95	95	100	100	100.0	290027	PASS
96	95	5	9	6.4	18643	PASS
173	174	0.00	2	0.9	1618	PASS
174	95	50	120	64.6	187477	PASS
175	174	4	9	7.2	13409	PASS
176	174	93	101	96.0	180053	PASS
177	176	5	9	6.2	11138	PASS

Average of 10.380 to 10.387 min.: VL042613.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	2217	44.05	2717	54.05	46	64.80	16
34.85	65	44.90	907	54.95	768	65.00	29
36.05	2995	45.05	2053	56.05	4899	65.75	7
37.10	17384	46.00	183	57.10	8826	66.80	19
38.10	16367	47.05	3411	58.10	374	67.15	709
39.10	6270	48.10	1648	59.05	105	68.05	33232
39.90	299	49.10	14046	60.05	2559	69.10	34528
41.05	115	50.10	70608	61.05	14562	70.05	2764
41.80	23	51.10	20936	62.05	15280	70.80	114
42.40	60	52.05	873	63.05	11629	71.15	148
43.00	168	53.00	136	64.05	1049	72.00	1471

Average of 10.380 to 10.387 min.: VL042613.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.10	13837	82.80	92	95.10	290027	108.20	32
74.10	55192	83.10	172	96.10	18643	109.65	69
75.10	162389	85.95	216	97.05	646	110.00	67
76.10	13623	87.00	9547	102.85	199	110.70	83
77.05	1749	88.00	9140	103.95	1201	110.95	248
77.90	300	89.30	35	104.95	352	111.95	298
78.05	701	90.20	78	105.80	457	112.90	286
79.00	7904	91.00	1206	105.95	748	114.95	395
79.95	2375	92.10	8693	106.70	110	115.95	895
81.00	8408	93.05	12665	106.95	193	117.00	1708
81.90	1627	94.10	34088	107.85	49	117.95	907

Average of 10.380 to 10.387 min.: VL042613.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	1306	128.95	390	140.00	146	147.95	494
119.80	42	129.95	1072	141.00	2905	148.80	175
120.20	26	130.85	374	142.00	254	149.90	309
122.75	50	131.85	56	143.00	2929	152.10	170
123.70	172	134.15	75	143.80	148	152.70	82
124.10	68	134.85	485	144.10	113	152.95	139
124.90	116	135.95	95	144.50	50	153.95	191
126.00	94	136.95	476	144.95	78	154.90	305
126.70	52	137.65	42	145.20	80	155.10	168
127.00	34	138.90	24	145.95	408	155.85	145
127.95	919	139.55	67	147.00	197	156.10	127

Average of 10.380 to 10.387 min.: VL042613.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.90	439	172.15	732				
157.70	50	173.00	1618				
158.90	351	174.00	187477				
160.90	133	175.00	13409				
161.10	73	176.00	180053				
165.30	19	177.00	11138				
169.30	53	177.85	253				
170.00	87	193.95	48				
170.30	132						
171.00	310						
171.80	137						