

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL060719\
Quantitation Report (Not Reviewed)

Data File : VL033885.D
Acq On : 7 Jun 2019 12:10
Operator : SY/AP
Sample : QC060619 CAN 10655
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC060619 CAN 10655

Quant Time: Jun 08 04:19:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL060719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019
QLast Update : Fri Jun 07 08:53:27 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.75	49	890416	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.27	114	2027637	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.22	117	2093453	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.56	95	1708440	9.94	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.40%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) Acetone	3.91	43	11265	0.087	ppbv #	89
20) Methylene Chloride	4.40	84	13818	0.273	ppbv	84
26) Hexane	5.77	57	7715	0.086	ppbv #	27
39) 1,2-Dichloropropane	7.27	63	543777	9.096	ppbv #	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VL033885.D
Acq On : 7 Jun 2019 12:10
Operator : SY/AP
Sample : QC060619 CAN 10655
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC060619 CAN 10655

Quant Time: Jun 08 04:19:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL060719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019
QLast Update : Fri Jun 07 08:53:27 2019
Response via : Initial Calibration

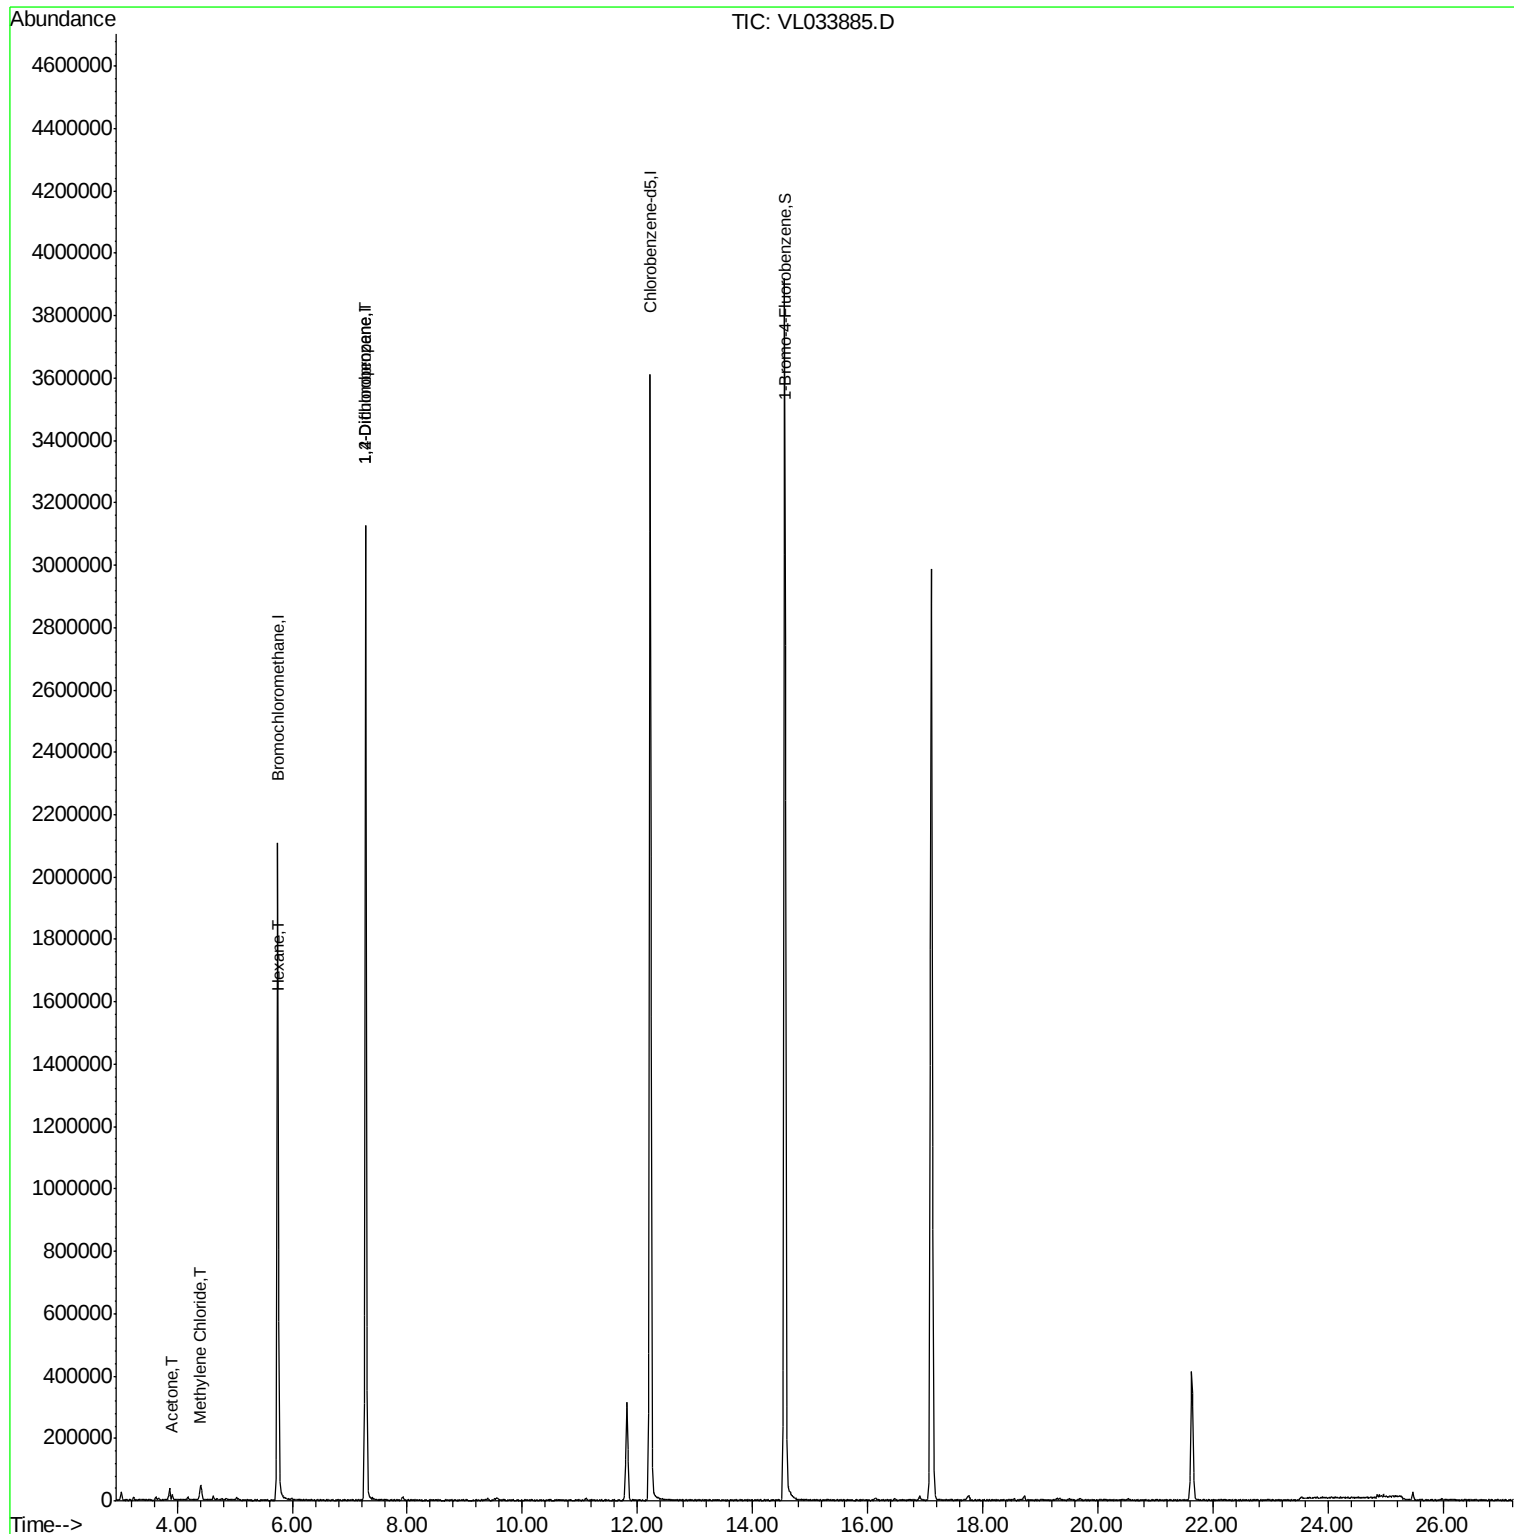

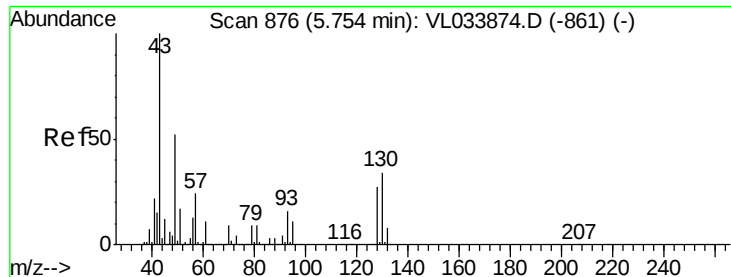

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.75 min Scan# 874

Delta R.T. -0.01 min

Lab File: VL033885.D

Acq: 7 Jun 2019 12:10

Instrument :

MSVOA_L

ClientSampleId :

QC060619 CAN 10655


Tgt Ion: 49 Resp: 890416

Ion Ratio Lower Upper

49 100

128 49.4 25.5 76.5




130 63.5 32.5 97.4

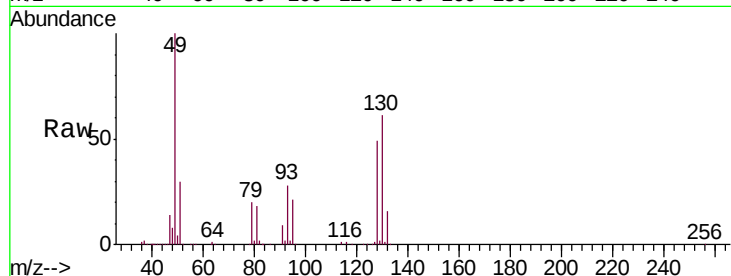

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

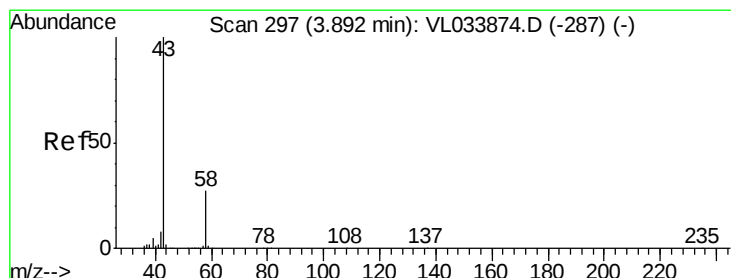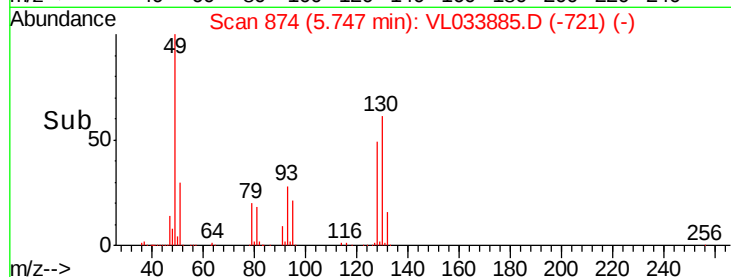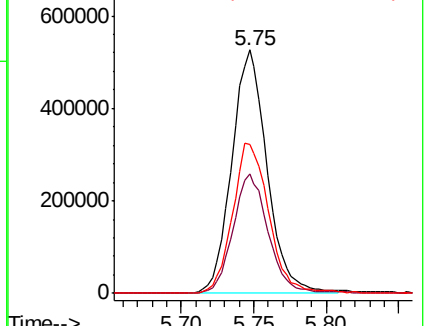

#15

Acetone

Concen: 0.087 ppbv

RT: 3.91 min Scan# 303

Delta R.T. 0.02 min

Lab File: VL033885.D


Acq: 7 Jun 2019 12:10

Tgt Ion: 43 Resp: 11265

Ion Ratio Lower Upper



43 100


58 32.5 21.3 31.9#

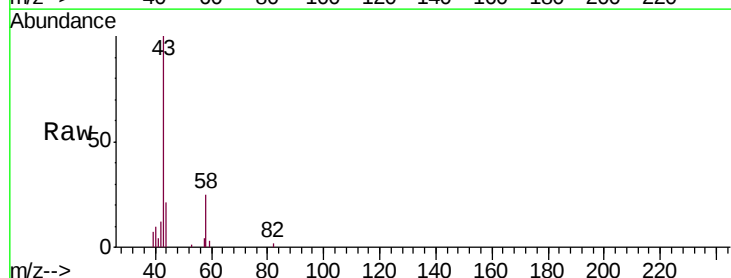

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 58.10 (57.80 to 58.80): VL0

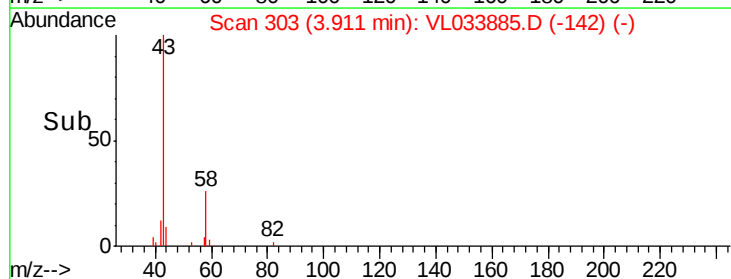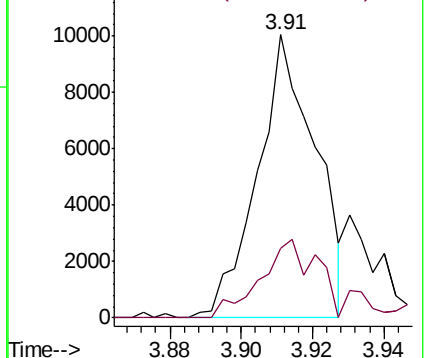


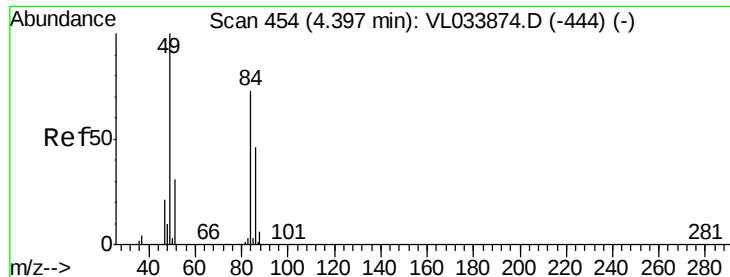




#20
Methylene Chloride
Concen: 0.273 ppbv
RT: 4.40 min Scan# 455
Delta R.T. 0.00 min
Lab File: VL033885.D
Acq: 7 Jun 2019 12:10

Instrument :
MSVOA_L
ClientSampleId :
QC060619 CAN 10655

Tgt Ion: 84 Resp: 13818
Ion Ratio Lower Upper
84 100
49 111.4 110.0 165.0
51 46.2 34.6 51.8
86 53.7 50.6 75.8

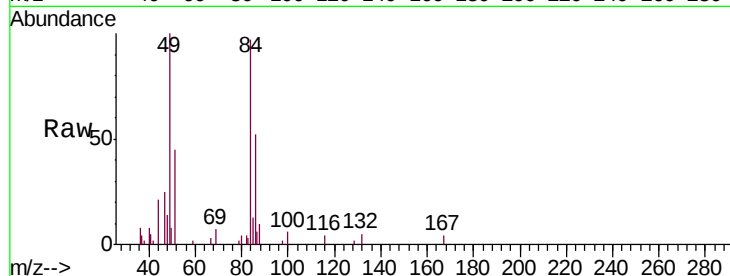


Abundance Ion 84.00 (83.70 to 84.70): VL0
Ion 49.10 (48.80 to 49.80): VL0
Ion 51.10 (50.80 to 51.80): VL0
Ion 86.00 (85.70 to 86.70): VL0

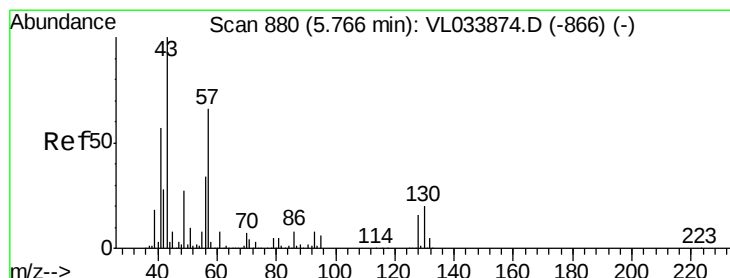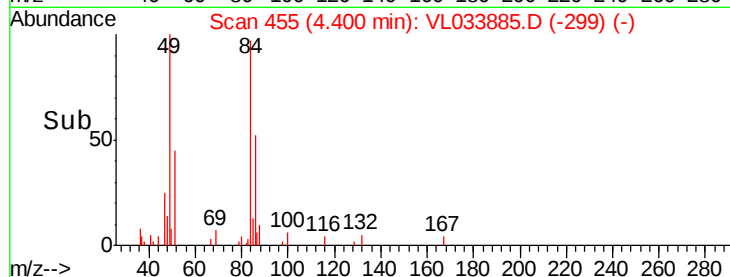
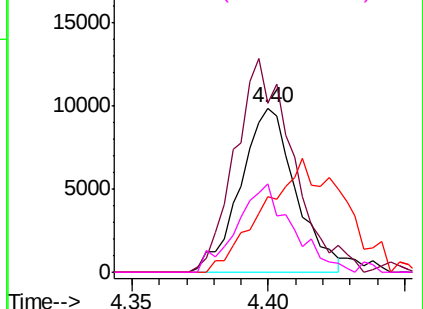



#26
Hexane
Concen: 0.086 ppbv
RT: 5.77 min Scan# 880
Delta R.T. -0.00 min
Lab File: VL033885.D
Acq: 7 Jun 2019 12:10

Tgt Ion: 57 Resp: 7715
Ion Ratio Lower Upper
57 100
41 167.6 71.4 107.2#
43 111.4 183.7 275.5#
56 96.4 42.7 64.1#

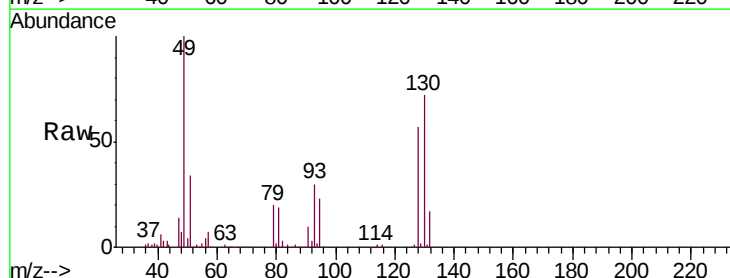

Abundance Ion 57.10 (56.80 to 57.80): VL0
Ion 41.10 (40.80 to 41.80): VL0
Ion 43.10 (42.80 to 43.80): VL0
Ion 56.10 (55.80 to 56.80): VL0

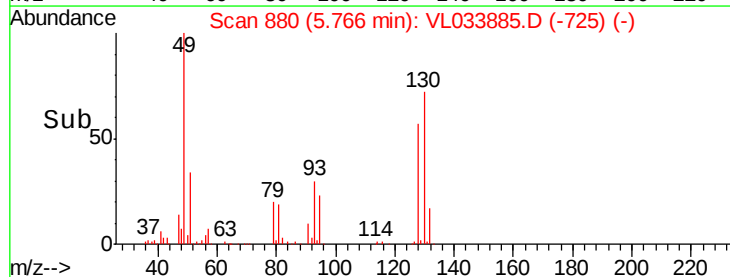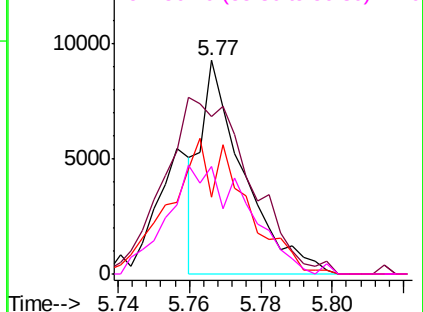

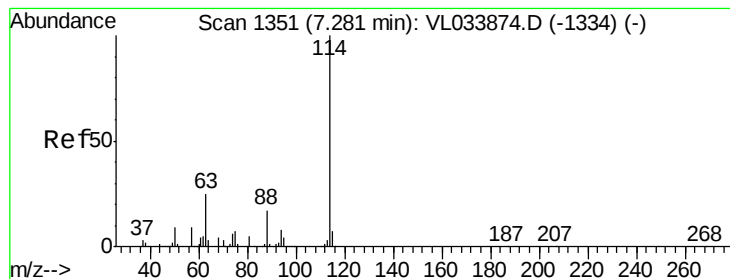

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.27 min Scan# 1349

Delta R.T. -0.01 min

Lab File: VL033885.D

Acq: 7 Jun 2019 12:10

Instrument :

MSVOA_L

ClientSampleId :

QC060619 CAN 10655


Tgt Ion:114 Resp: 2027637

Ion Ratio Lower Upper

114 100

63 26.9 21.1 31.7




88 18.3 14.2 21.4

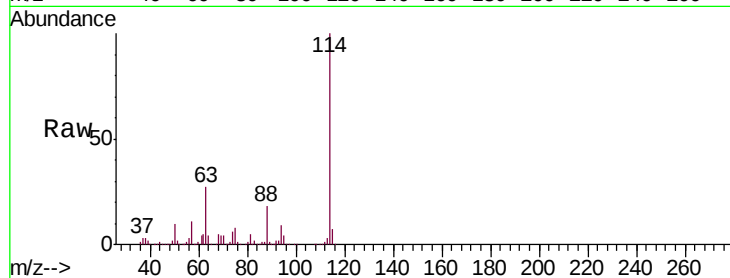

Abundance Ion 114.10 (113.80 to 114.80): V

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

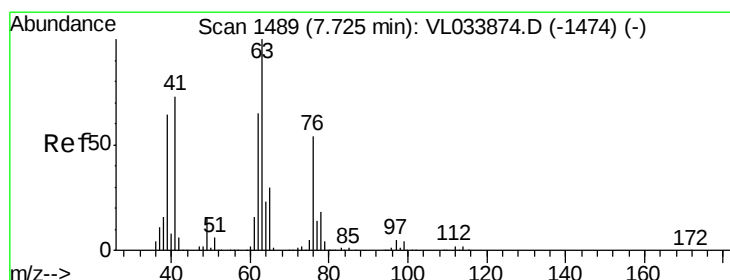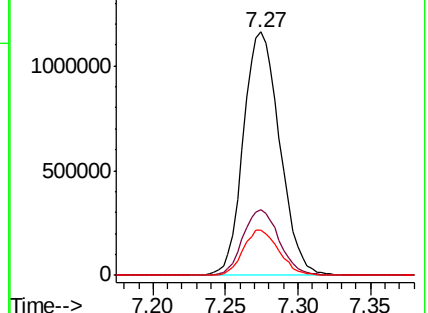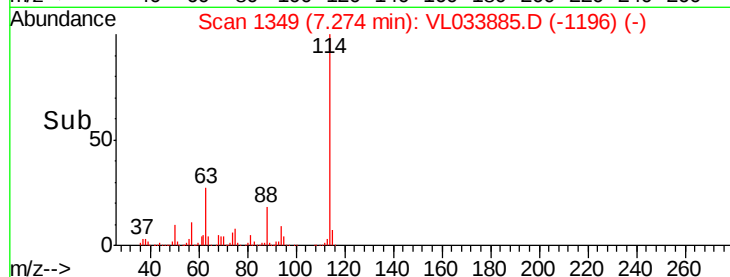

#39

1,2-Dichloropropane

Concen: 9.096 ppbv

RT: 7.27 min Scan# 1349

Delta R.T. -0.45 min

Lab File: VL033885.D

Acq: 7 Jun 2019 12:10


Tgt Ion: 63 Resp: 543777

Ion Ratio Lower Upper

63 100

41 0.1 58.7 88.1#



62 17.7 51.9 77.9#

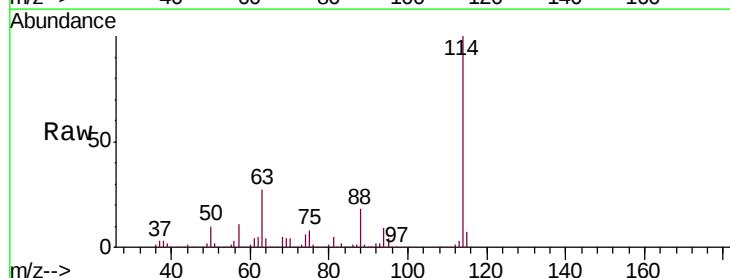


Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 62.10 (61.80 to 62.80): VL0



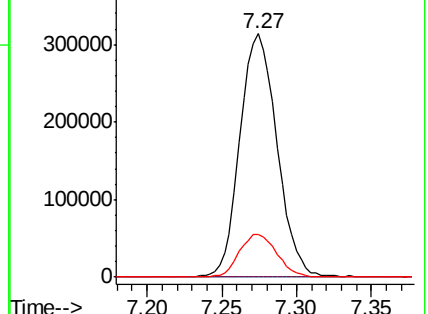
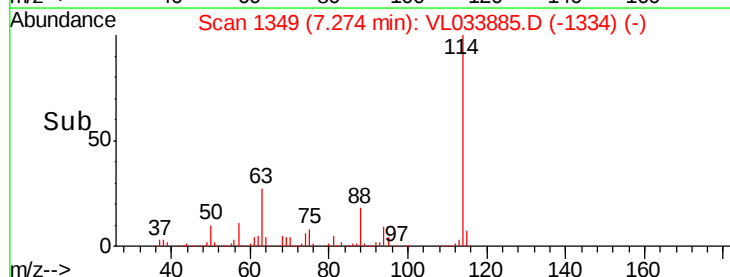


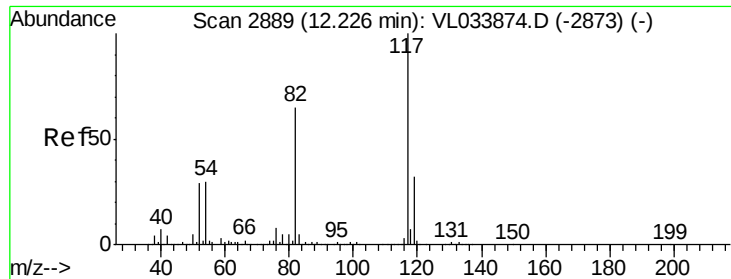

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.22 min Scan# 2888
Delta R.T. -0.00 min
Lab File: VL033885.D
Acq: 7 Jun 2019 12:10

Instrument :
MSVOA_L
ClientSampleId :
QC060619 CAN 10655

Tgt Ion: 117 Resp: 2093453
Ion Ratio Lower Upper
117 100
82 68.5 50.2 75.2
119 31.9 24.8 37.2

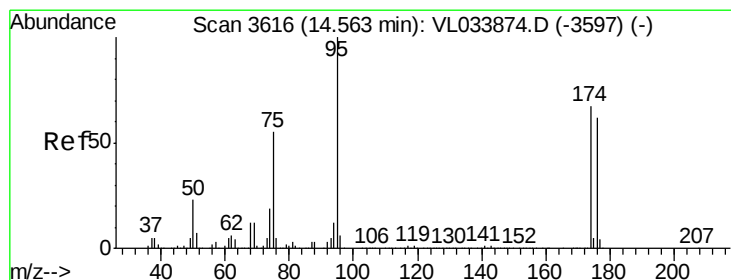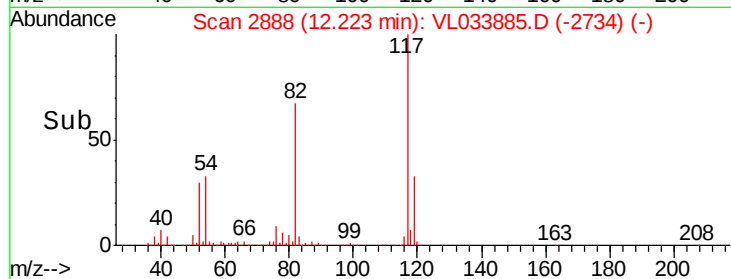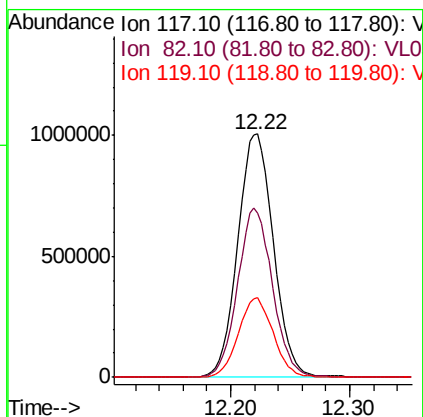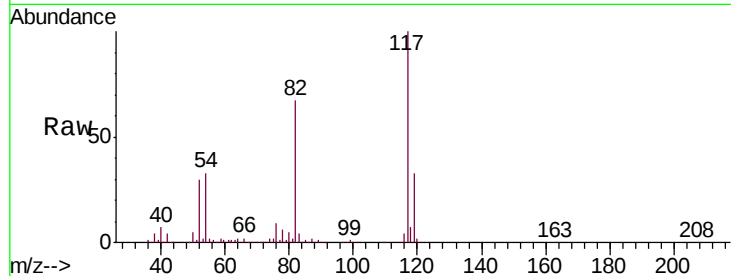

#68
1-Bromo-4-Fluorobenzene
Concen: 9.935 ppbv
RT: 14.56 min Scan# 3614
Delta R.T. -0.01 min
Lab File: VL033885.D
Acq: 7 Jun 2019 12:10

Tgt Ion: 95 Resp: 1708440
Ion Ratio Lower Upper
95 100
174 65.3 54.0 81.0
175 4.6 3.8 5.8

