

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL060719\
Quantitation Report (Not Reviewed)

Data File : VL033893.D
Acq On : 7 Jun 2019 17:38
Operator : SY/AP
Sample : CAN 10150
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10150

Quant Time: Jun 08 04:20:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL060719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019
QLast Update : Fri Jun 07 08:53:27 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.75	49	774923	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.27	114	1771665	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.22	117	1762578	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.56	95	1442974	9.97	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.70%

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
20) Methylene Chloride	4.40	84	10142	0.230	ppbv #	78
26) Hexane	5.76	57	2523	0.032	ppbv #	25
30) Cyclohexane	7.26	84	4996	0.090	ppbv #	1
39) 1,2-Dichloropropane	7.27	63	471799	9.033	ppbv #	26

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VL033893.D

Acq On : 7 Jun 2019 17:38

Operator : SY/AP

Sample : CAN 10150

Misc : 400ml/MSVOA_L

ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10150


Quant Time: Jun 08 04:20:41 2019


Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL060719AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019

QLast Update : Fri Jun 07 08:53:27 2019

Response via : Initial Calibration

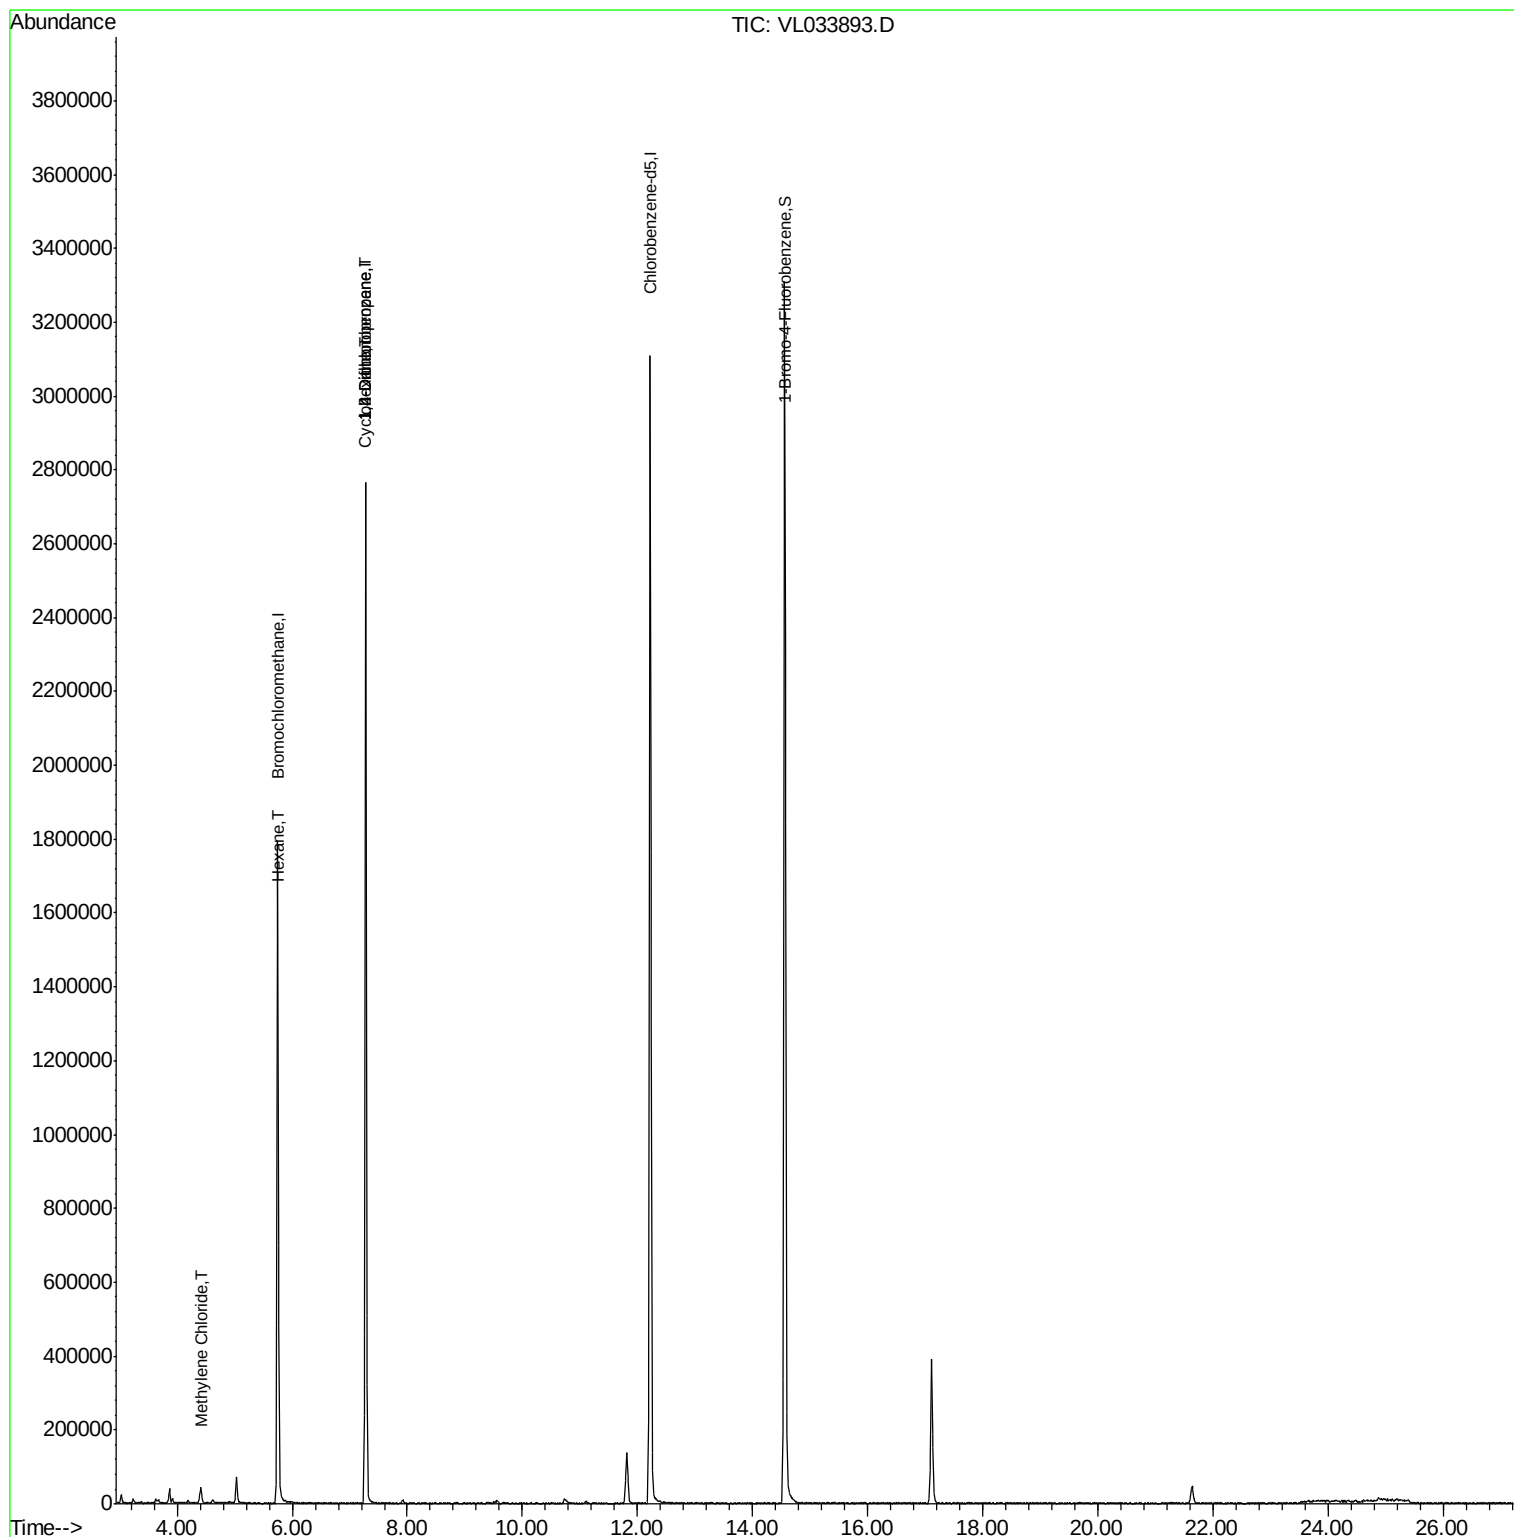

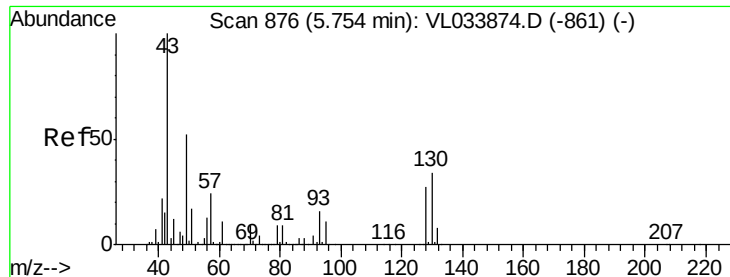

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.75 min Scan# 874

Delta R.T. -0.01 min

Lab File: VL033893.D

Acq: 7 Jun 2019 17:38

Instrument :

MSVOA_L

ClientSampleId :

CAN 10150


Tgt Ion: 49 Resp: 774923

Ion Ratio Lower Upper

49 100

128 48.9 25.5 76.5




130 63.2 32.5 97.4

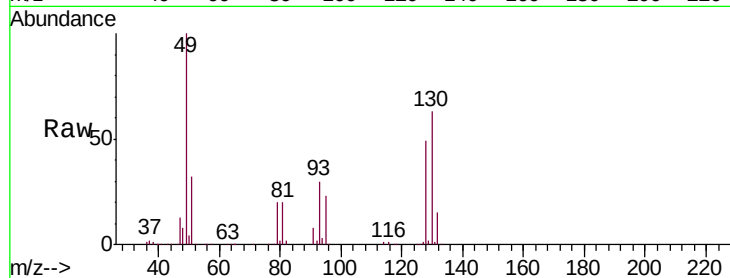

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

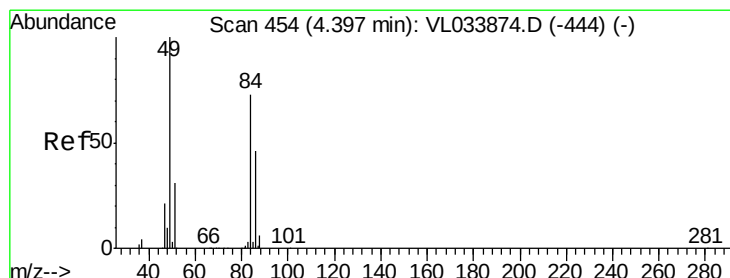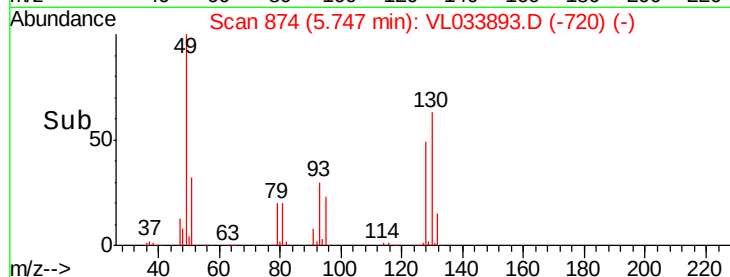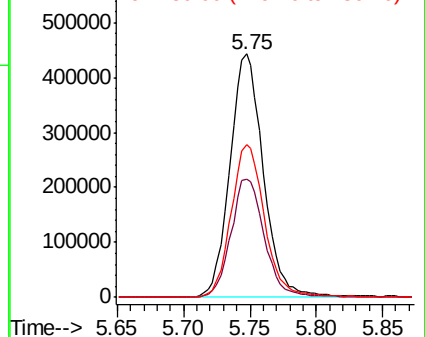

#20

Methylene Chloride

Concen: 0.230 ppbv

RT: 4.40 min Scan# 456

Delta R.T. 0.01 min

Lab File: VL033893.D

Acq: 7 Jun 2019 17:38

Tgt Ion: 84 Resp: 10142


Ion Ratio Lower Upper

84 100

49 105.7 110.0 165.0#

51 64.4 34.6 51.8#

86 59.6 50.6 75.8


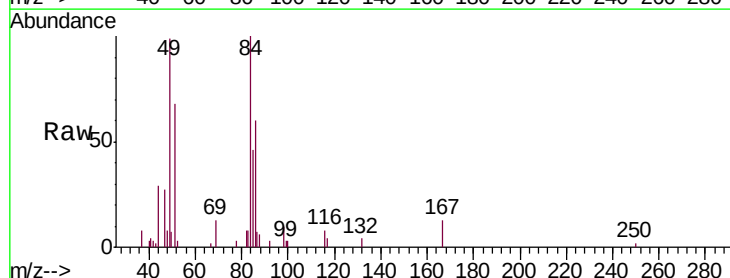



Abundance Ion 84.00 (83.70 to 84.70): VL0

Ion 49.10 (48.80 to 49.80): VL0

Ion 51.10 (50.80 to 51.80): VL0

Ion 86.00 (85.70 to 86.70): VL0



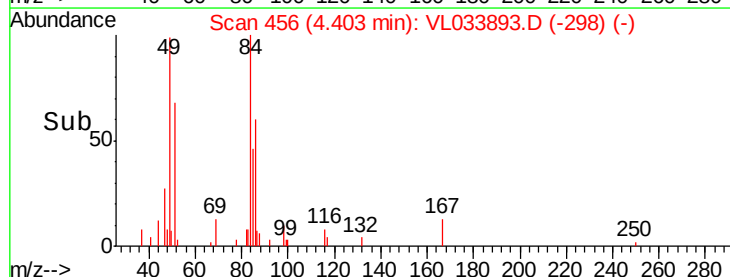
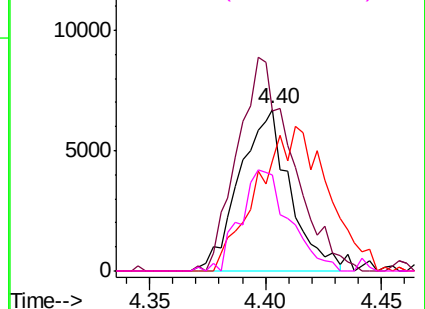


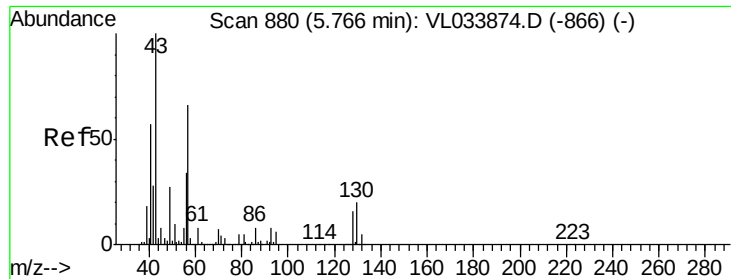

#26
Hexane
Concen: 0.032 ppbv
RT: 5.76 min Scan# 879
Delta R.T. -0.00 min
Lab File: VL033893.D
Acq: 7 Jun 2019 17:38




Instrument :
MSVOA_L
ClientSampleId :
CAN 10150


Tgt Ion: 57 Resp: 2523
Ion Ratio Lower Upper
57 100
41 190.2 71.4 107.2#
43 125.8 183.7 275.5#
56 0.0 42.7 64.1#

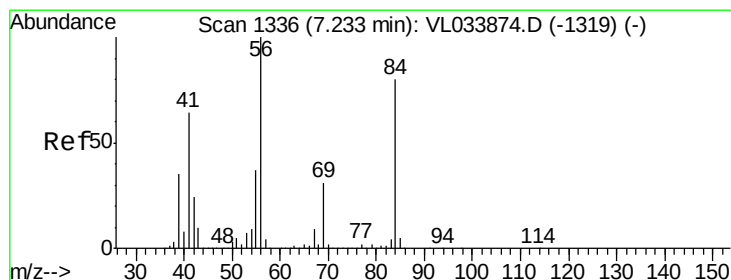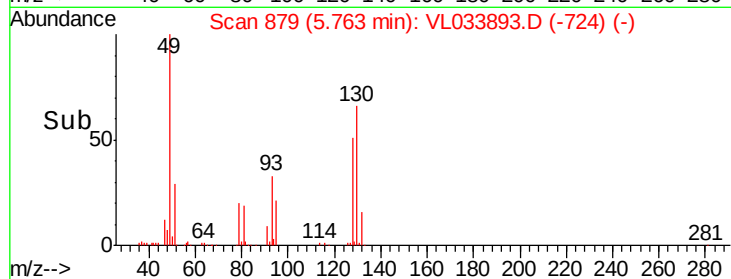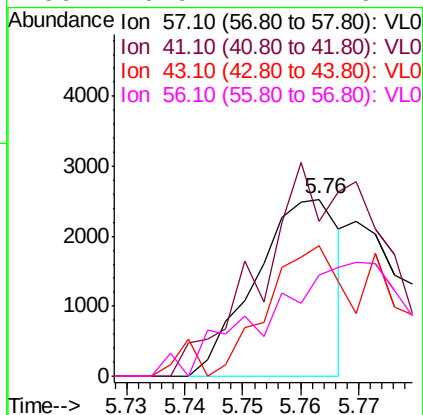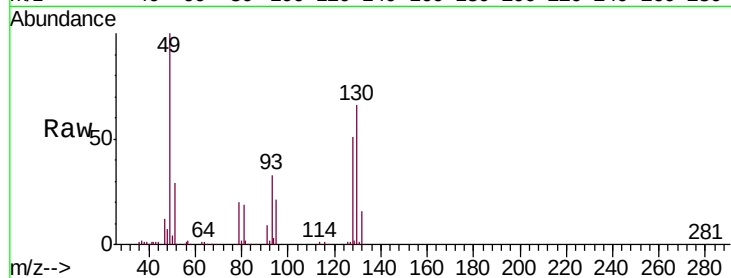

#30
Cyclohexane
Concen: 0.090 ppbv
RT: 7.26 min Scan# 1345
Delta R.T. 0.03 min
Lab File: VL033893.D
Acq: 7 Jun 2019 17:38

Tgt Ion: 84 Resp: 4996
Ion Ratio Lower Upper
84 100
56 0.0 105.8 158.8#
41 0.0 65.7 98.5#

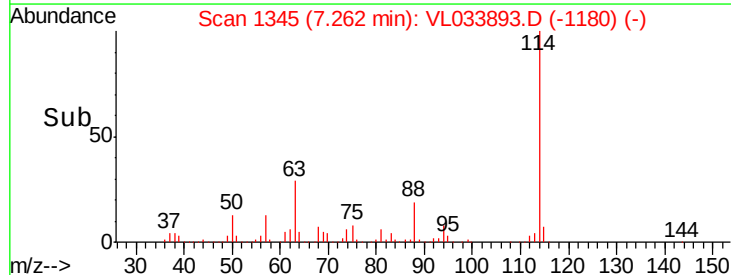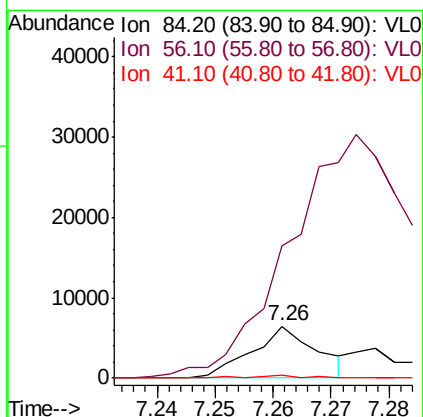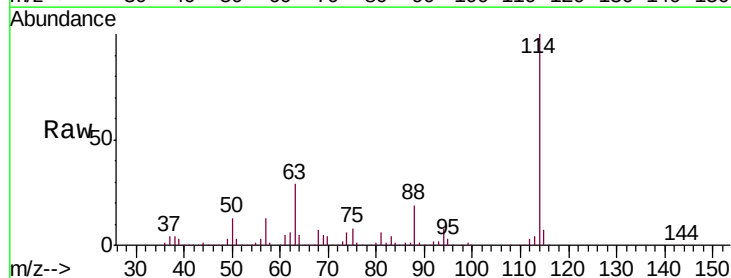

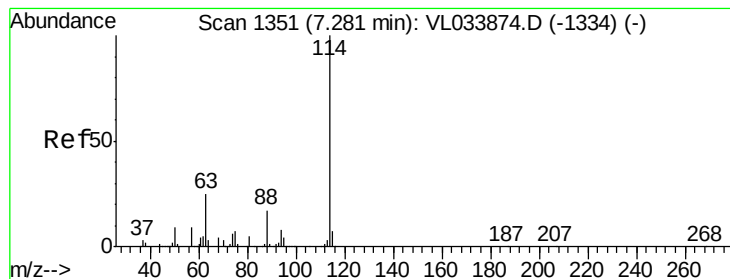

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.27 min Scan# 1349

Delta R.T. -0.01 min

Lab File: VL033893.D

Acq: 7 Jun 2019 17:38

Instrument :

MSVOA_L

ClientSampleId :

CAN 10150


Tgt Ion:114 Resp: 1771665

Ion Ratio Lower Upper

114 100

63 26.7 21.1 31.7




88 18.2 14.2 21.4

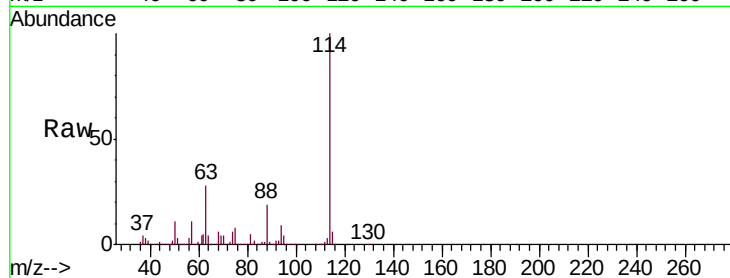

Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

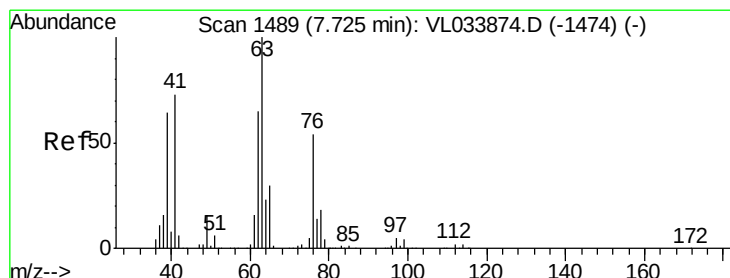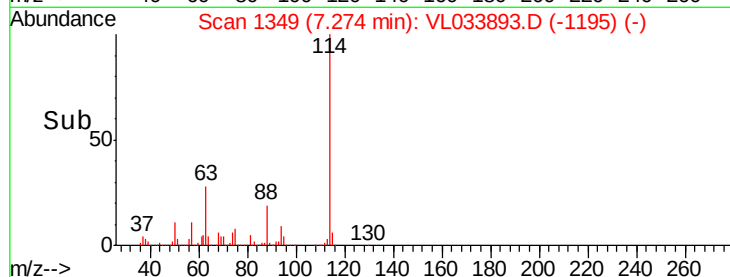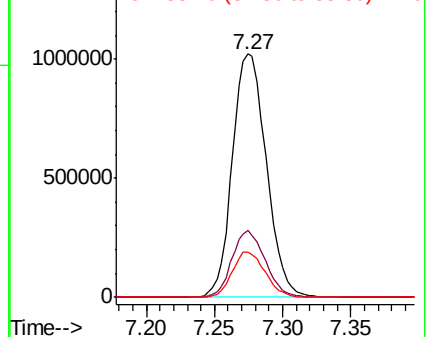

#39

1,2-Dichloropropane

Concen: 9.033 ppbv

RT: 7.27 min Scan# 1349

Delta R.T. -0.45 min

Lab File: VL033893.D

Acq: 7 Jun 2019 17:38


Tgt Ion: 63 Resp: 471799

Ion Ratio Lower Upper

63 100

41 0.0 58.7 88.1#



62 17.5 51.9 77.9#

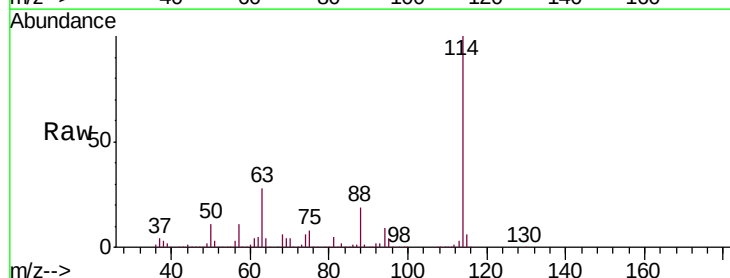


Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 62.10 (61.80 to 62.80): VL0

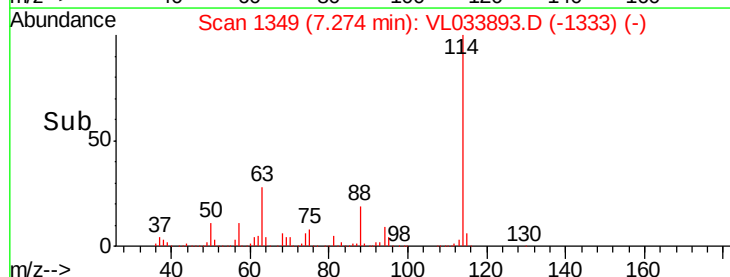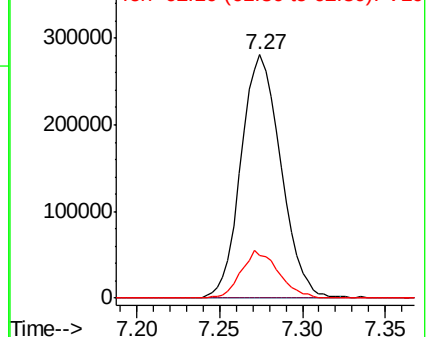


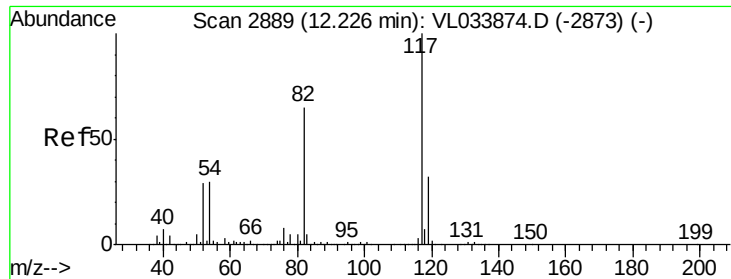




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.22 min Scan# 2888
Delta R.T. -0.00 min
Lab File: VL033893.D
Acq: 7 Jun 2019 17:38

Instrument :
MSVOA_L
ClientSampleId :
CAN 10150

Tgt Ion: 117 Resp: 1762578
Ion Ratio Lower Upper
117 100
82 69.3 50.2 75.2
119 32.3 24.8 37.2

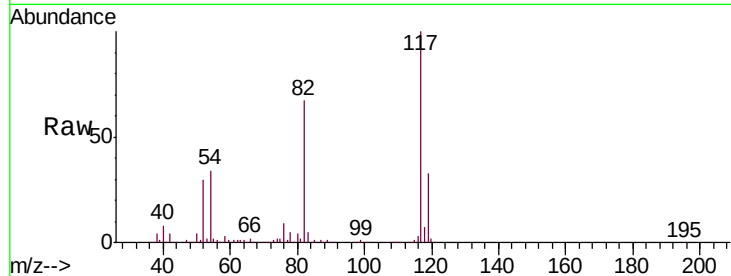


Abundance Ion 117.10 (116.80 to 117.80): V
Ion 82.10 (81.80 to 82.80): VL0
Ion 119.10 (118.80 to 119.80): V

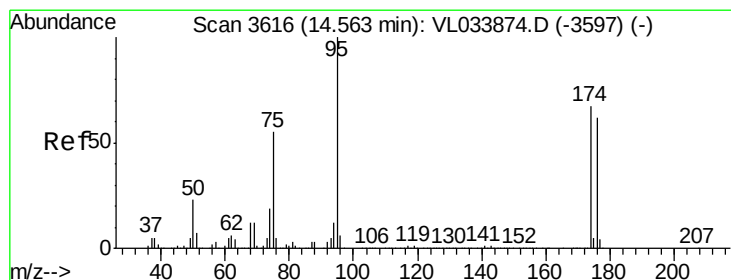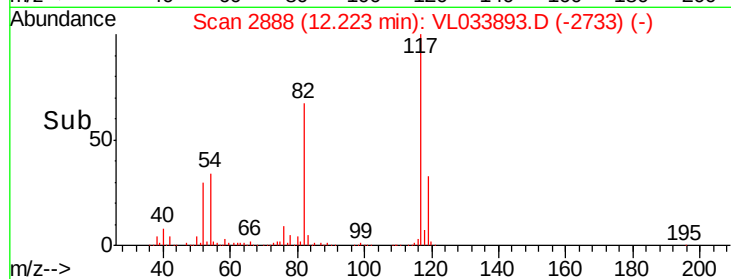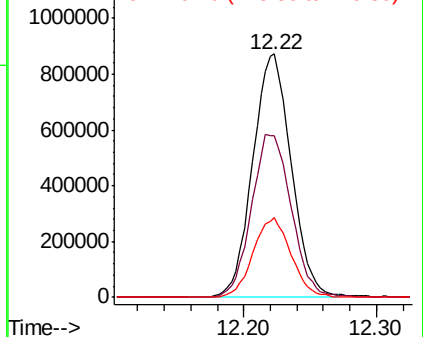

#68
1-Bromo-4-Fluorobenzene
Concen: 9.967 ppbv
RT: 14.56 min Scan# 3614
Delta R.T. -0.01 min
Lab File: VL033893.D
Acq: 7 Jun 2019 17:38

Tgt Ion: 95 Resp: 1442974
Ion Ratio Lower Upper
95 100
174 64.9 54.0 81.0
175 4.6 3.8 5.8

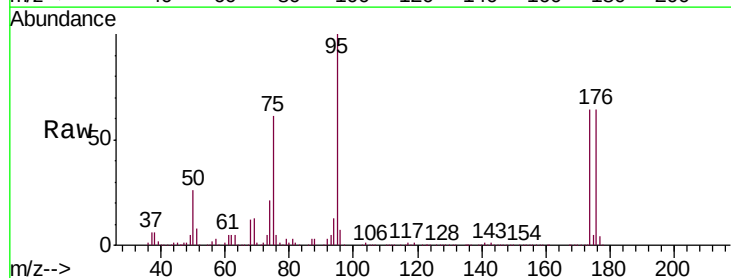

Abundance Ion 95.10 (94.80 to 95.80): VL0
Ion 174.00 (173.70 to 174.70): V
Ion 175.00 (174.70 to 175.70): V

