

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL060719\
Data File : VL033891.D
Acq On : 7 Jun 2019 16:16
Operator : SY/AP
Sample : CAN 10737
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10737

Quant Time: Jun 09 21:54:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL060719AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019
QLast Update : Fri Jun 07 08:53:27 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.75	49	772383	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.27	114	1768808	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.22	117	1759458	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.56	95	1451634	10.04	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.40%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL060719\
Data File : VL033891.D
Acq On : 7 Jun 2019 16:16
Operator : SY/AP
Sample : CAN 10737
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10737

Quant Time: Jun 09 21:54:24 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL060719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019
QLast Update : Fri Jun 07 08:53:27 2019
Response via : Initial Calibration

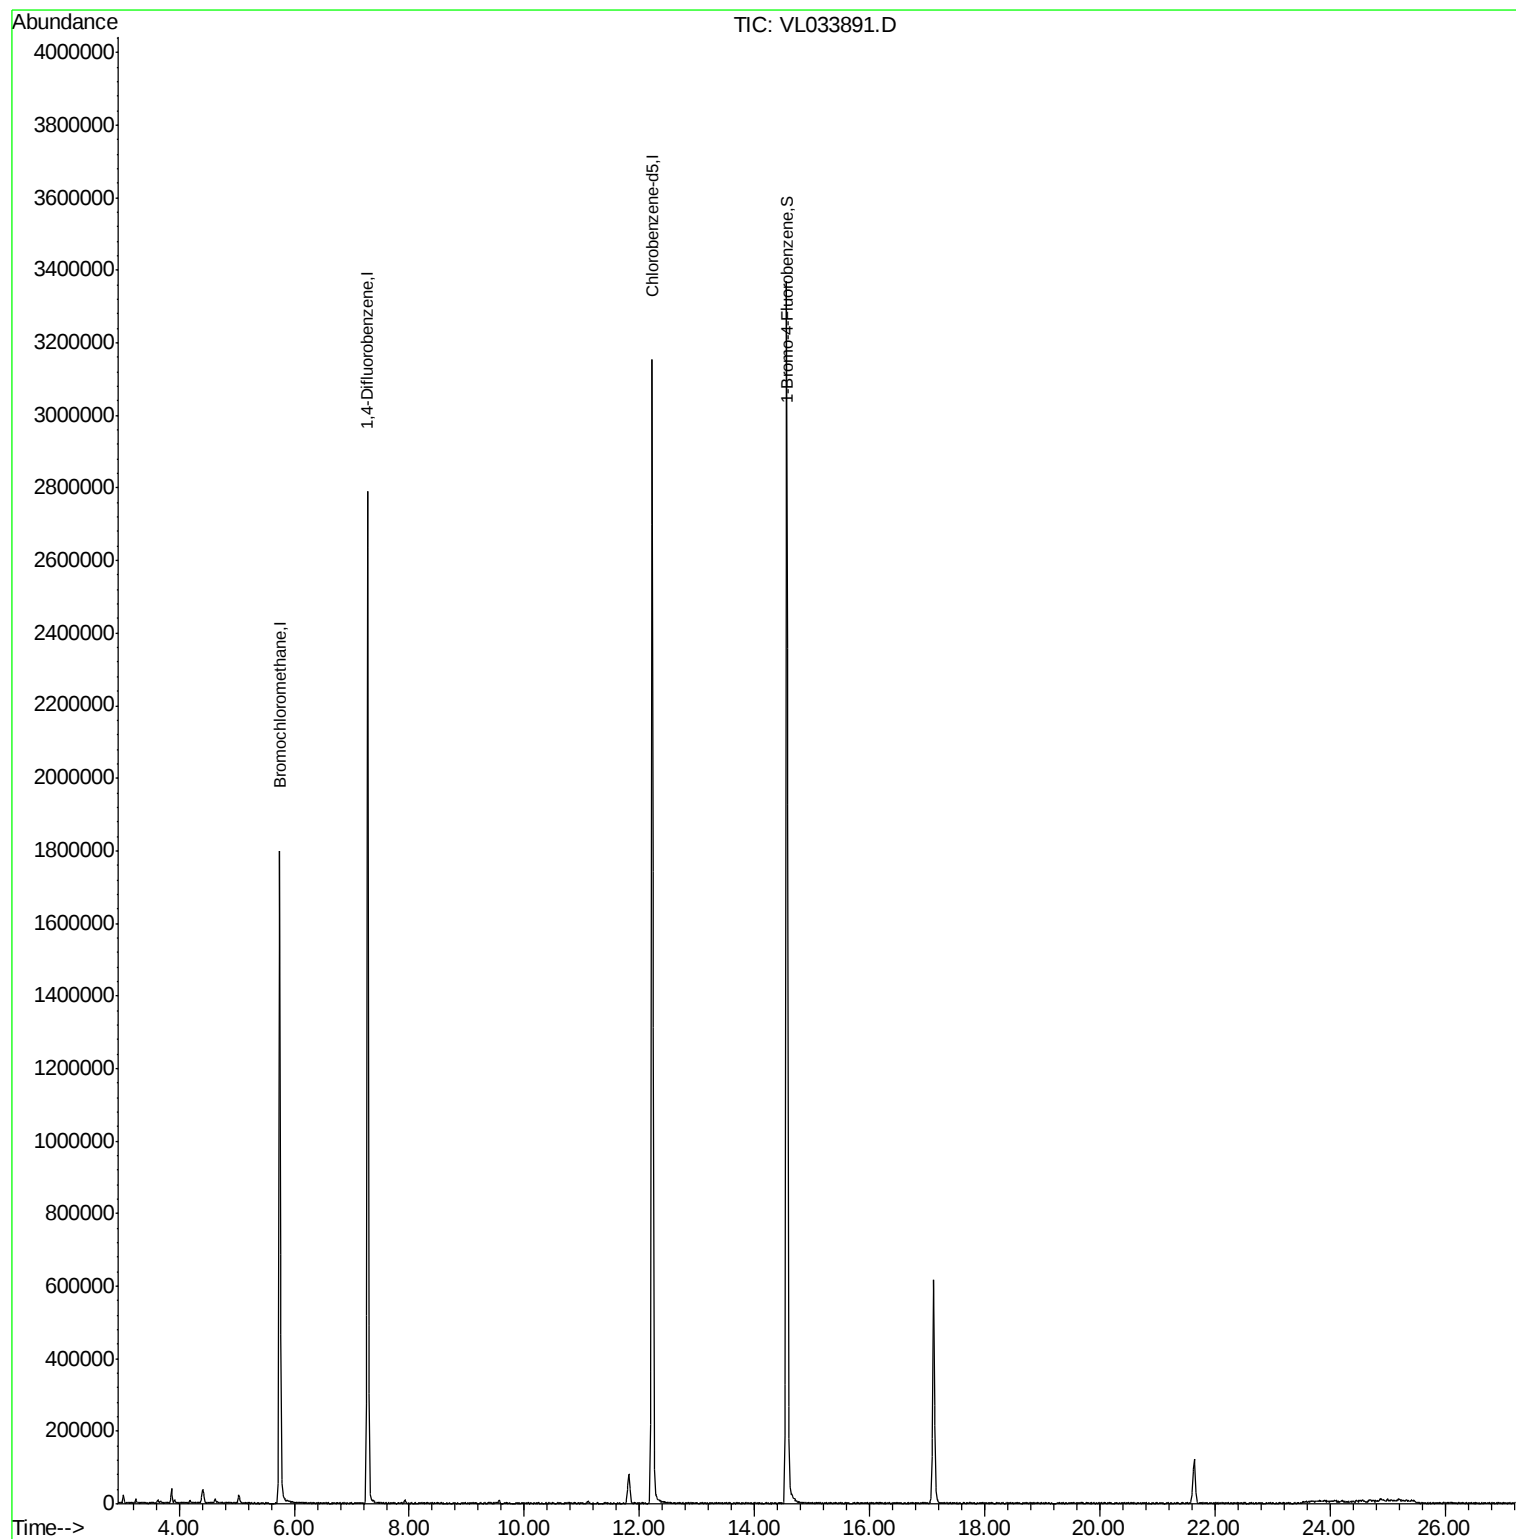

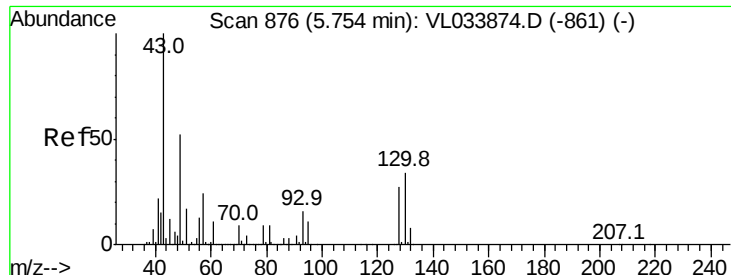

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.75 min Scan# 874

Delta R.T. -0.01 min

Lab File: VL033891.D

Acq: 7 Jun 2019 16:16

Instrument :

MSVOA_L

ClientSampleId :

CAN 10737


Tot Ion: 49 Resp: 772383

Ion Ratio Lower Upper

49 100

128 49.8 25.5 76.5




130 63.8 32.5 97.4

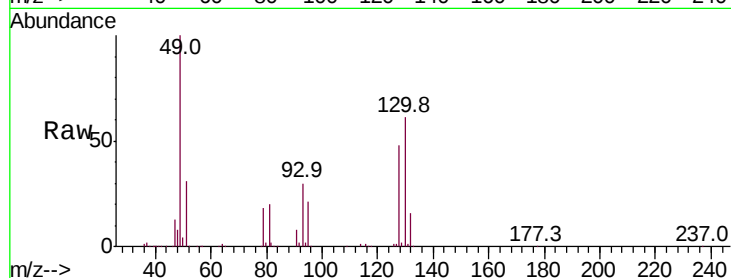

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

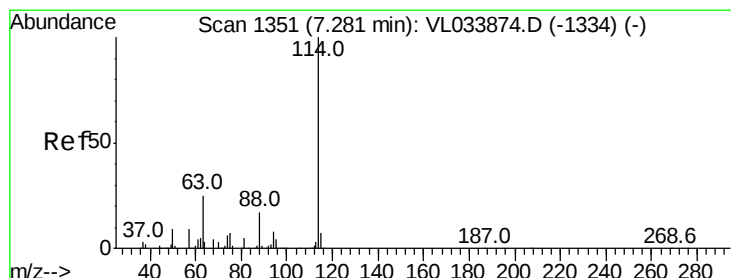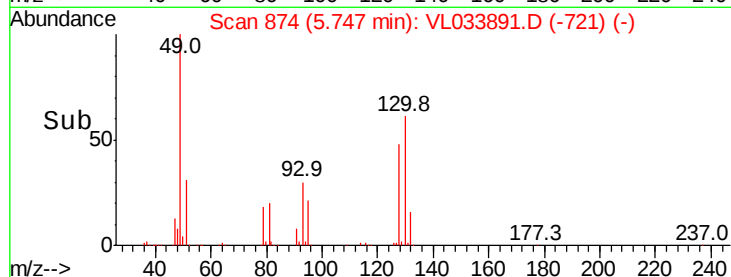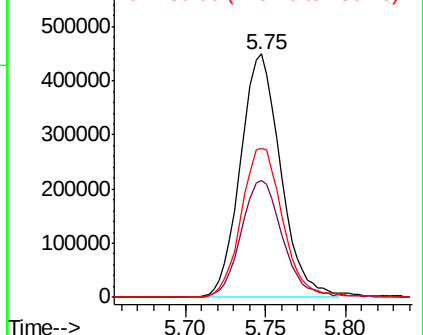

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.27 min Scan# 1349

Delta R.T. -0.01 min

Lab File: VL033891.D

Acq: 7 Jun 2019 16:16


Tgt Ion: 114 Resp: 1768808

Ion Ratio Lower Upper

114 100

63 27.4 21.1 31.7



88 18.4 14.2 21.4

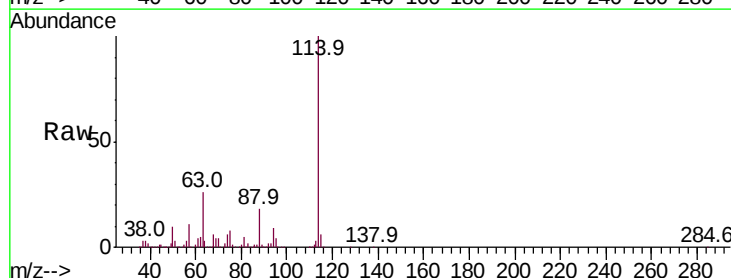


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

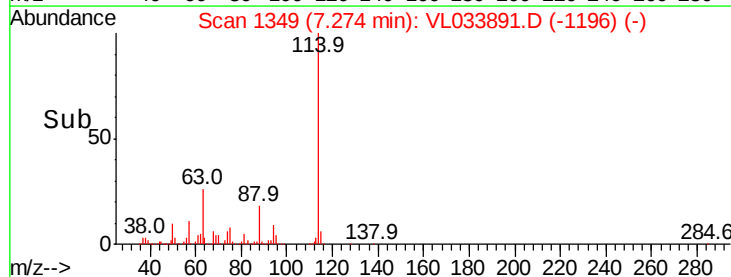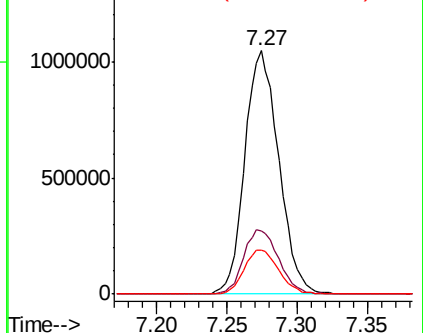


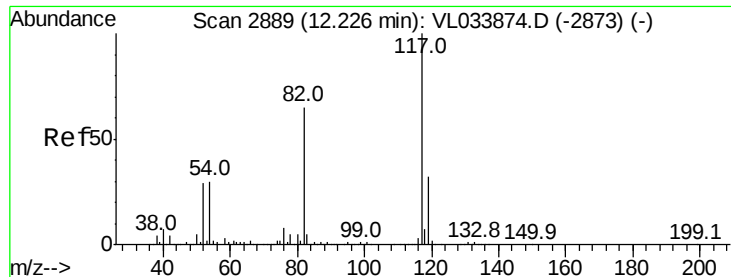




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.22 min Scan# 2887
Delta R.T. -0.01 min
Lab File: VL033891.D
Acq: 7 Jun 2019 16:16

Instrument :
MSVOA_L
ClientSampleId :
CAN 10737

Tot Ion:117 Resp: 1759458
Ion Ratio Lower Upper
117 100
82 69.6 50.2 75.2
119 32.3 24.8 37.2

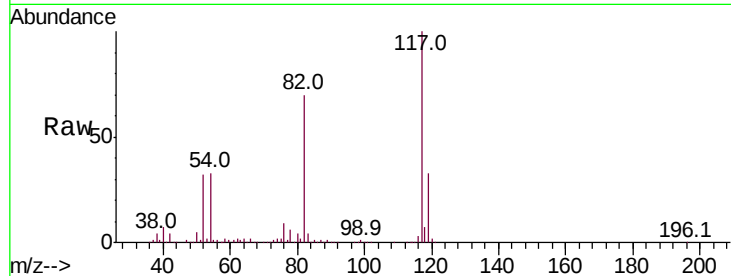


Abundance Ion 117.10 (116.80 to 117.80): V
Ion 82.10 (81.80 to 82.80): VL0
Ion 119.10 (118.80 to 119.80): V

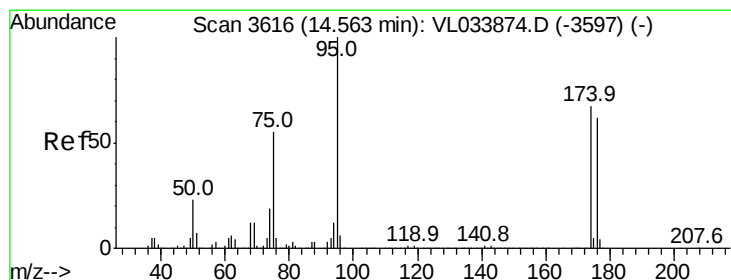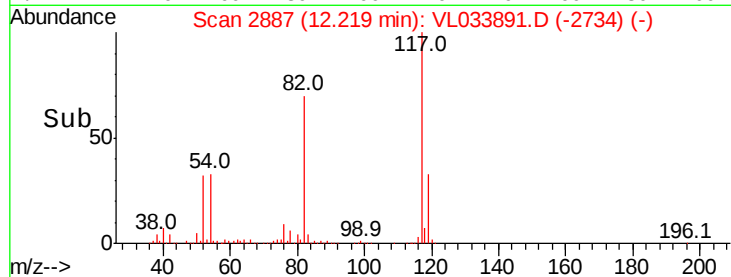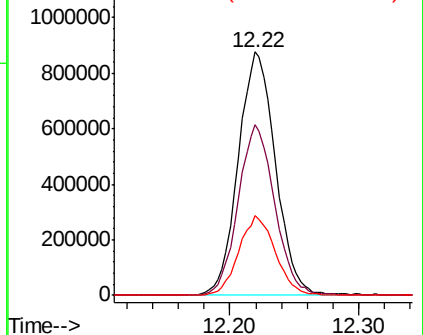

#68
1-Bromo-4-Fluorobenzene
Concen: 10.045 ppbv
RT: 14.56 min Scan# 3615
Delta R.T. -0.00 min
Lab File: VL033891.D
Acq: 7 Jun 2019 16:16

Tgt Ion: 95 Resp: 1451634
Ion Ratio Lower Upper
95 100
174 66.1 54.0 81.0
175 4.7 3.8 5.8

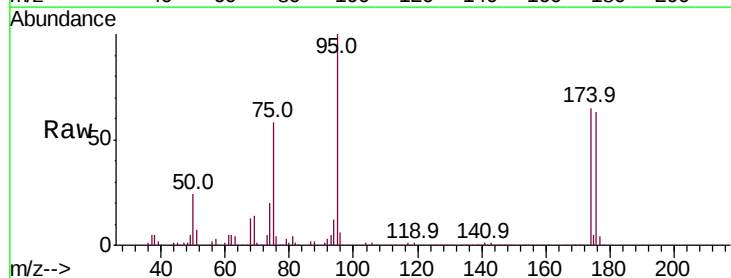

Abundance Ion 95.10 (94.80 to 95.80): VL0
Ion 174.00 (173.70 to 174.70): V
Ion 175.00 (174.70 to 175.70): V

