


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL060719\
 Data File : VL033873.D
 Acq On : 7 Jun 2019 1:24
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL060719AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019
 Last Update : Fri Jun 07 08:53:27 2019

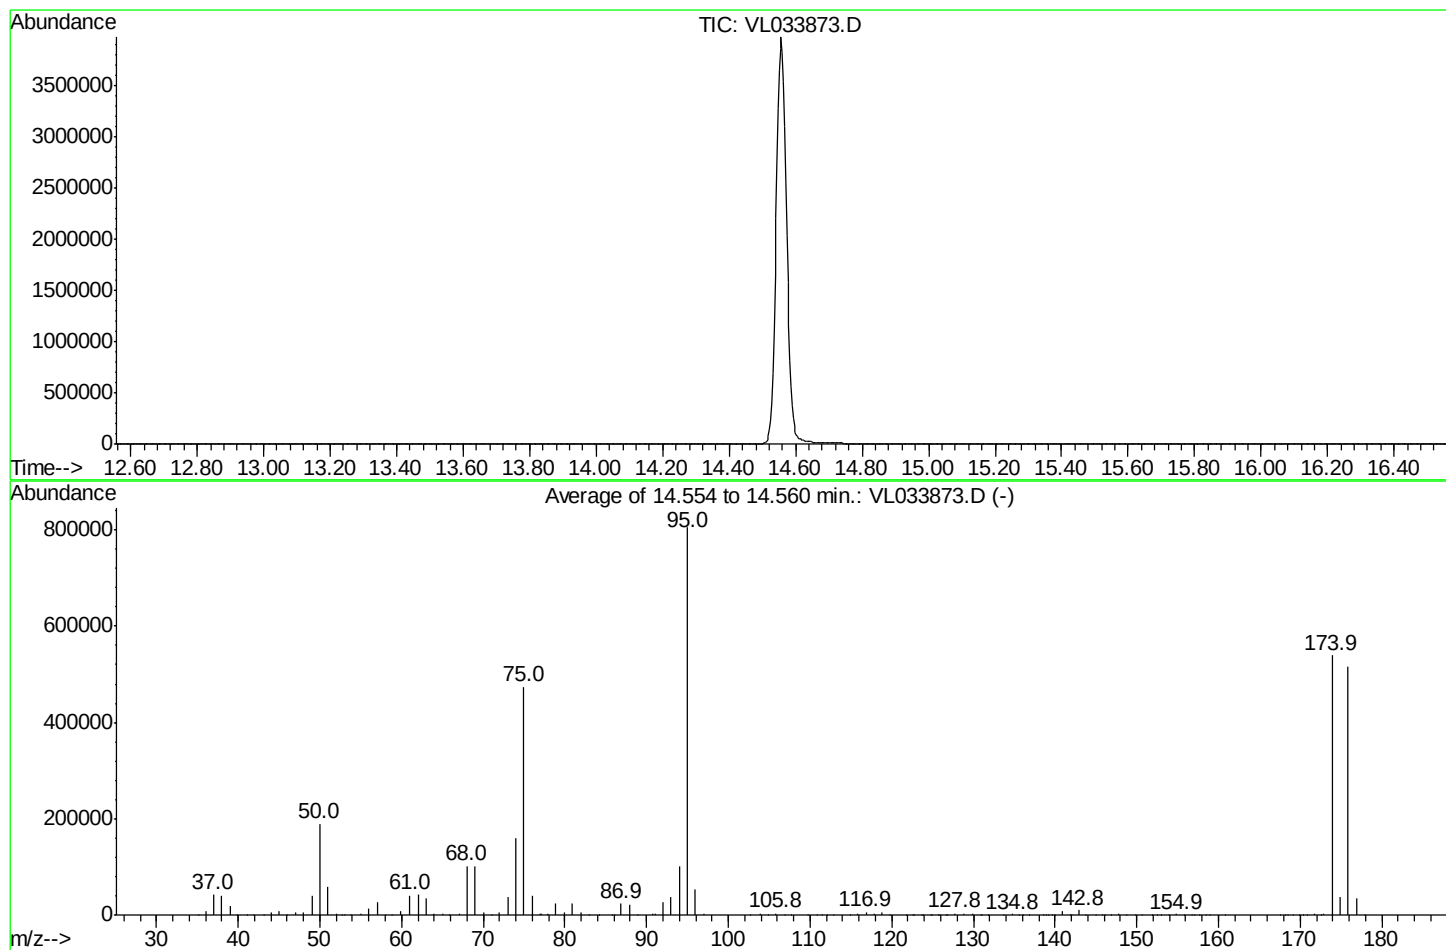

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.5	189312	PASS
75	95	30	66	58.8	473557	PASS
95	95	100	100	100.0	805440	PASS
96	95	5	9	6.8	54392	PASS
173	174	0.00	2	0.5	2468	PASS
174	95	50	120	67.0	539456	PASS
175	174	4	9	7.0	37973	PASS
176	174	93	101	95.9	517098	PASS
177	176	5	9	6.7	34528	PASS