


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL060722\
 Data File : VL039203.D
 Acq On : 7 Jun 2022 9:53
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

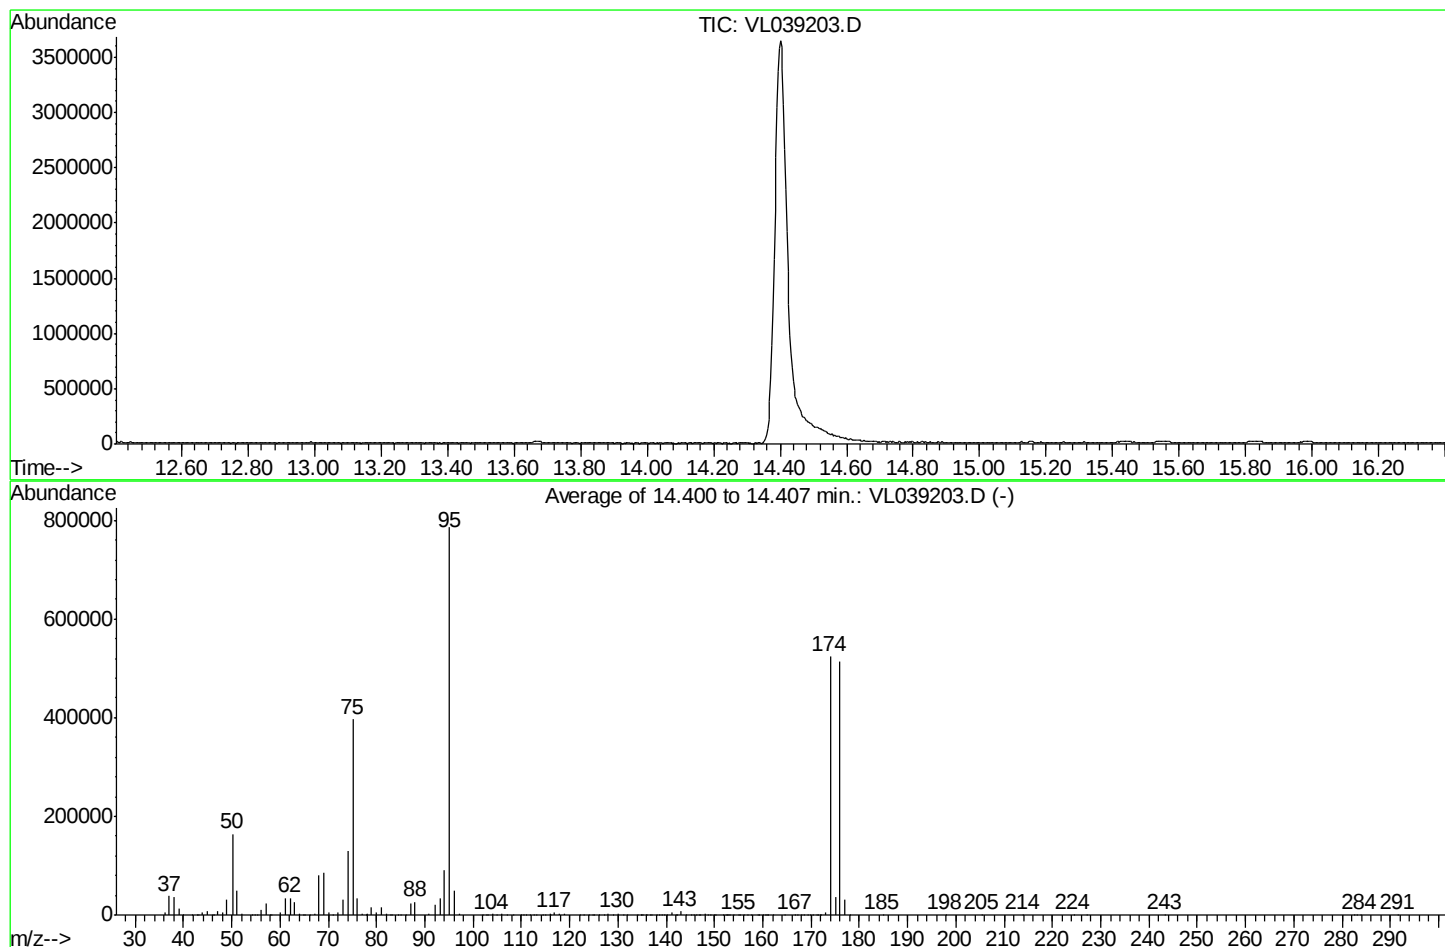

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.9	164565	PASS
75	95	30	66	50.4	396010	PASS
95	95	100	100	100.0	785856	PASS
96	95	5	9	6.2	48898	PASS
173	174	0.00	2	1.0	5463	PASS
174	95	50	120	66.6	523712	PASS
175	174	4	9	7.1	36952	PASS
176	174	93	101	97.9	512576	PASS
177	176	5	9	6.0	30746	PASS