


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL060822\
 Data File : VL039230.D
 Acq On : 8 Jun 2022 9:49
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

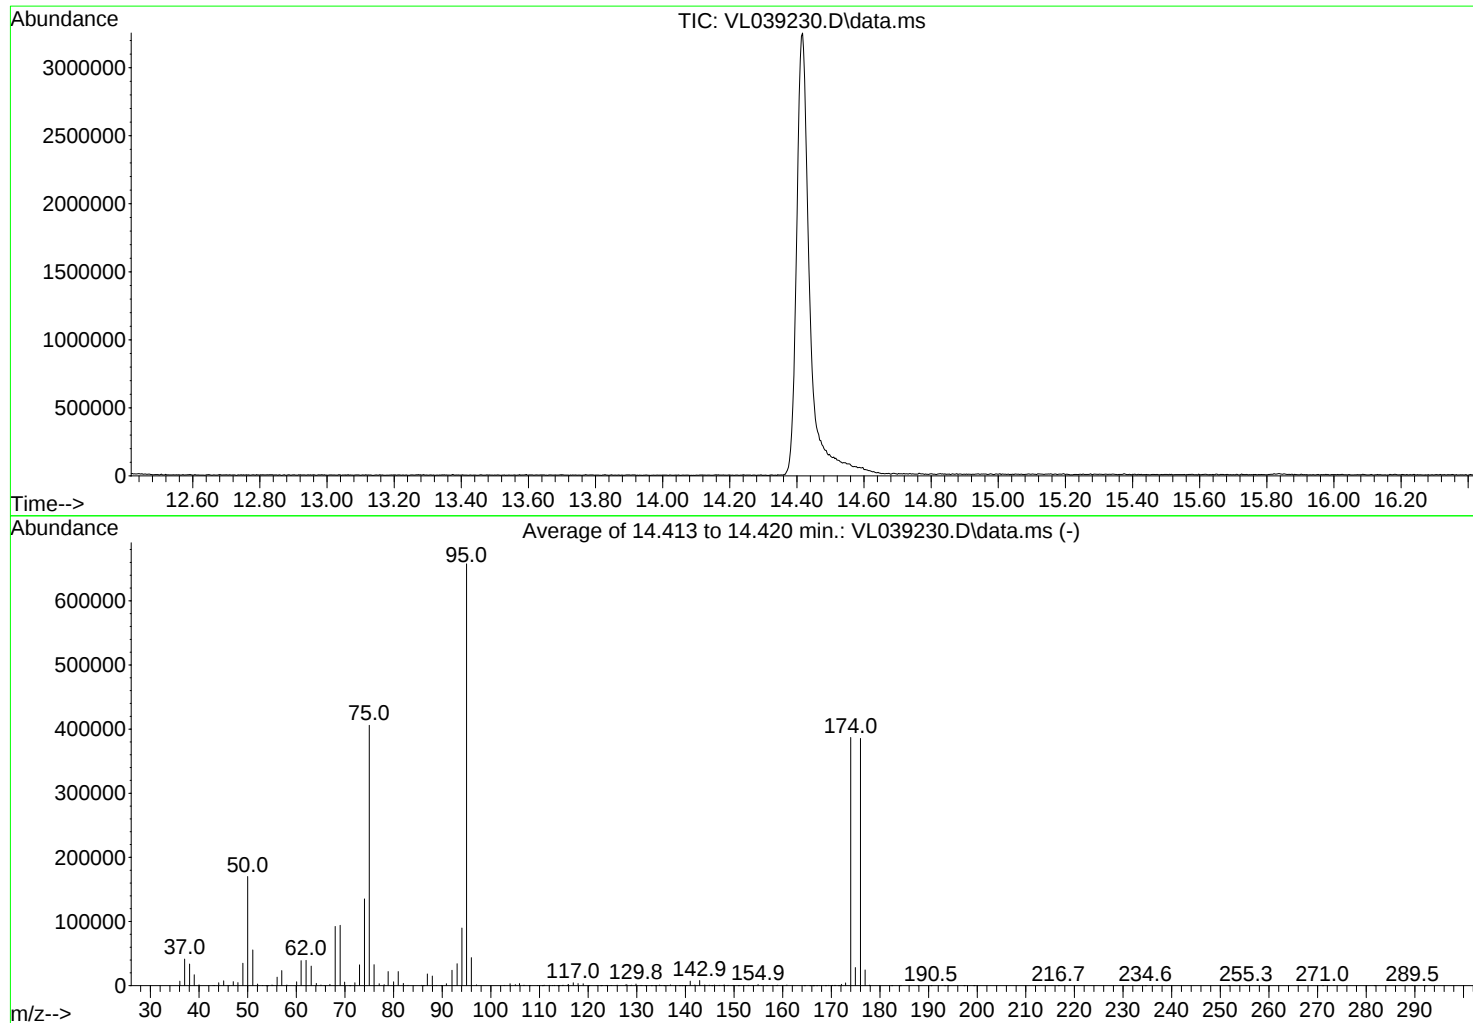

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.9	170197	PASS
75	95	30	66	61.7	405995	PASS
95	95	100	100	100.0	657707	PASS
96	95	5	9	6.6	43728	PASS
173	174	0.00	2	1.1	4332	PASS
174	95	50	120	58.8	386987	PASS
175	174	4	9	7.3	28245	PASS
176	174	93	101	99.6	385579	PASS
177	176	5	9	6.3	24416	PASS

Average of 14.413 to 14.420 min.: VL039230.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6923	47.05	6261	56.05	13250	68.00	9226
37.05	41517	48.00	4852	57.00	23360	69.00	9398
38.05	33744	49.00	34976	58.05	1022	69.95	550
39.00	16883	50.00	170197	60.05	5935	71.00	13
40.00	1359	51.05	55611	61.00	38917	71.20	240
42.90	228	52.05	2433	62.00	39541	72.05	4553
43.20	189	53.10	203	63.05	30544	73.00	32432
44.05	4430	53.80	80	64.10	3403	74.00	135232
45.05	7636	54.10	72	65.05	1095	75.00	405995
45.95	505	55.00	1071	65.85	178	76.00	32717
46.20	359	55.20	429	66.90	1926	77.05	3024

Average of 14.413 to 14.420 min.: VL039230.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.05	1604	89.80	74	105.90	3219	114.00	96
78.90	22037	90.85	2909	106.80	771	114.70	248
80.00	6102	92.00	23851	107.90	153	114.85	676
80.95	22011	93.05	34125	109.60	249	115.80	1067
82.00	3536	94.05	89731	109.95	191	115.95	1733
82.95	563	95.00	657707	110.60	54	116.95	4616
85.80	472	96.00	43728	110.95	775	117.95	3282
86.10	64	97.05	1261	112.10	513	119.00	3082
86.95	18229	102.75	453	112.70	170	120.10	51
87.95	15070	103.95	3111	113.05	573	121.80	252
88.80	230	105.05	1410	113.80	95	122.00	194

Average of 14.413 to 14.420 min.: VL039230.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.60	51	130.85	480	138.00	348	144.90	859
122.95	217	131.05	340	138.80	123	145.45	57
123.70	195	131.80	67	139.10	222	145.95	1079
123.90	410	133.00	61	139.30	86	146.95	505
124.75	320	133.80	148	139.70	243	147.80	847
125.95	859	134.10	282	140.00	276	148.05	1001
127.80	1843	134.70	1000	140.20	340	148.75	619
128.00	995	135.00	352	141.00	6887	149.80	586
128.70	340	135.60	71	141.95	950	150.90	97
128.95	888	136.40	220	142.95	7957	152.05	314
129.85	2567	136.90	1314	144.00	1018	152.95	388

Average of 14.413 to 14.420 min.: VL039230.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.90	314	165.60	77	171.50	130	187.80	63
154.95	1649	166.20	107	172.10	2137	190.50	71
155.70	279	166.40	55	172.95	4332	193.30	68
156.75	588	167.00	65	174.00	386987	194.00	62
157.00	380	167.50	255	174.95	28245	197.30	51
157.90	331	168.80	83	176.00	385579	199.30	59
158.70	181	168.95	214	176.95	24416	216.70	157
159.00	813	169.50	463	177.85	805	234.60	54
160.85	949	170.25	525	178.10	280	251.70	72
162.05	230	170.70	530	182.40	154	255.30	185
164.50	101	170.90	398	184.20	58	271.00	74

Average of 14.413 to 14.420 min.: VL039230.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
281.70	60						
289.50	259						
292.10	51						