


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061124\
Data File : VL041339.D
Acq On : 11 Jun 2024 9:33
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060424AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Jun 12 01:18:29 2024

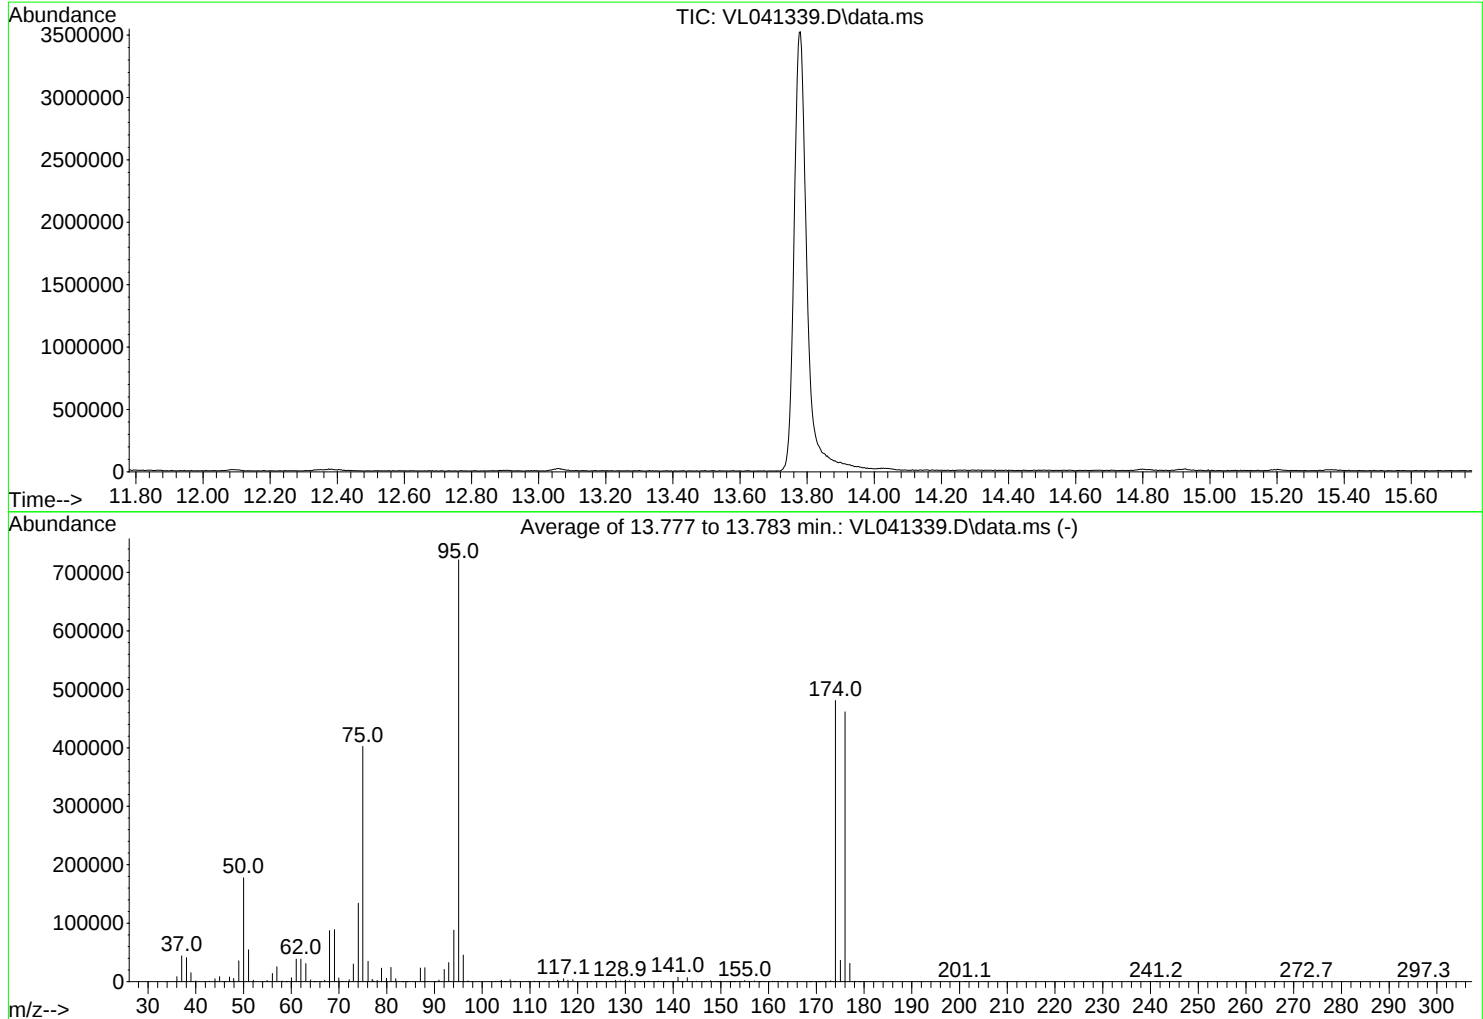

AutoFind: Scans 3475, 3476, 3477; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.6	177749	PASS
75	95	30	66	55.8	402325	PASS
95	95	100	100	100.0	721536	PASS
96	95	5	9	6.3	45403	PASS
173	174	0.00	2	0.3	1614	PASS
174	95	50	120	66.7	481045	PASS
175	174	4	9	7.6	36427	PASS
176	174	93	101	96.0	461568	PASS
177	176	5	9	6.8	31165	PASS

Average of 13.777 to 13.783 min.: VL041339.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8453	47.95	5560	61.05	38549	70.80	294
37.05	44104	49.00	35739	62.00	38725	72.15	332
38.05	41192	50.00	177749	63.05	30880	73.00	3018
39.00	15444	51.05	54496	64.05	2982	74.05	13401
40.00	1060	52.05	2349	64.80	134	75.00	402325
42.90	469	54.95	2158	65.15	306	76.10	34856
44.00	4817	56.05	13866	66.10	62	76.95	3949
45.00	8560	57.00	25456	67.00	2480	77.20	1024
45.90	237	58.05	992	68.00	87200	78.00	2277
46.25	618	58.95	139	69.05	89008	78.90	23144
47.05	7933	60.05	6685	69.95	6240	79.95	5901

Average of 13.777 to 13.783 min.: VL041339.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	24317	93.00	32632	105.85	3290	115.80	2418
81.90	5006	94.05	88277	106.75	467	116.10	802
83.20	362	95.05	721536	107.00	350	117.05	4927
83.40	84	96.05	45403	109.75	508	117.95	2466
84.20	159	97.05	1266	110.10	183	119.00	3653
85.90	441	102.85	532	111.00	876	121.95	211
87.05	23376	103.80	966	111.80	415	122.70	76
88.00	23915	104.00	2373	112.10	324	123.75	321
90.00	58	104.60	303	112.95	821	124.05	461
90.95	2684	104.80	375	114.80	320	124.50	51
92.05	20896	105.05	648	115.05	481	125.05	278

Average of 13.777 to 13.783 min.: VL041339.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.80	106	134.70	357	142.10	469	149.50	70
126.05	187	134.95	819	142.95	6850	149.90	704
126.85	212	135.90	96	144.05	521	151.85	162
127.10	95	136.70	314	144.95	713	152.10	73
127.95	2197	136.95	943	145.85	679	152.60	215
128.95	1303	138.10	57	146.10	192	152.85	32
130.00	2573	139.05	383	146.40	122	153.85	214
130.85	1356	139.75	576	146.95	328	154.30	175
131.80	162	140.00	88	147.85	1687	155.00	1857
133.00	78	141.00	7811	148.80	302	155.85	460
133.75	173	141.85	565	149.10	557	157.05	1365

Average of 13.777 to 13.783 min.: VL041339.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
158.10	60	170.40	204	179.10	64		
158.80	674	170.70	87	201.10	54		
159.10	381	171.20	551	241.20	57		
160.00	52	171.65	531	266.10	51		
160.75	949	171.90	303	272.70	106		
161.20	216	173.00	1614	292.20	64		
161.80	209	174.00	481045	297.30	191		
162.70	61	175.05	36427				
168.60	72	176.00	461568				
168.95	347	177.00	31165				
169.90	295	178.10	770				