


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061322\
 Data File : VL039252.D
 Acq On : 13 Jun 2022 11:18
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

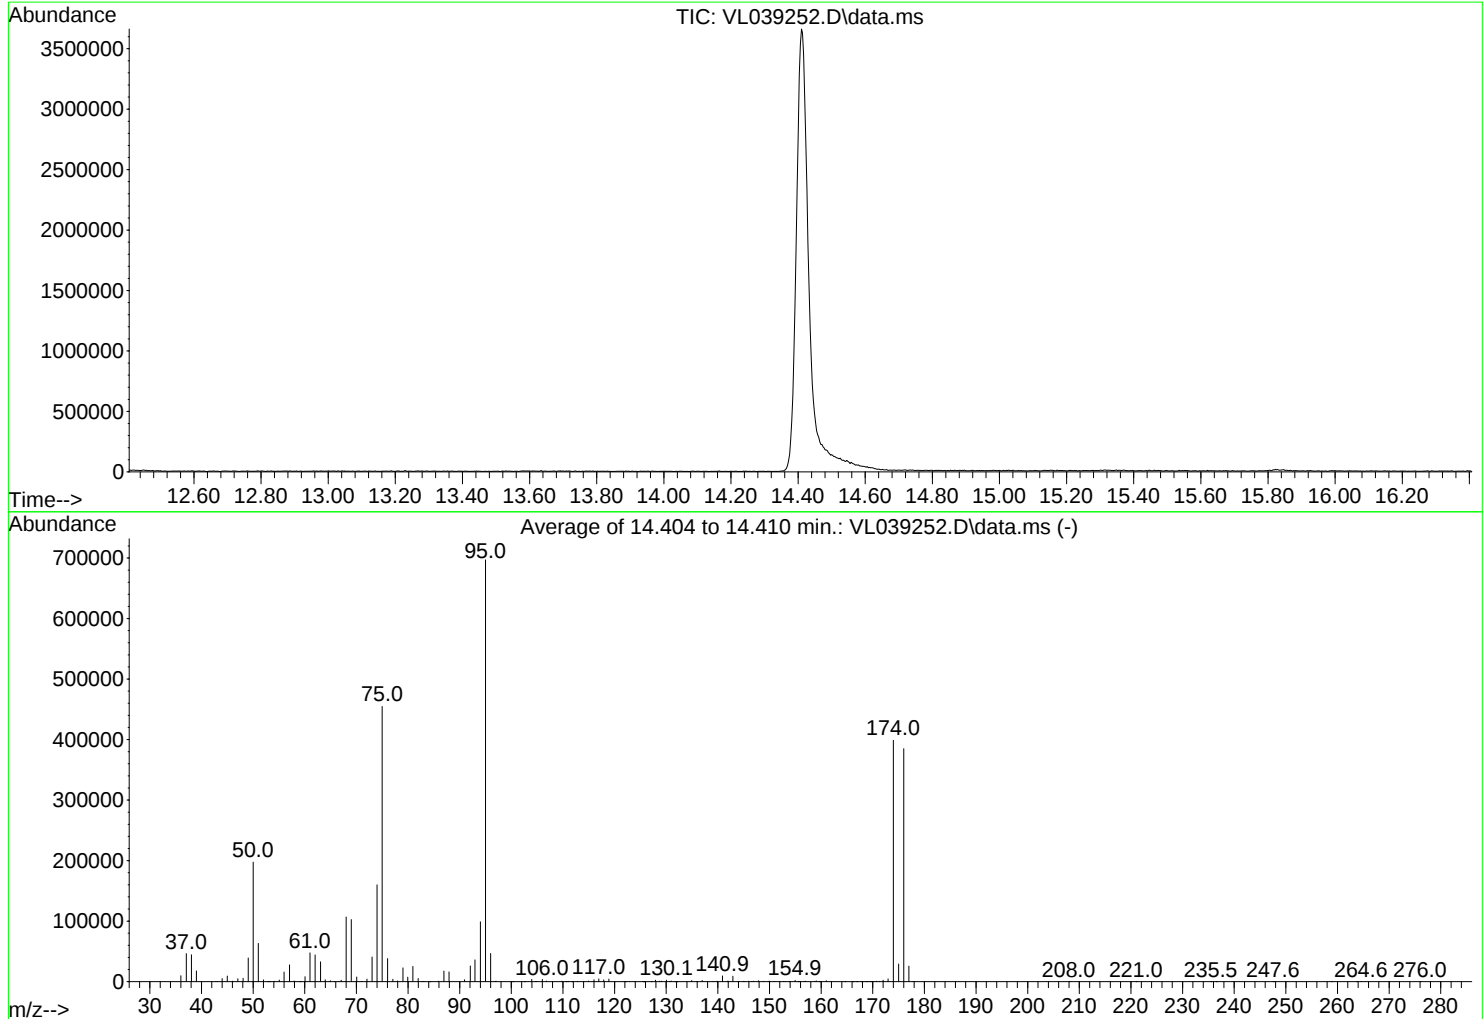

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	28.3	197376	PASS
75	95	30	66	65.2	454763	PASS
95	95	100	100	100.0	696960	PASS
96	95	5	9	6.7	46581	PASS
173	174	0.00	2	1.1	4399	PASS
174	95	50	120	57.2	398720	PASS
175	174	4	9	7.3	29157	PASS
176	174	93	101	96.5	384896	PASS
177	176	5	9	6.7	25661	PASS

Average of 14.404 to 14.410 min.: VL039252.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	9852	48.05	5694	57.95	1142	68.00	10680
37.05	46232	49.05	39213	59.10	63	69.00	10249
38.05	44389	50.00	197376	60.05	8331	70.05	758
39.00	17629	51.00	63208	61.00	47512	71.05	64
39.90	326	52.00	3052	62.00	44080	72.05	4185
42.80	250	52.80	131	63.05	32824	73.05	40632
43.10	386	53.20	147	63.95	3130	74.00	160021
44.00	5013	54.10	473	64.95	1708	75.00	454763
45.00	9188	55.05	2712	65.80	234	76.05	38053
46.05	680	56.00	15913	66.60	401	77.05	3944
47.05	4868	57.05	27875	67.05	2273	77.95	1036

Average of 14.404 to 14.410 min.: VL039252.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.00	22685	90.95	3247	104.70	194	114.95	1157
79.95	7336	92.05	26000	104.80	331	116.00	3141
80.95	25107	92.95	35968	104.95	404	116.95	4581
81.95	5202	94.00	98987	106.00	3594	117.90	2869
82.70	244	95.00	696960	106.85	1040	118.90	4365
82.90	573	96.00	46581	109.80	703	121.85	199
83.10	405	96.90	464	110.60	145	122.10	144
84.20	67	97.05	931	111.05	496	122.85	318
85.85	797	100.30	150	111.70	144	123.80	188
86.95	17380	102.55	150	112.00	508	125.50	101
87.95	16278	103.95	3643	112.80	471	125.70	115

Average of 14.404 to 14.410 min.: VL039252.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.05	198	135.80	211	144.95	537	152.70	327
127.10	107	136.05	211	145.20	296	153.00	231
127.90	2289	136.95	2054	145.95	930	153.80	133
128.75	791	139.05	609	146.60	210	153.95	551
129.10	816	139.85	915	146.95	675	154.95	2145
130.05	2400	140.90	9489	147.90	1628	155.55	155
130.70	506	141.85	929	148.90	566	155.90	147
130.95	1182	142.10	830	149.75	588	156.70	543
131.70	129	142.90	9053	150.05	751	156.95	697
132.10	51	143.90	642	150.90	441	158.70	248
134.95	1731	144.10	571	152.00	462	159.05	1331

Average of 14.404 to 14.410 min.: VL039252.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
159.65	159	170.20	317	208.00	71		
161.00	1670	170.70	875	221.00	54		
161.95	175	171.25	641	235.50	64		
164.60	53	172.00	2383	236.50	59		
166.20	55	172.95	4399	247.55	150		
166.90	116	174.00	398720	258.80	79		
167.80	155	175.00	29157	263.70	73		
168.30	403	176.00	384896	264.60	171		
168.80	140	177.00	25661	276.00	81		
169.30	397	177.80	395				
169.60	126	178.10	235				