


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061421\
 Data File : VL037144.D
 Acq On : 14 Jun 2021 9:34
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL061421AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue May 18 12:00:15 2021
 Last Update : Tue May 18 12:00:15 2021

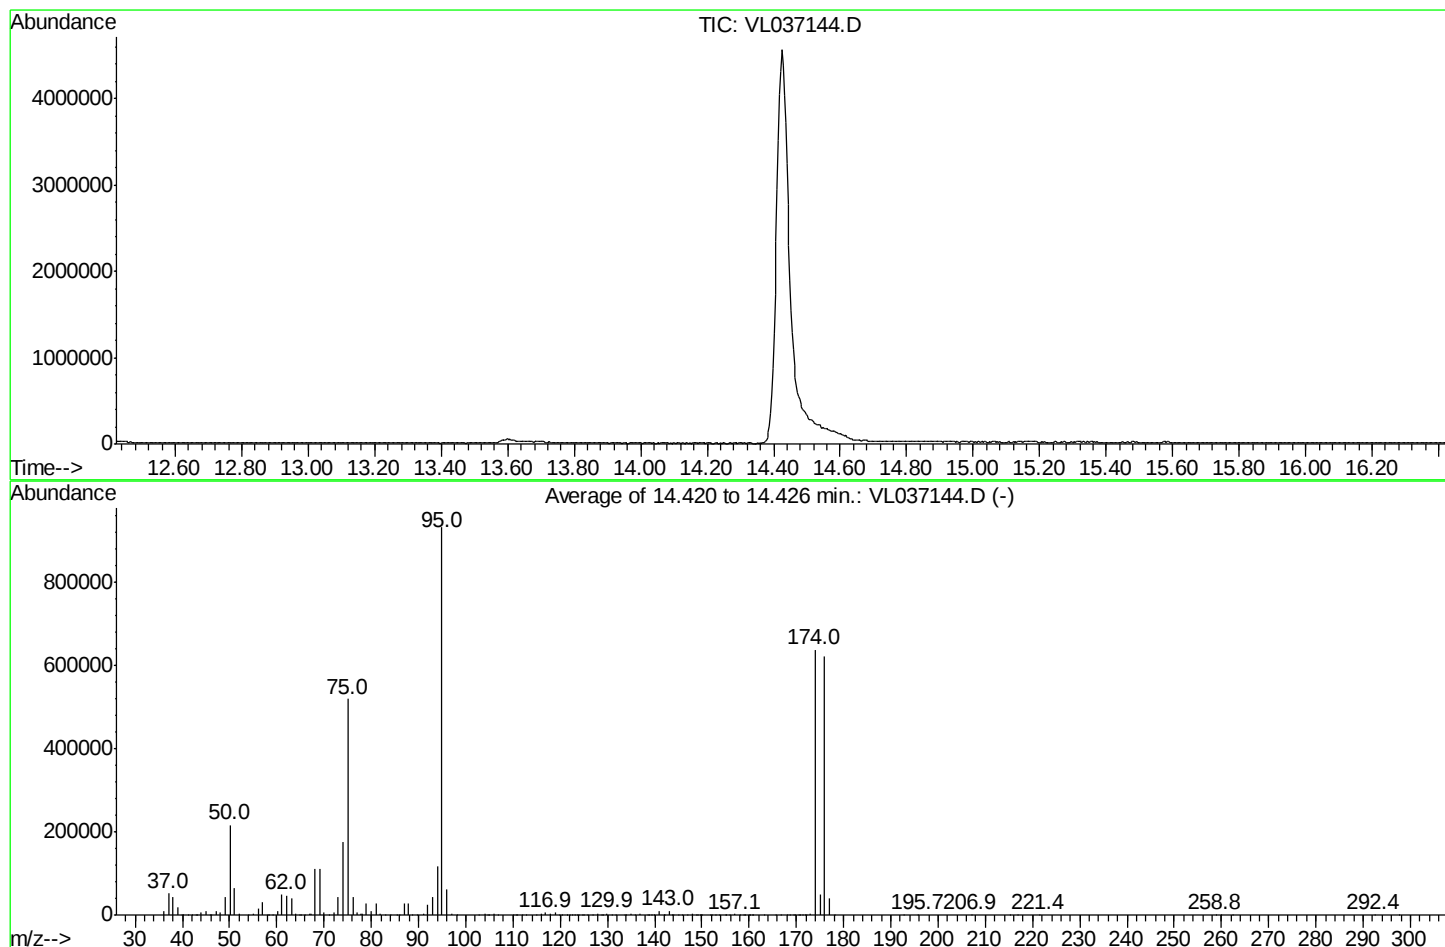

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.2	216362	PASS
75	95	30	66	55.7	519722	PASS
95	95	100	100	100.0	932650	PASS
96	95	5	9	6.8	63165	PASS
173	174	0.00	2	0.4	2296	PASS
174	95	50	120	68.4	637610	PASS
175	174	4	9	7.9	50632	PASS
176	174	93	101	97.4	620906	PASS
177	176	5	9	6.6	41069	PASS