

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061422\
 Data File : VL039291.D
 Acq On : 15 Jun 2022 9:07
 Operator : SY/AP
 Sample : N3306-02
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SS-1

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 06/16/2022
 Supervised By : Mahesh Dadoda 06/16/2022

Quant Time: Jun 16 01:15:47 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jun 15 2022

QLast Update : Wed Jun 01 01:22:18 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.658	49	1352107	10.000	ppbv	-0.02
33) 1,4-Difluorobenzene	7.166	114	3650863	10.000	ppbv	-0.02
55) Chlorobenzene-d5	12.076	117	3312180	10.000	ppbv	-0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.404	95	2663916	9.728	ppbv	-0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.300%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	3.044	85	56644	0.239	ppbv	98
3) Chlorodifluoromethane	2.957	51	127448	0.741	ppbv #	70
4) Chloromethane	3.140	50	18844m	0.213	ppbv	
9) Propene	3.012	41	133384	1.778	ppbv	88
11) Trichlorofluoromethane	3.944	101	42209	0.196	ppbv #	75
13) Ethanol	3.610	45	236420	57.790	ppbv #	100
15) Acetone	3.838	43	2761697	19.608	ppbv	94
19) Isopropyl Alcohol	3.973	45	283527	4.292	ppbv #	1
20) Methylene Chloride	4.340	84	628215	10.584	ppbv	94
26) Hexane	5.681	57	509661	3.653	ppbv #	38
27) Carbon Disulfide	4.542	76	42277m	0.292	ppbv	
32) 1,1,1-Trichloroethane	6.500	97	10631m	0.046	ppbv	
34) 2-Butanone	5.240	43	320960	1.618	ppbv	98
35) Carbon Tetrachloride	7.005	117	14658m	0.055	ppbv	
36) Benzene	6.883	78	81181	0.274	ppbv	93
41) Tetrahydrofuran	6.050	42	13166	0.110	ppbv #	63
50) 4-Methyl-2-Pentanone	8.748	43	28607m	0.096	ppbv	
52) Tetrachloroethene	11.211	164	125697	1.086	ppbv	91
53) Toluene	9.793	91	399469	1.170	ppbv	99
58) Ethyl Benzene	12.700	91	275812	0.605	ppbv	91
59) m/p-Xylene	12.957	91	906227	2.256	ppbv	93
60) o-Xylene	13.677	91	480955	1.274	ppbv	99
61) Styrene	13.516	104	67861	0.336	ppbv	94
65) tert-Butylbenzene	16.748	119	126730	0.247	ppbv #	61
70) n-Butylbenzene	18.545	91	137981m	0.228	ppbv	
72) 4-Ethyltoluene	15.818	105	285811m	0.646	ppbv	
73) 1,3,5-Trimethylbenzene	15.982	105	336466	0.843	ppbv	98
74) 1,2,4-Trimethylbenzene	16.741	105	1195582	2.685	ppbv #	64
79) Naphthalene	22.172	128	173007m	0.505	ppbv	
80) Naphthalene,2-methyl-	24.956	142	29970m	0.235	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061422\
Data File : VL039291.D
Acq On : 15 Jun 2022 9:07
Operator : SY/AP
Sample : N3306-02
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SS-1

Quant Time: Jun 16 01:15:47 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun
QLast Update : Wed Jun 01 01:22:18 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

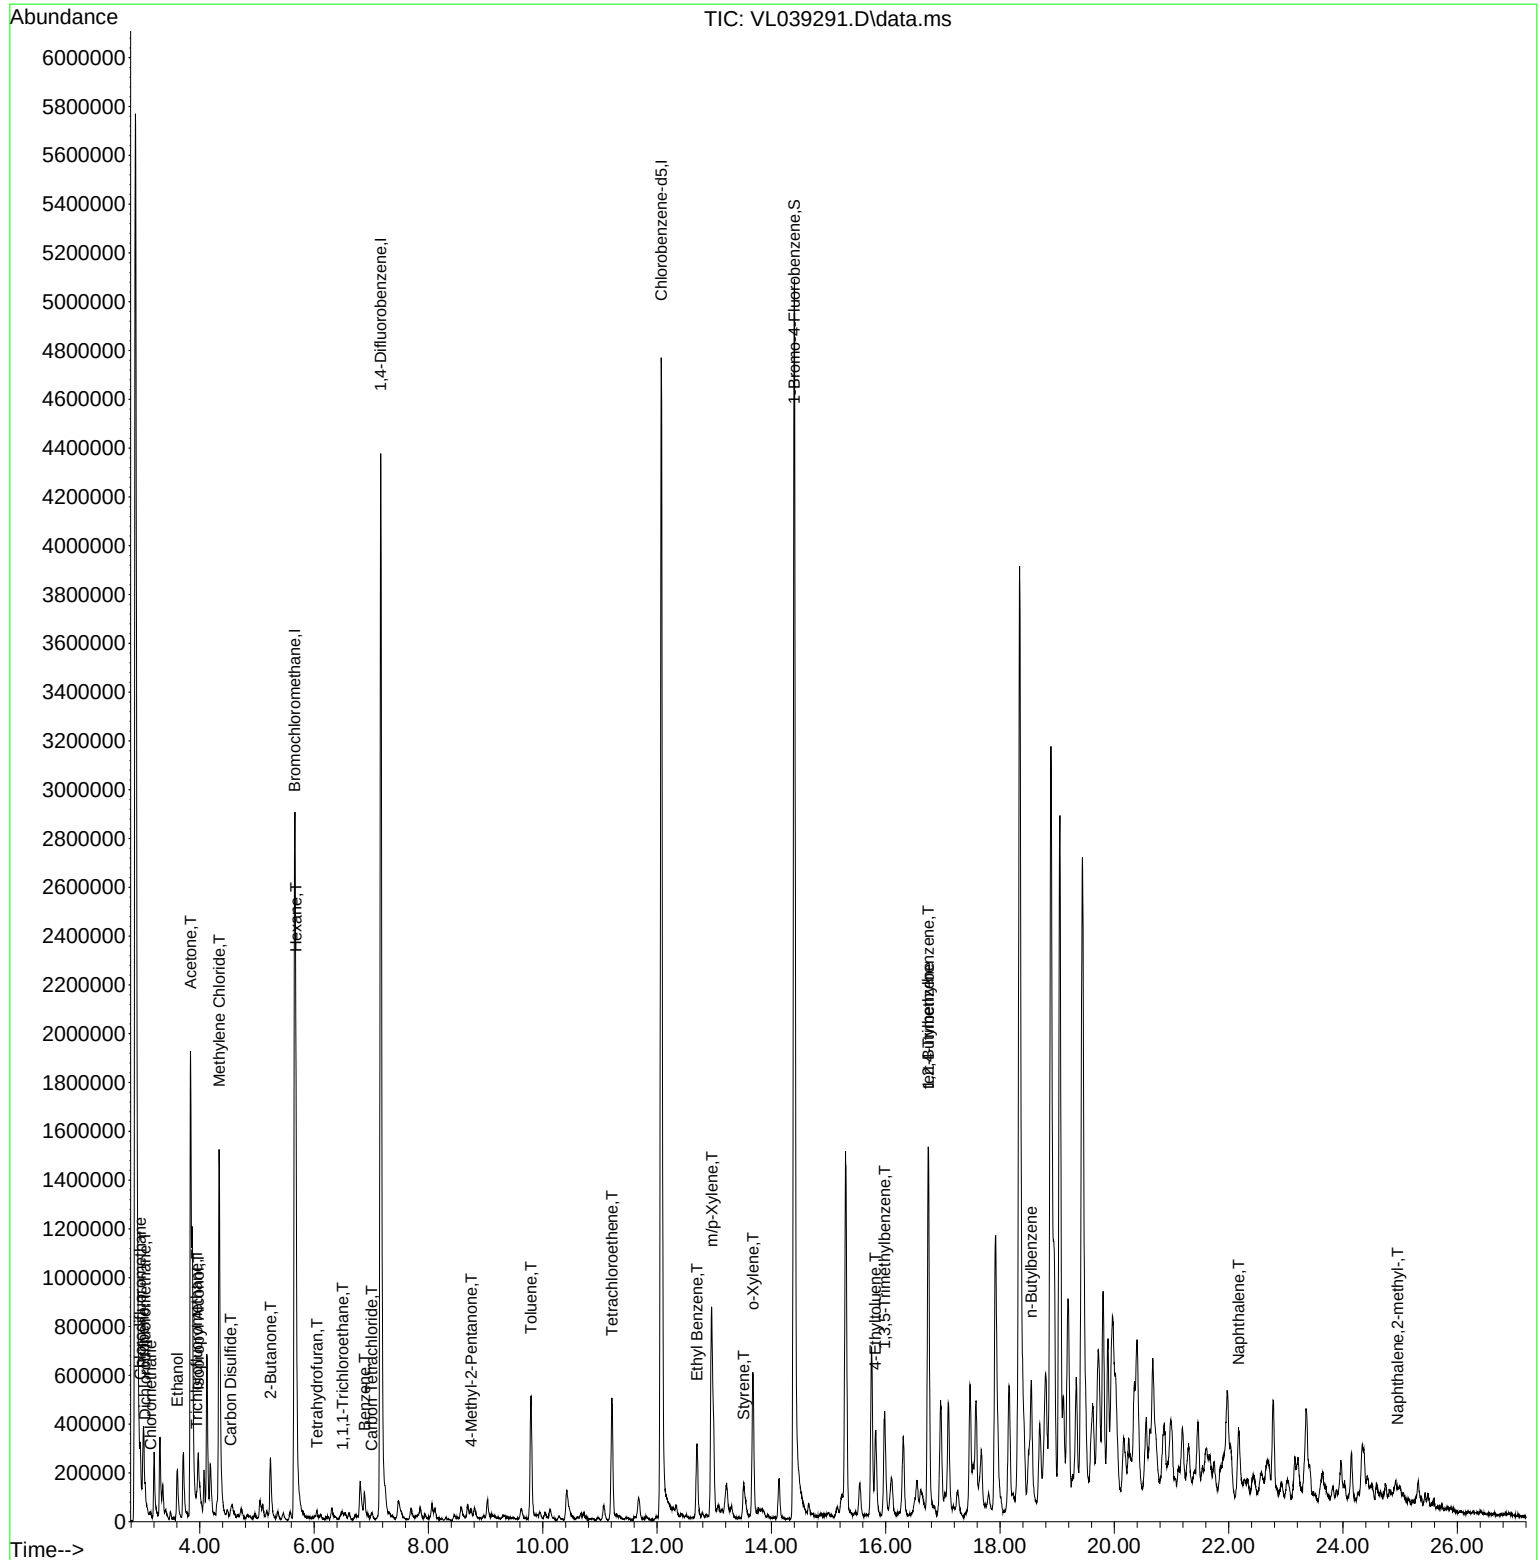

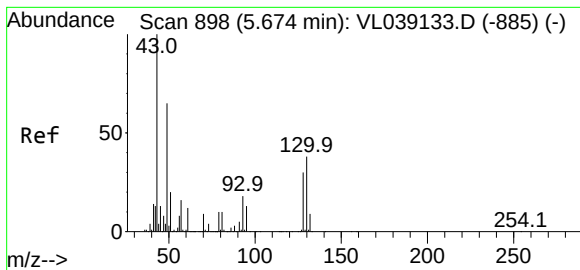





#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.658 min Scan# 89
Delta R.T. -0.016 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

Instrument :
MSVOA_L
ClientSampleId :
SS-1

Tgt Ion: 49 Resp: 135210
Ion Ratio Lower Upper
49 100
128 51.8 24.7 74.1
130 67.6 31.4 94.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

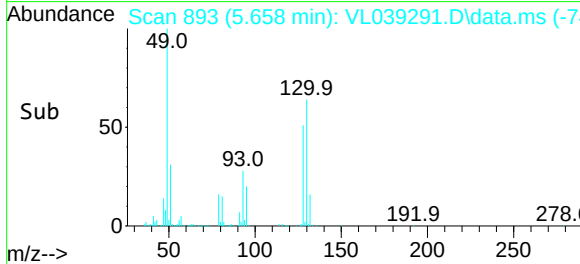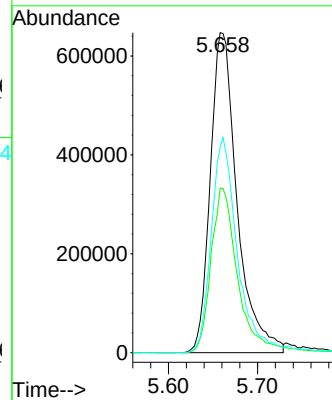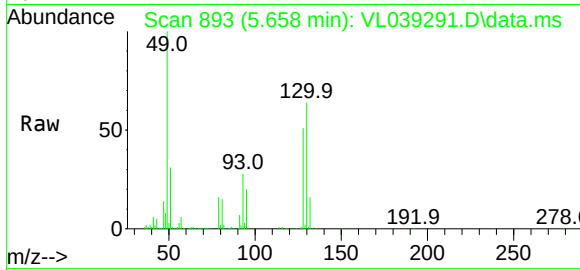

#2
Dichlorodifluoromethane
Concen: 0.239 ppbv
RT: 3.044 min Scan# 80
Delta R.T. -0.016 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

Tgt Ion: 85 Resp: 56644
Ion Ratio Lower Upper
85 100
87 34.6 26.9 40.3

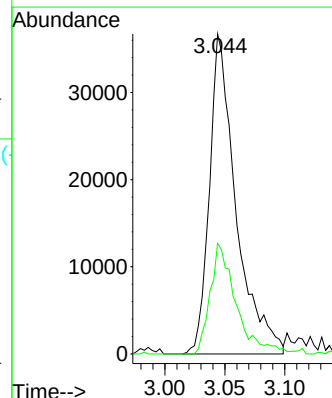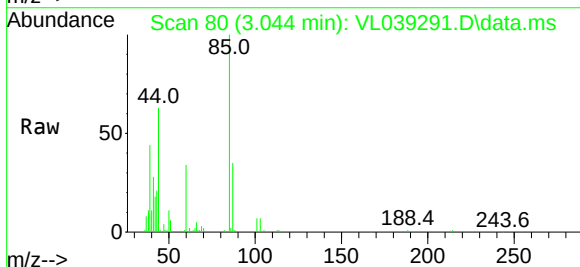

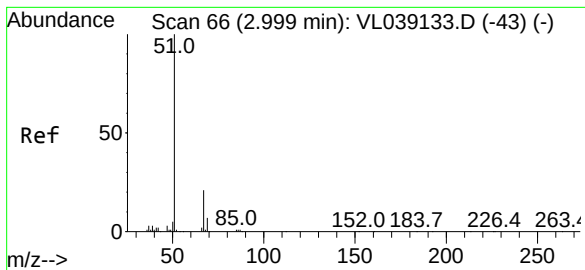





#3
Chlorodifluoromethane
Concen: 0.741 ppbv
RT: 2.957 min Scan# 51
Delta R.T. -0.042 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

Instrument :
MSVOA_L
ClientSampleId :
SS-1

Tgt Ion: 51 Resp: 12744
Ion Ratio Lower Upper
51 100
67 6.3 16.2 24.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

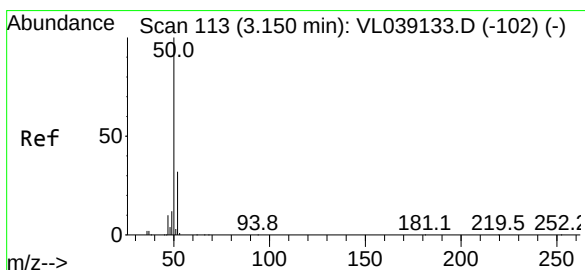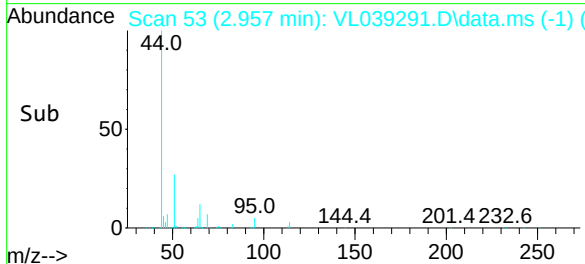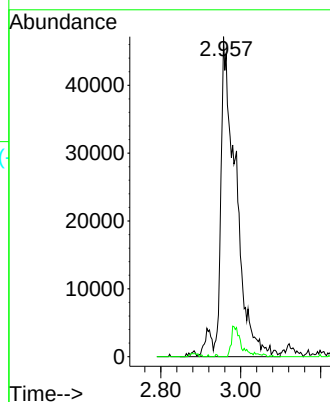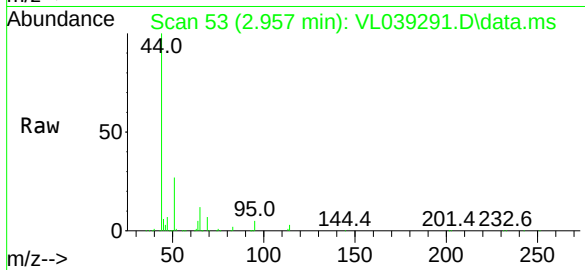

#4
Chloromethane
Concen: 0.213 ppbv m
RT: 3.140 min Scan# 110
Delta R.T. -0.010 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07


Tgt Ion: 50 Resp: 18844
Ion Ratio Lower Upper
50 100
52 35.9 25.9 38.9

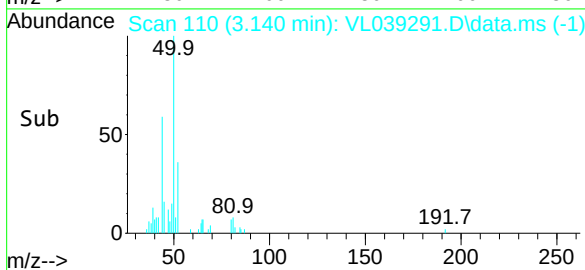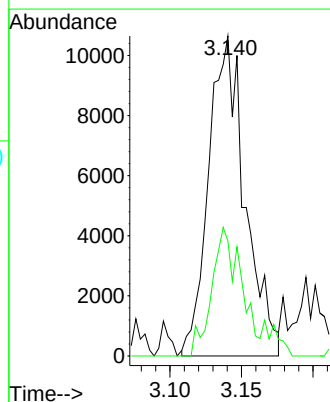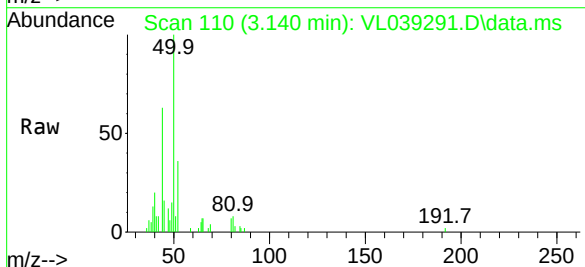

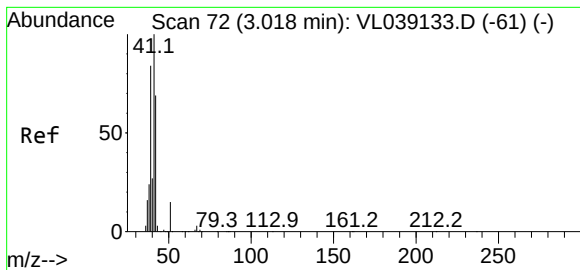

#9
 Propene
 Concen: 1.778 ppbv
 RT: 3.012 min Scan# 70
 Delta R.T. -0.006 min
 Lab File: VL039291.D
 Acq: 15 Jun 2022 9:07




Instrument :
 MSVOA_L
 ClientSampleId :
 SS-1

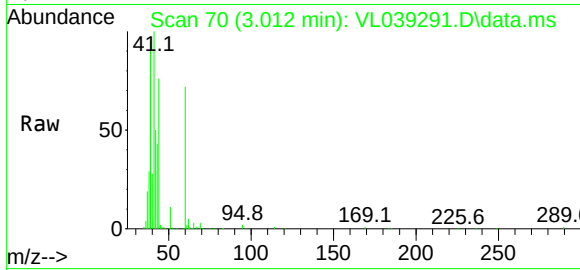


Tgt Ion: 41 Resp: 133384
 Ion Ratio Lower Upper
 41 100
 42 59.2 55.4 83.2

Manual Integrations
 APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
 Supervised By :Mahesh Dadoda 06/16/2022

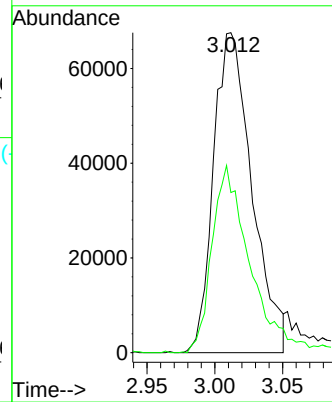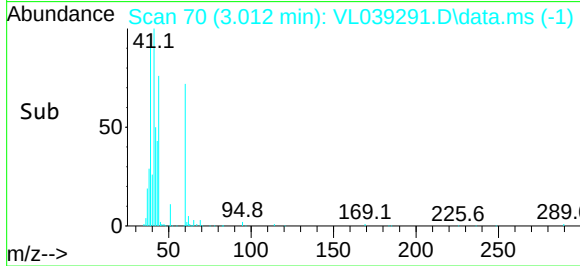


#11
 Trichlorofluoromethane
 Concen: 0.196 ppbv
 RT: 3.944 min Scan# 360
 Delta R.T. -0.016 min
 Lab File: VL039291.D
 Acq: 15 Jun 2022 9:07

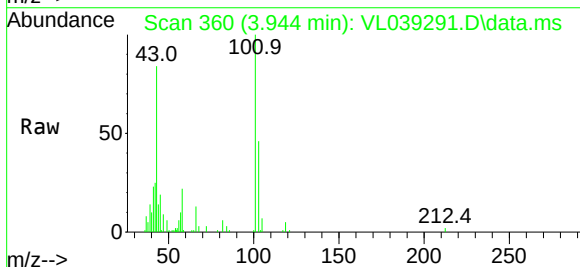


Tgt Ion:101 Resp: 42209
 Ion Ratio Lower Upper
 101 100
 103 44.6 51.7 77.5#

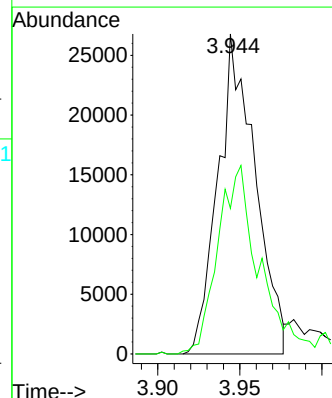



#13
Ethanol
Concen: 57.790 ppbv
RT: 3.610 min Scan# 210
Delta R.T. -0.000 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07




Instrument :
MSVOA_L
ClientSampleId :
SS-1




Tgt Ion: 45 Resp: 236420
Ion Ratio Lower Upper
45 100
46 38.3 0.0 0.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

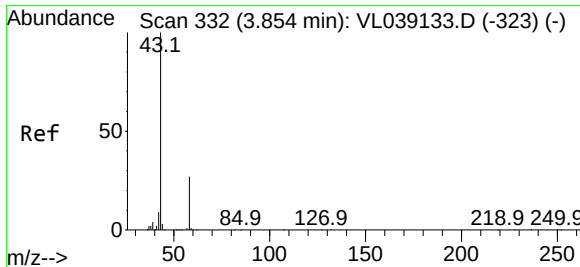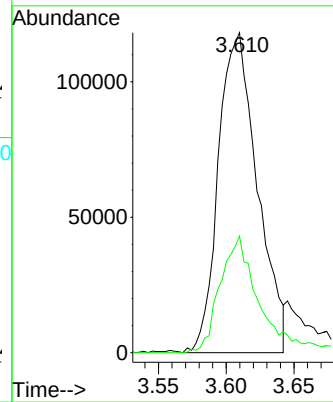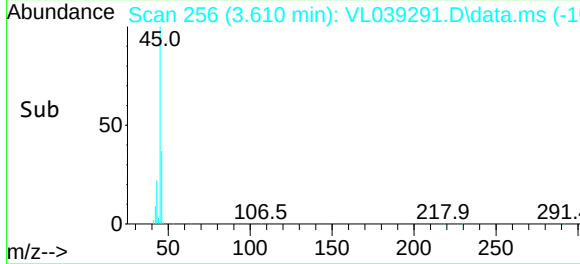


#15
Acetone
Concen: 19.608 ppbv
RT: 3.838 min Scan# 327
Delta R.T. -0.016 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

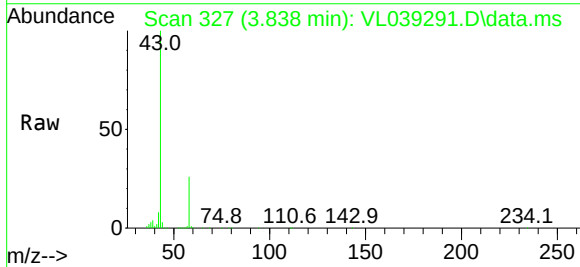

Tgt Ion: 43 Resp: 2761697
Ion Ratio Lower Upper
43 100
58 24.8 22.5 33.7

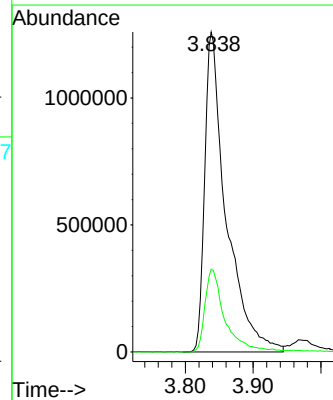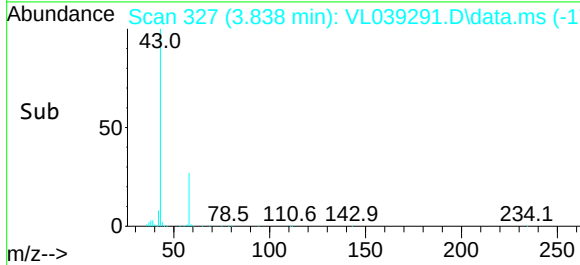



#19

Isopropyl Alcohol

Concen: 4.292 ppbv

RT: 3.973 min Scan# 30

Delta R.T. 0.010 min

Lab File: VL039291.D

Acq: 15 Jun 2022 9:07

Instrument :

MSVOA_L

ClientSampleId :

SS-1

Tgt Ion: 45 Resp: 28352

Ion Ratio Lower Upper

45 100





58 242.0 1.8 2.8

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022

Supervised By :Mahesh Dadoda 06/16/2022

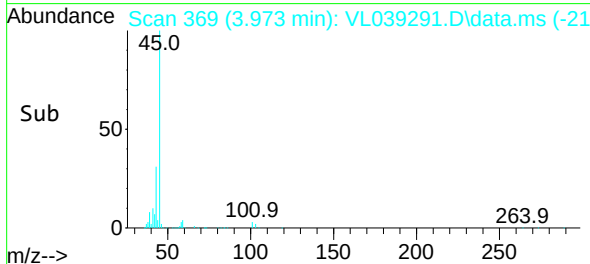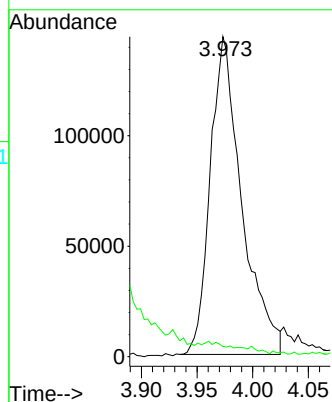

#20

Methylene Chloride

Concen: 10.584 ppbv

RT: 4.340 min Scan# 483

Delta R.T. -0.013 min

Lab File: VL039291.D

Acq: 15 Jun 2022 9:07

Tgt Ion: 84 Resp: 628215




Ion Ratio Lower Upper


84 100

49 148.0 111.1 166.7

51 46.5 35.3 52.9


86 60.2 51.9 77.9

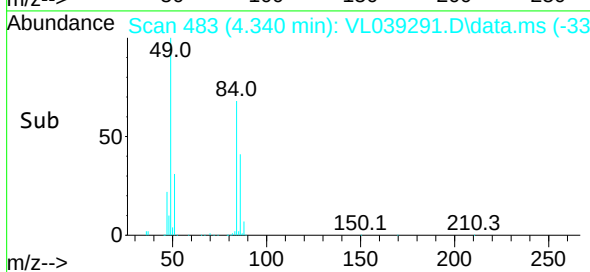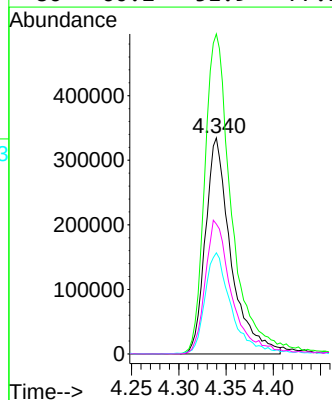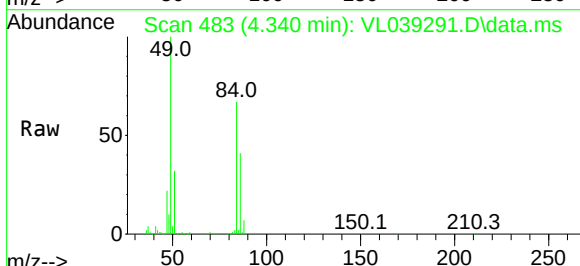

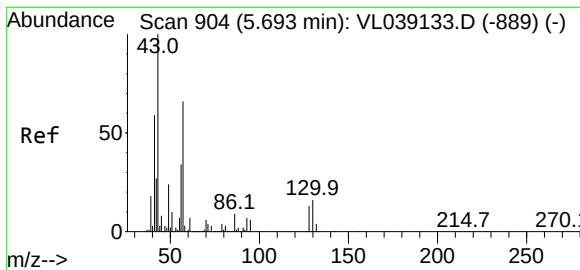

#26
Hexane
Concen: 3.653 ppbv
RT: 5.681 min Scan# 904
Delta R.T. -0.013 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07




Instrument :
MSVOA_L
ClientSampleId :
SS-1

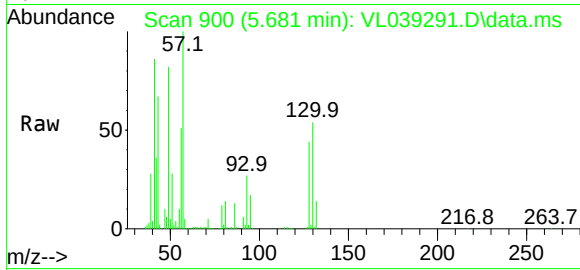

Tgt Ion: 57 Resp: 50966
Ion Ratio Lower Upper
57 100
41 99.0 72.4 108.6
43 76.5 187.0 280.6
56 57.2 41.8 62.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

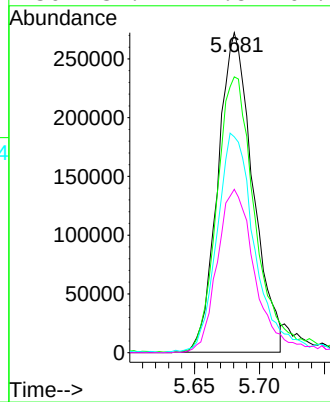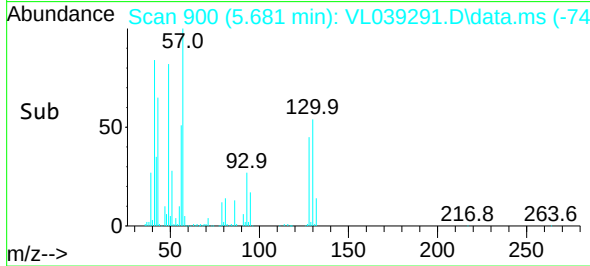

#27
Carbon Disulfide
Concen: 0.292 ppbv m
RT: 4.542 min Scan# 546
Delta R.T. -0.016 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07


Tgt Ion: 76 Resp: 42277
Ion Ratio Lower Upper
76 100
44 27.0 14.4 21.6
78 10.5 7.7 11.5

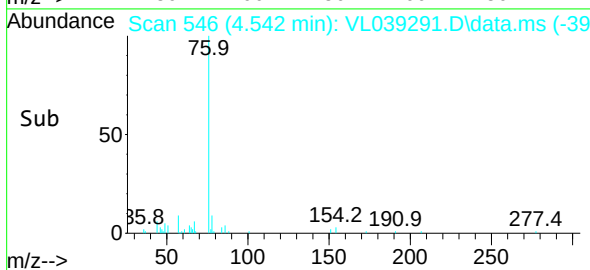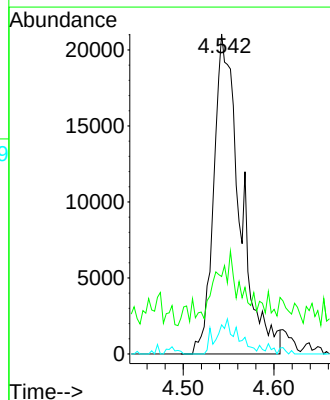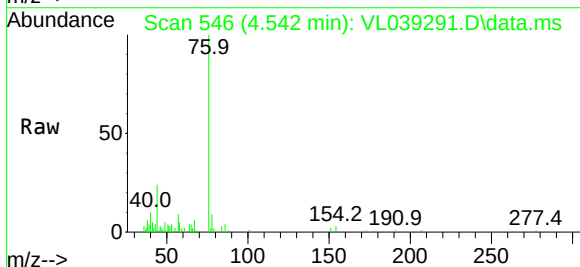

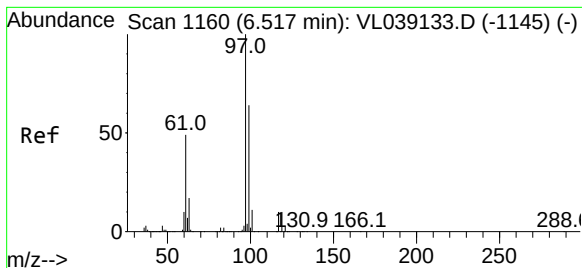

#32
 1,1,1-Trichloroethane
 Concen: 0.046 ppbv m
 RT: 6.500 min Scan# 1160
 Delta R.T. -0.016 min
 Lab File: VL039291.D
 Acq: 15 Jun 2022 9:07




Instrument :
 MSVOA_L
 ClientSampleId :
 SS-1

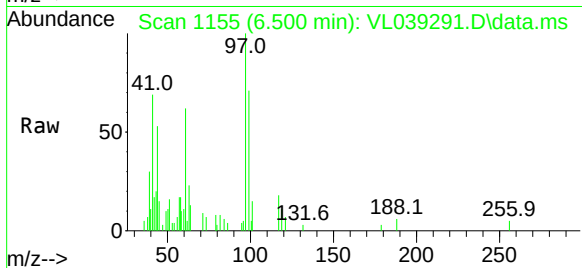

Tgt Ion: 97 Resp: 1063
 Ion Ratio Lower Upper
 97 100
 99 67.6 52.1 78.1
 61 55.9 40.0 60.0




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
 Supervised By :Mahesh Dadoda 06/16/2022

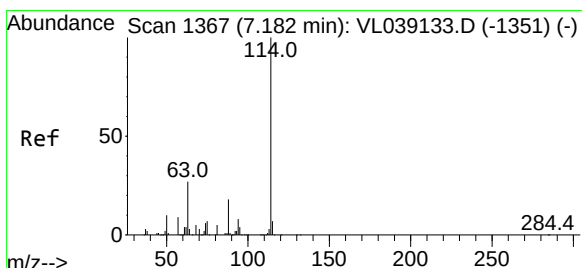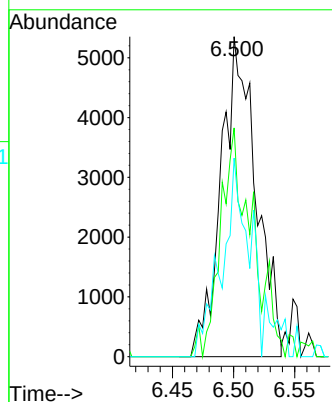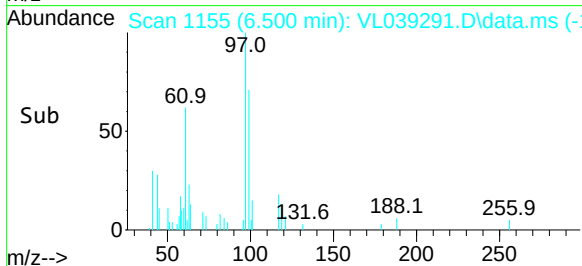

#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.166 min Scan# 1362
 Delta R.T. -0.016 min
 Lab File: VL039291.D
 Acq: 15 Jun 2022 9:07


Tgt Ion:114 Resp: 3650863
 Ion Ratio Lower Upper
 114 100
 63 25.3 21.7 32.5
 88 18.4 14.8 22.2

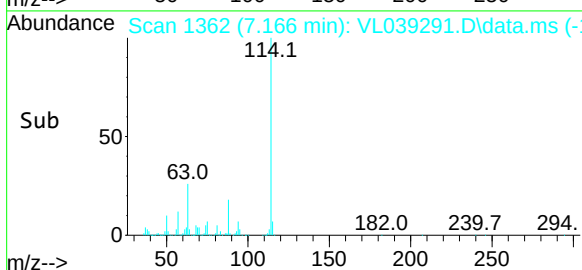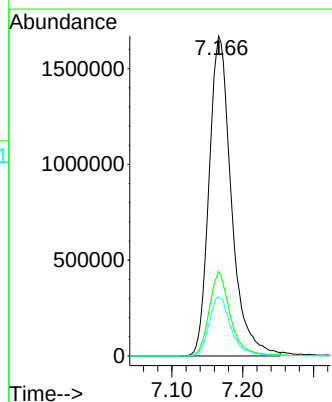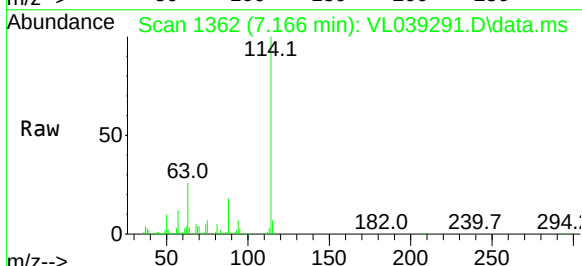

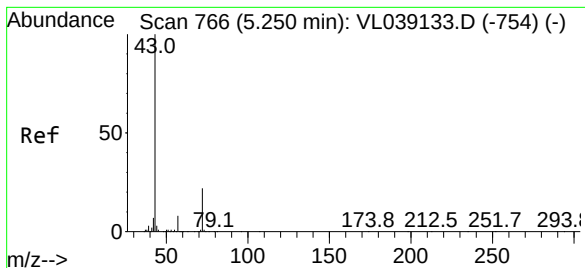

#34
2-Butanone
Concen: 1.618 ppbv
RT: 5.240 min Scan# 766
Delta R.T. -0.010 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07




Instrument :
MSVOA_L
ClientSampleId :
SS-1

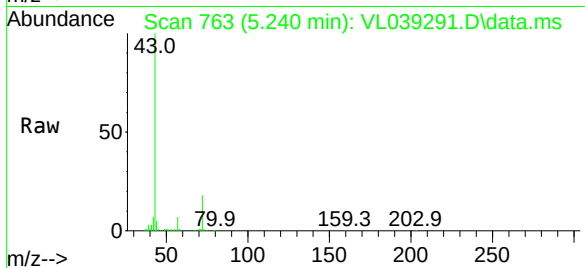

Tgt Ion: 43 Resp: 320960
Ion Ratio Lower Upper
43 100
72 23.7 18.2 27.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

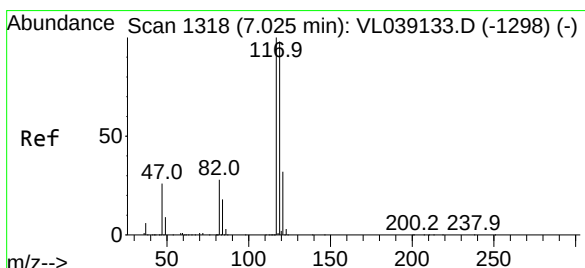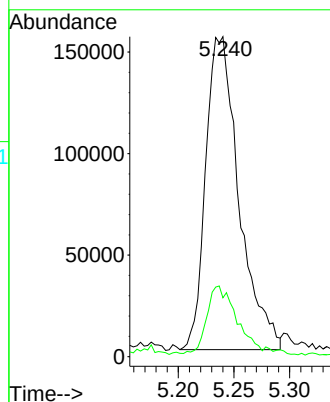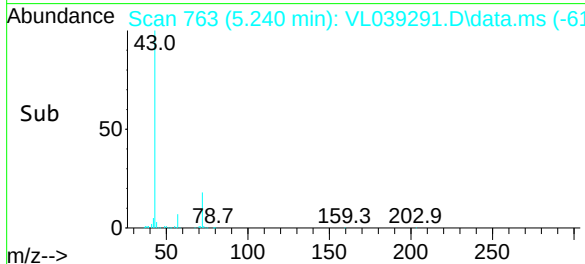

#35
Carbon Tetrachloride
Concen: 0.055 ppbv m
RT: 7.005 min Scan# 1312
Delta R.T. -0.019 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

Tgt Ion:117 Resp: 14658
Ion Ratio Lower Upper
117 100
119 61.4 78.6 118.0#
121 25.8 25.4 38.0

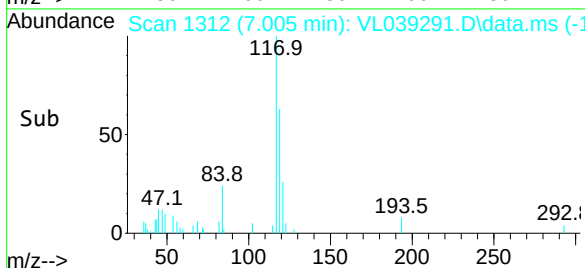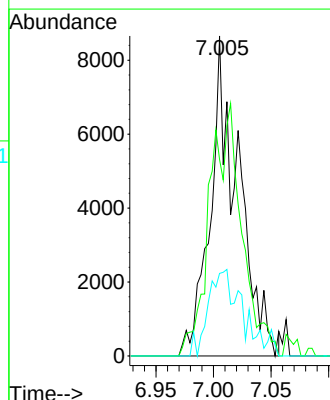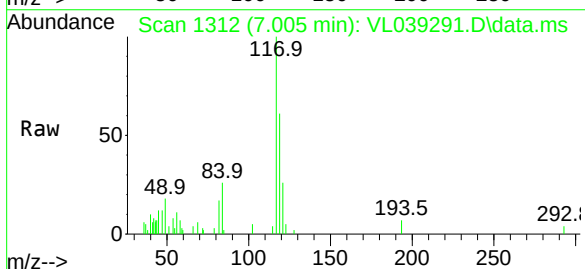



#36

Benzene

Concen: 0.274 ppbv

RT: 6.883 min Scan# 1015

Delta R.T. -0.016 min

Lab File: VL039291.D

Acq: 15 Jun 2022 9:07

Instrument :

MSVOA_L

ClientSampleId :





SS-1

Tgt Ion: 78	Resp: 8118
Ion Ratio	Lower Upper
78 100	
77 19.5	18.6 27.8
50 16.8	15.8 23.8

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

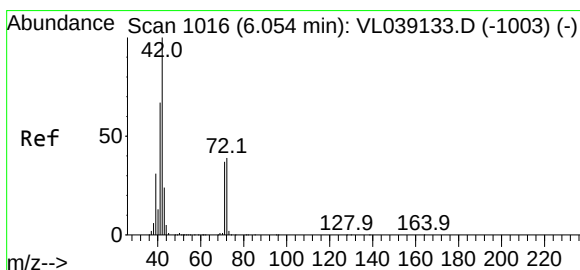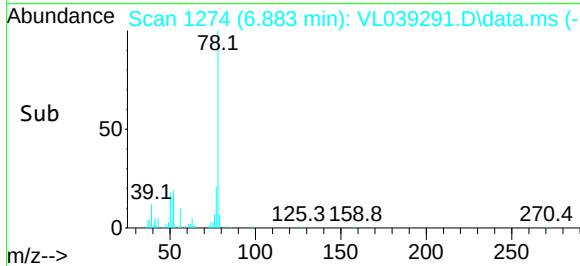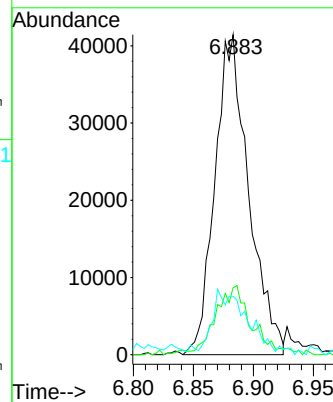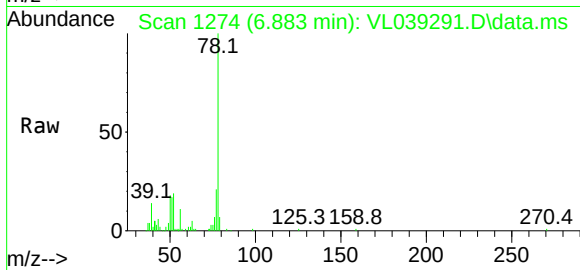

#41

Tetrahydrofuran

Concen: 0.110 ppbv




RT: 6.050 min Scan# 1015


Delta R.T. -0.003 min

Lab File: VL039291.D

Acq: 15 Jun 2022 9:07


Tgt Ion: 42	Resp: 13166
Ion Ratio	Lower Upper
42 100	
72 66.8	32.0 48.0#
71 57.2	31.1 46.7#

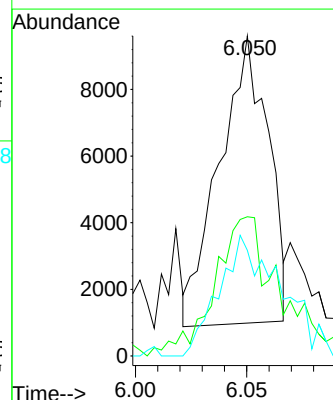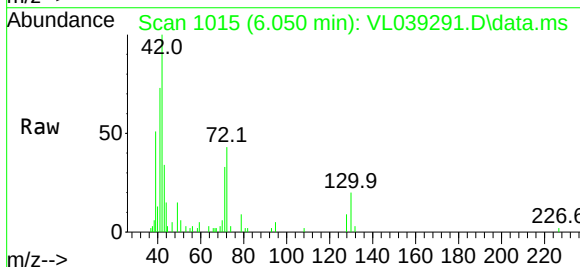

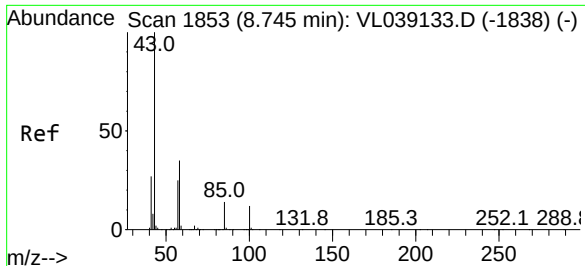

#50
4-Methyl-2-Pentanone
Concen: 0.096 ppbv m
RT: 8.748 min Scan# 1853
Delta R.T. 0.003 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07




Instrument :
MSVOA_L
ClientSampleId :
SS-1

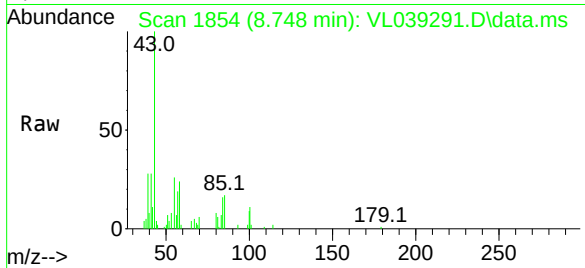


Tgt Ion: 43 Resp: 2860
Ion Ratio Lower Upper
43 100
58 0.0 28.7 43.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

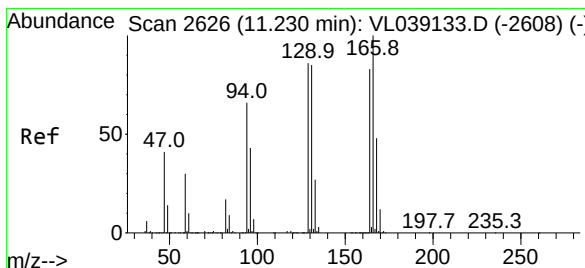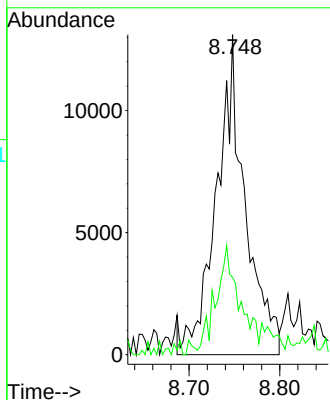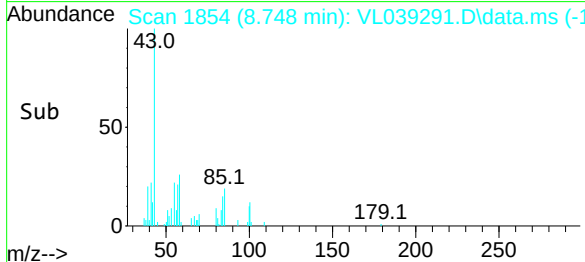


#52
Tetrachloroethene
Concen: 1.086 ppbv
RT: 11.211 min Scan# 2620
Delta R.T. -0.019 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

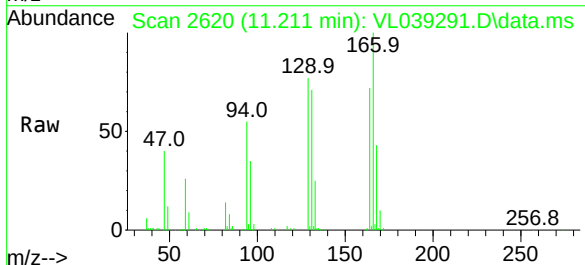


Tgt Ion:164 Resp: 125697
Ion Ratio Lower Upper
164 100
166 138.3 96.3 144.5
129 105.9 82.5 123.7
131 97.1 82.1 123.1

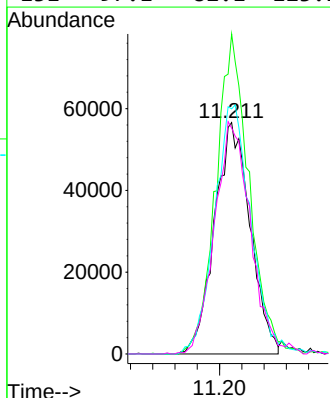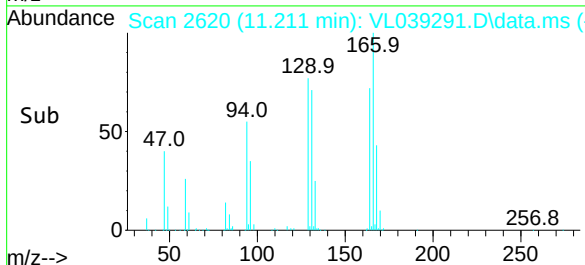



#53
Toluene
Concen: 1.170 ppbv
RT: 9.793 min Scan# 2185
Delta R.T. -0.019 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07




Instrument :
MSVOA_L
ClientSampleId :
SS-1

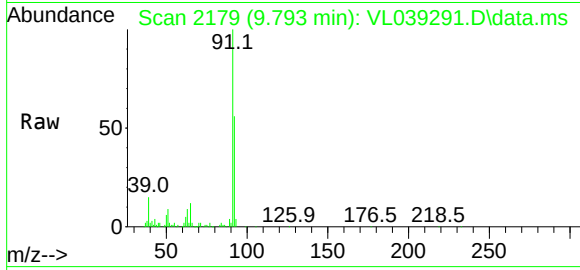


Tgt Ion: 91 Resp: 399469
Ion Ratio Lower Upper
91 100
92 59.2 48.1 72.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

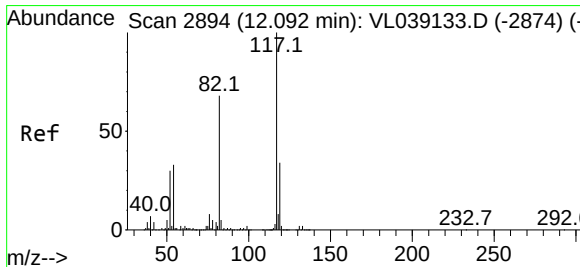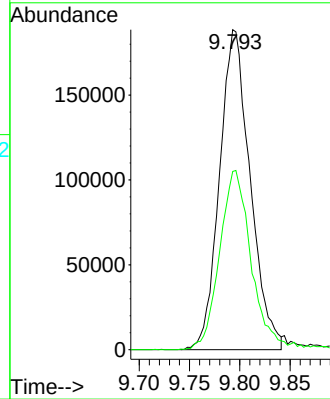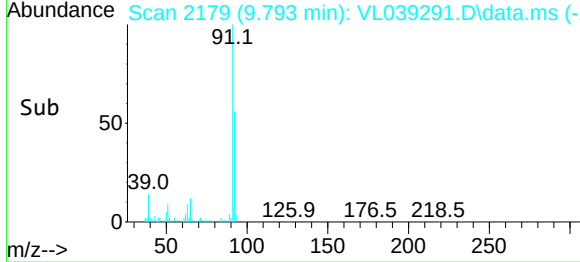


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.076 min Scan# 2889
Delta R.T. -0.016 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

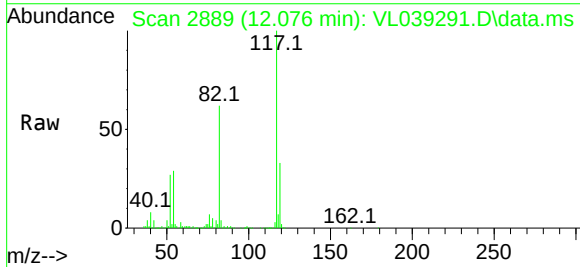

Tgt Ion:117 Resp: 3312180
Ion Ratio Lower Upper
117 100
82 63.8 55.1 82.7
119 33.7 24.7 37.1

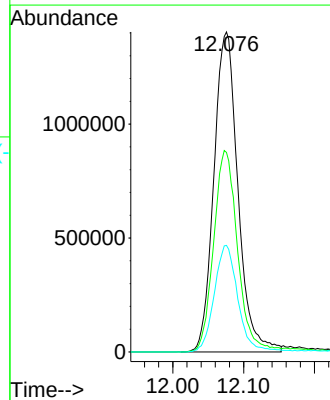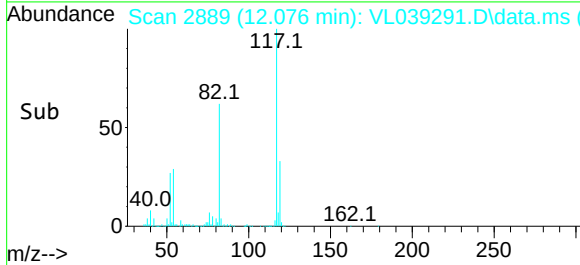







#58
Ethyl Benzene
Concen: 0.605 ppbv
RT: 12.700 min Scan# 3088
Delta R.T. -0.016 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

Instrument :
MSVOA_L
ClientSampleId :
SS-1

Tgt Ion: 91 Resp: 275812
Ion Ratio Lower Upper
91 100
106 25.6 24.2 36.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

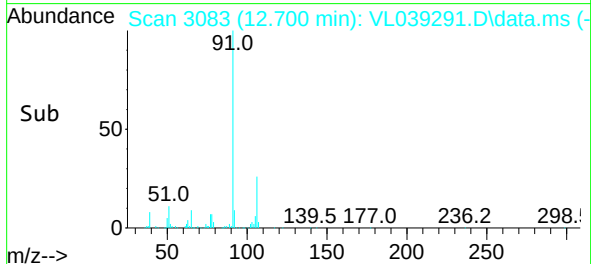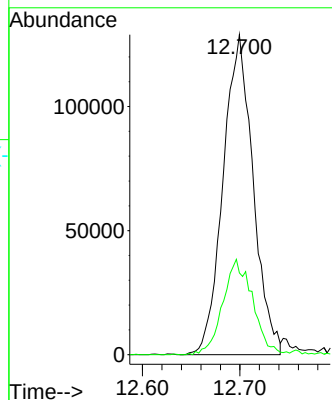

#59
m/p-Xylene
Concen: 2.256 ppbv
RT: 12.957 min Scan# 3163
Delta R.T. -0.042 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

Tgt Ion: 91 Resp: 906227
Ion Ratio Lower Upper
91 100
106 47.1 34.3 51.5

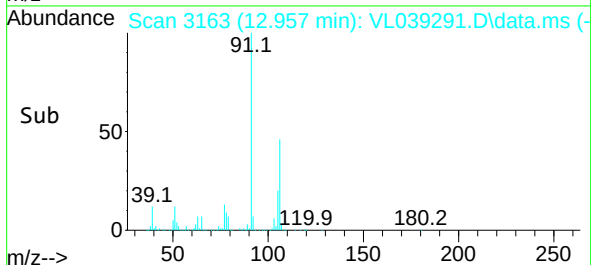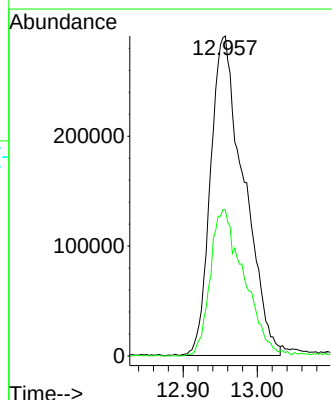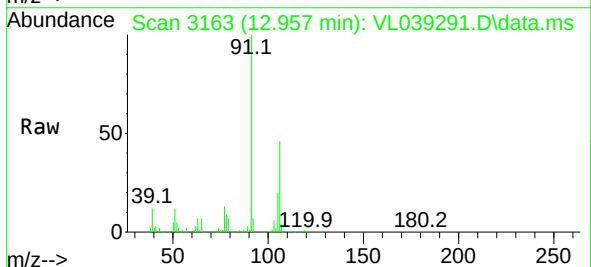



#60

o-Xylene

Concen: 1.274 ppbv

RT: 13.677 min Scan# 31

Delta R.T. -0.019 min

Lab File: VL039291.D

Acq: 15 Jun 2022 9:07

Instrument :

MSVOA_L

ClientSampleId :

SS-1

Tgt Ion: 91 Resp: 48095

Ion Ratio Lower Upper

91 100





106 43.8 22.3 66.9

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022

Supervised By :Mahesh Dadoda 06/16/2022

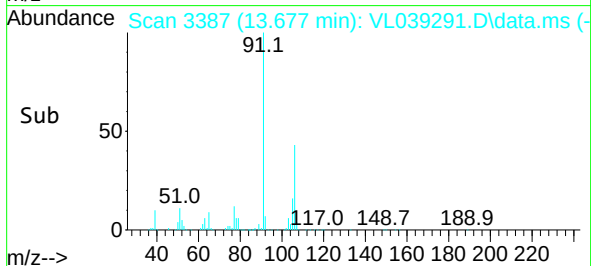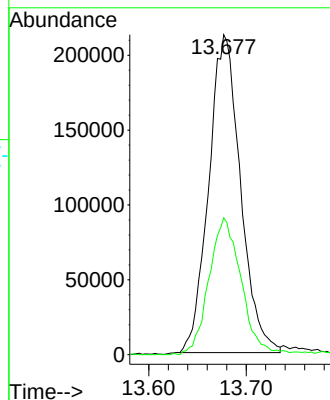

#61

Styrene

Concen: 0.336 ppbv

RT: 13.516 min Scan# 3337

Delta R.T. -0.016 min

Lab File: VL039291.D

Acq: 15 Jun 2022 9:07




Tgt Ion:104 Resp: 67861


Ion Ratio Lower Upper

104 100

78 60.1 45.7 68.5

103 55.3 39.6 59.4

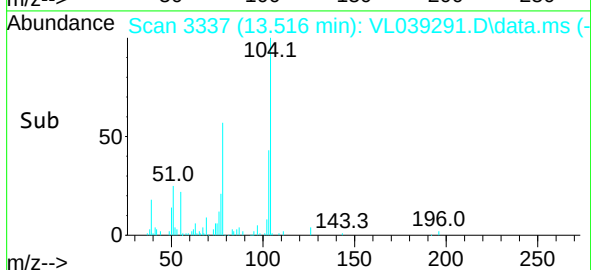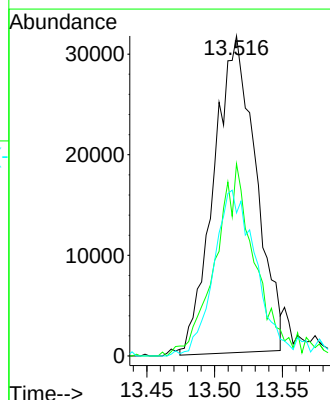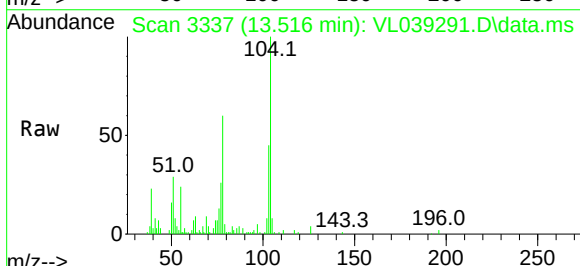



#65

tert-Butylbenzene

Concen: 0.247 ppbv

RT: 16.748 min Scan# 4342

Delta R.T. -0.000 min

Lab File: VL039291.D

Acq: 15 Jun 2022 9:07

Instrument :

MSVOA_L

ClientSampleId :

SS-1





Tgt Ion: 119 Resp: 126730

Ion	Ratio	Lower	Upper
119	100		
91	118.6	67.1	100.7
134	0.3	15.8	23.8

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

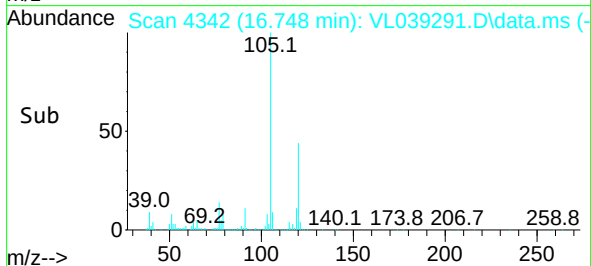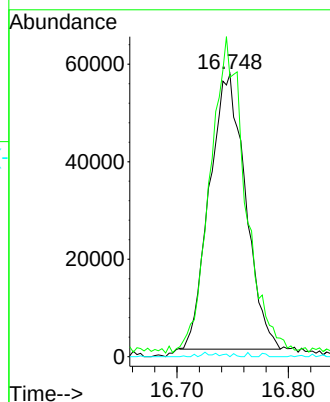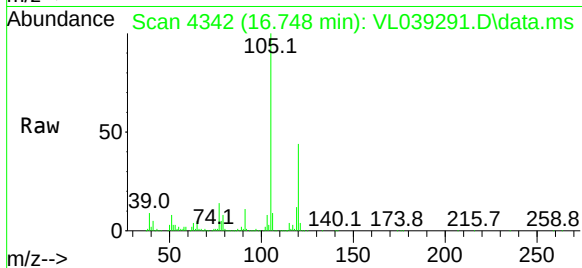

#68

1-Bromo-4-Fluorobenzene

Concen: 9.728 ppbv

RT: 14.404 min Scan# 3613




Delta R.T. -0.013 min


Lab File: VL039291.D

Acq: 15 Jun 2022 9:07

Tgt Ion: 95 Resp: 2663916


Ion	Ratio	Lower	Upper
95	100		
174	69.6	53.8	80.8
175	5.4	4.1	6.1

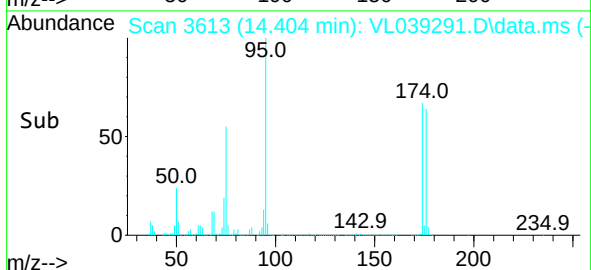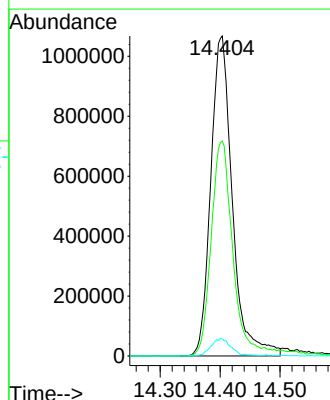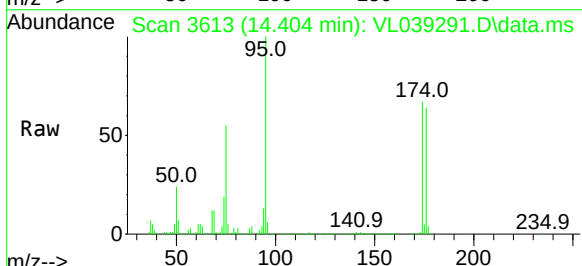

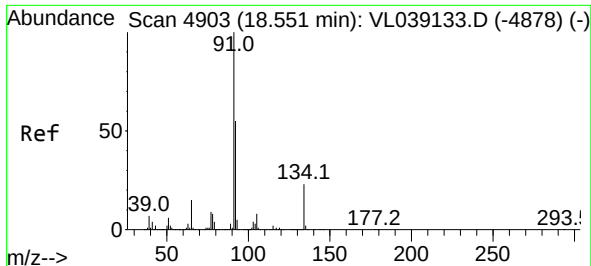

#70
n-Butylbenzene
Concen: 0.228 ppbv m
RT: 18.545 min Scan# 4903
Delta R.T. -0.006 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07




Instrument :
MSVOA_L
ClientSampleId :
SS-1

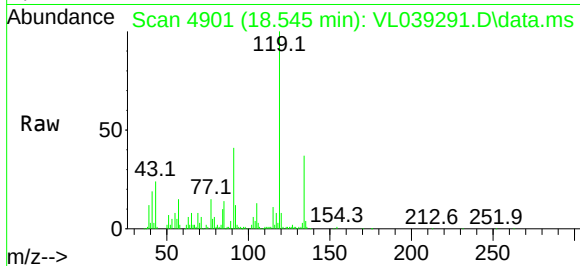


Tgt Ion: 91 Resp: 13798
Ion Ratio Lower Upper
91 100
92 35.1 43.6 65.4
134 0.0 17.7 26.5

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

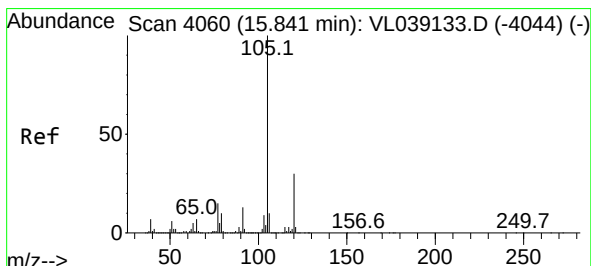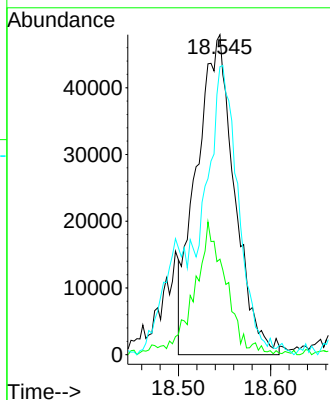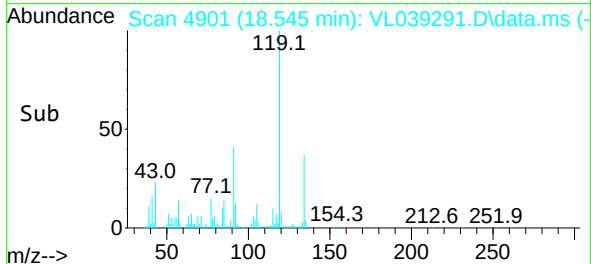


#72
4-Ethyltoluene
Concen: 0.646 ppbv m
RT: 15.818 min Scan# 4053
Delta R.T. -0.023 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

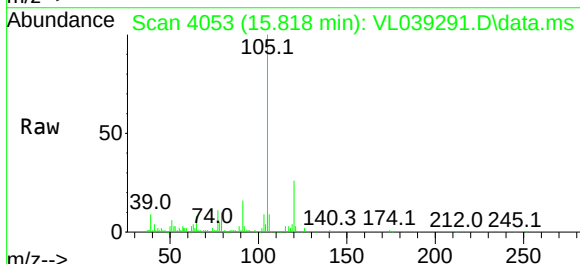

Tgt Ion:105 Resp: 285811
Ion Ratio Lower Upper
105 100
120 0.0 23.9 35.9
91 14.1 10.6 16.0
77 14.0 11.7 17.5

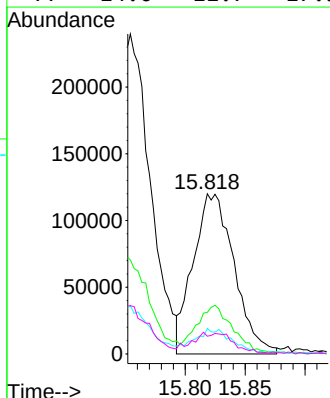



#73

1,3,5-Trimethylbenzene

Concen: 0.843 ppbv

RT: 15.982 min Scan# 4108

Delta R.T. -0.013 min

Lab File: VL039291.D

Acq: 15 Jun 2022 9:07

Instrument :

MSVOA_L

ClientSampleId :

SS-1

Tgt Ion:105 Resp: 336460

Ion Ratio Lower Upper

105 100





120 47.1 36.7 55.1

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022

Supervised By :Mahesh Dadoda 06/16/2022

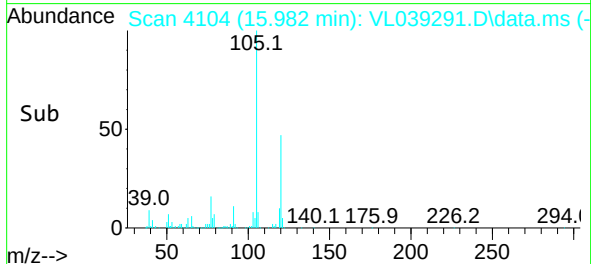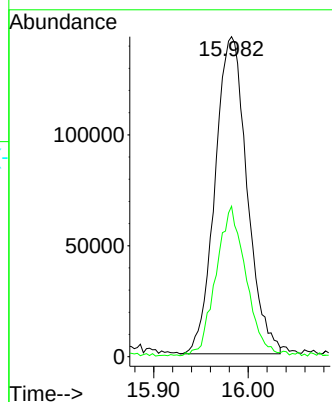

#74

1,2,4-Trimethylbenzene

Concen: 2.685 ppbv

RT: 16.741 min Scan# 4340

Delta R.T. -0.019 min

Lab File: VL039291.D

Acq: 15 Jun 2022 9:07

Tgt Ion:105 Resp: 1195582




Ion Ratio Lower Upper


105 100

120 42.8 38.1 57.1

91 11.3 47.4 71.0#


77 13.1 19.5 29.3#

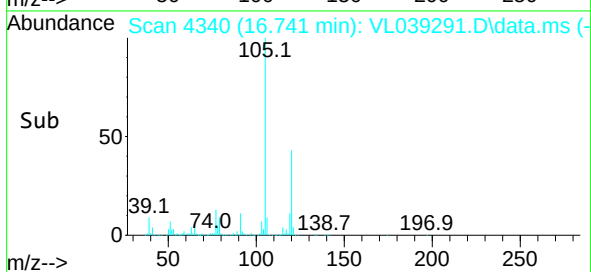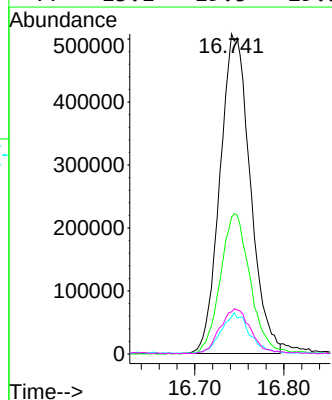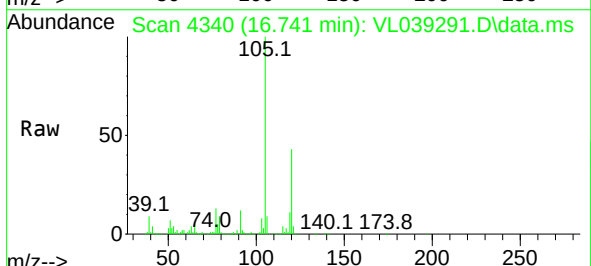



#79
Naphthalene
Concen: 0.505 ppbv m
RT: 22.172 min Scan# 6036
Delta R.T. -0.023 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07




Instrument :
MSVOA_L
ClientSampleId :
SS-1

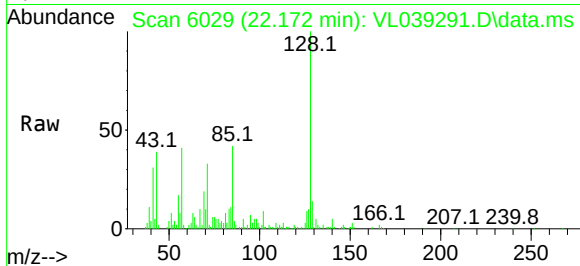


Tgt Ion:128 Resp: 17300
Ion Ratio Lower Upper
128 100
127 9.8 10.4 15.6
129 13.9 9.0 13.6

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

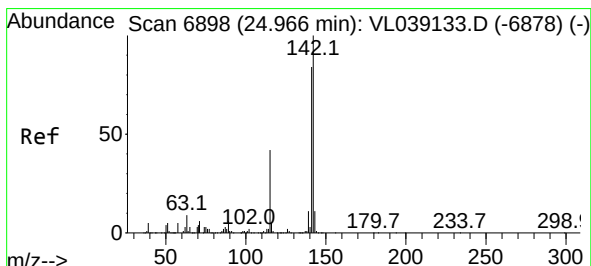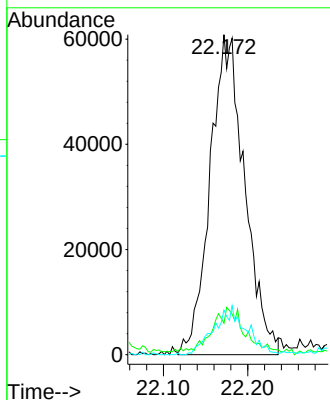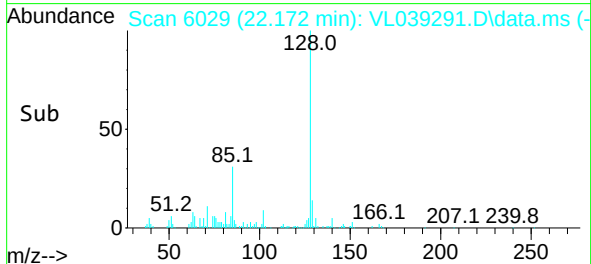

#80
Naphthalene,2-methyl-
Concen: 0.235 ppbv m
RT: 24.956 min Scan# 6895
Delta R.T. -0.010 min
Lab File: VL039291.D
Acq: 15 Jun 2022 9:07

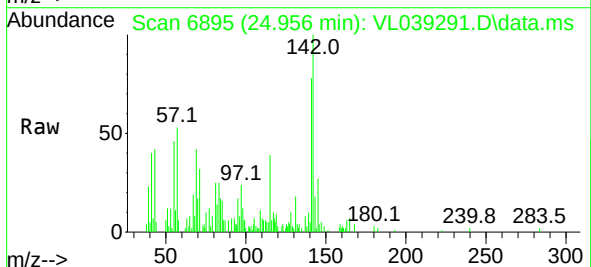

Tgt Ion:142 Resp: 29970
Ion Ratio Lower Upper
142 100
141 56.2 64.6 96.8#
115 28.0 32.7 49.1#

