

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061422\
 Data File : VL039295.D
 Acq On : 15 Jun 2022 11:50
 Operator : SY/AP
 Sample : N3326-04
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 IA2

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 06/16/2022
 Supervised By : Mahesh Dadoda 06/16/2022

Quant Time: Jun 16 01:17:06 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jun 15 2022

QLast Update : Wed Jun 01 01:22:18 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.658	49	1162359	10.000	ppbv	-0.02
33) 1,4-Difluorobenzene	7.163	114	3238952	10.000	ppbv	-0.02
55) Chlorobenzene-d5	12.069	117	2915459	10.000	ppbv	-0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.397	95	2319225	9.622	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.200%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	3.044	85	43396	0.213	ppbv	95
3) Chlorodifluoromethane	2.989	51	65928	0.446	ppbv #	85
4) Chloromethane	3.140	50	37761	0.497	ppbv #	88
9) Propene	3.021	41	170180m	2.639	ppbv	
10) Heptane	8.105	43	78444	0.521	ppbv	99
11) Trichlorofluoromethane	3.941	101	44363m	0.240	ppbv	
13) Ethanol	3.587	45	1373752	390.613	ppbv #	100
15) Acetone	3.838	43	3772630	31.158	ppbv	93
17) tert-Butyl alcohol	4.288	59	43668	0.465	ppbv #	70
19) Isopropyl Alcohol	3.954	45	2178922	38.368	ppbv	99
20) Methylene Chloride	4.343	84	61239m	1.200	ppbv	
26) Hexane	5.674	57	240866	2.008	ppbv #	39
30) Cyclohexane	7.124	84	36822	0.365	ppbv	88
34) 2-Butanone	5.237	43	188671	1.072	ppbv	97
35) Carbon Tetrachloride	7.002	117	13539m	0.057	ppbv	
36) Benzene	6.873	78	118323	0.450	ppbv #	90
37) 1,2-Dichloroethane	6.298	62	32650m	0.189	ppbv	
41) Tetrahydrofuran	6.047	42	34237	0.324	ppbv	93
44) 2,2,4-Trimethylpentane	7.857	57	520521	1.132	ppbv	92
52) Tetrachloroethene	11.208	164	15189m	0.148	ppbv	
53) Toluene	9.790	91	719731	2.377	ppbv	99
58) Ethyl Benzene	12.693	91	174181	0.434	ppbv	100
59) m/p-Xylene	12.950	91	547369m	1.548	ppbv	
60) o-Xylene	13.671	91	218665m	0.658	ppbv	
61) Styrene	13.513	104	115070	0.647	ppbv	98
72) 4-Ethyltoluene	15.818	105	82181	0.211	ppbv #	91
73) 1,3,5-Trimethylbenzene	15.979	105	76916	0.219	ppbv	96
74) 1,2,4-Trimethylbenzene	16.744	105	290945	0.742	ppbv #	64
79) Naphthalene	22.178	128	32981m	0.109	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061422\
Data File : VL039295.D
Acq On : 15 Jun 2022 11:50
Operator : SY/AP
Sample : N3326-04
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
IA2

Quant Time: Jun 16 01:17:06 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun
QLast Update : Wed Jun 01 01:22:18 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

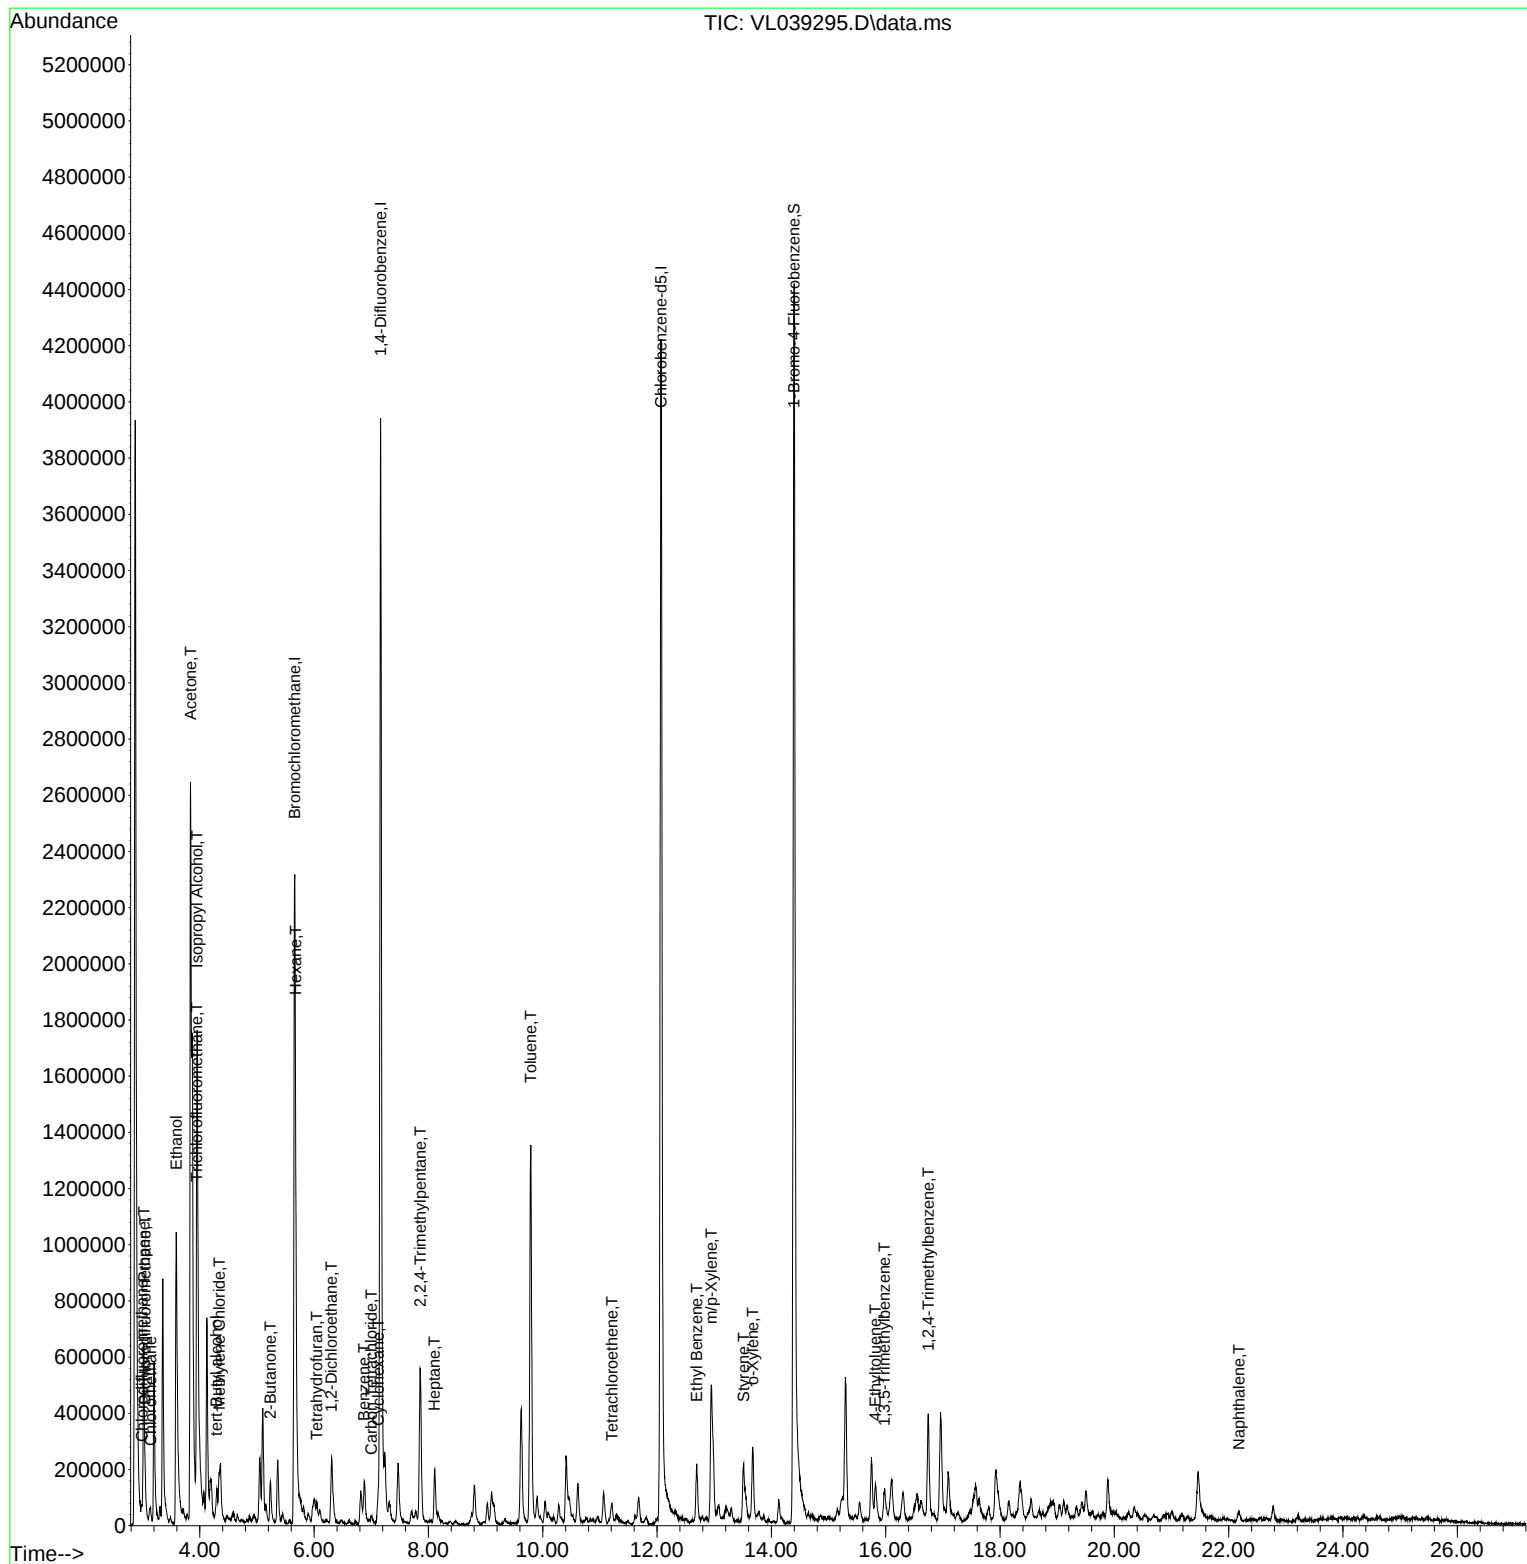



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.658 min Scan# 80
Delta R.T. -0.016 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument :
MSVOA_L
ClientSampleId :
IA2




Tgt Ion: 49 Resp: 116235
Ion Ratio Lower Upper
49 100
128 51.9 24.7 74.1
130 68.1 31.4 94.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

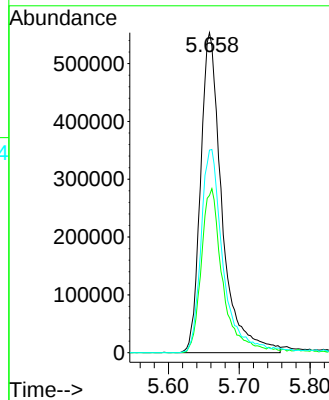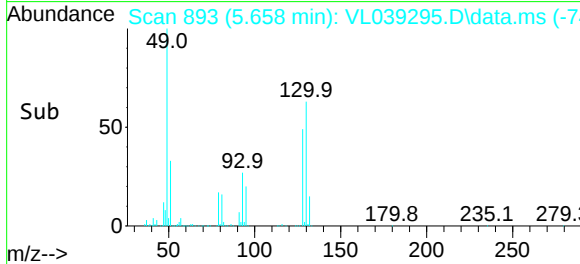


#2
Dichlorodifluoromethane
Concen: 0.213 ppbv
RT: 3.044 min Scan# 80
Delta R.T. -0.016 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

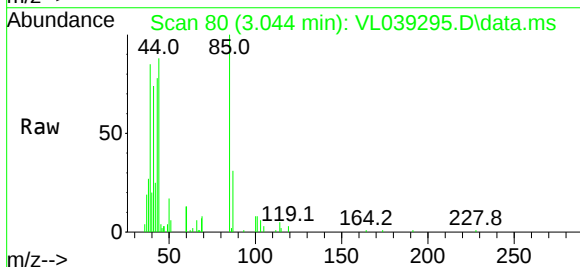


Tgt Ion: 85 Resp: 43396
Ion Ratio Lower Upper
85 100
87 31.0 26.9 40.3

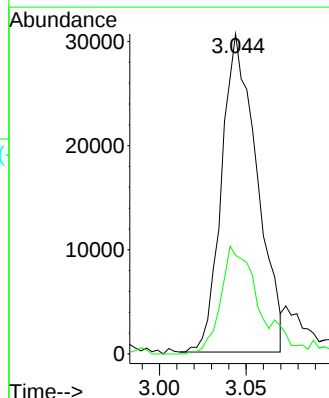

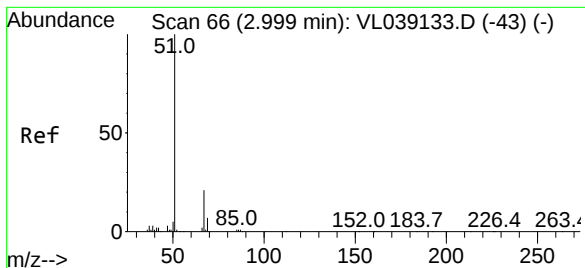

#3
Chlorodifluoromethane
Concen: 0.446 ppbv
RT: 2.989 min Scan# 61
Delta R.T. -0.010 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument :
MSVOA_L
ClientSampleId :
IA2

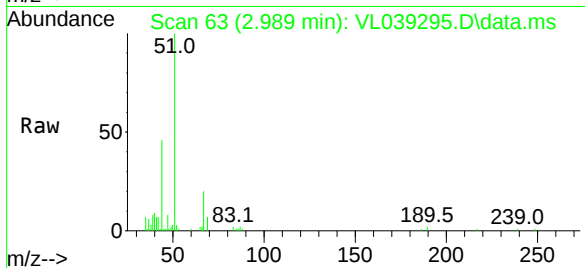

Tgt Ion: 51 Resp: 65928
Ion Ratio Lower Upper
51 100
67 13.5 16.2 24.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

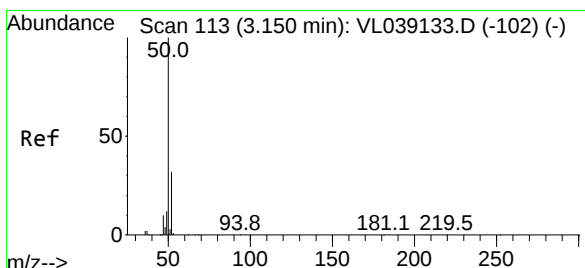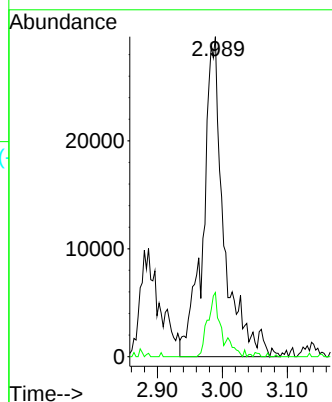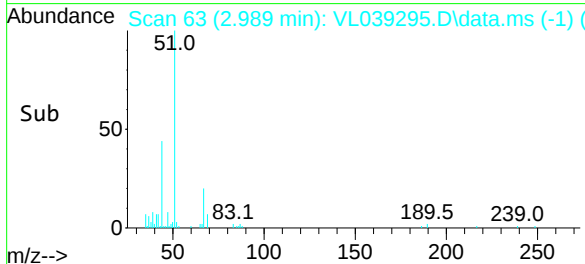

#4
Chloromethane
Concen: 0.497 ppbv
RT: 3.140 min Scan# 110
Delta R.T. -0.010 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

Tgt Ion: 50 Resp: 37761
Ion Ratio Lower Upper
50 100
52 39.1 25.9 38.9

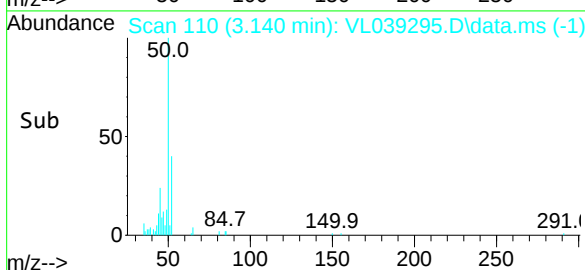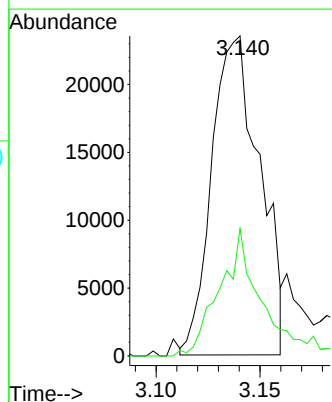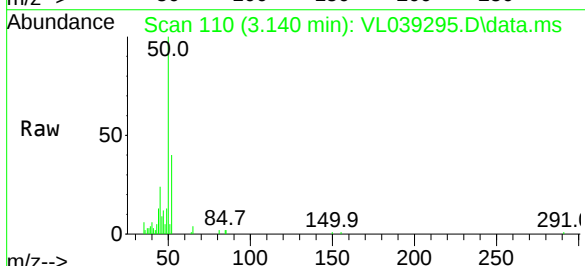







#9
Propene
Concen: 2.639 ppbv m
RT: 3.021 min Scan# 71
Delta R.T. 0.003 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

Instrument :
MSVOA_L
ClientSampleId :
IA2

Tgt Ion: 41 Resp: 170180
Ion Ratio Lower Upper
41 100
42 78.4 55.4 83.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

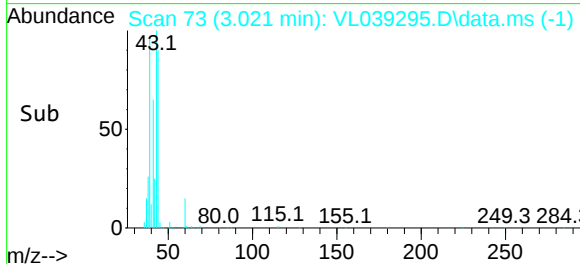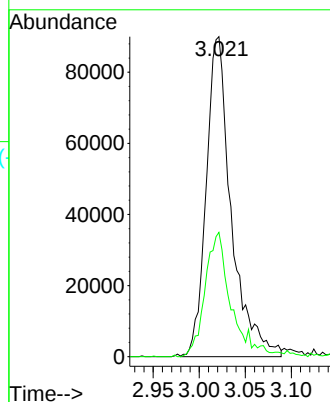

#10
Heptane
Concen: 0.521 ppbv
RT: 8.105 min Scan# 1654
Delta R.T. -0.023 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50


Tgt Ion: 43 Resp: 78444
Ion Ratio Lower Upper
43 100
57 52.7 41.4 62.2

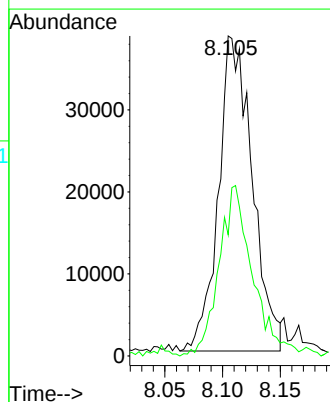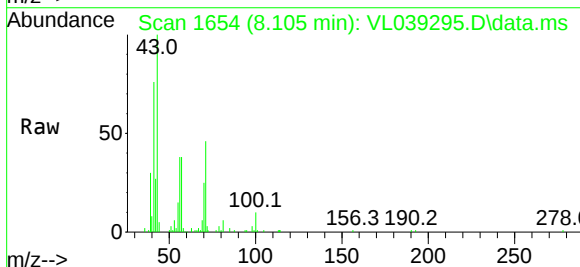

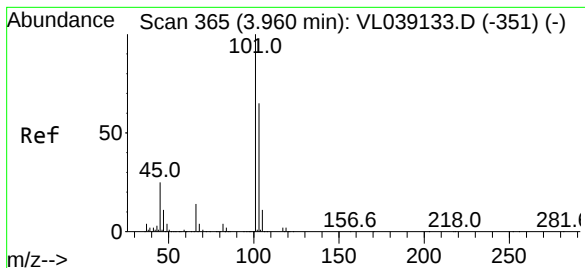

#11
Trichlorofluoromethane
Concen: 0.240 ppbv m
RT: 3.941 min Scan# 3
Delta R.T. -0.019 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument :
MSVOA_L
ClientSampleId :
IA2

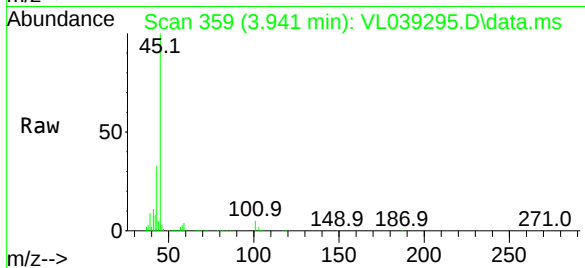

Tgt Ion:101 Resp: 4436
Ion Ratio Lower Upper
101 100
103 44.7 51.7 77.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

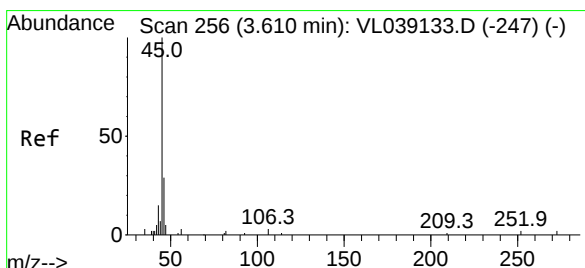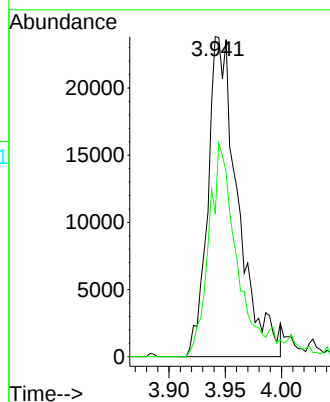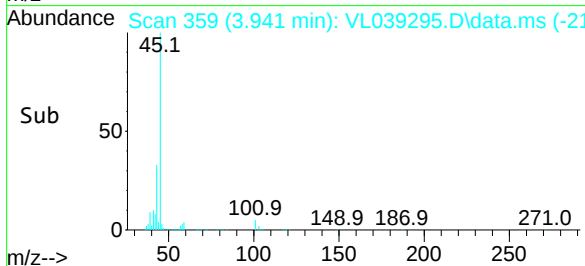

#13
Ethanol
Concen: 390.613 ppbv
RT: 3.587 min Scan# 249
Delta R.T. -0.023 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50


Tgt Ion: 45 Resp: 1373752
Ion Ratio Lower Upper
45 100
46 35.7 0.0 0.0#

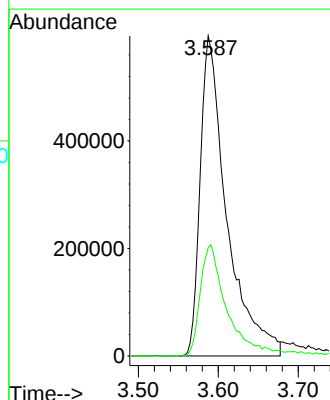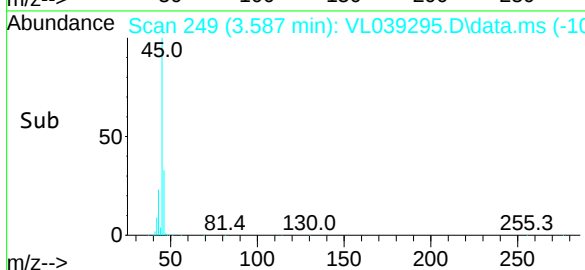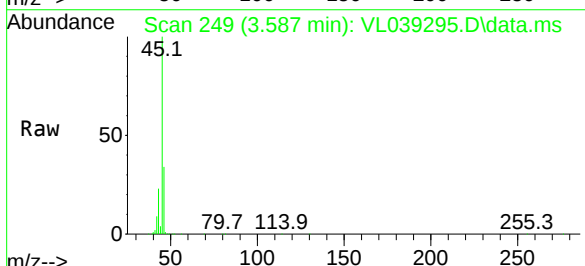



#15
Acetone
Concen: 31.158 ppbv
RT: 3.838 min Scan# 311
Delta R.T. -0.016 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument :
MSVOA_L
ClientSampleId :
IA2



Tgt Ion: 43 Resp: 3772630
Ion Ratio Lower Upper
43 100
58 24.5 22.5 33.7




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

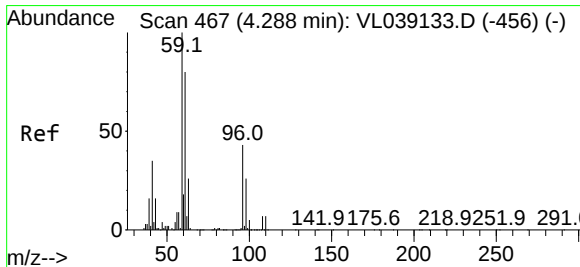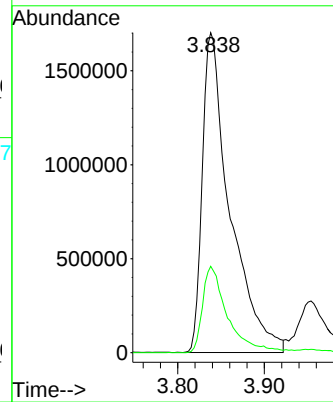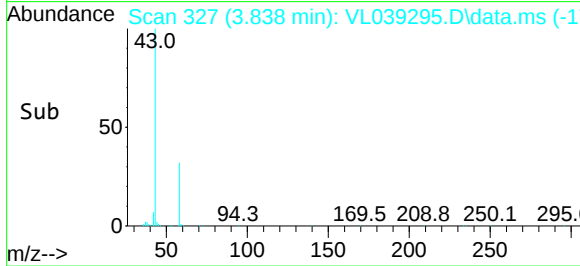

#17
tert-Butyl alcohol
Concen: 0.465 ppbv
RT: 4.288 min Scan# 467
Delta R.T. -0.000 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50


Tgt Ion: 59 Resp: 43668
Ion Ratio Lower Upper
59 100
57 0.0 9.1 13.7#

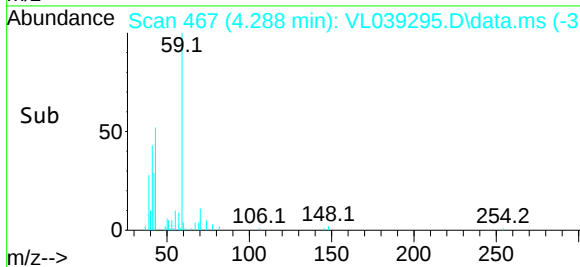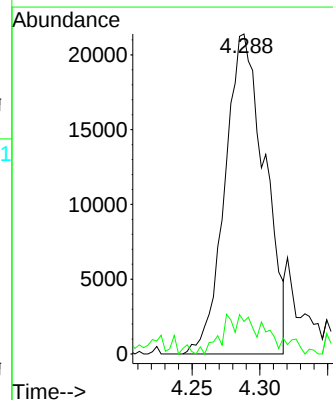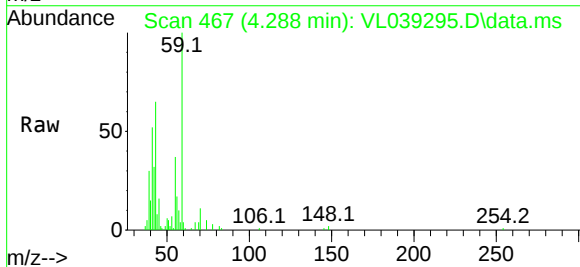



#19
Isopropyl Alcohol
Concen: 38.368 ppbv
RT: 3.954 min Scan# 30
Delta R.T. -0.010 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument :
MSVOA_L
ClientSampleId :
IA2



Tgt Ion: 45 Resp: 217892
Ion Ratio Lower Upper
45 100
58 2.1 1.8 2.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

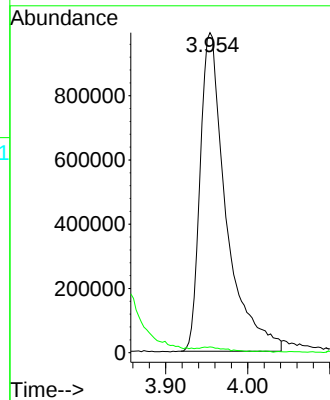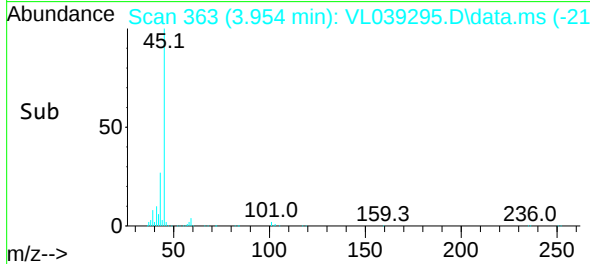

#20
Methylene Chloride
Concen: 1.200 ppbv m
RT: 4.343 min Scan# 484
Delta R.T. -0.010 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50


Tgt Ion: 84 Resp: 61239
Ion Ratio Lower Upper
84 100
49 143.3 111.1 166.7
51 33.6 35.3 52.9#
86 67.6 51.9 77.9

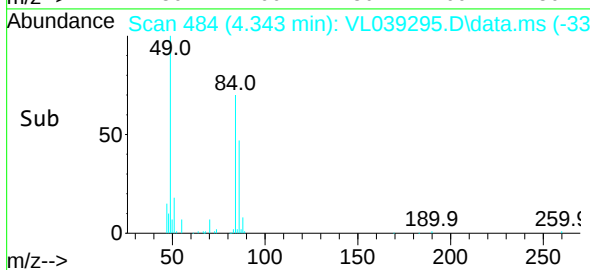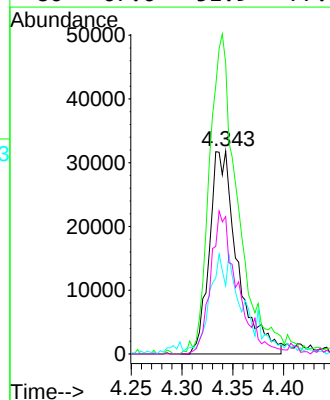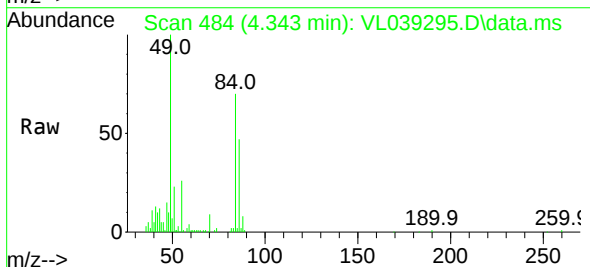



#26
Hexane
Concen: 2.008 ppbv
RT: 5.674 min Scan# 898
Delta R.T. -0.019 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument :
MSVOA_L
ClientSampleId :
IA2



Tgt Ion:	57	Resp:	24086
Ion	Ratio	Lower	Upper
57	100		
41	103.5	72.4	108.6
43	82.5	187.0	280.6
56	57.3	41.8	62.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

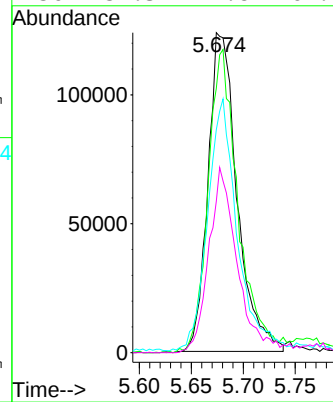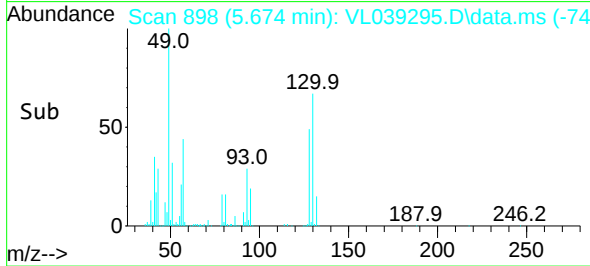

#30
Cyclohexane
Concen: 0.365 ppbv
RT: 7.124 min Scan# 1349
Delta R.T. -0.013 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50


Tgt Ion:	84	Resp:	36822
Ion	Ratio	Lower	Upper
84	100		
56	114.4	110.6	165.8
41	86.6	68.9	103.3

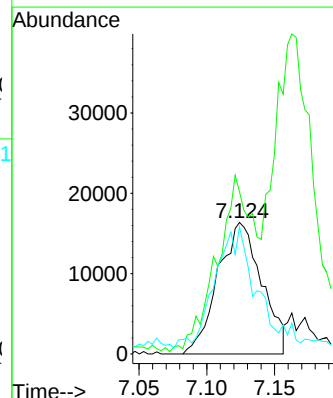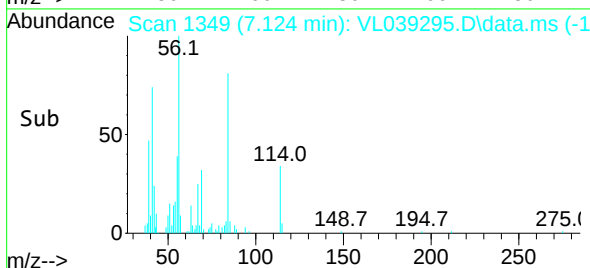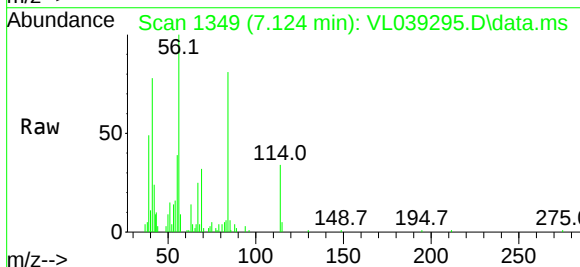



#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.163 min Scan# 114
Delta R.T. -0.019 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument :
MSVOA_L
ClientSampleId :
IA2




Tgt Ion:114 Resp: 323895
Ion Ratio Lower Upper
114 100
63 25.4 21.7 32.5
88 18.0 14.8 22.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

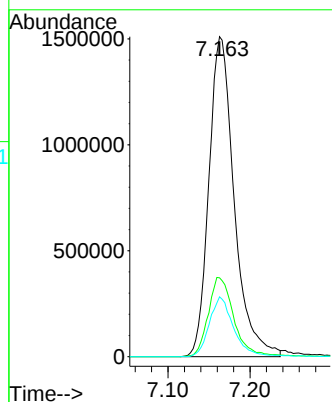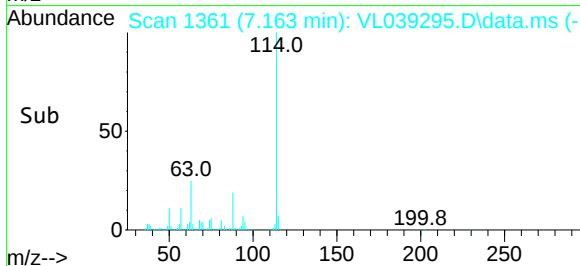


#34
2-Butanone
Concen: 1.072 ppbv
RT: 5.237 min Scan# 762
Delta R.T. -0.013 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

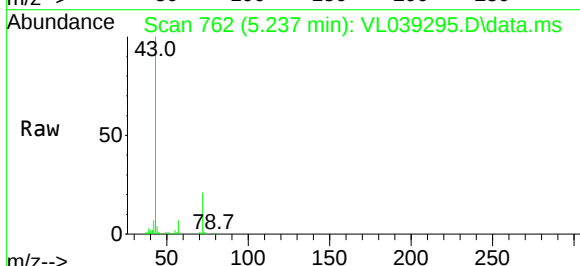


Tgt Ion: 43 Resp: 188671
Ion Ratio Lower Upper
43 100
72 24.0 18.2 27.2

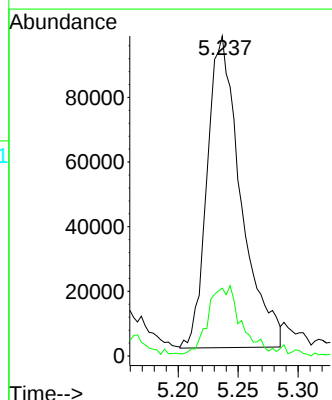



#35
Carbon Tetrachloride
Concen: 0.057 ppbv m
RT: 7.002 min Scan# 117
Delta R.T. -0.023 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument :
MSVOA_L
ClientSampleId :
IA2




Tgt Ion: 117 Resp: 13539
Ion Ratio Lower Upper
117 100
119 62.8 78.6 118.0
121 24.6 25.4 38.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

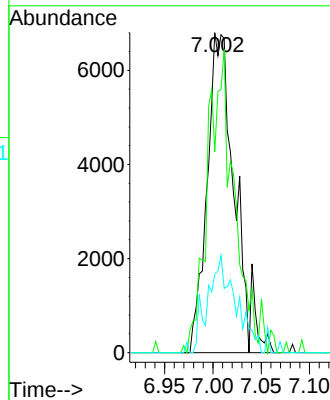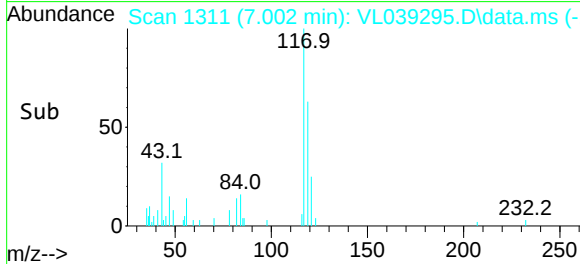


#36
Benzene
Concen: 0.450 ppbv
RT: 6.873 min Scan# 1271
Delta R.T. -0.026 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

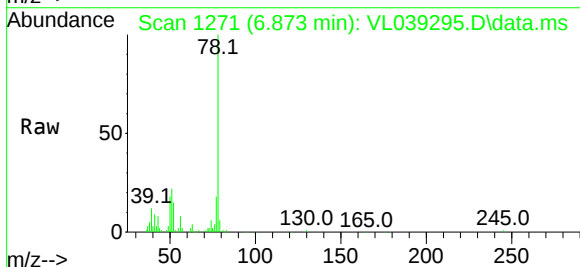


Tgt Ion: 78 Resp: 118323
Ion Ratio Lower Upper
78 100
77 16.5 18.6 27.8
50 17.2 15.8 23.8

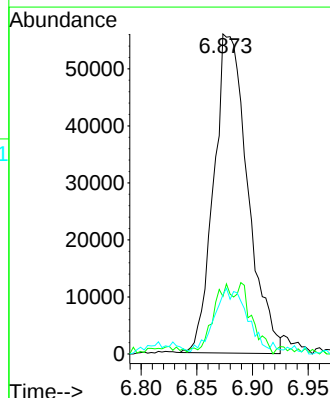



#37
1,2-Dichloroethane
Concen: 0.189 ppbv
RT: 6.298 min Scan# 1097
Delta R.T. -0.016 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument :
MSVOA_L
ClientSampleId :
IA2



Tgt Ion: 62 Resp: 32650
Ion Ratio Lower Upper
62 100
98 6.9 4.3 6.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

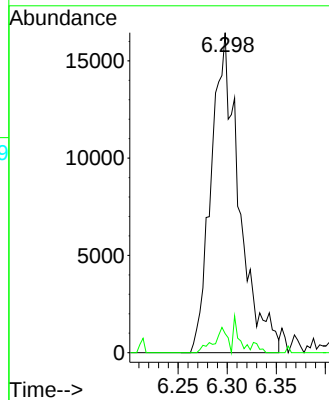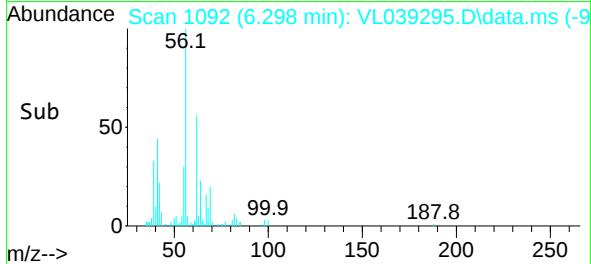

#41
Tetrahydrofuran
Concen: 0.324 ppbv
RT: 6.047 min Scan# 1014
Delta R.T. -0.007 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50


Tgt Ion: 42 Resp: 34237
Ion Ratio Lower Upper
42 100
72 42.2 32.0 48.0
71 33.1 31.1 46.7

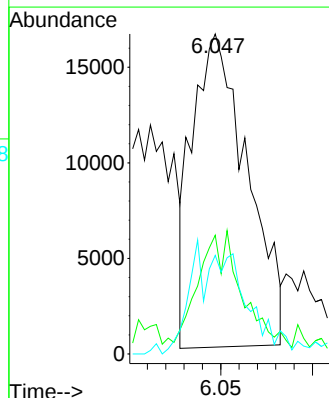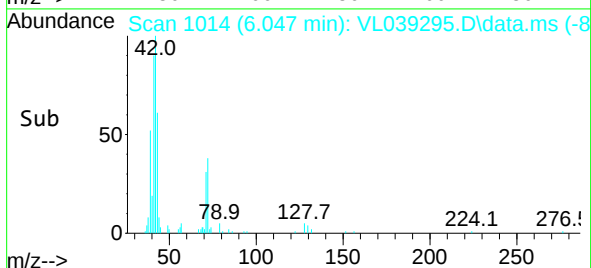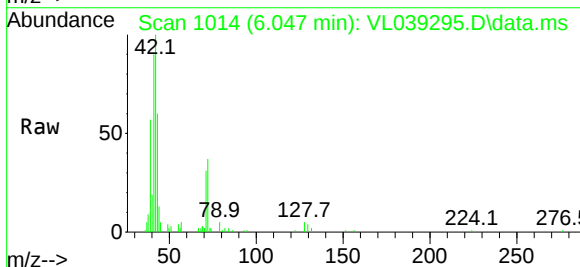



#44
2,2,4-Trimethylpentane
Concen: 1.132 ppbv
RT: 7.857 min Scan# 1577
Delta R.T. -0.019 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument : MSVOA_L
ClientSampleId : IA2




Tgt Ion: 57 Resp: 52052
Ion Ratio Lower Upper
57 100
41 38.0 26.2 39.4
56 34.3 24.7 37.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

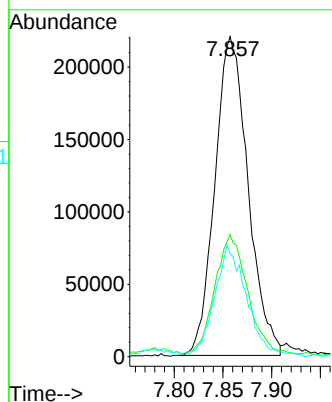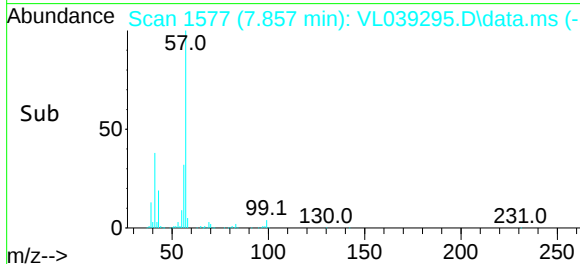


#52
Tetrachloroethene
Concen: 0.148 ppbv m
RT: 11.208 min Scan# 2619
Delta R.T. -0.023 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

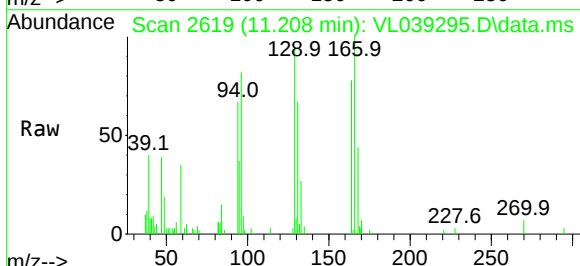


Tgt Ion:164 Resp: 15189
Ion Ratio Lower Upper
164 100
166 128.2 96.3 144.5
129 121.6 82.5 123.7
131 86.0 82.1 123.1

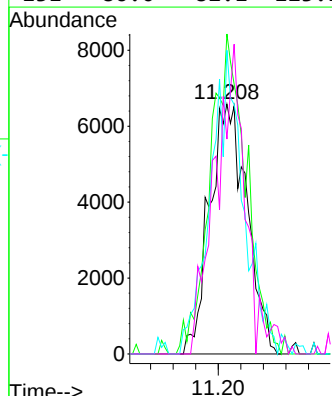



#53
Toluene
Concen: 2.377 ppbv
RT: 9.790 min Scan# 2185
Delta R.T. -0.023 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument : MSVOA_L
ClientSampleId : 1A2




Tgt Ion: 91 Resp: 71973
Ion Ratio Lower Upper
91 100
92 60.8 48.1 72.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

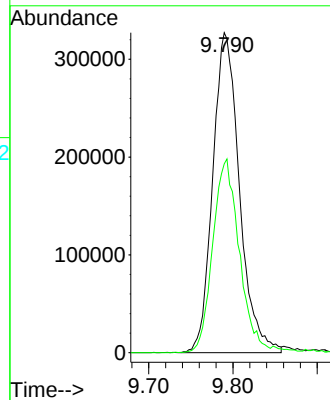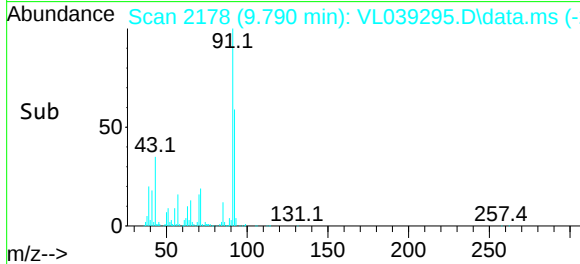


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.069 min Scan# 2887
Delta R.T. -0.023 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

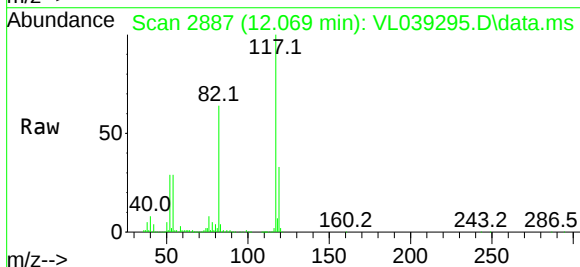

Tgt Ion:117 Resp: 2915459
Ion Ratio Lower Upper
117 100
82 66.4 55.1 82.7
119 34.2 24.7 37.1

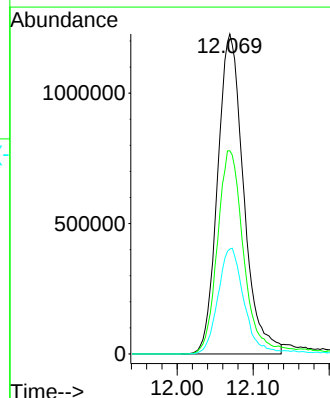

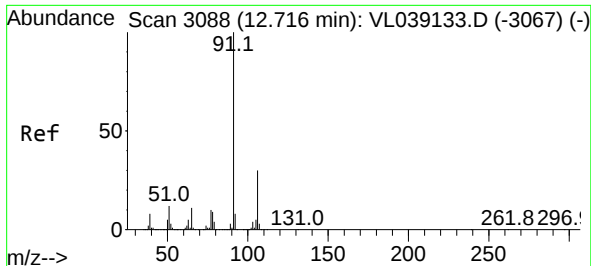





#58
Ethyl Benzene
Concen: 0.434 ppbv
RT: 12.693 min Scan# 3088
Delta R.T. -0.023 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

Instrument :
MSVOA_L
ClientSampleId :
IA2

Tgt Ion: 91 Resp: 17418
Ion Ratio Lower Upper
91 100
106 30.1 24.2 36.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

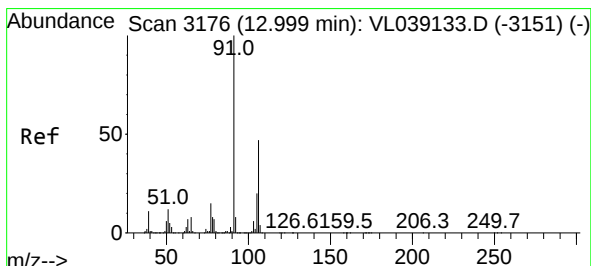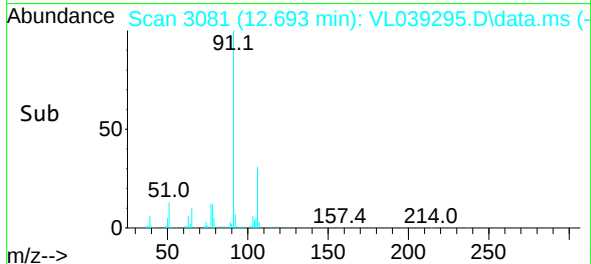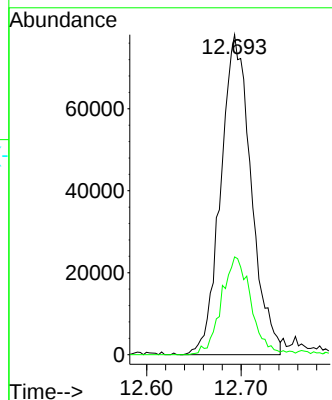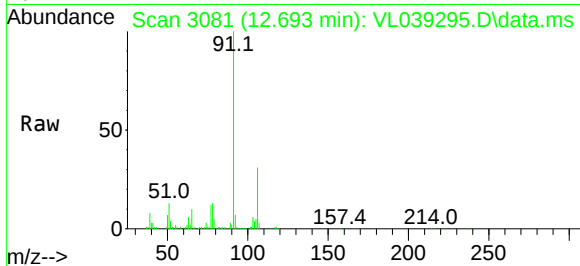

#59
m/p-Xylene
Concen: 1.548 ppbv m
RT: 12.950 min Scan# 3161
Delta R.T. -0.048 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

Tgt Ion: 91 Resp: 547369
Ion Ratio Lower Upper
91 100
106 46.6 34.3 51.5

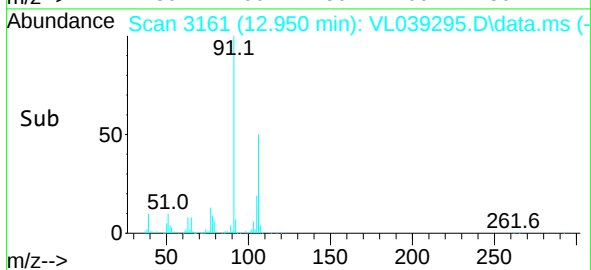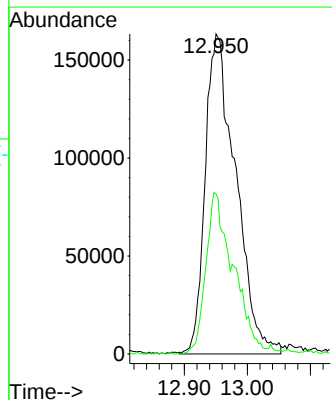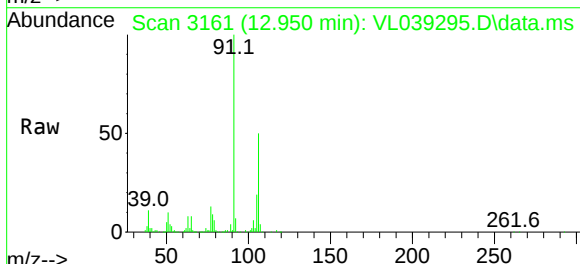

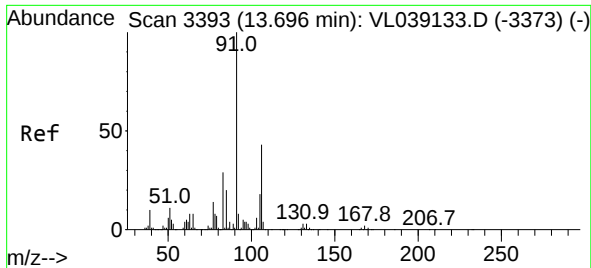





#60
o-Xylene
Concen: 0.658 ppbv m
RT: 13.671 min Scan# 3385
Delta R.T. -0.026 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

Instrument :
MSVOA_L
ClientSampleId :
IA2

Tgt Ion: 91 Resp: 21866
Ion Ratio Lower Upper
91 100
106 43.1 22.3 66.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

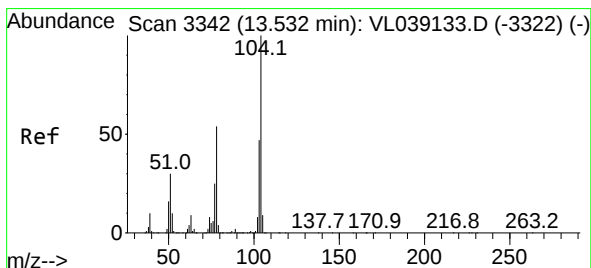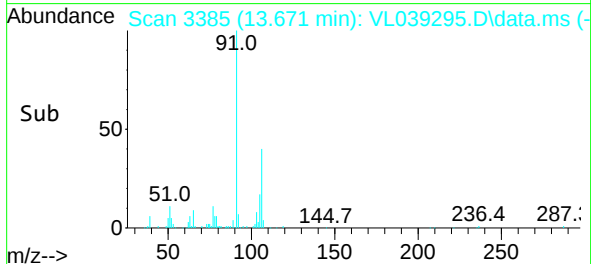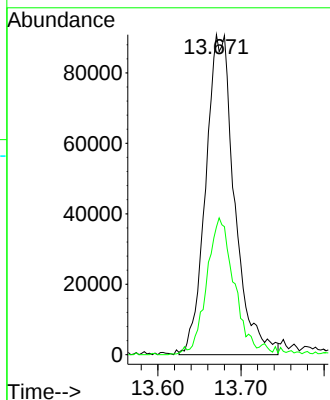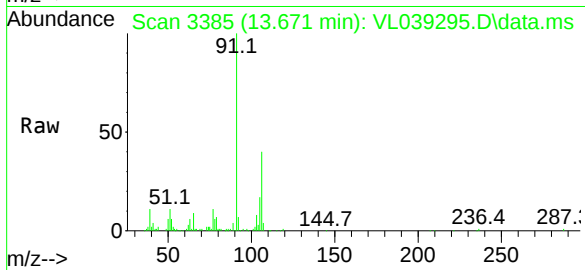

#61
Styrene
Concen: 0.647 ppbv
RT: 13.513 min Scan# 3336
Delta R.T. -0.019 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50


Tgt Ion:104 Resp: 115070
Ion Ratio Lower Upper
104 100
78 57.3 45.7 68.5
103 52.0 39.6 59.4

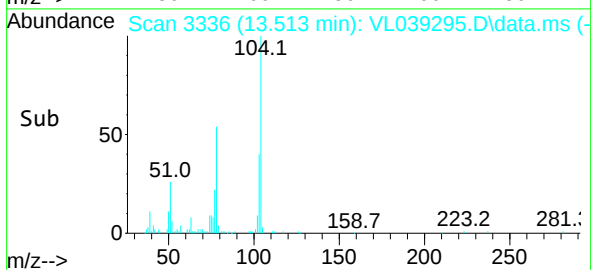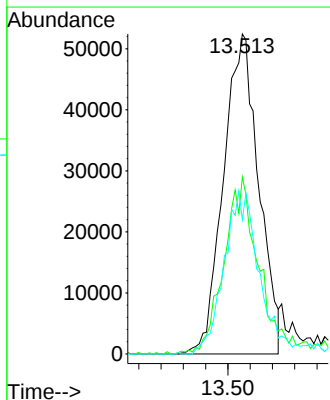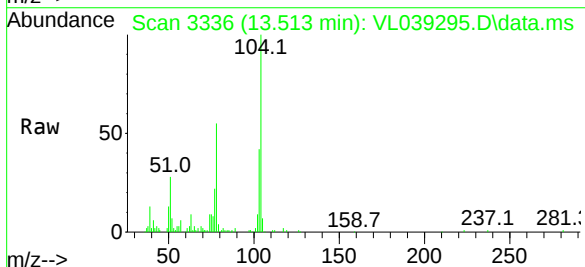

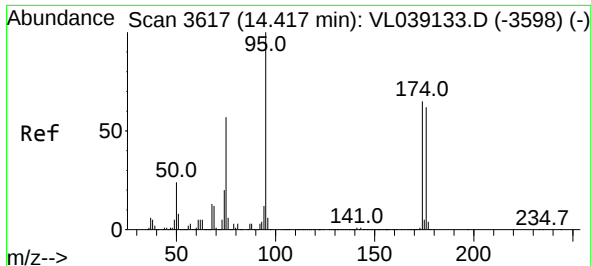

#68
1-Bromo-4-Fluorobenzene
Concen: 9.622 ppbv
RT: 14.397 min Scan# 30
Delta R.T. -0.019 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50




Instrument :
MSVOA_L
ClientSampleId :
IA2




Tgt Ion: 95 Resp: 231922
Ion Ratio Lower Upper
95 100
174 71.8 53.8 80.8
175 5.3 4.1 6.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
Supervised By :Mahesh Dadoda 06/16/2022

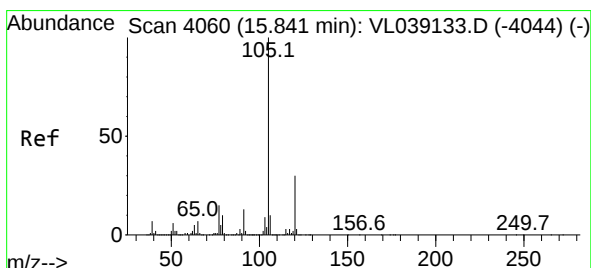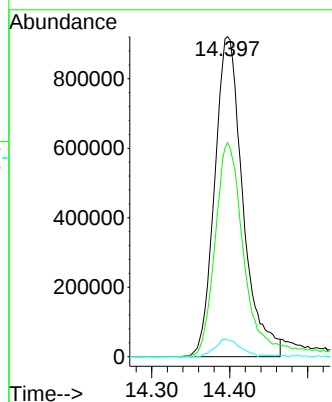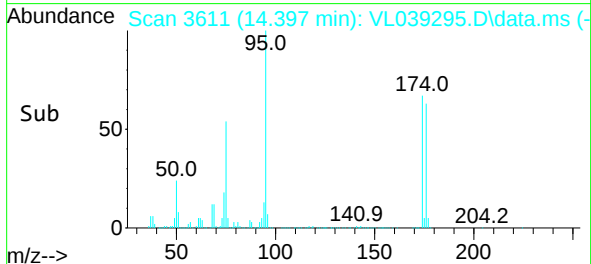


#72
4-Ethyltoluene
Concen: 0.211 ppbv
RT: 15.818 min Scan# 4053
Delta R.T. -0.023 min
Lab File: VL039295.D
Acq: 15 Jun 2022 11:50

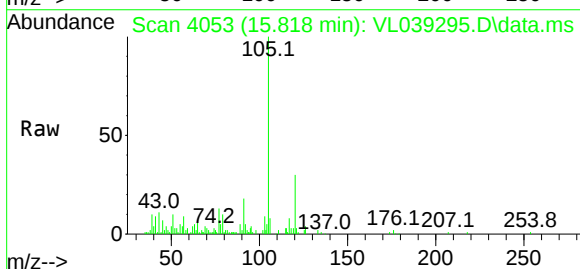


Tgt Ion:105 Resp: 82181
Ion Ratio Lower Upper
105 100
120 34.7 23.9 35.9
91 18.1 10.6 16.0#
77 18.0 11.7 17.5#

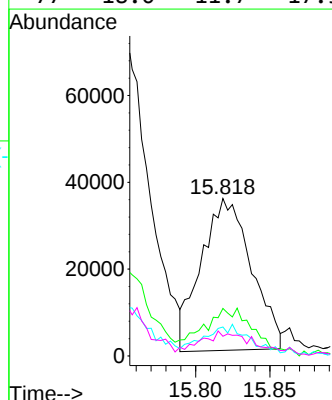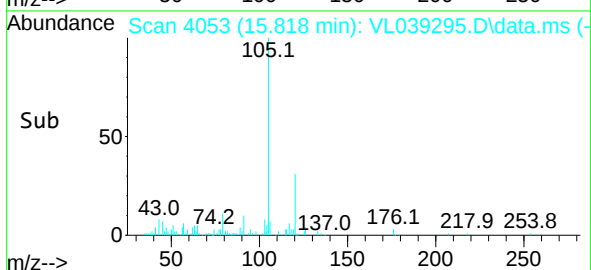

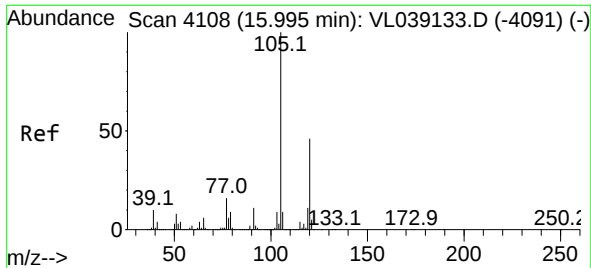

#73
 1,3,5-Trimethylbenzene
 Concen: 0.219 ppbv
 RT: 15.979 min Scan# 4108
 Delta R.T. -0.016 min
 Lab File: VL039295.D
 Acq: 15 Jun 2022 11:50




Instrument :
 MSVOA_L
 ClientSampleId :
 IA2

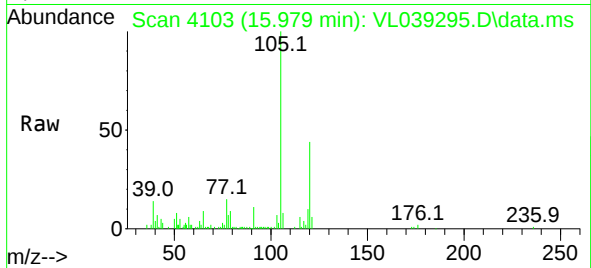


Tgt Ion:105 Resp: 76910
 Ion Ratio Lower Upper
 105 100
 120 43.5 36.7 55.1

Manual Integrations
 APPROVED



Reviewed By :Semsettin Yesilyurt 06/16/2022
 Supervised By :Mahesh Dadoda 06/16/2022

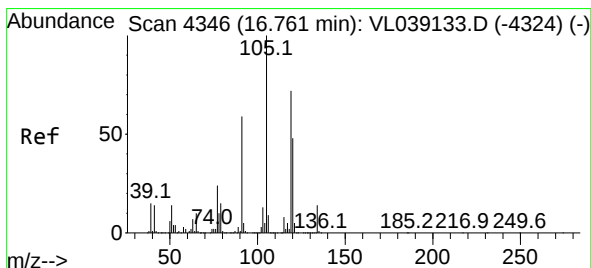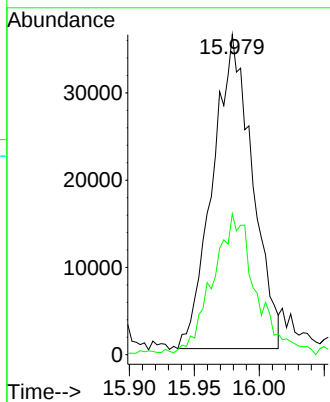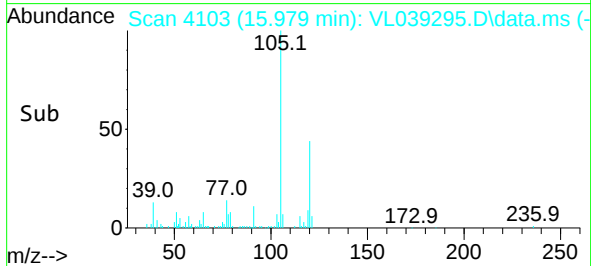


#74
 1,2,4-Trimethylbenzene
 Concen: 0.742 ppbv
 RT: 16.744 min Scan# 4341
 Delta R.T. -0.016 min
 Lab File: VL039295.D
 Acq: 15 Jun 2022 11:50

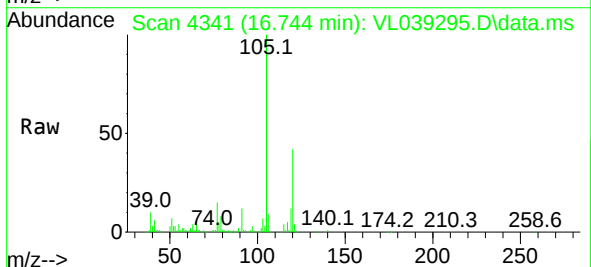

Tgt Ion:105 Resp: 290945
 Ion Ratio Lower Upper
 105 100
 120 41.3 38.1 57.1
 91 10.6 47.4 71.0#
 77 14.4 19.5 29.3#

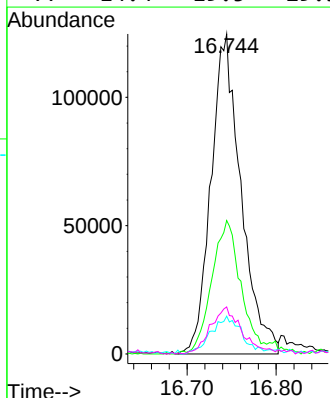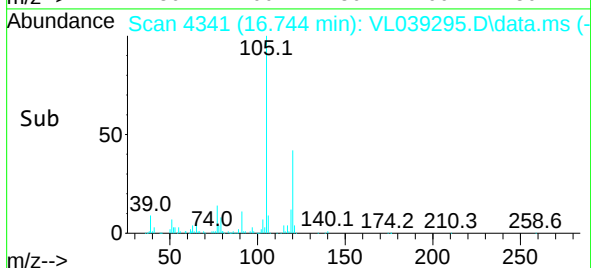

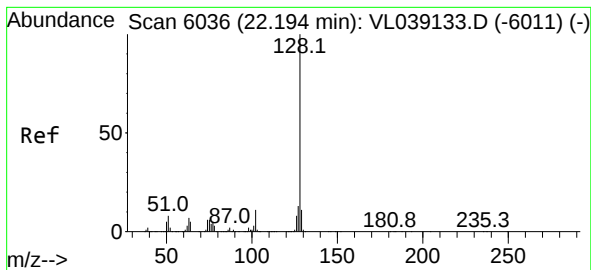

#79

Naphthalene

Concen: 0.109 ppbv m

RT: 22.178 min Scan# 6031

Delta R.T. -0.016 min

Lab File: VL039295.D

Acq: 15 Jun 2022 11:50

Instrument :

MSVOA_L

ClientSampleId :

IA2

Tgt Ion:128 Resp: 3298

Ion Ratio Lower Upper

128 100

127 15.9 10.4 15.6

129 9.9 9.0 13.6

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/16/2022

Supervised By :Mahesh Dadoda 06/16/2022

